

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN111918\
Quantitation Report (Not Reviewed)

Data File : BN003616.D
Acq On : 20 Nov 2018 04:01
Operator : MJ/SJ
Sample : J5928-18
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A40Y6

Quant Time: Nov 20 08:28:38 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 20 03:27:39 2018
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.84	152	7389	0.40	ng/ul	0.00
2) Naphthalene-d8	10.64	136	30318	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.48	164	16957	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.22	188	40734	0.40	ng/ul	0.00
16) Chrysene-d12	21.40	240	43985	0.40	ng/ul	0.00
20) Perylene-d12	23.71	264	39994	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.23	152	6589	0.14	ng/ul	0.00
14) Fluoranthene-d10	19.24	212	18066	0.15	ng/ul	0.00
Target Compounds						
23) Benzo(a)pyrene	23.56	252	5790	0.040	ng/ul#	Qvalue 28


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BN003616.D
Acq On : 20 Nov 2018 04:01
Operator : MJ/SJ
Sample : J5928-18
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A40Y6

Quant Time: Nov 20 08:28:38 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 20 03:27:39 2018
Response via : Initial Calibration

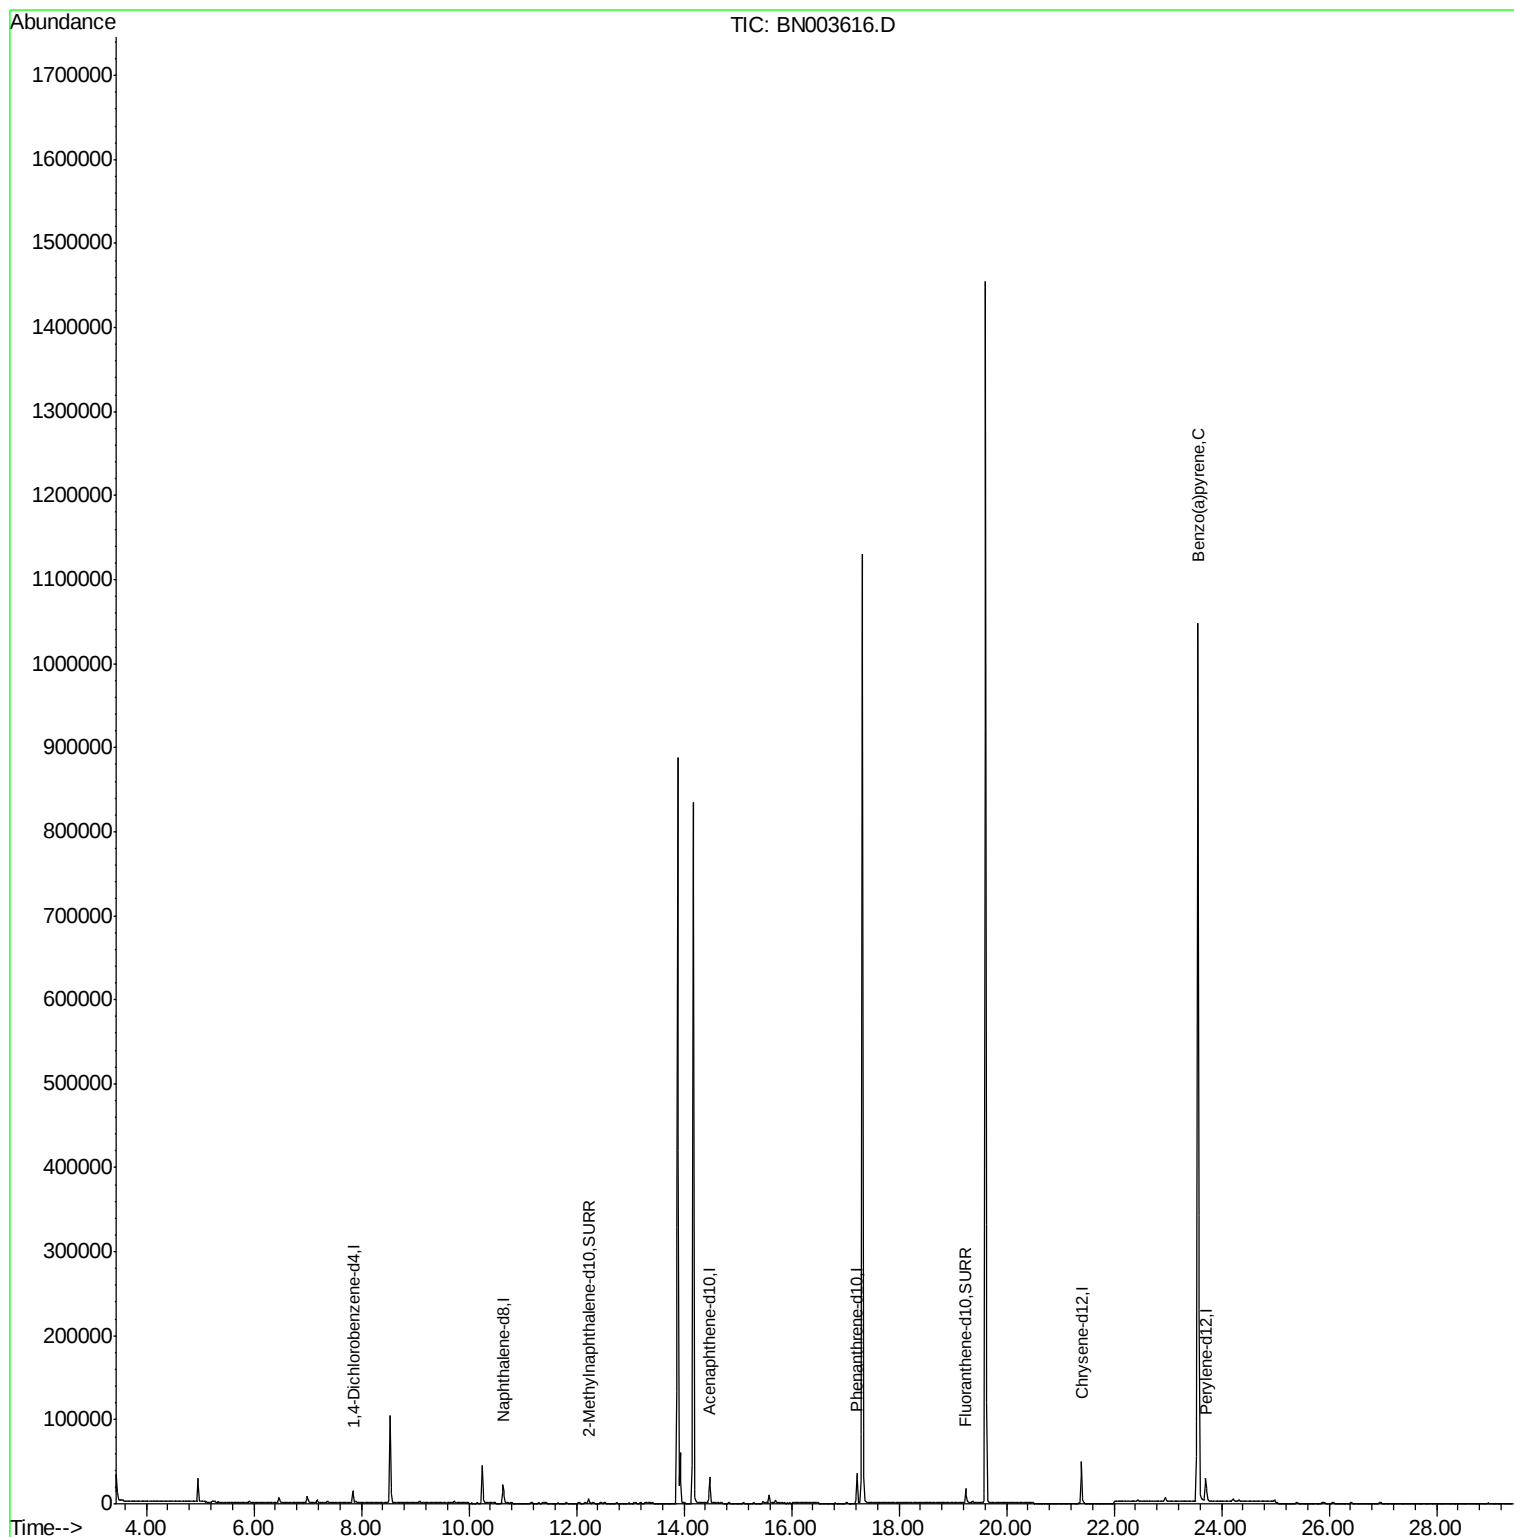

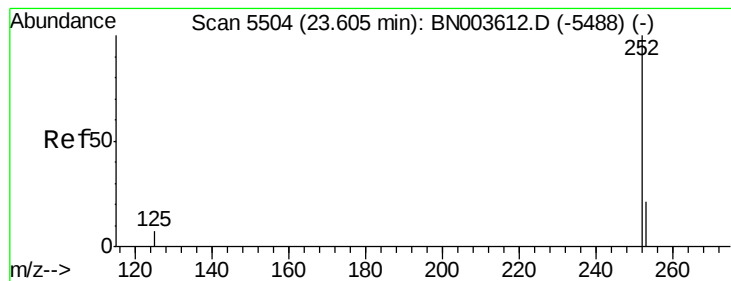

#23

Benzo(a)pyrene

Concen: 0.040 ng/ul

RT: 23.56 min Scan# 5489

Delta R.T. -0.04 min

Lab File: BN003616.D


Acq: 20 Nov 2018 04:01

Instrument :

BNA_N

ClientSampleId :

A40Y6

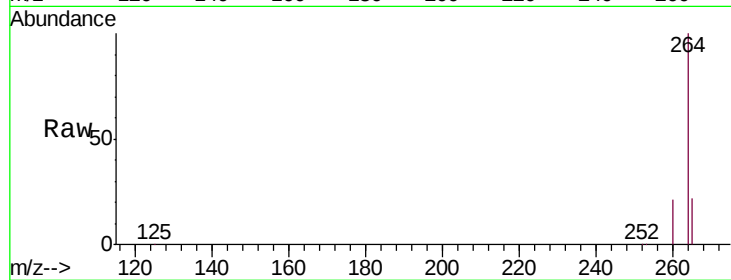

Tgt Ion: 252 Resp: 5790

Ion Ratio Lower Upper

252 100

253 44.7 19.0 28.4#

125 62.9 10.2 15.4#

