

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN111918\
Quantitation Report (QT Reviewed)


Data File : BN003598.D
Acq On : 19 Nov 2018 17:31
Operator : MJ/SJ
Sample : PB114864BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Quant Time: Nov 20 01:57:26 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 20 01:46:26 2018
Response via : Initial Calibration

Instrument :
BNA_N
ClientSampleId :
SBLK64

Manual Integrations
APPROVED

Sohil
11/20/2018 5:13:08 PM

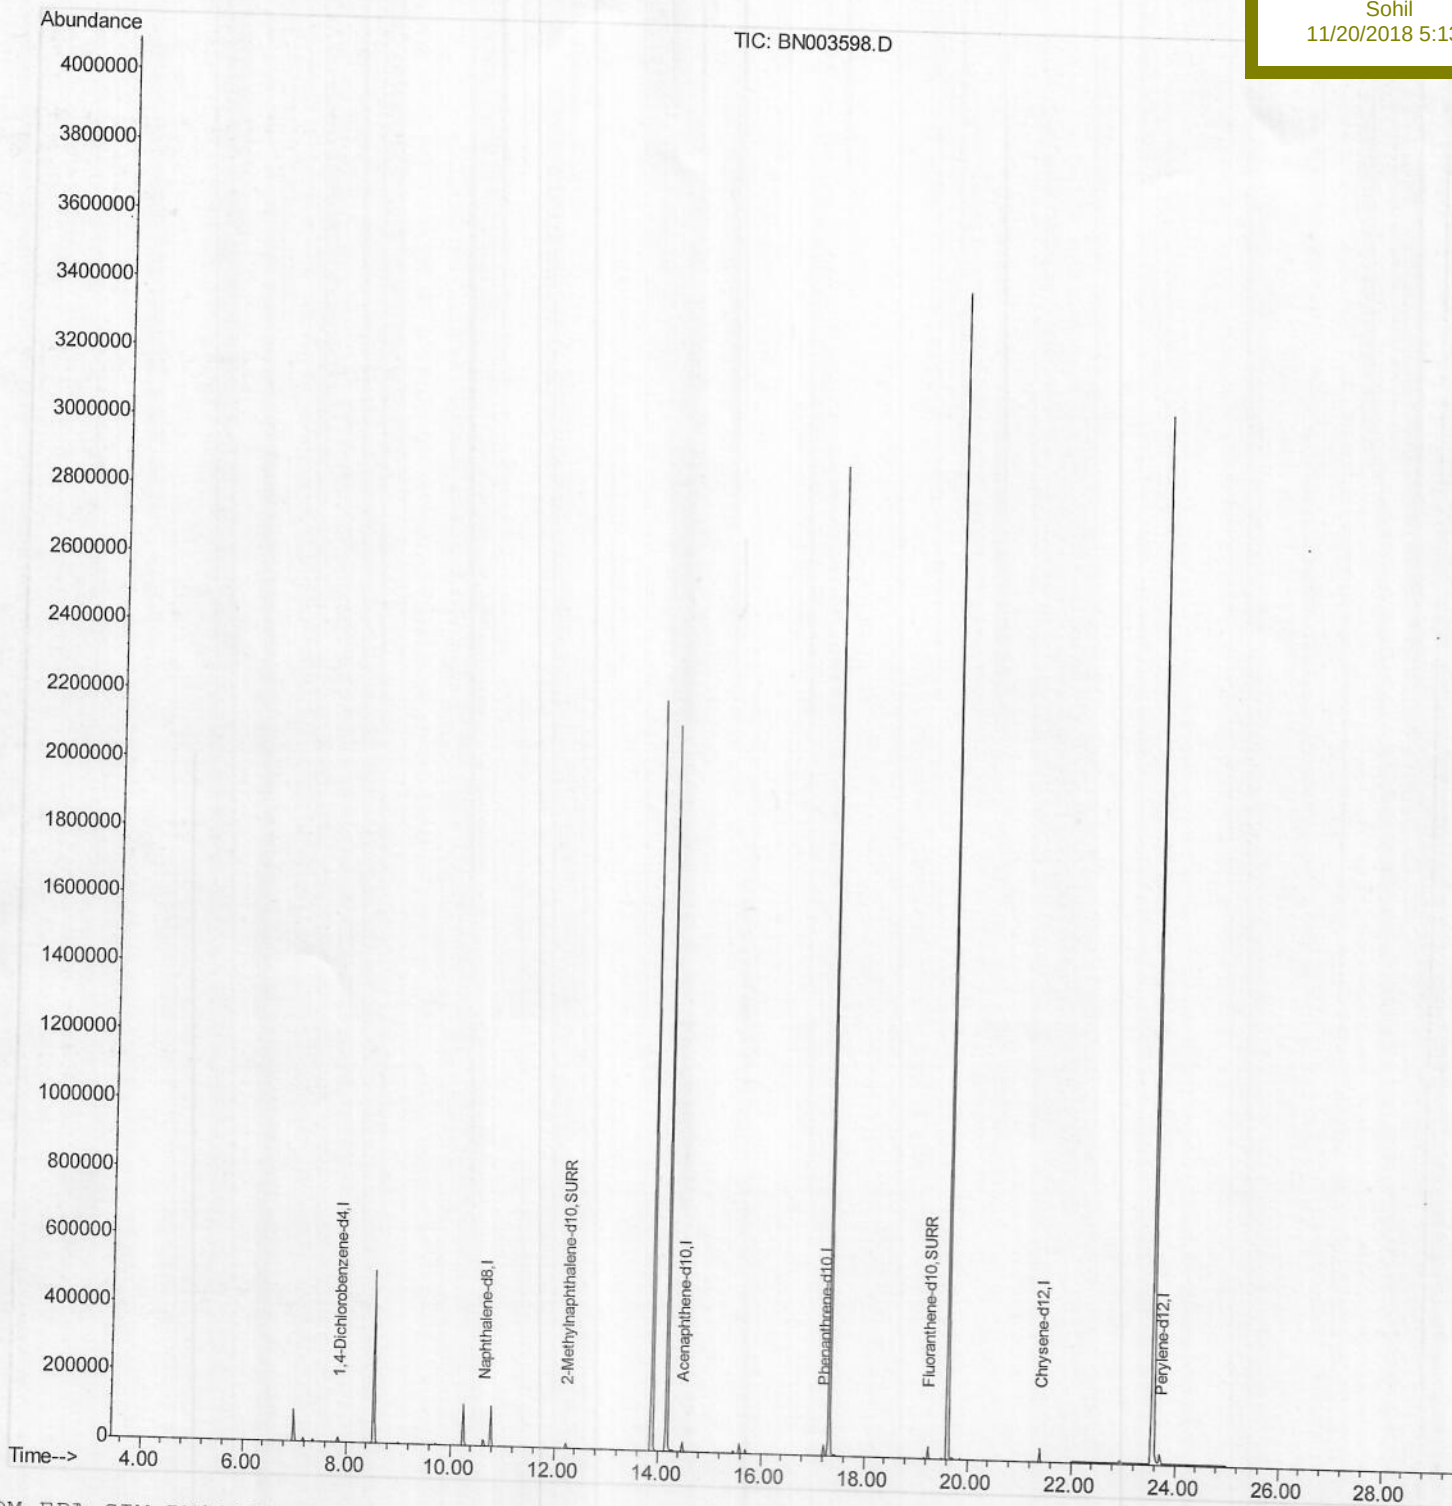

SOM-EPA-SIM-BN111918.M Tue Nov 20 01:55:24 2018

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN111918\
Quantitation Report (Qedit)


Data File : BN003598.D
Acq On : 19 Nov 2018 17:31
Operator : MJ/SJ
Sample : PB114864BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Quant Time: Nov 20 01:49:35 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 20 01:46:26 2018
Response via : Initial Calibration

Instrument :
BNA_N
ClientSampleId :
SBLK64

Manual Integrations
APPROVED

Sohil
11/20/2018 5:13:08 PM

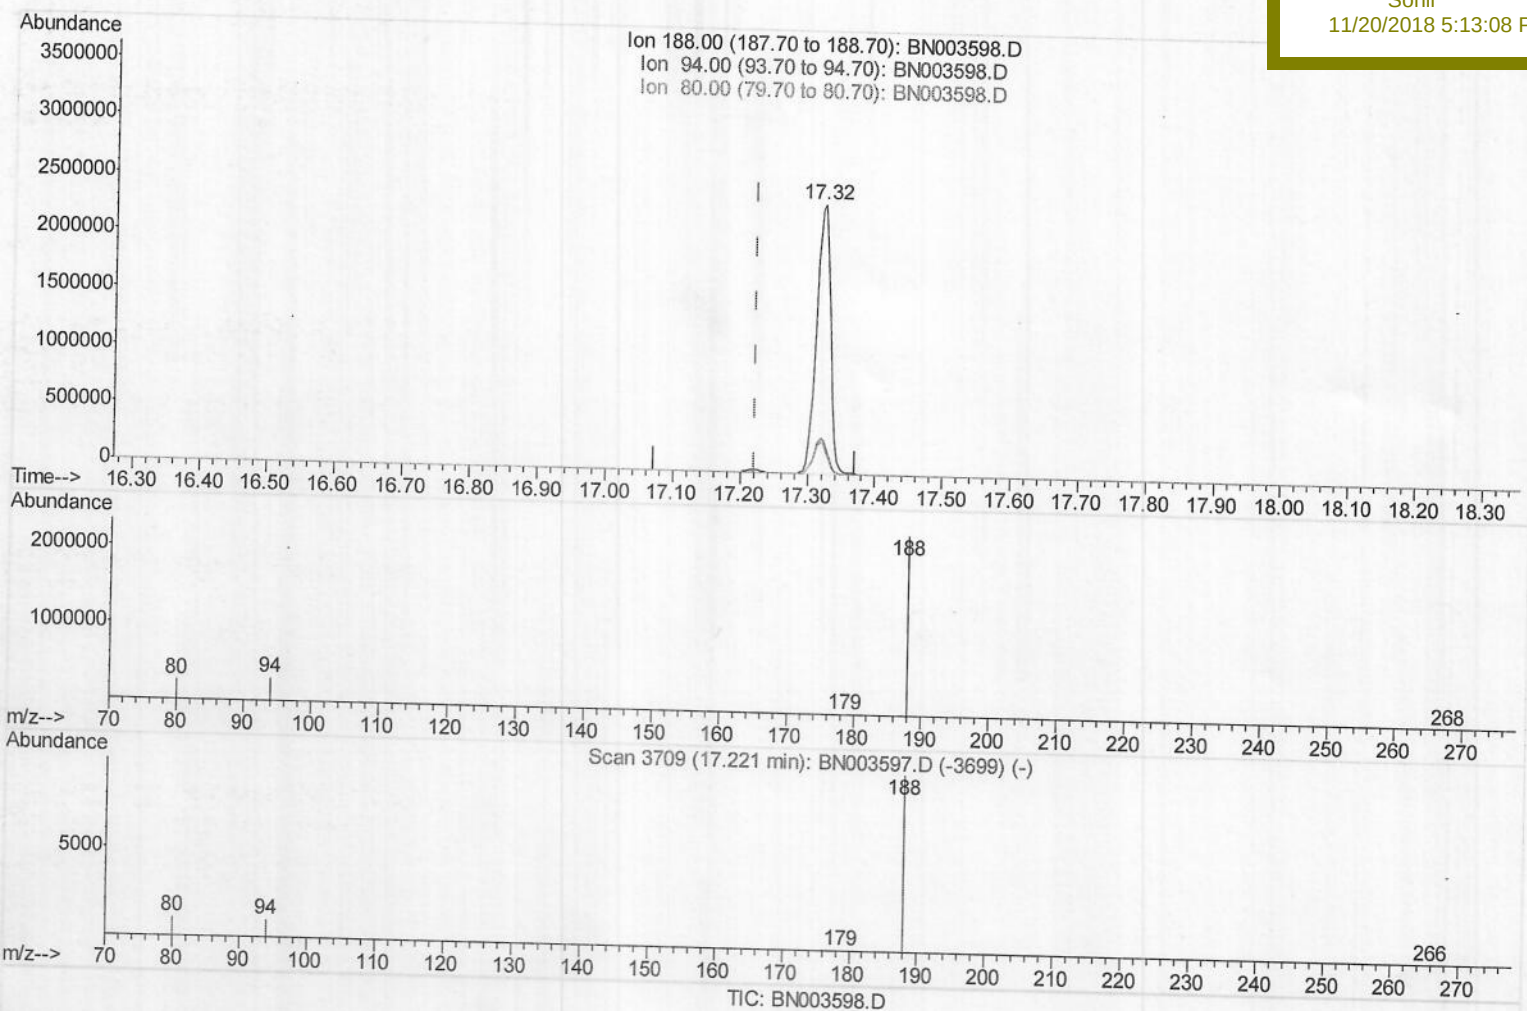

(10) Phenanthrene-d10 (I)

17.322min (+0.101) 0.40ng/ul

response 3353725

Ion	Exp%	Act%
188.00	100	100
94.00	10.40	12.45
80.00	11.60	10.95
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN111918\
Quantitation Report (Qedit)


Data File : BN003598.D
Acq On : 19 Nov 2018 17:31
Operator : MJ/SJ
Sample : PB114864BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK64

Manual Integrations
APPROVED

Sohil
11/20/2018 5:13:08 PM

Quant Time: Nov 20 01:49:35 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 20 01:46:26 2018
Response via : Initial Calibration

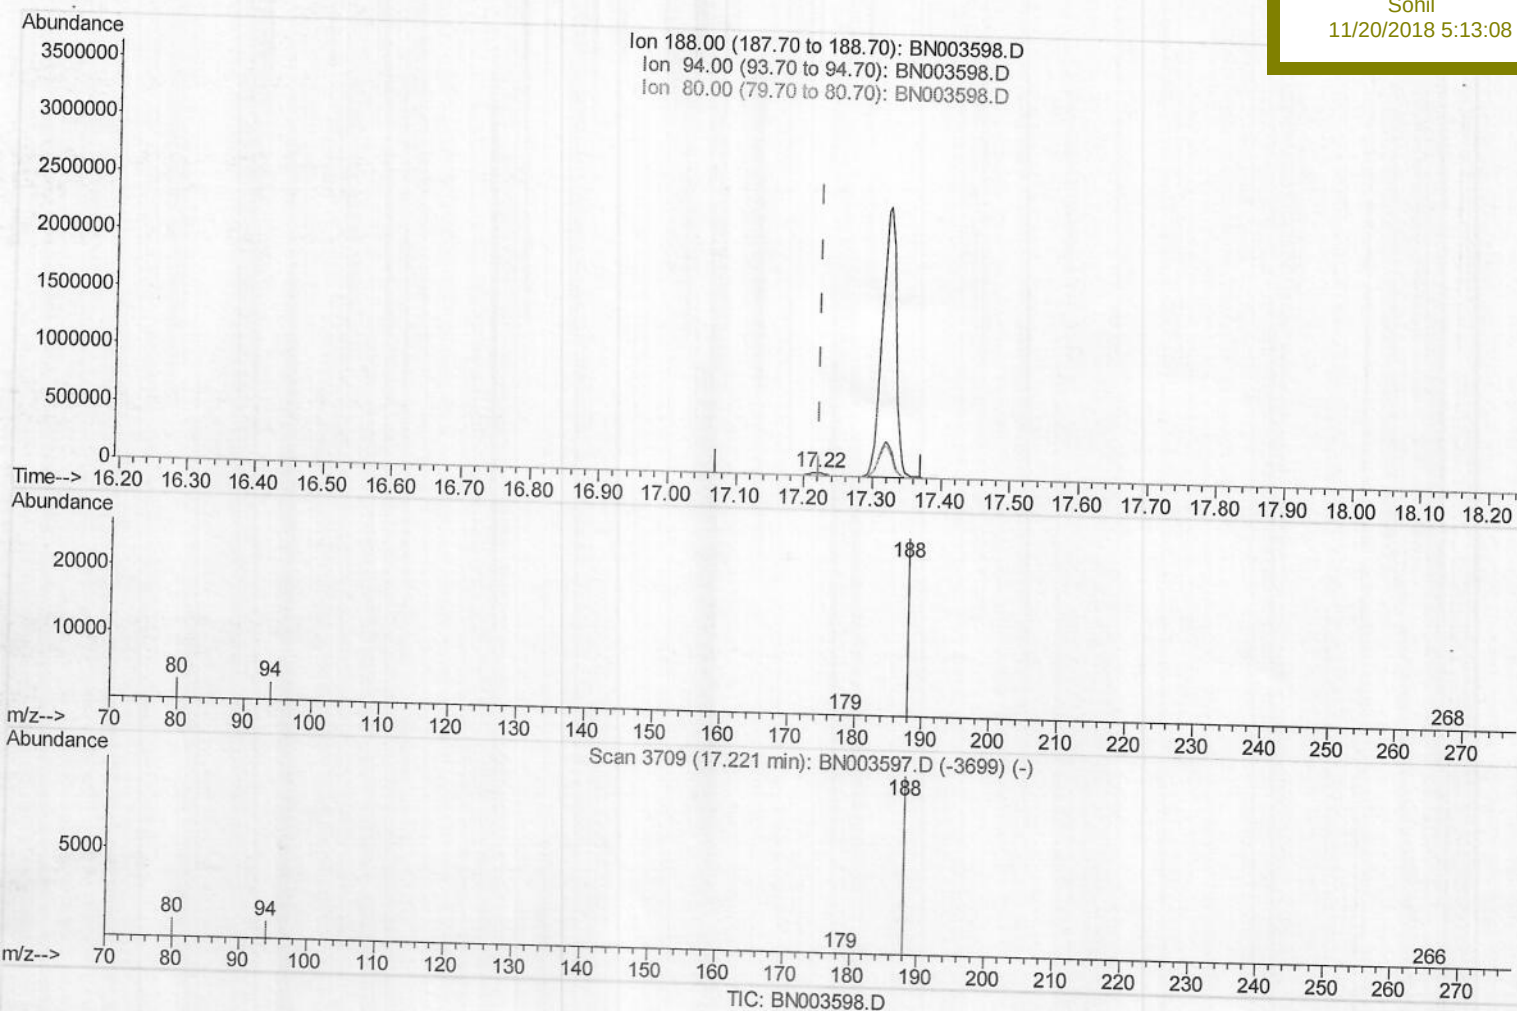

(10) Phenanthrene-d10 (I)

17.221min (-0.000) 0.40ng/ul m

response 36842

Ion	Exp%	Act%
188.00	100	100
94.00	10.40	10.02
80.00	11.60	10.91
0.00	0.00	0.00

JU
11/20/18

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN111918\
Quantitation Report (Qedit)



Data File : BN003598.D
Acq On : 19 Nov 2018 17:31
Operator : MJ/SJ
Sample : PB114864BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Quant Time: Nov 20 01:55:28 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 20 01:46:26 2018
Response via : Initial Calibration

Instrument :
BNA_N
ClientSampleId :
SBLK64

Manual Integrations
APPROVED

Sohil
11/20/2018 5:13:08 PM

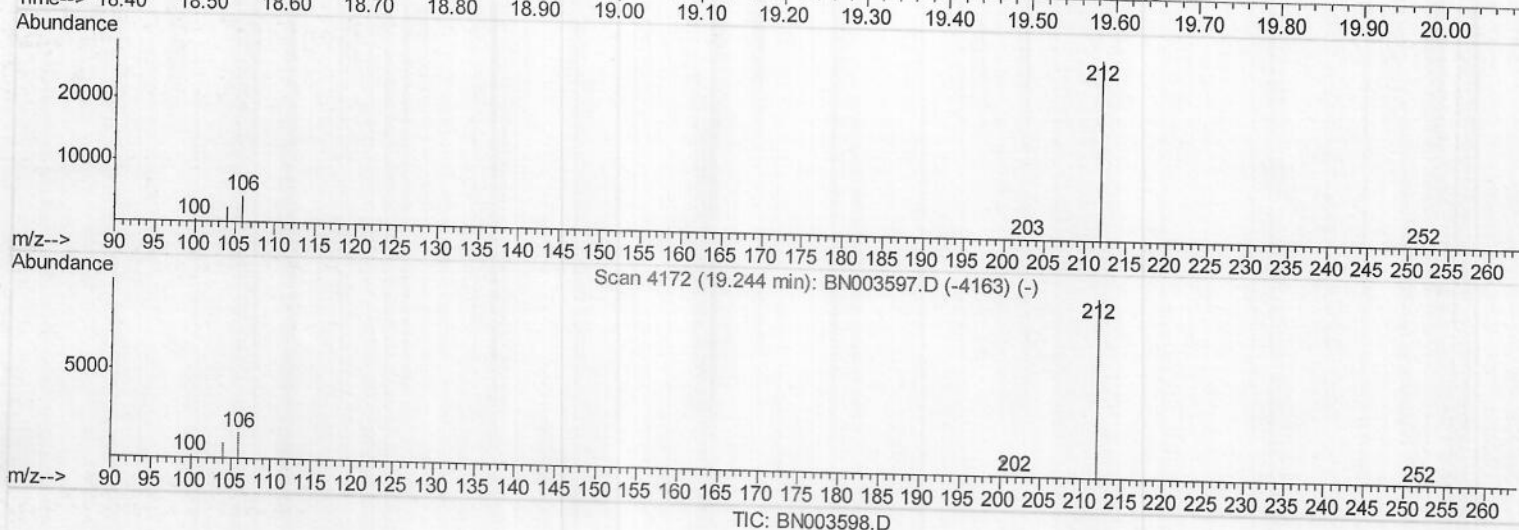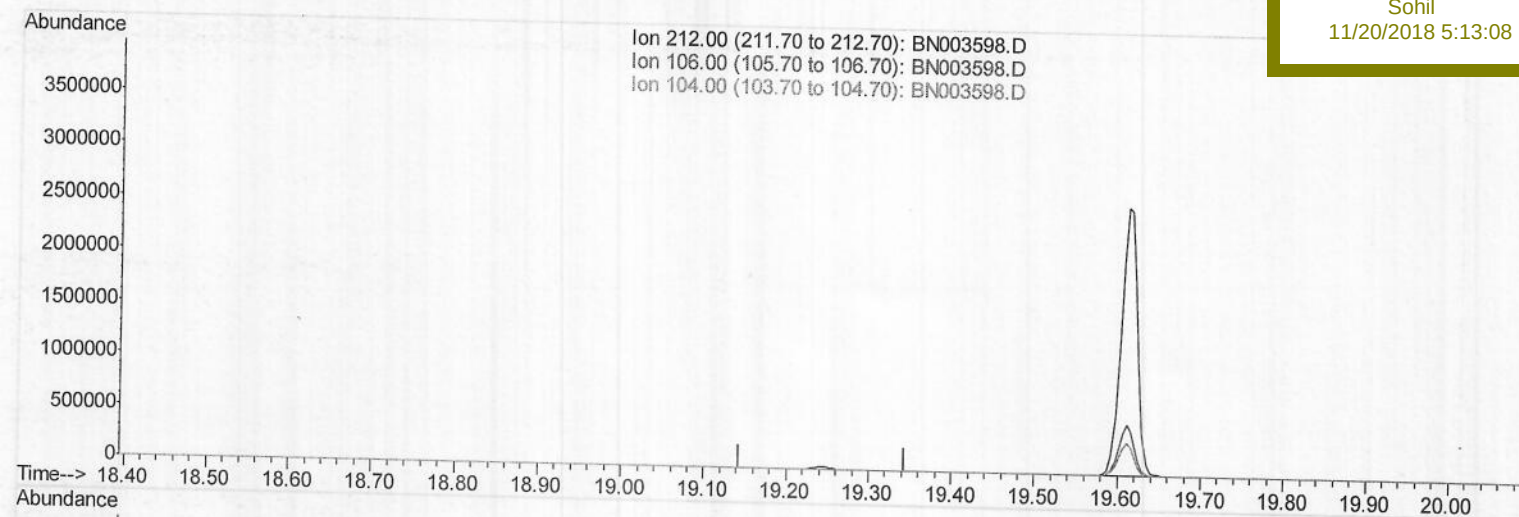

(14) Fluoranthene-d10 (SURR)

19.244min (-19.244) 0.00ng/ul

response 0

Ion	Exp%	Act%
212.00	100	0.00
106.00	14.20	0.00#
104.00	8.00	0.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN111918\
Quantitation Report (Qedit)



Data File : BN003598.D
Acq On : 19 Nov 2018 17:31
Operator : MJ/SJ
Sample : PB114864BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Quant Time: Nov 20 01:55:28 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 20 01:46:26 2018
Response via : Initial Calibration

Instrument :
BNA_N
ClientSampleId :
SBLK64

Manual Integrations
APPROVED

Sohil
11/20/2018 5:13:08 PM

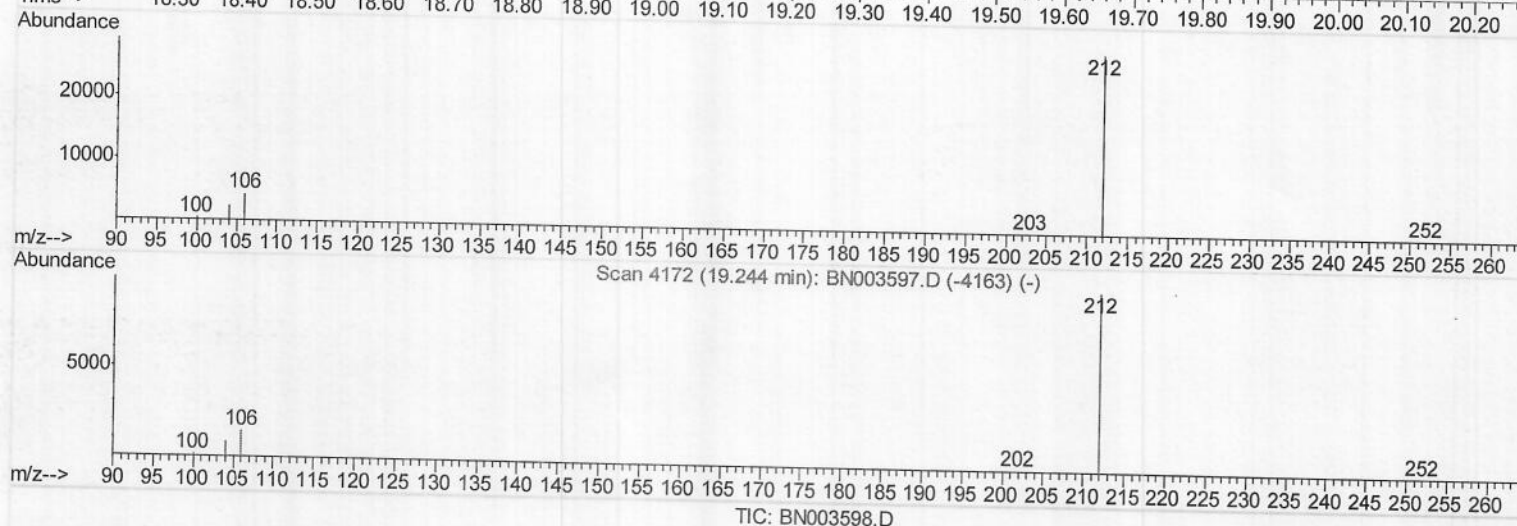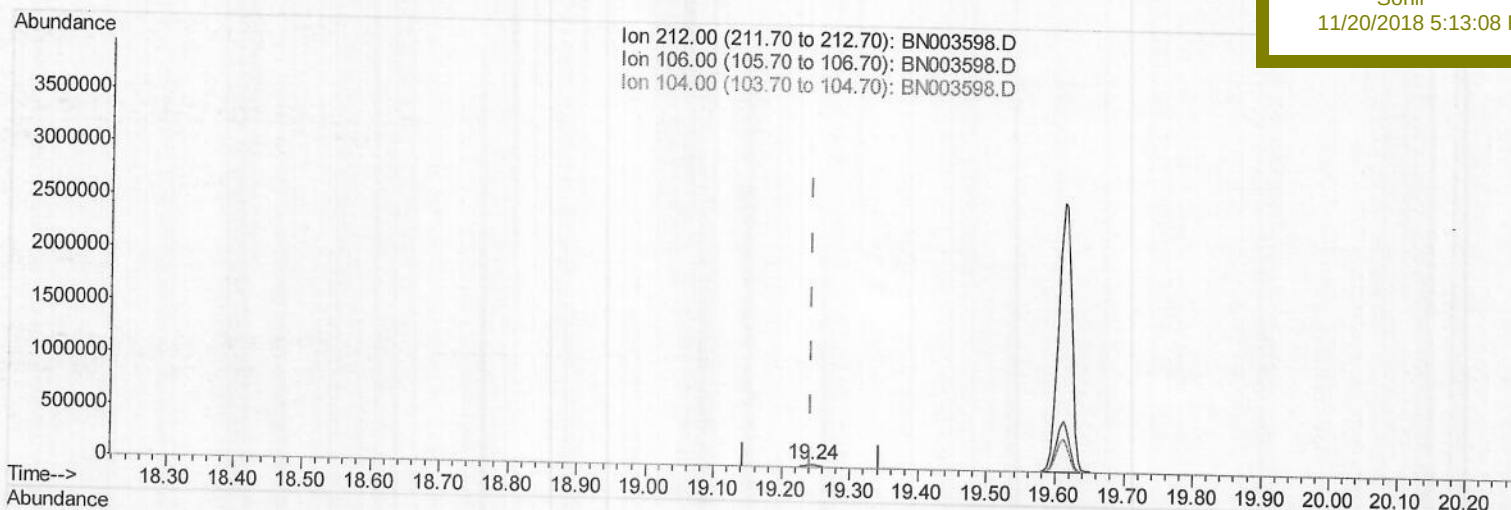

(14) Fluoranthene-d10 (SURR)

19.243min (-0.000) 0.36ng/ul m

response 38650

Ion	Exp%	Act%
212.00	100	100
106.00	14.20	0.00#
104.00	8.00	0.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN111918\
Quantitation Report (Qedit)




Data File : BN003598.D
Acq On : 19 Nov 2018 17:31
Operator : MJ/SJ
Sample : PB114864BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Quant Time: Nov 20 01:55:28 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 20 01:46:26 2018
Response via : Initial Calibration

Instrument :
BNA_N
ClientSampleId :
SBLK64

Manual Integrations
APPROVED

Sohil
11/20/2018 5:13:08 PM

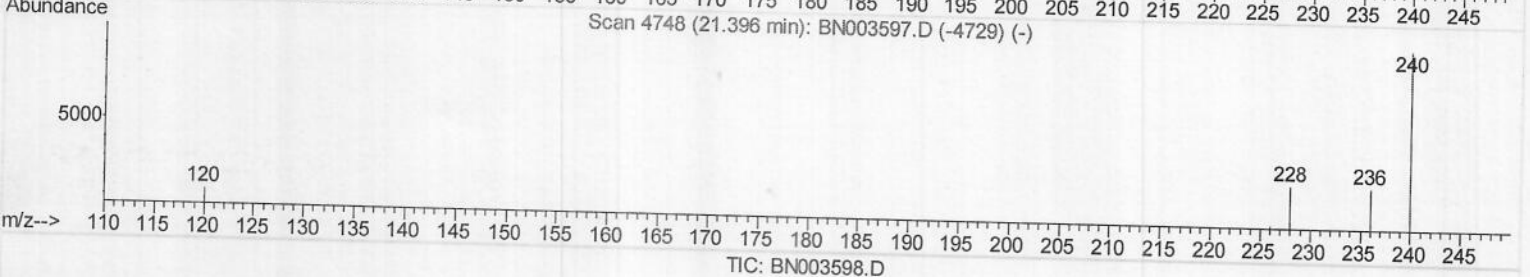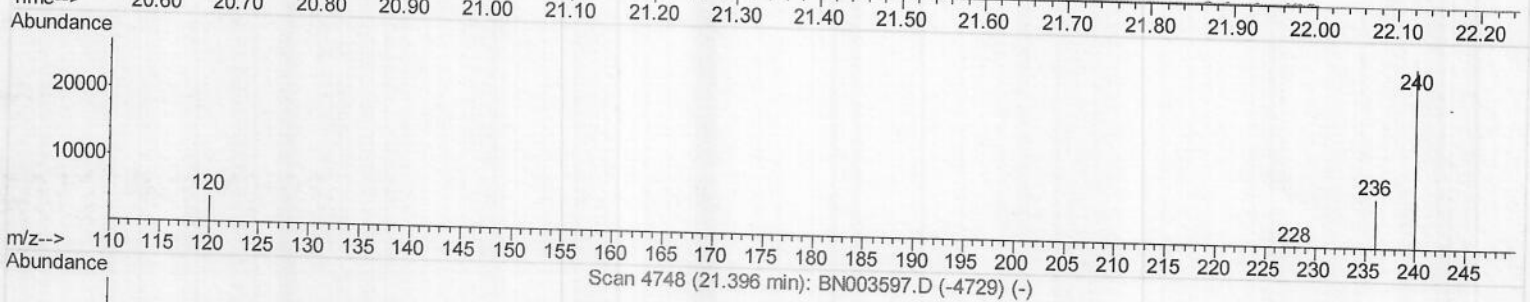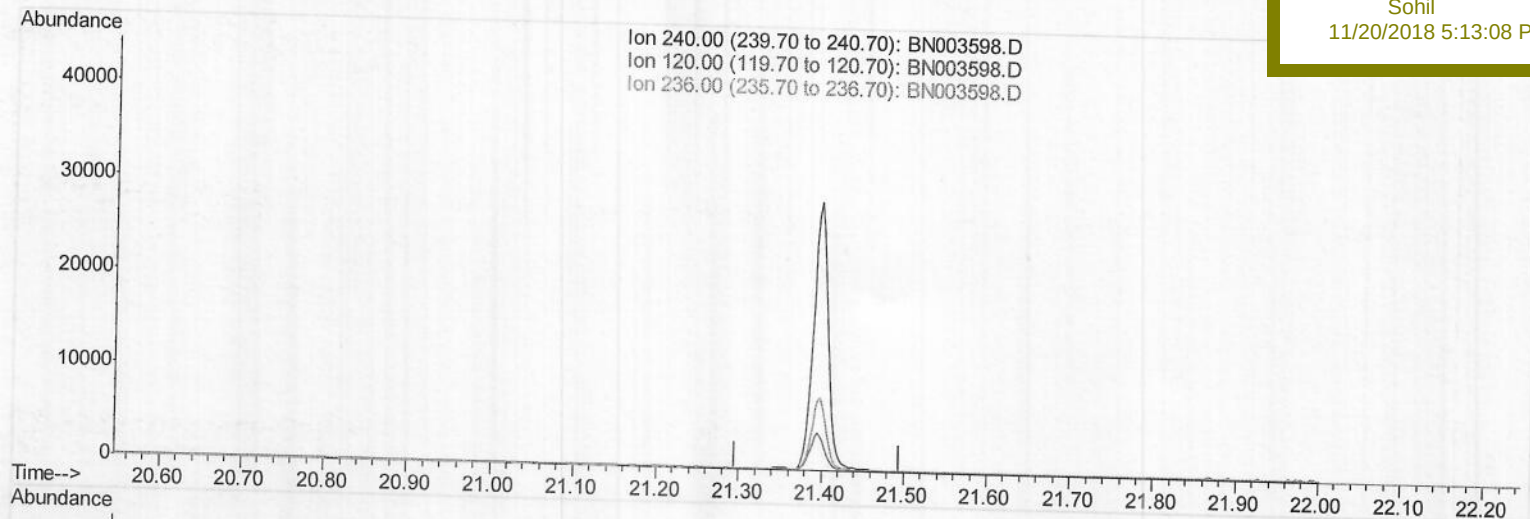

(16) Chrysene-d12 (I)
21.396min (-21.396) 0.00ng/ul
response 0

Ion	Exp%	Act%
240.00	100	0.00
120.00	14.00	0.00#
236.00	27.60	0.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN111918\
Quantitation Report (Qedit)


Data File : BN003598.D
Acq On : 19 Nov 2018 17:31
Operator : MJ/SJ
Sample : PB114864BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Quant Time: Nov 20 01:55:28 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 20 01:46:26 2018
Response via : Initial Calibration

Instrument :
BNA_N
ClientSampleId :
SBLK64

Manual Integrations
APPROVED

Sohil
11/20/2018 5:13:08 PM

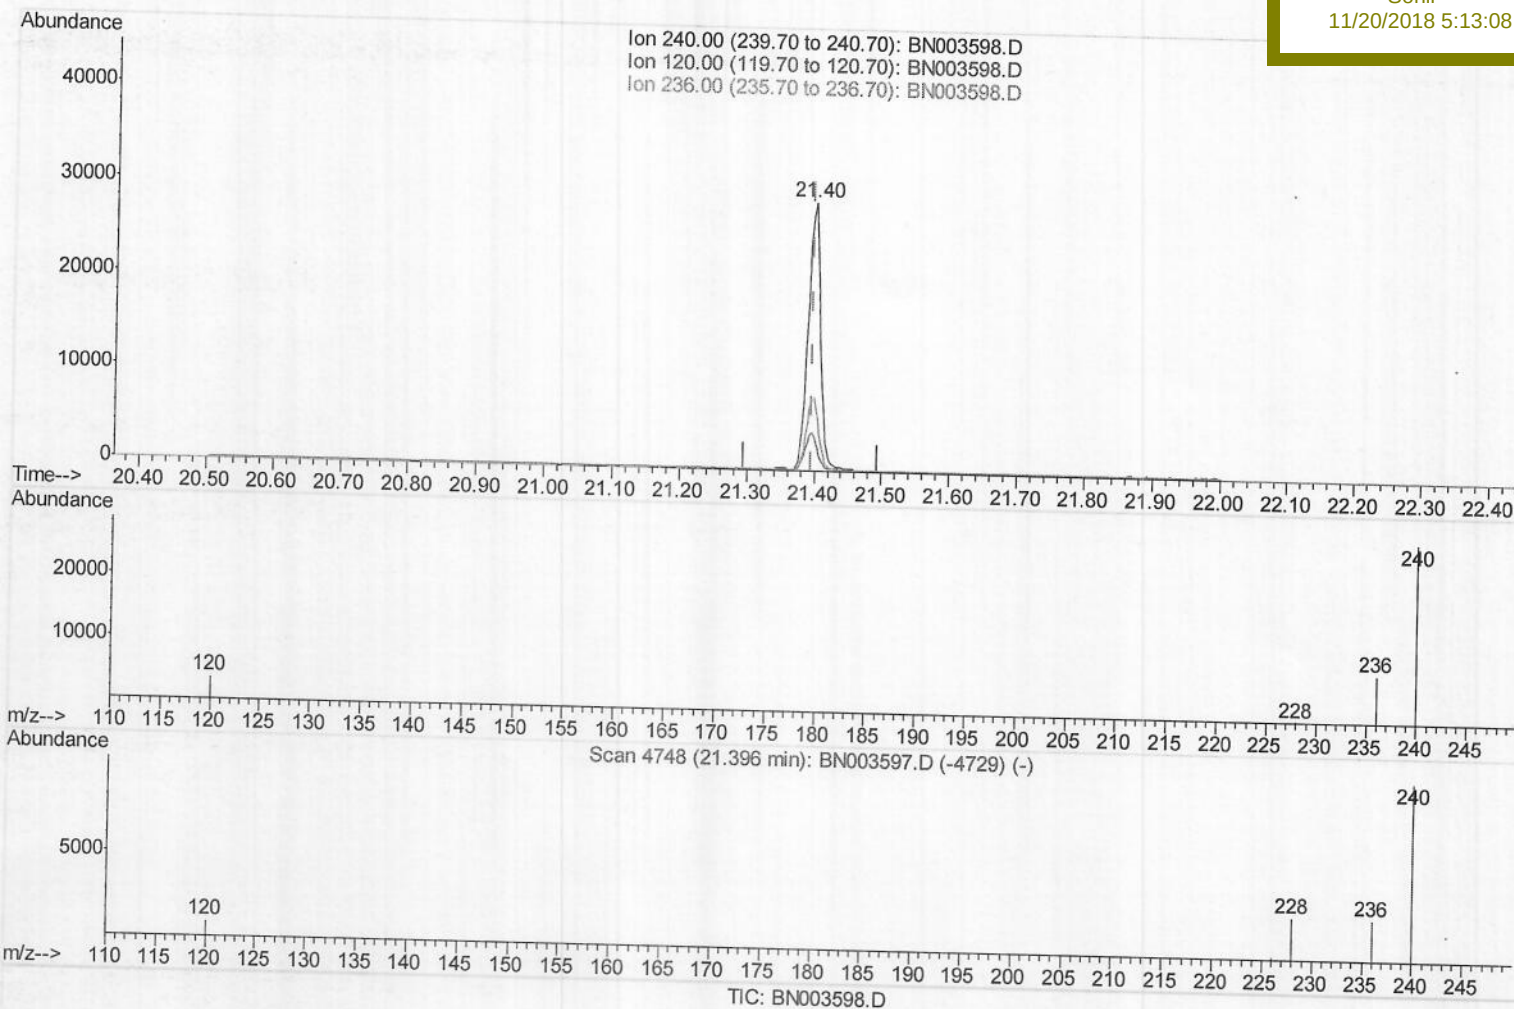

(16) Chrysene-d12 (I)
21.398min (+0.003) 0.40ng/ul m
response 36611

Ion	Exp%	Act%
240.00	100	100
120.00	14.00	12.89
236.00	27.60	27.21
0.00	0.00	0.00

\$JU
11/20/18

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN111918\
Quantitation Report (Qedit)



Data File : BN003598.D
Acq On : 19 Nov 2018 17:31
Operator : MJ/SJ
Sample : PB114864BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
Client Sampled :
SBLK64

Manual Integrations
APPROVED

Sohil
11/20/2018 5:13:08 PM

Quant Time: Nov 20 01:56:08 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 20 01:46:26 2018
Response via : Initial Calibration

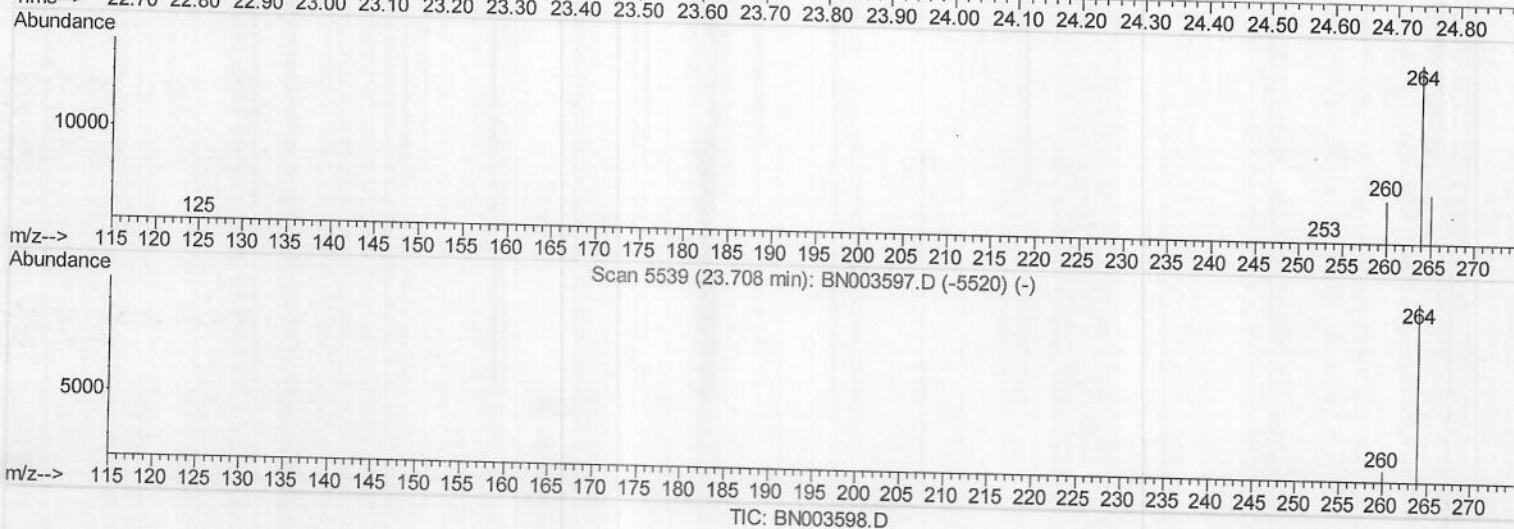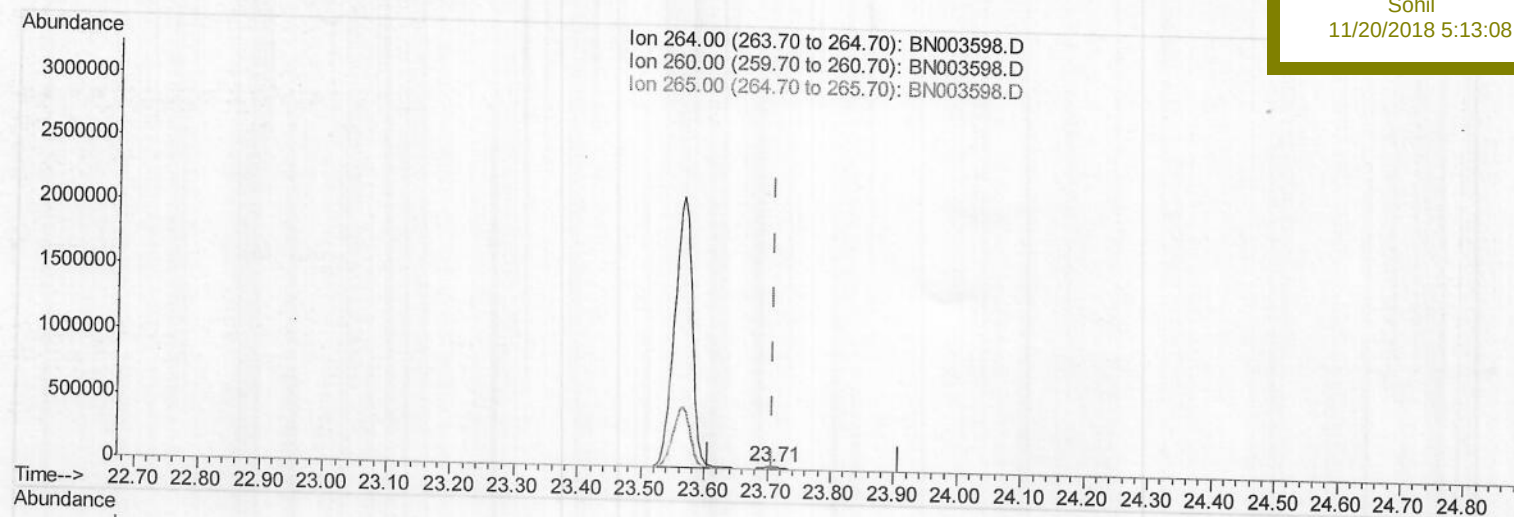

(20) Perylene-d12 (I)

23.707min (-0.000) 0.40ng/ul

response 43966

Ion	Exp%	Act%
264.00	100	100
260.00	26.20	25.35
265.00	33.50	28.87
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN111918\
Quantitation Report (Qedit)


Data File : BN003598.D
Acq On : 19 Nov 2018 17:31
Operator : MJ/SJ
Sample : PB114864BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Quant Time: Nov 20 01:56:08 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 20 01:46:26 2018
Response via : Initial Calibration

Instrument :
BNA_N
Client Sampled :
SBLK64

Manual Integrations
APPROVED

Sohil
11/20/2018 5:13:08 PM

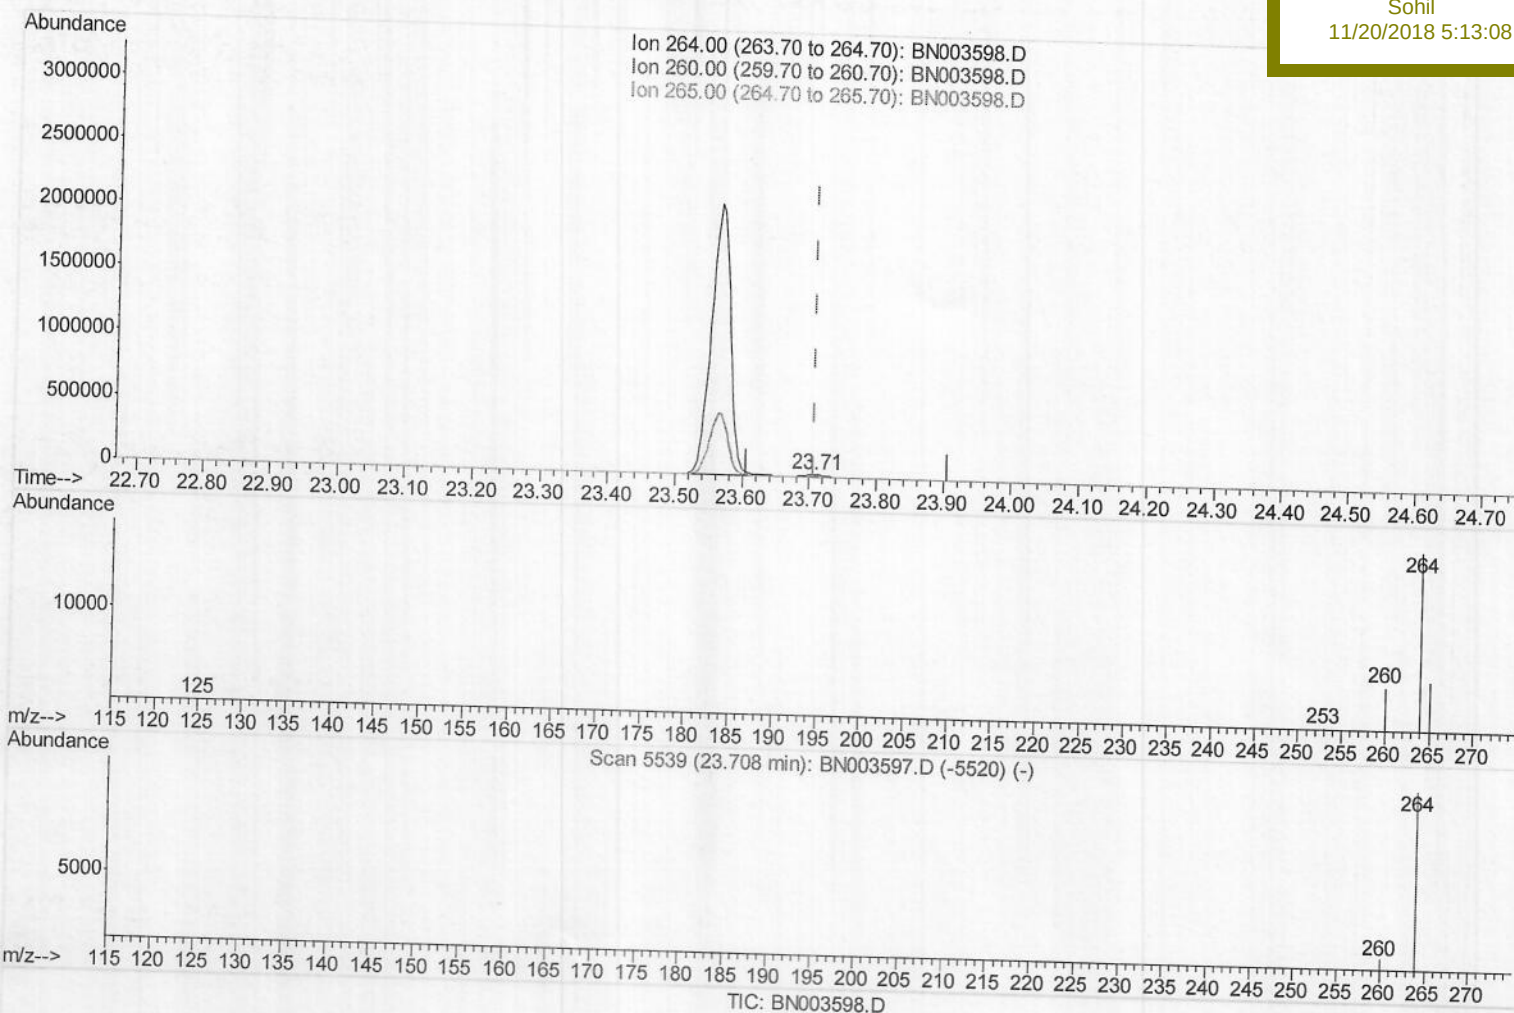

(20) Perylene-d12 (I)

23.707min (-0.000) 0.40ng/ul m

response 32141

Ion	Exp%	Act%
264.00	100	100
260.00	26.20	25.35
265.00	33.50	28.87
0.00	0.00	0.00

JU
11/20/18

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN111918\
Quantitation Report (QT Reviewed)

Data File : BN003598.D
Acq On : 19 Nov 2018 17:31
Operator : MJ/SJ
Sample : PB114864BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Quant Time: Nov 20 01:57:26 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 20 01:46:26 2018
Response via : Initial Calibration

Instrument :
BNA_N
ClientSampleId :
SBLK64

Manual Integrations
APPROVED

Sohil
11/20/2018 5:13:08 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.84	152	7521	0.40	ng/ul	0.00
2) Naphthalene-d8	10.64	136	26194	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.48	164	15985	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.22	188	36842m	0.40	ng/ul	0.00
16) Chrysene-d12	21.40	240	36611m	0.40	ng/ul	0.00
20) Perylene-d12	23.71	264	32141m	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.23	152	17081	0.42	ng/ul	0.00
14) Fluoranthene-d10	19.24	212	38650m	0.36	ng/ul	0.00

Target Compounds

Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

JV
11/20/18