

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN111918\

Quantitation Report (QT Reviewed)

Data File : BN003601.D

Acq On : 19 Nov 2018 19:16

Operator : MJ/SJ

Sample : J5928-01

Misc :

ALS Vial : 13 Sample Multiplier: 1

Quant Time: Nov 20 02:05:44 2018

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue Nov 20 01:46:26 2018

Response via : Initial Calibration

Instrument :

BNA_N


ClientSampleId :

A40Z4

Manual Integrations
APPROVED

Sohil

11/20/2018 5:13:16 PM

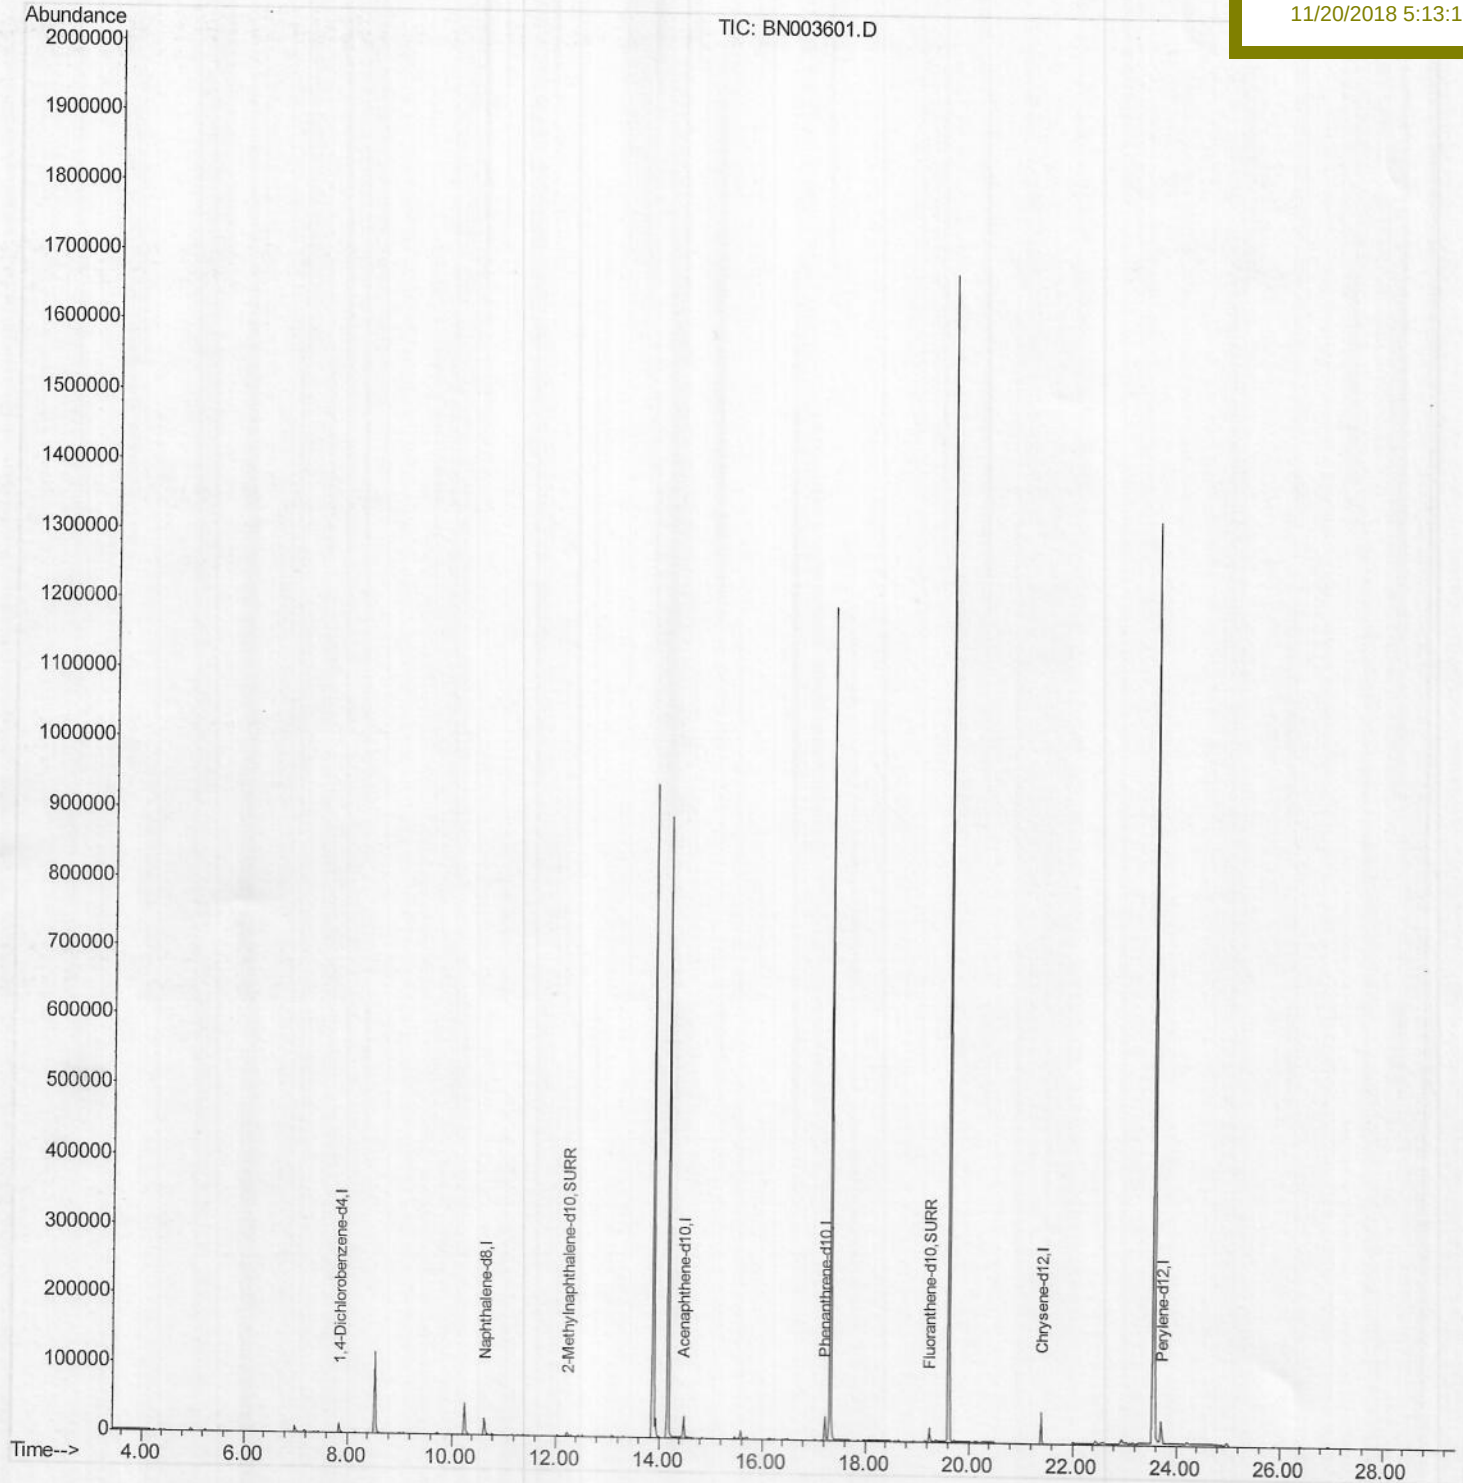

SOM-EPA-SIM-BN111918.M Tue Nov 20 02:03:41 2018

Page: 2

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN111918\
Quantitation Report (Qedit)



Data File : BN003601.D
Acq On : 19 Nov 2018 19:16
Operator : MJ/SJ
Sample : J5928-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Quant Time: Nov 20 01:49:47 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 20 01:46:26 2018
Response via : Initial Calibration

Instrument :
BNA_N
ClientSampleId :
A40Z4

Manual Integrations
APPROVED

Sohil
11/20/2018 5:13:16 PM

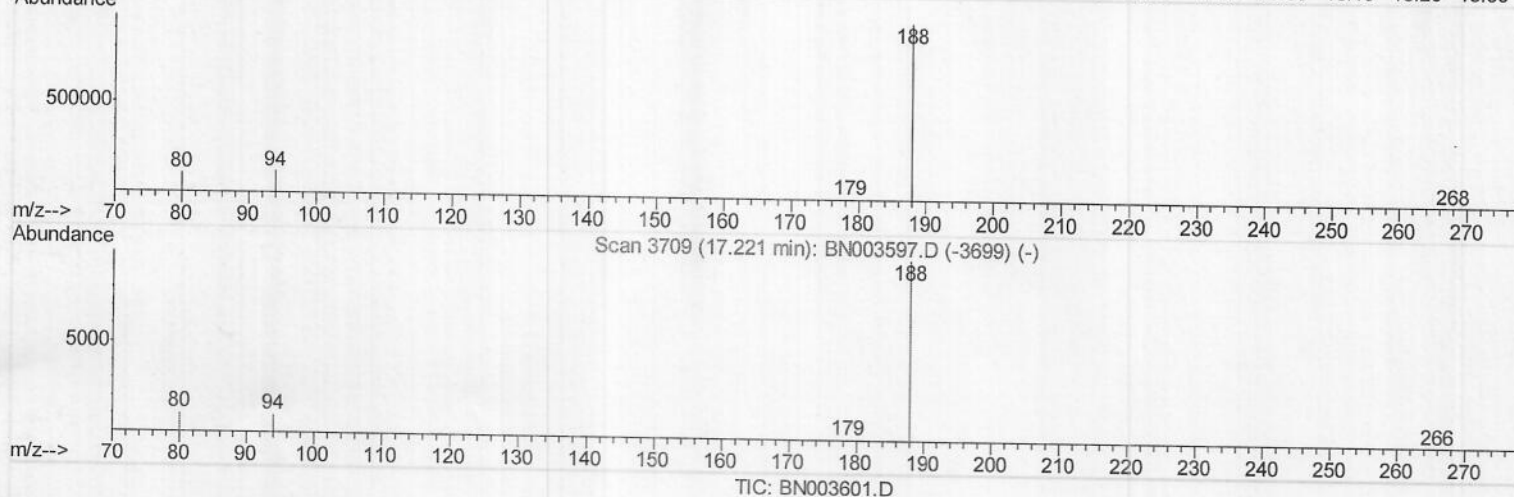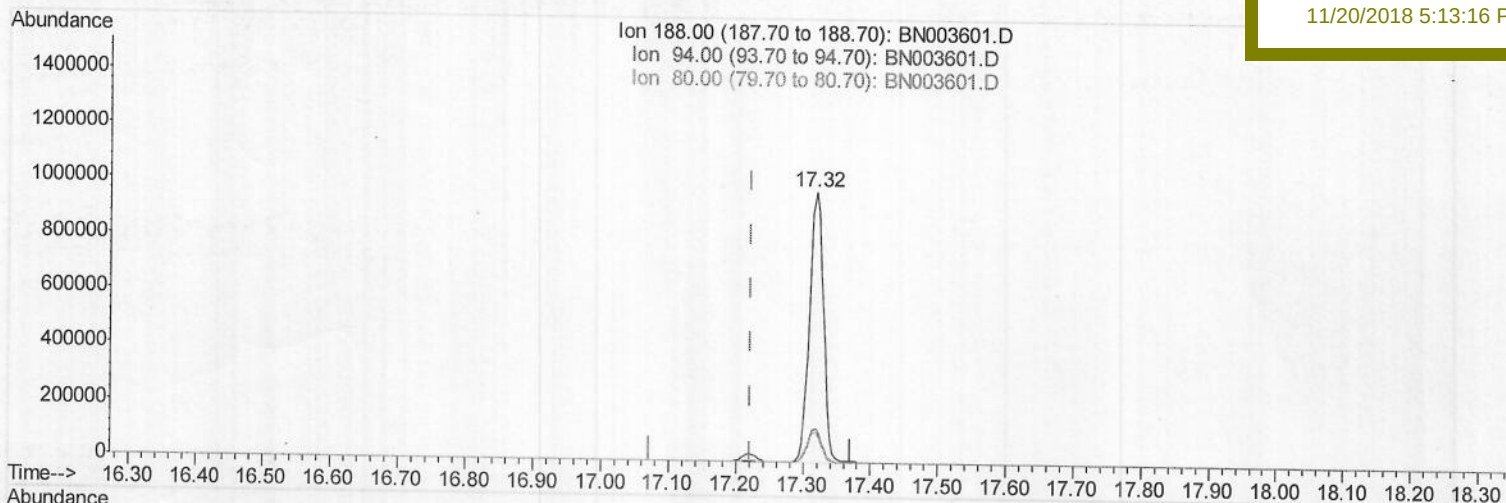

(10) Phenanthrene-d10 (I)

17.318min (+0.097) 0.40ng/ul

response 1392442

Ion	Exp%	Act%
188.00	100	100
94.00	10.40	12.22
80.00	11.60	10.88
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN111918\
Quantitation Report (Qedit)




Data File : BN003601.D
Acq On : 19 Nov 2018 19:16
Operator : MJ/SJ
Sample : J5928-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Quant Time: Nov 20 01:49:47 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 20 01:46:26 2018
Response via : Initial Calibration

Instrument :
BNA_N
ClientSampleId :
A40Z4

Manual Integrations
APPROVED

Sohil
11/20/2018 5:13:16 PM

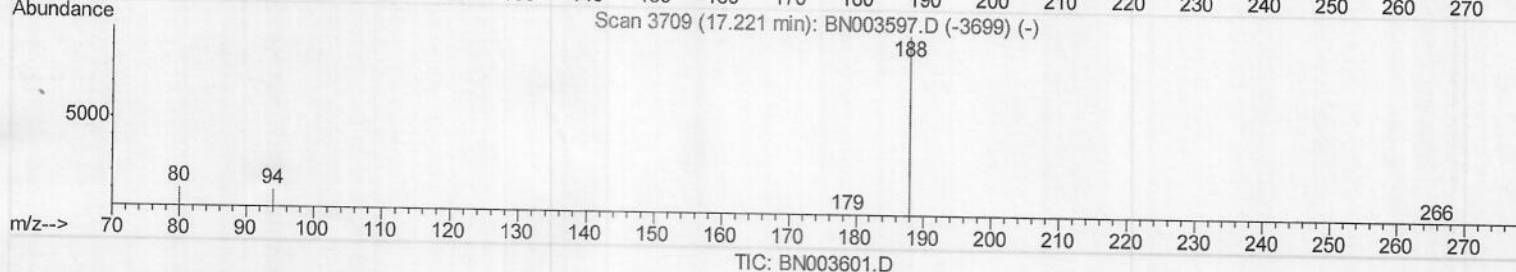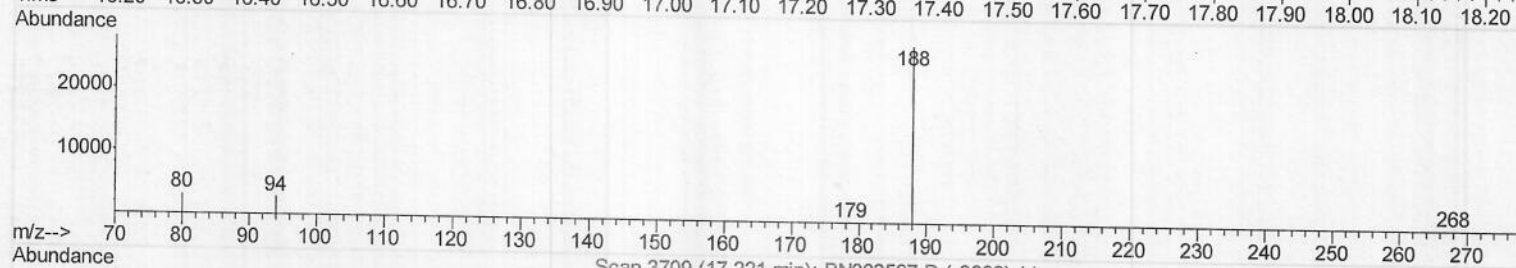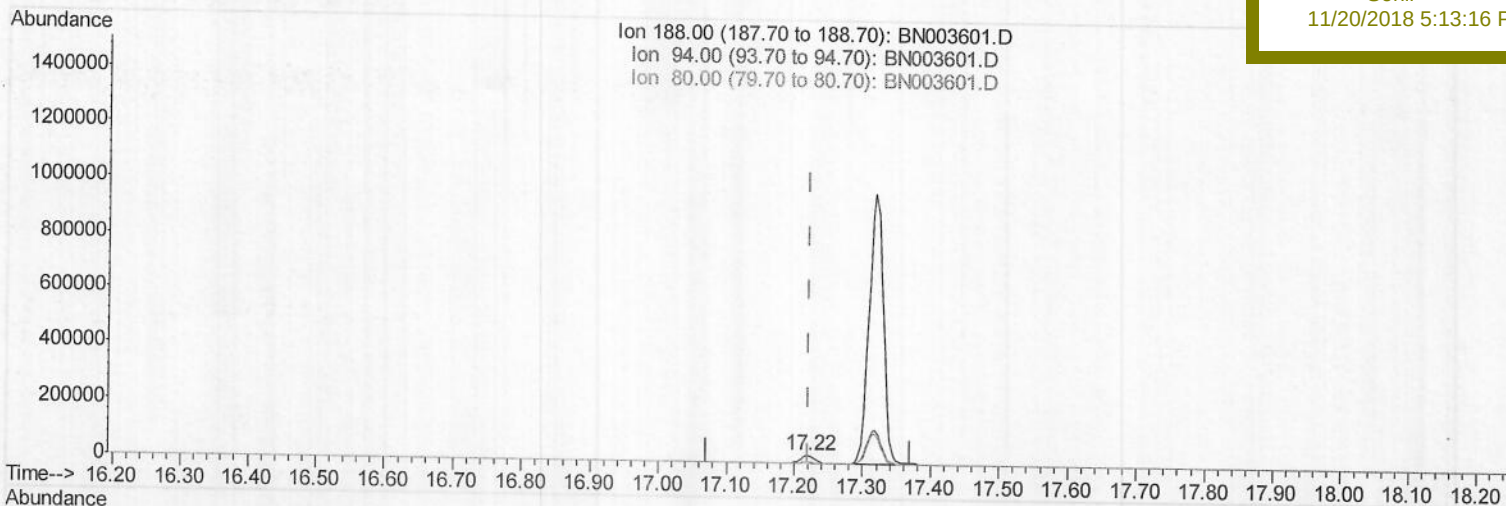

(10) Phenanthrene-d10 (I)

17.221min (-0.000) 0.40ng/ul m

response 39318

Ion	Exp%	Act%
188.00	100	100
94.00	10.40	10.25
80.00	11.60	11.21
0.00	0.00	0.00

JU
11/20/18

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN111918\
Quantitation Report (Qedit)




Data File : BN003601.D
Acq On : 19 Nov 2018 19:16
Operator : MJ/SJ
Sample : J5928-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Quant Time: Nov 20 02:03:50 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 20 01:46:26 2018
Response via : Initial Calibration

Instrument :
BNA_N
ClientSampleId :
A40Z4

Manual Integrations
APPROVED

Sohil
11/20/2018 5:13:16 PM

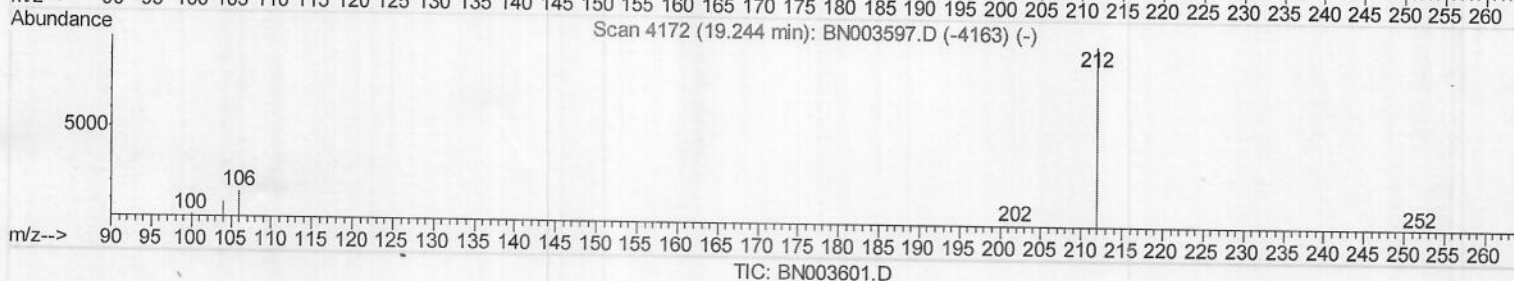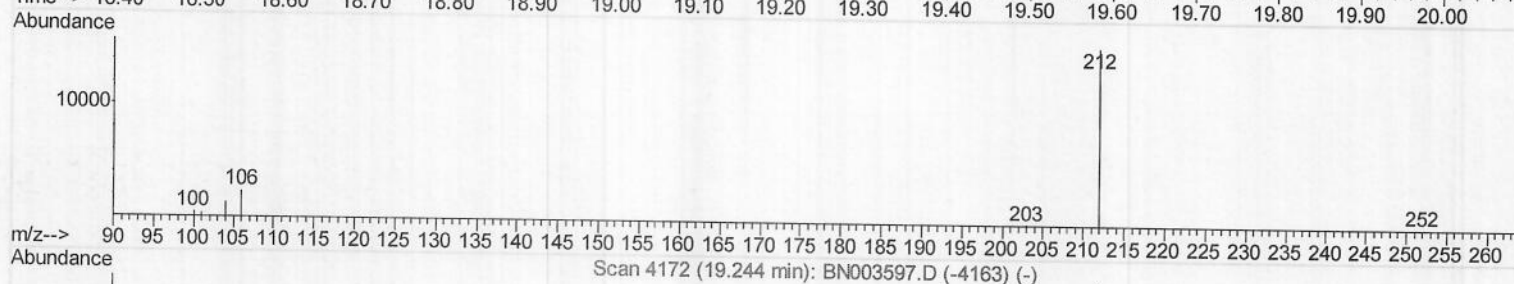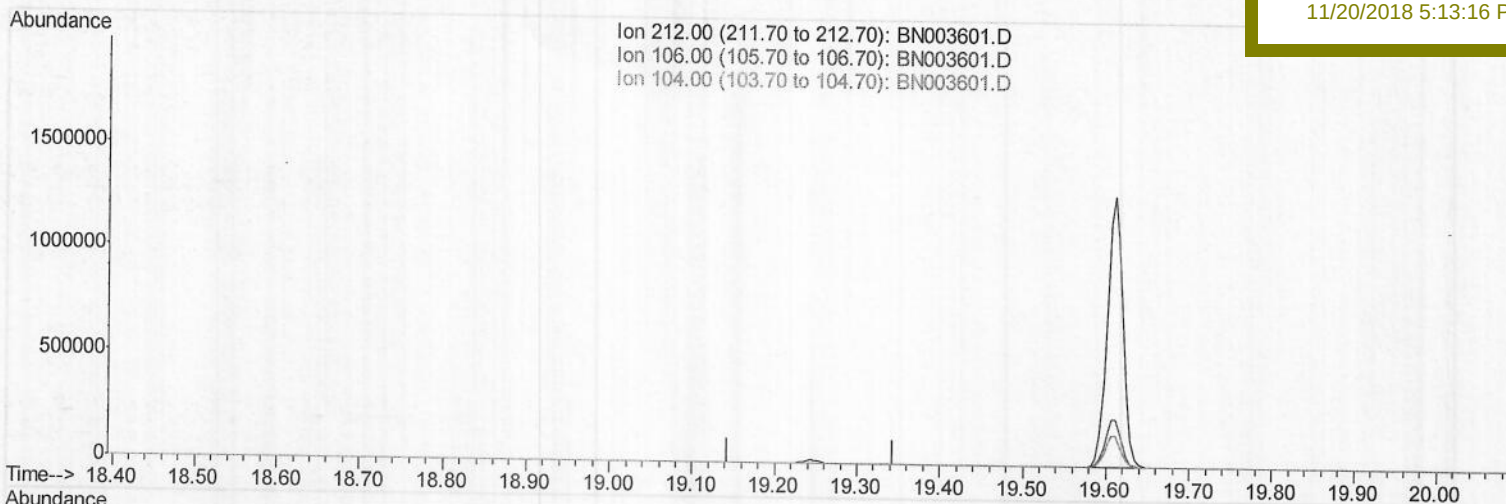

(14) Fluoranthene-d10 (SURR)

19.244min (-19.244) 0.00ng/ul

response 0

Ion	Exp%	Act%
212.00	100	0.00
106.00	14.20	0.00#
104.00	8.00	0.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN111918\
Quantitation Report (Qedit)




Data File : BN003601.D
Acq On : 19 Nov 2018 19:16
Operator : MJ/SJ
Sample : J5928-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Quant Time: Nov 20 02:03:50 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 20 01:46:26 2018
Response via : Initial Calibration

Instrument :
BNA_N
ClientSampleId :
A40Z4

Manual Integrations
APPROVED

Sohil
11/20/2018 5:13:16 PM

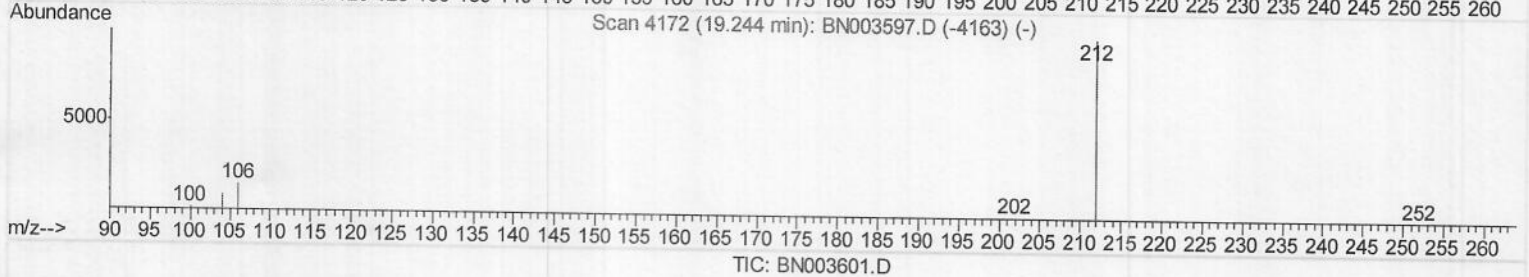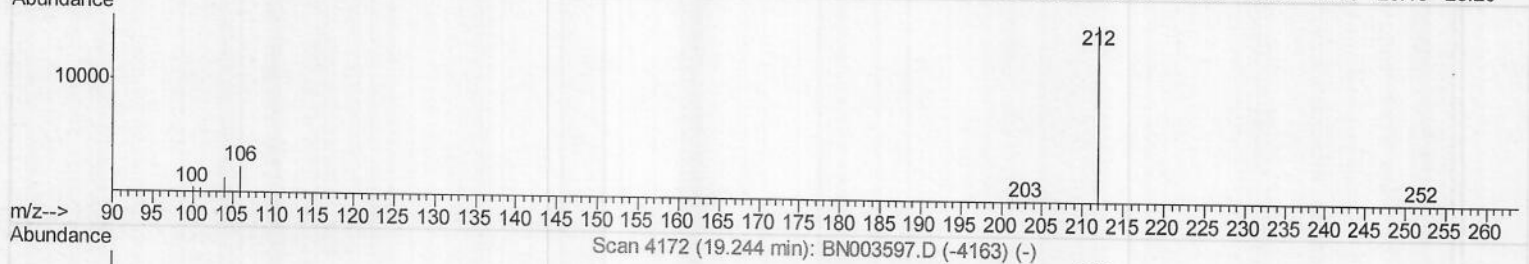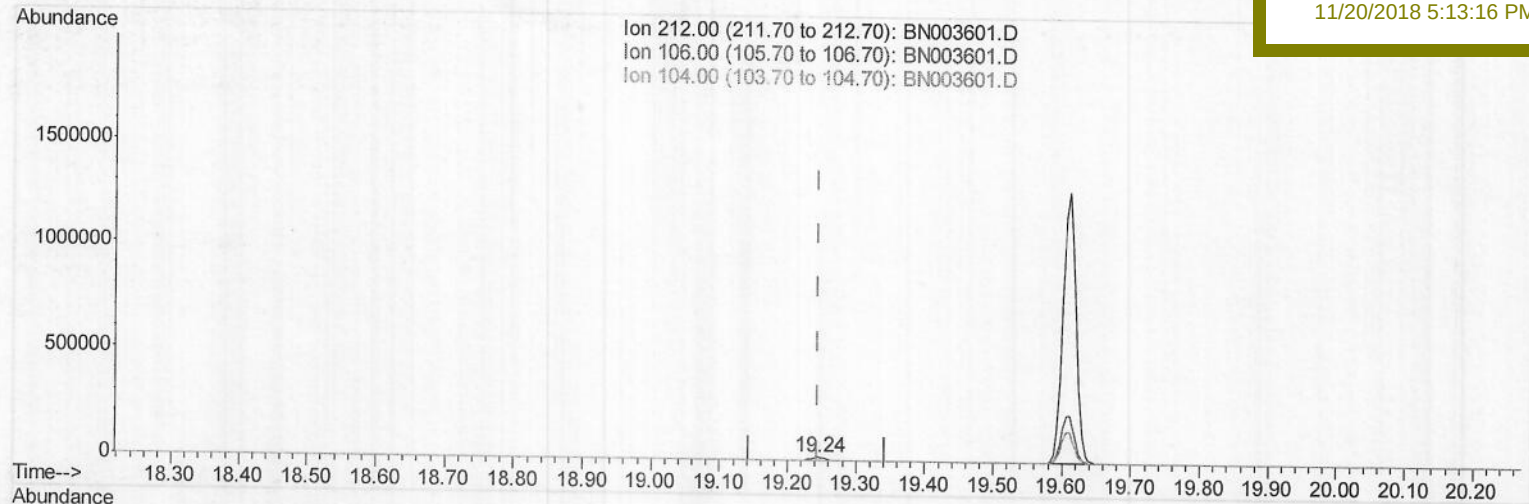

(14) Fluoranthene-d10 (SURR)

19.243min (-0.000) 0.18ng/ul m

response 20571

Ion	Exp%	Act%
212.00	100	100
106.00	14.20	0.00#
104.00	8.00	0.00#
0.00	0.00	0.00

JV
11/20/18

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN111918\
Quantitation Report (Qedit)




Data File : BN003601.D
Acq On : 19 Nov 2018 19:16
Operator : MJ/SJ
Sample : J5928-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Quant Time: Nov 20 02:03:50 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 20 01:46:26 2018
Response via : Initial Calibration

Instrument :
BNA_N
ClientSampleId :
A40Z4

Manual Integrations
APPROVED

Sohil
11/20/2018 5:13:16 PM

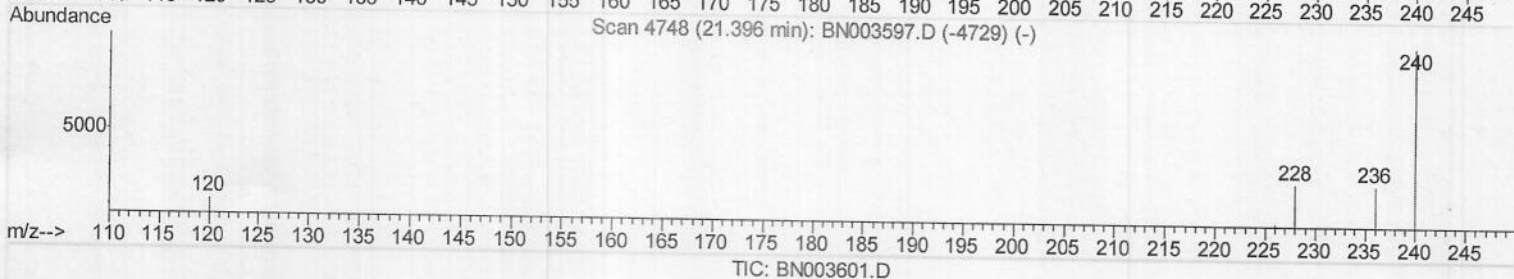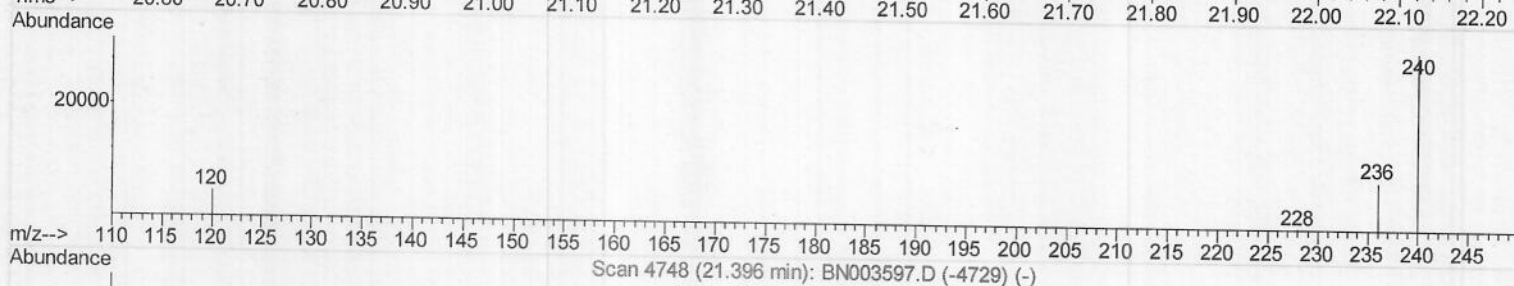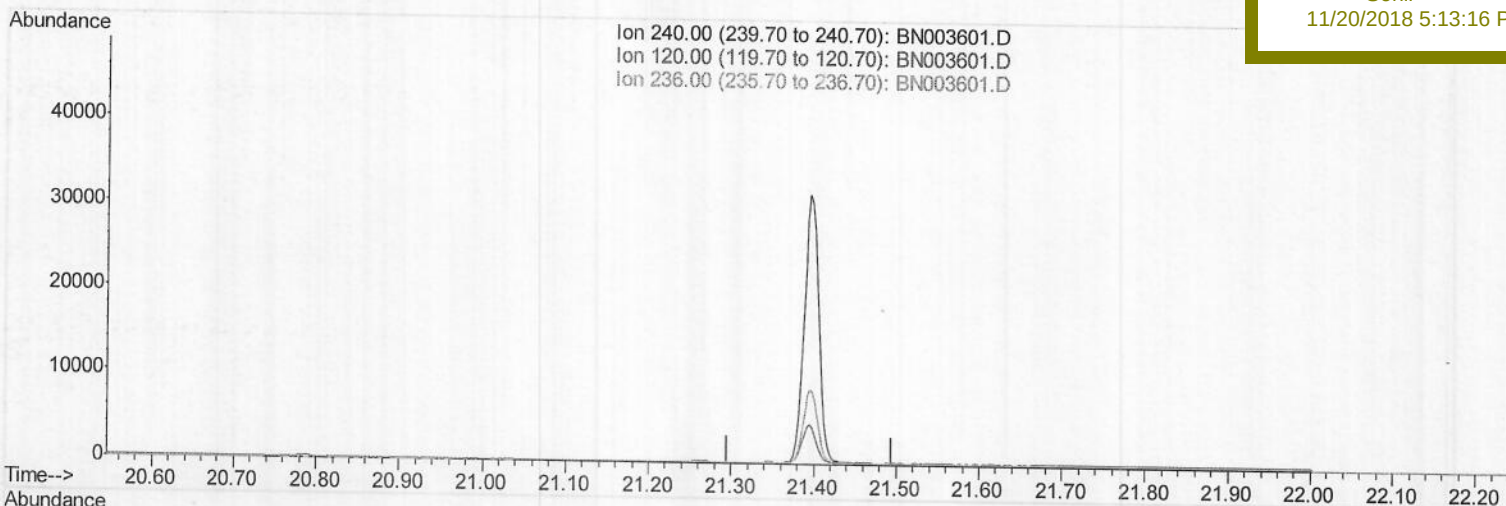

(16) Chrysene-d12 (I)

21.396min (-21.396) 0.00ng/ul

response 0

Ion	Exp%	Act%
240.00	100	0.00
120.00	14.00	0.00#
236.00	27.60	0.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN111918\
Quantitation Report (Qedit)




Data File : BN003601.D
Acq On : 19 Nov 2018 19:16
Operator : MJ/SJ
Sample : J5928-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Quant Time: Nov 20 02:03:50 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 20 01:46:26 2018
Response via : Initial Calibration

Instrument :
BNA_N
ClientSampleId :
A40Z4

Manual Integrations
APPROVED

Sohil
11/20/2018 5:13:16 PM

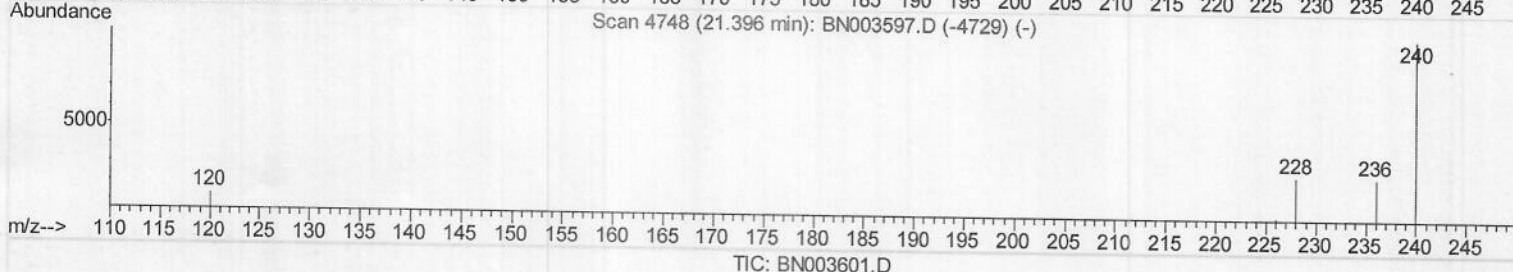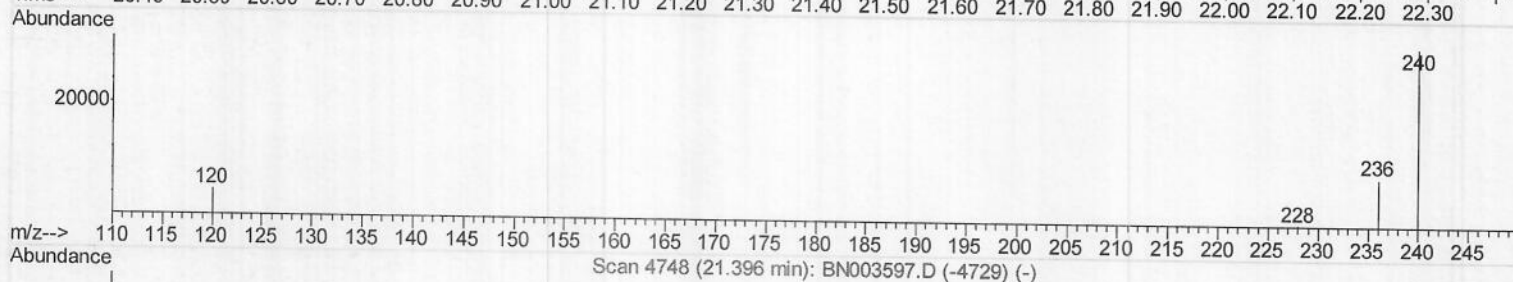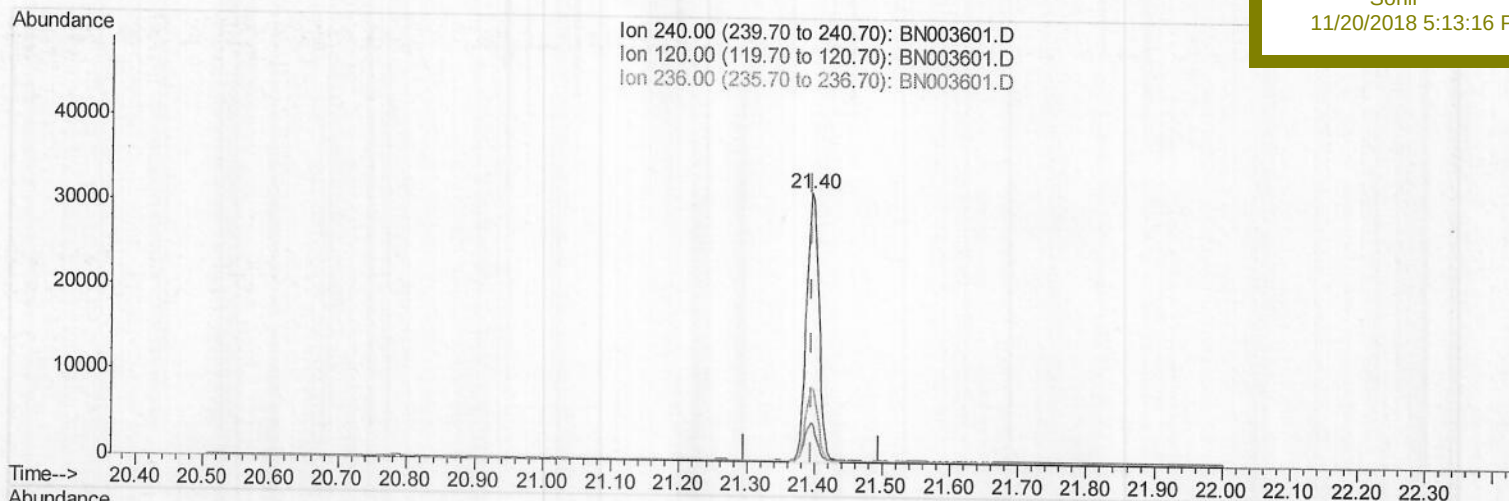

(16) Chrysene-d12 (I)

21.395min (-0.000) 0.40ng/ul m

response 40259

Ion	Exp%	Act%
240.00	100	100
120.00	14.00	14.37
236.00	27.60	27.26
0.00	0.00	0.00

JU
11/20/18

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN111918\
Quantitation Report (Qedit)




Data File : BN003601.D
Acq On : 19 Nov 2018 19:16
Operator : MJ/SJ
Sample : J5928-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Quant Time: Nov 20 02:04:53 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 20 01:46:26 2018
Response via : Initial Calibration

Instrument :
BNA_N
ClientSampleId :
A40Z4

Manual Integrations
APPROVED

Sohil
11/20/2018 5:13:16 PM

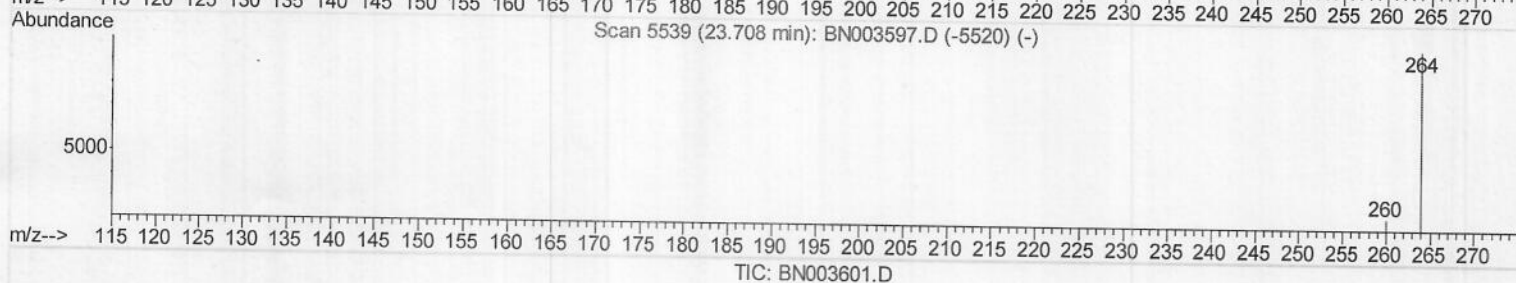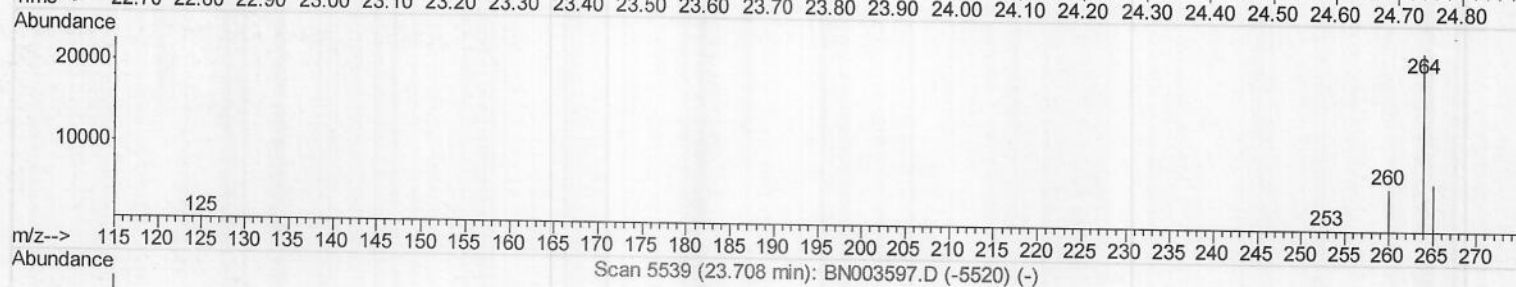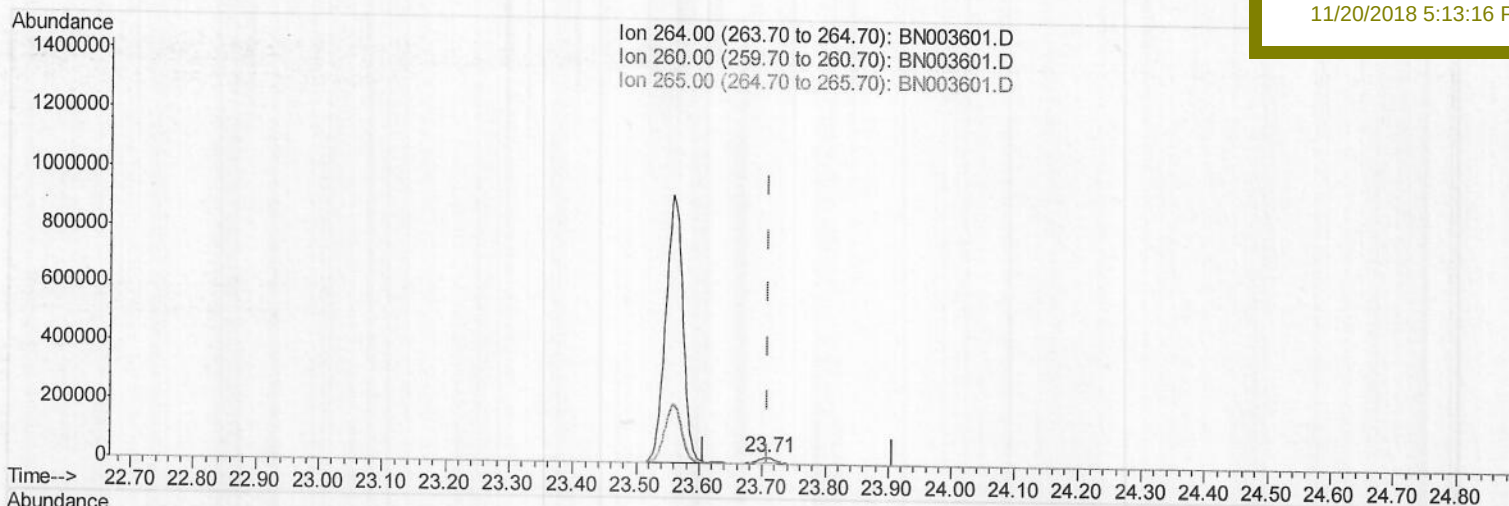

(20) Perylene-d12 (I)

23.707min (-0.000) 0.40ng/ul

response 47472

Ion	Exp%	Act%
264.00	100	100
260.00	26.20	25.38
265.00	33.50	27.63
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN111918\
Quantitation Report (Qedit)




Data File : BN003601.D
Acq On : 19 Nov 2018 19:16
Operator : MJ/SJ
Sample : J5928-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Quant Time: Nov 20 02:04:53 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 20 01:46:26 2018
Response via : Initial Calibration

Instrument :
BNA_N
ClientSampleId :
A40Z4

Manual Integrations
APPROVED

Sohil
11/20/2018 5:13:16 PM

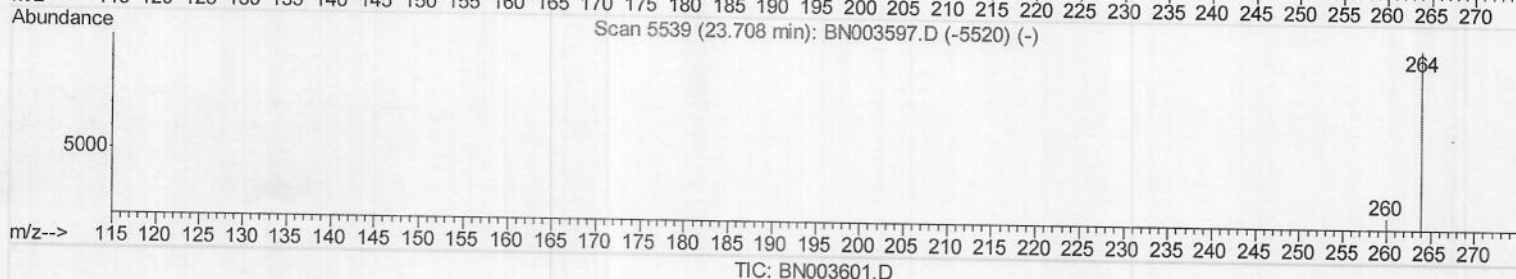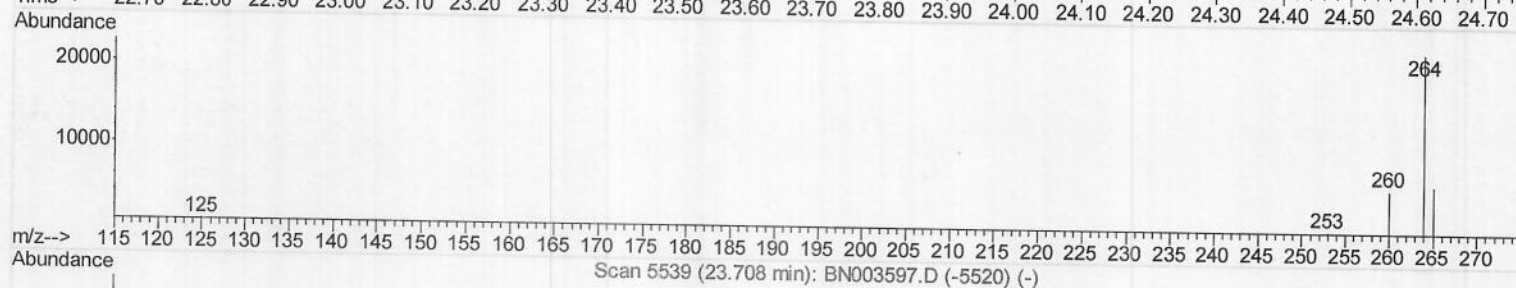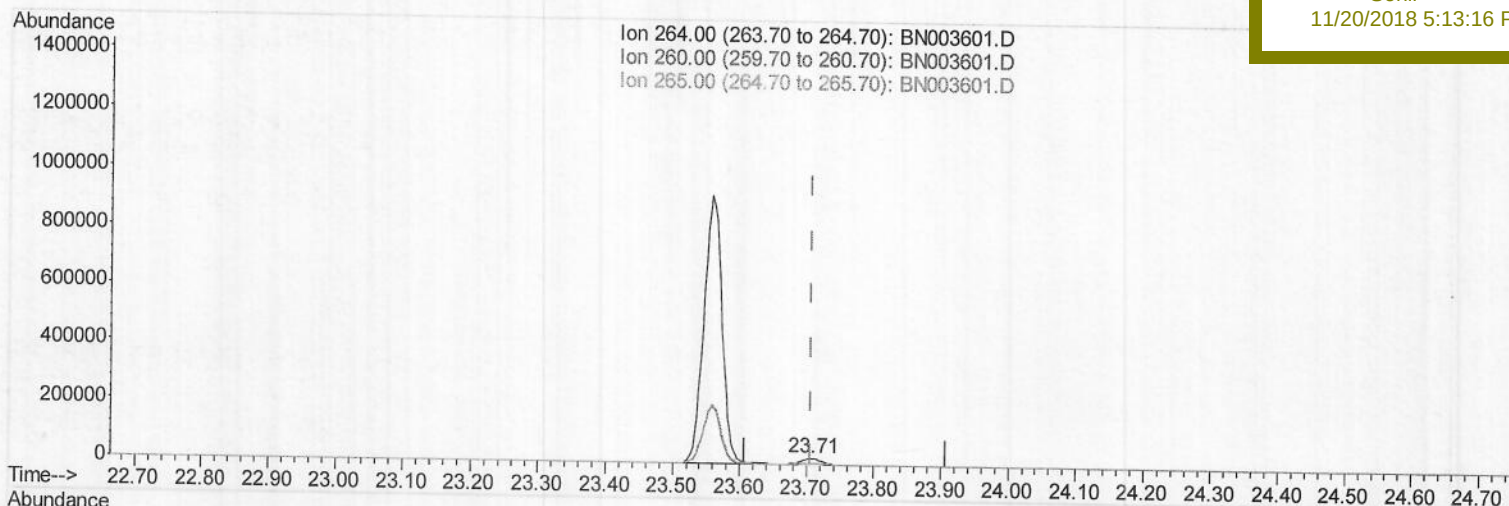

(20) Perylene-d12 (I)

23.707min (-0.000) 0.40ng/ul m

response 41171

Ion	Exp%	Act%
264.00	100	100
260.00	26.20	25.38
265.00	33.50	27.63
0.00	0.00	0.00

JV
11/20/18

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN111918\
Quantitation Report (QT Reviewed)

Data File : BN003601.D
Acq On : 19 Nov 2018 19:16
Operator : MJ/SJ
Sample : J5928-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Quant Time: Nov 20 02:05:44 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 20 01:46:26 2018
Response via : Initial Calibration

Instrument :
BNA_N
ClientSampleId :
A40Z4

Manual Integrations
APPROVED

Sohil
11/20/2018 5:13:16 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.84	152	7196	0.40	ng/ul	0.00
2) Naphthalene-d8	10.64	136	31132	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.48	164	16537	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.22	188	39318m	0.40	ng/ul	0.00
16) Chrysene-d12	21.40	240	40259m	0.40	ng/ul	0.00
20) Perylene-d12	23.71	264	41171m	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.23	152	7071	0.15	ng/ul	0.00
14) Fluoranthene-d10	19.24	212	20571m	0.18	ng/ul	0.00

Target Compounds

						Qvalue
--	--	--	--	--	--	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

JV
11/20/18