

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN111918\
 Data File : BN003621.D
 Acq On : 20 Nov 2018 06:56
 Operator : MJ/SJ
 Sample : J5928-07MSD
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4102MSD

Quant Time: Nov 20 08:29:01 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 20 03:27:39 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.84	152	6794	0.40	ng/ul	0.00
2) Naphthalene-d8	10.64	136	28090	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.48	164	15173	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.22	188	36510	0.40	ng/ul	0.00
16) Chrysene-d12	21.40	240	36176	0.40	ng/ul	0.00
20) Perylene-d12	23.71	264	31540	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.23	152	7359	0.17	ng/ul	0.00
14) Fluoranthene-d10	19.24	212	20679	0.19	ng/ul	0.00
Target Compounds				Ovalue		
8) Acenaphthene	14.54	153	10308	0.172	ng/ul	98
11) Pentachlorophenol	16.87	266	1650	0.251	ng/ul	99
17) Pyrene	19.64	202	27610	0.213	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN111918\
Data File : BN003621.D
Acq On : 20 Nov 2018 06:56
Operator : MJ/SJ
Sample : J5928-07MSD
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4102MSD

Quant Time: Nov 20 08:29:01 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 20 03:27:39 2018
Response via : Initial Calibration

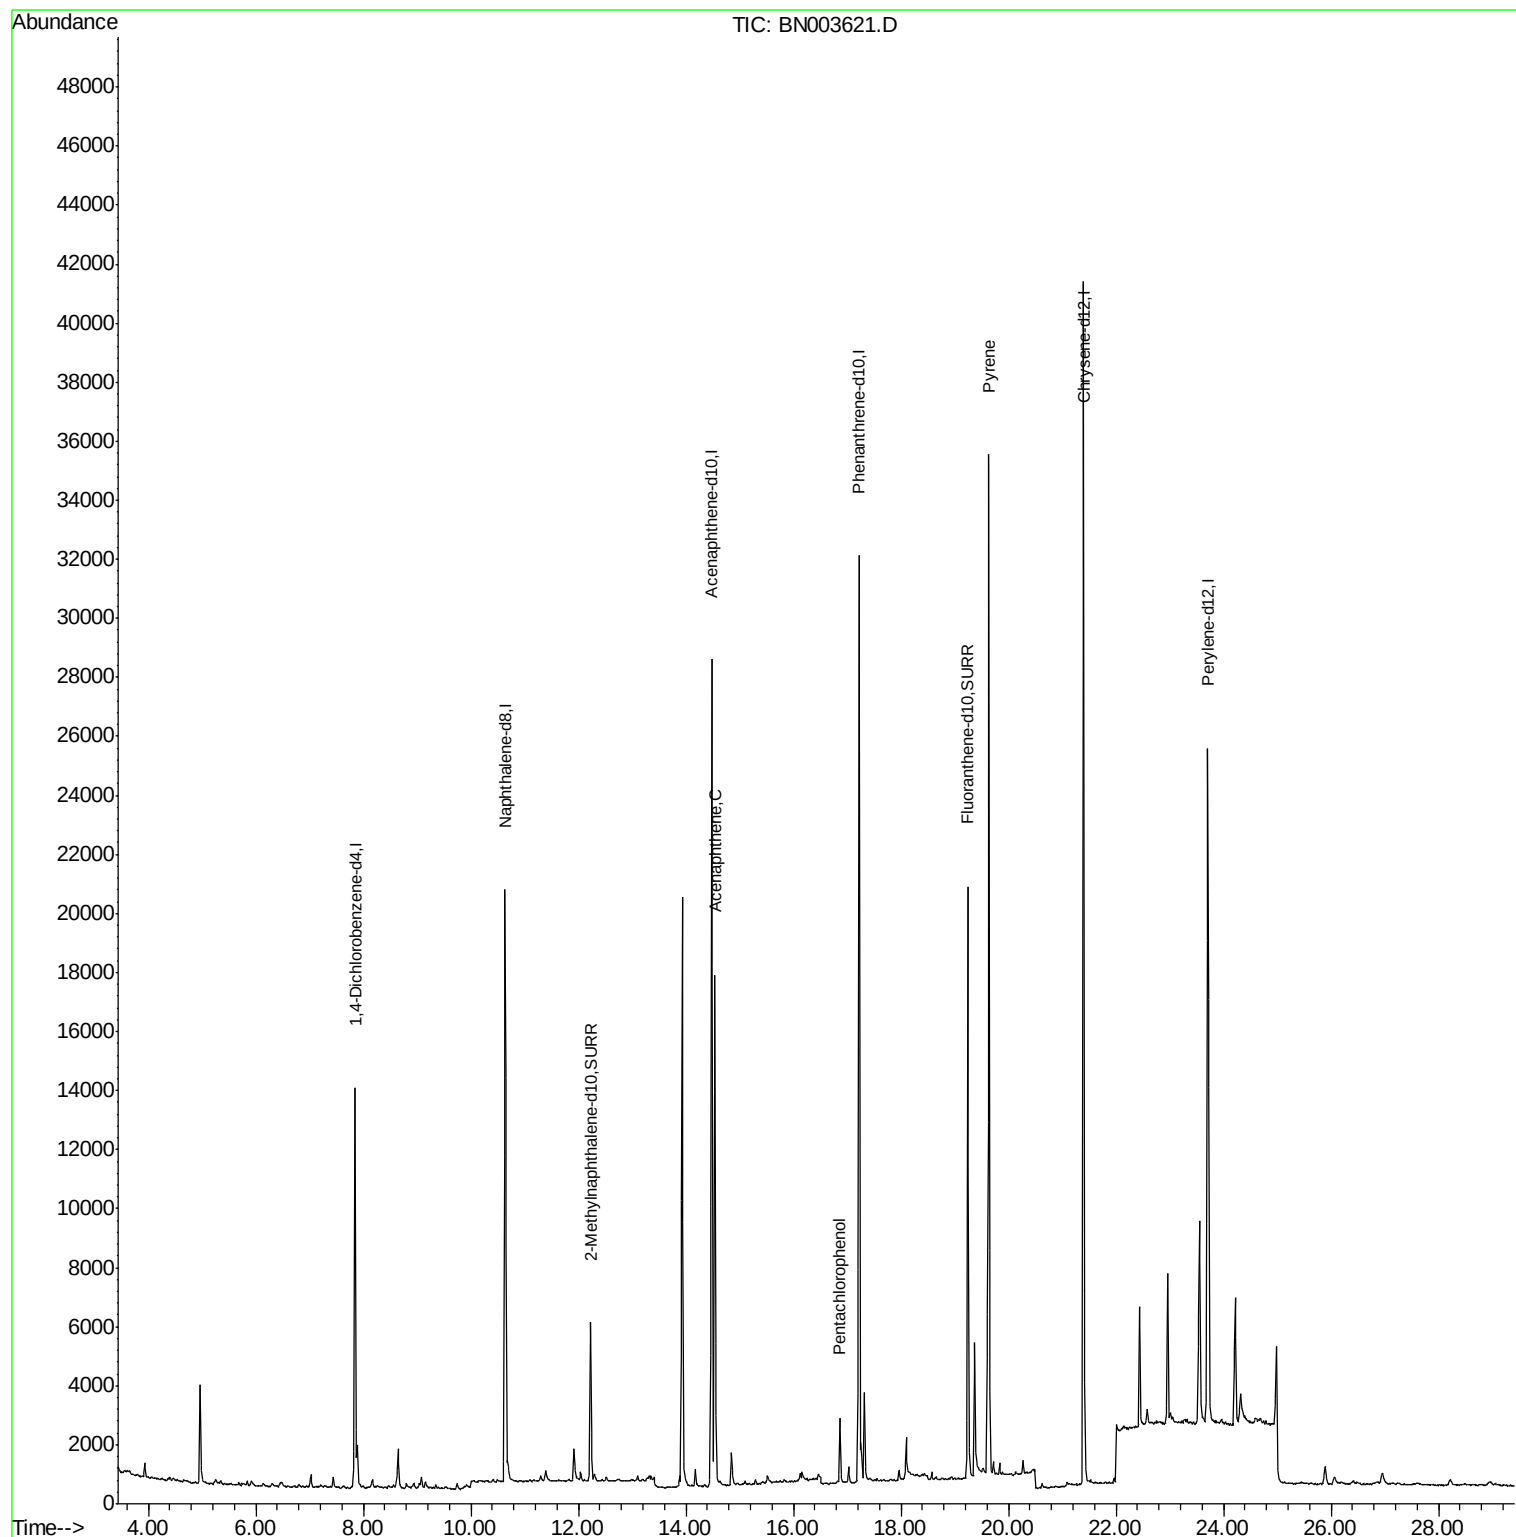

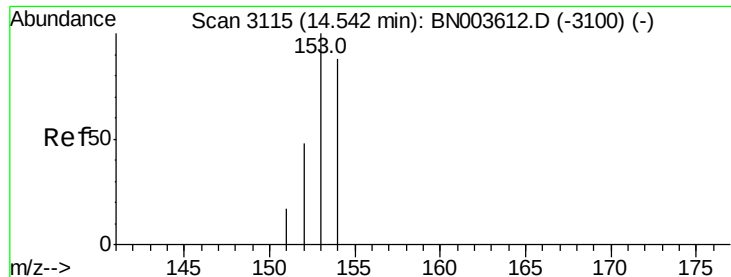

#8

Acenaphthene

Concen: 0.172 ng/ul

RT: 14.54 min Scan# 3115

Delta R.T. -0.00 min

Lab File: BN003621.D

Acq: 20 Nov 2018 06:56

Instrument :

BNA_N

ClientSampleId :

A4102MSD


Tot Ion:153 Resp: 10308

Ion Ratio Lower Upper

153 100

152 48.1 39.3 58.9




154 89.7 70.3 105.5

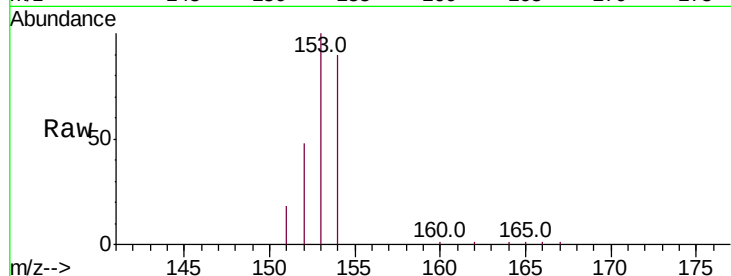

Abundance Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

Ion 154.00 (153.70 to 154.70): E

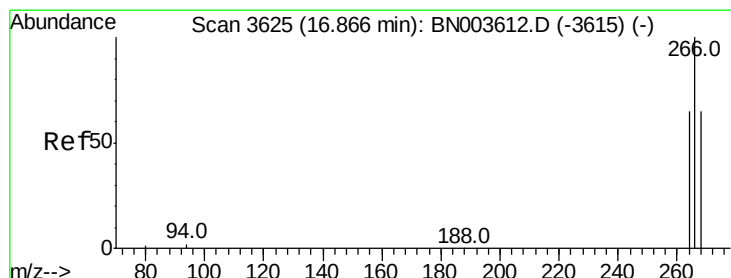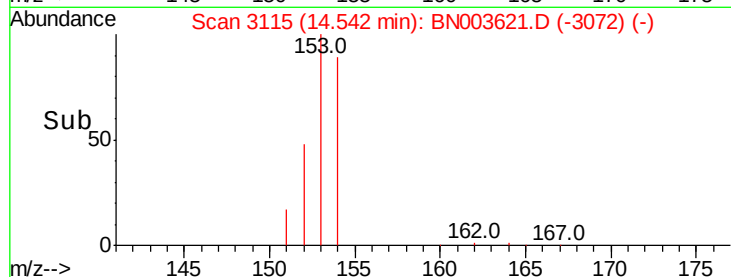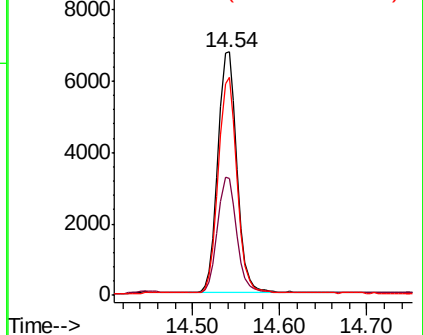

#11

Pentachlorophenol

Concen: 0.251 ng/ul

RT: 16.87 min Scan# 3625

Delta R.T. -0.00 min

Lab File: BN003621.D

Acq: 20 Nov 2018 06:56


Tgt Ion:266 Resp: 1650

Ion Ratio Lower Upper

266 100

264 62.1 49.4 74.2



268 62.7 51.7 77.5



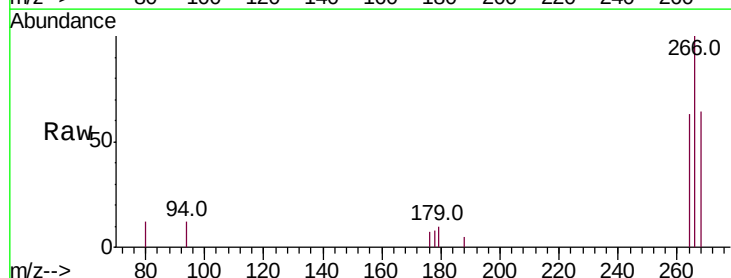


Abundance Ion 266.00 (265.70 to 266.70): E

Ion 264.00 (263.70 to 264.70): E

Ion 268.00 (267.70 to 268.70): E

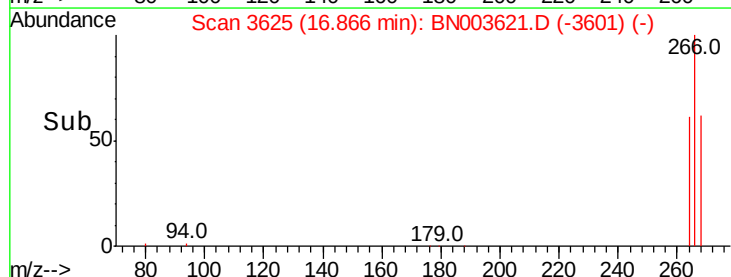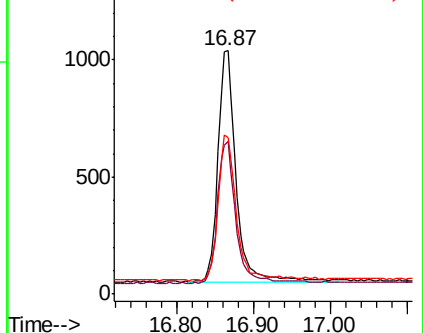

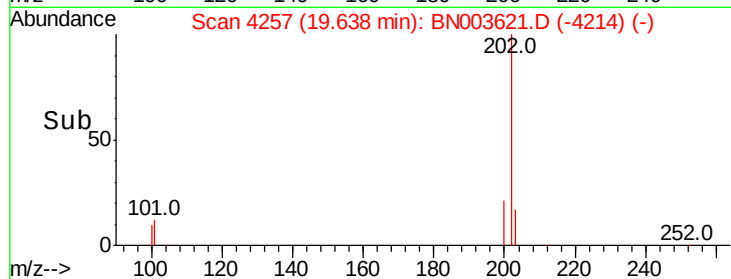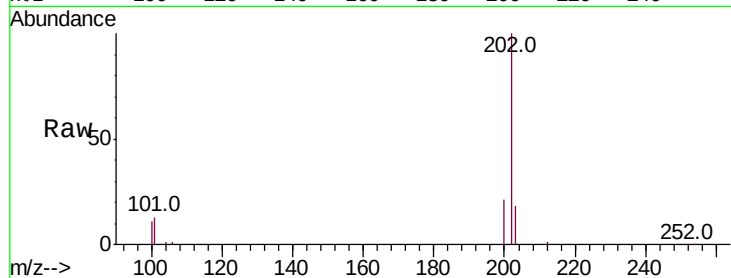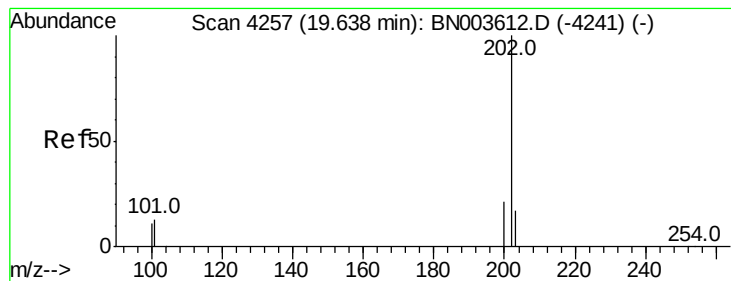

#17

Pvrene

Concen: 0.213 ng/ul

RT: 19.64 min Scan# 4257

Delta R.T. 0.00 min

Lab File: BN003621.D

Acq: 20 Nov 2018 06:56

Instrument :

BNA_N

ClientSampleId :

A4102MSD

Tot Ion:202 Resp: 27610

Ion Ratio Lower Upper

202 100

101 13.1 10.3 15.5

100 10.5 8.5 12.7

