




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111924\
Data File : BN035159.D
Acq On : 19 Nov 2024 13:17
Operator : RC/JU
Sample : PB165077BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK077

Manual IntegrationsAPPROVED

Quant Time: Nov 19 13:45:50 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 18 00:44:37 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/20/2024
Supervised By :mohammad ahmed 11/22/2024

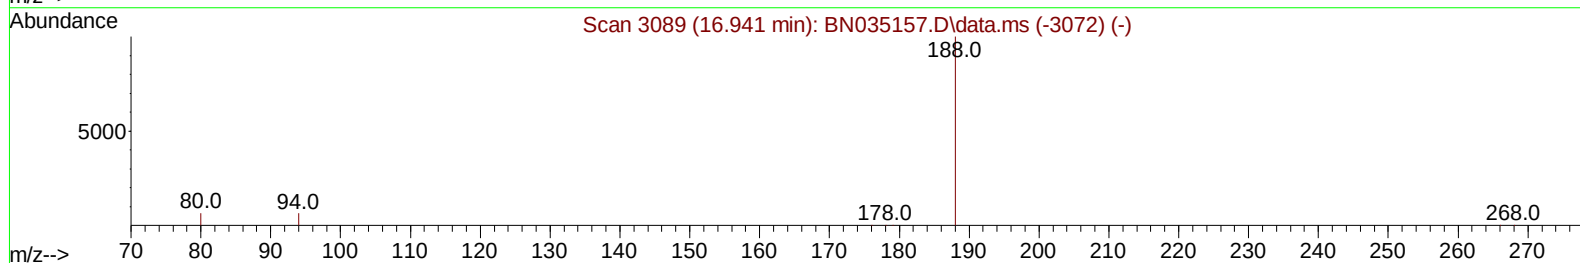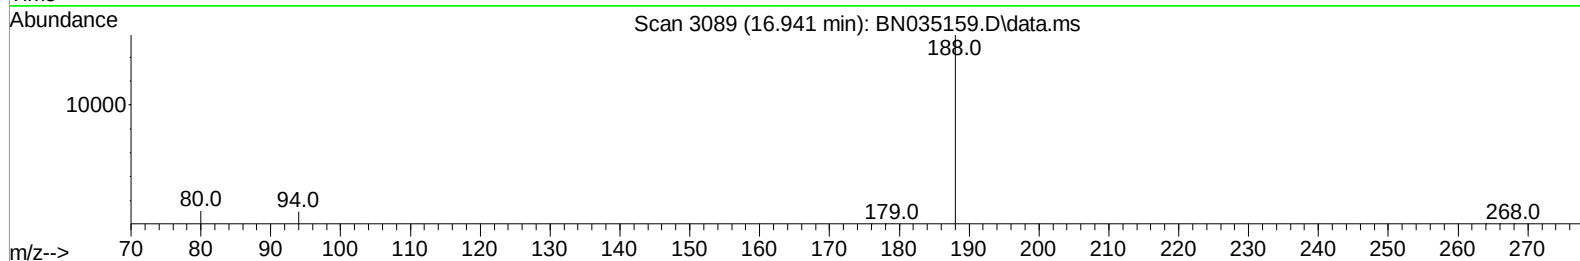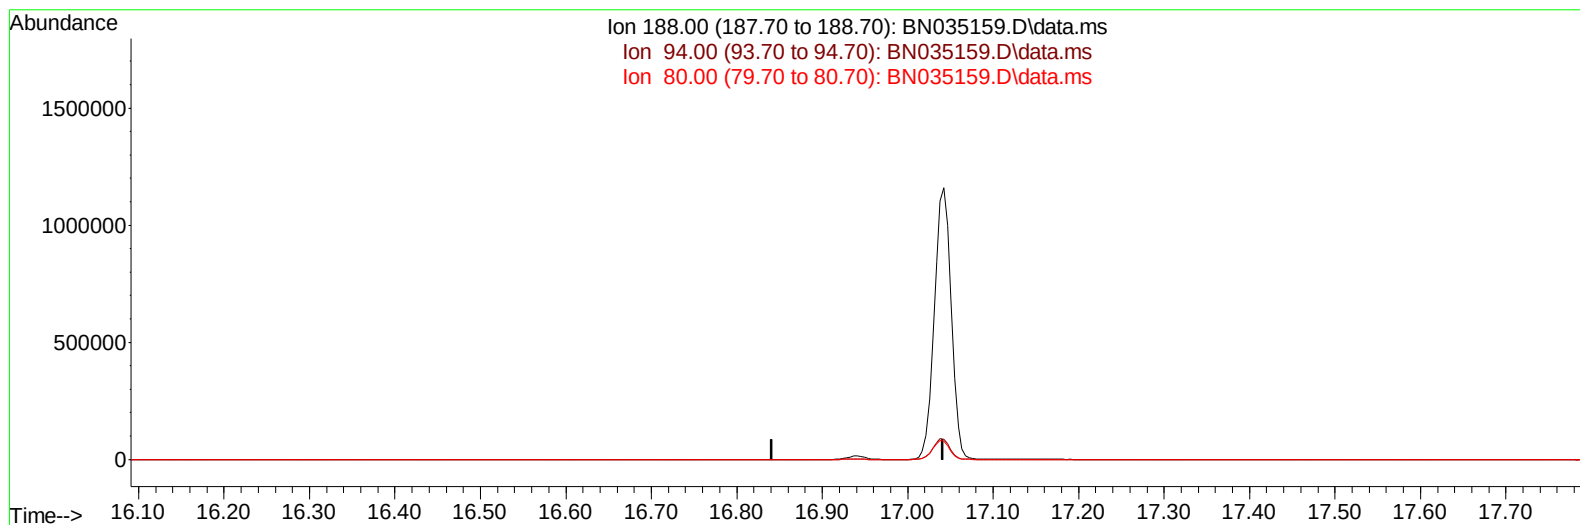

TIC: BN035159.D\data.ms

(13) Phenanthrene-d10 (I)

16.941min (-16.941) 0.00 ng/u1

response 0

Ion	Exp%	Act%
188.00	100.00	0.00
94.00	7.00	0.00#
80.00	7.60	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111924\
Data File : BN035159.D
Acq On : 19 Nov 2024 13:17
Operator : RC/JU
Sample : PB165077BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK077

Manual IntegrationsAPPROVED

Quant Time: Nov 19 13:45:50 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 18 00:44:37 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/20/2024
Supervised By :mohammad ahmed 11/22/2024

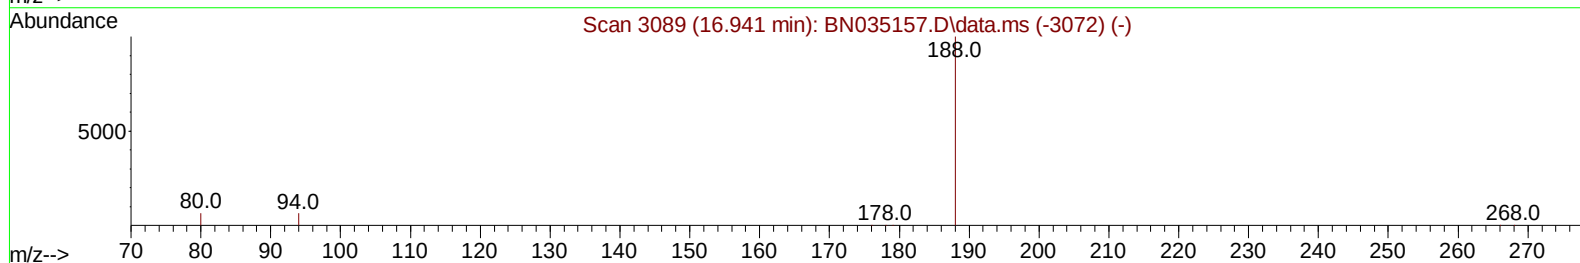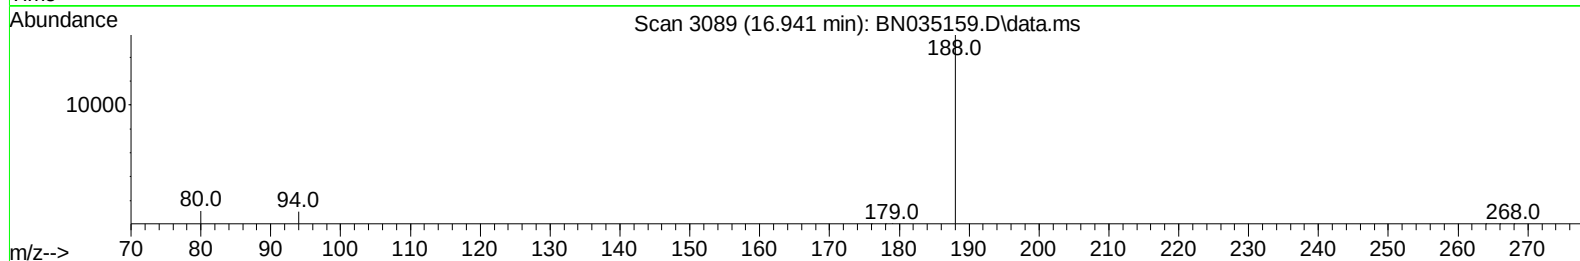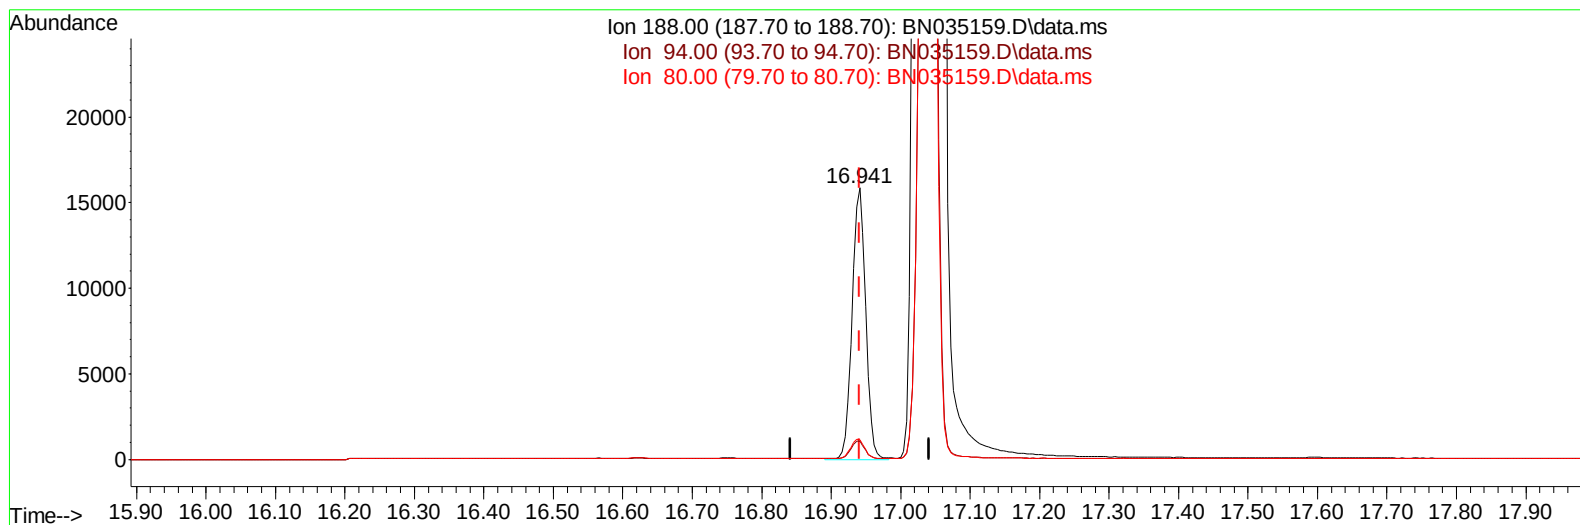

TIC: BN035159.D\data.ms

(13) Phenanthrene-d10 (I)

16.941min (-0.000) 0.40 ng/ul m

response 21492

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	7.00	6.73
80.00	7.60	7.14
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111924\
Data File : BN035159.D
Acq On : 19 Nov 2024 13:17
Operator : RC/JU
Sample : PB165077BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK077

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/20/2024
Supervised By :mohammad ahmed 11/22/2024

Quant Time: Nov 19 13:45:50 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 18 00:44:37 2024
Response via : Initial Calibration

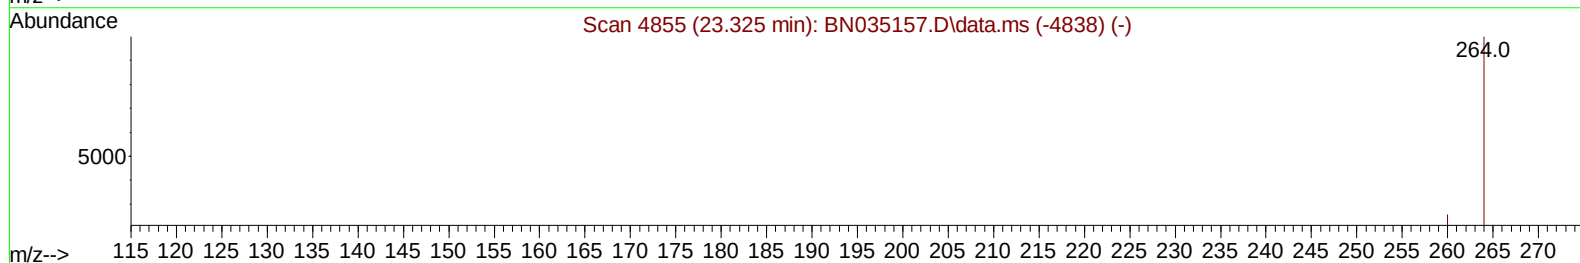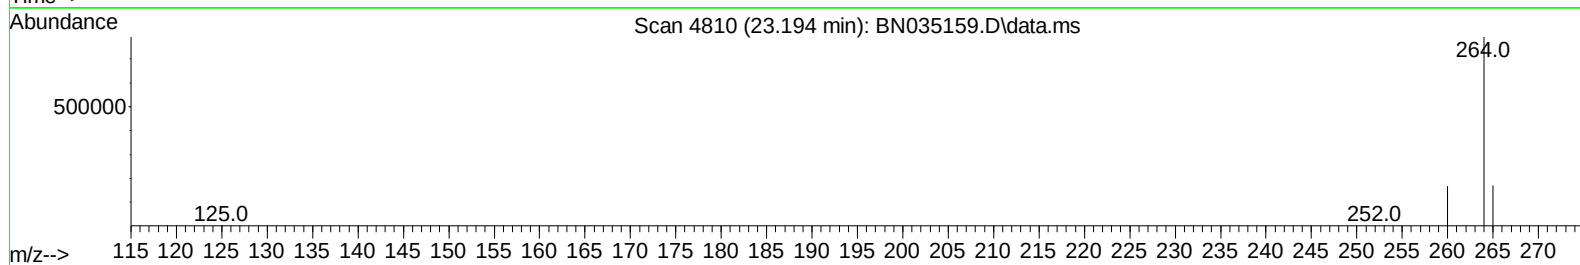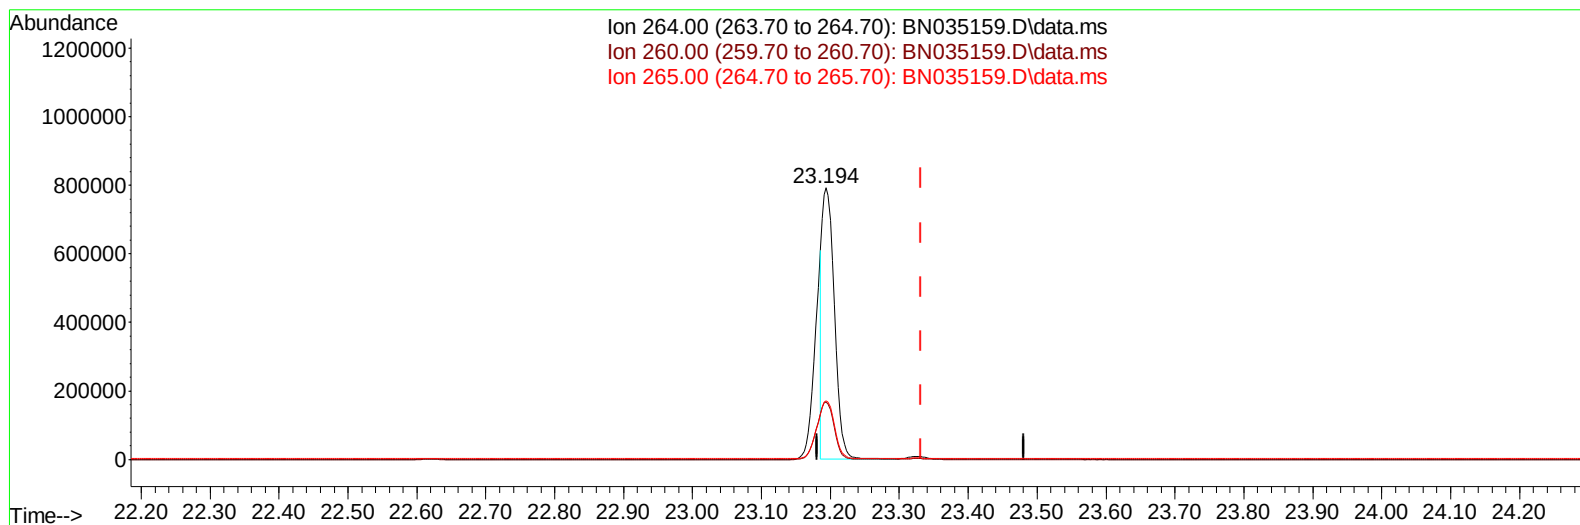

TIC: BN035159.D\data.ms

(23) Perylene-d12 (I)

23.194min (-0.138) 0.40 ng/u1

response 983787

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.20	21.21
265.00	75.50	21.61#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111924\
Data File : BN035159.D
Acq On : 19 Nov 2024 13:17
Operator : RC/JU
Sample : PB165077BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK077

Manual IntegrationsAPPROVED

Quant Time: Nov 19 13:45:50 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 18 00:44:37 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/20/2024
Supervised By :mohammad ahmed 11/22/2024

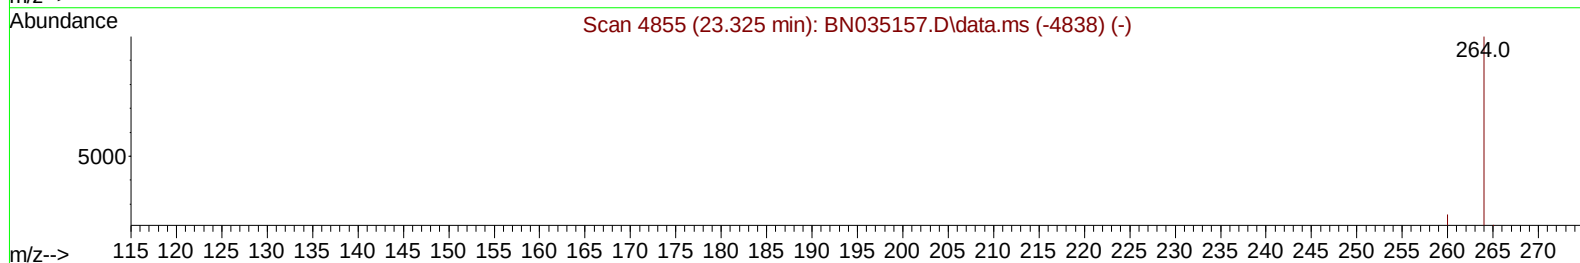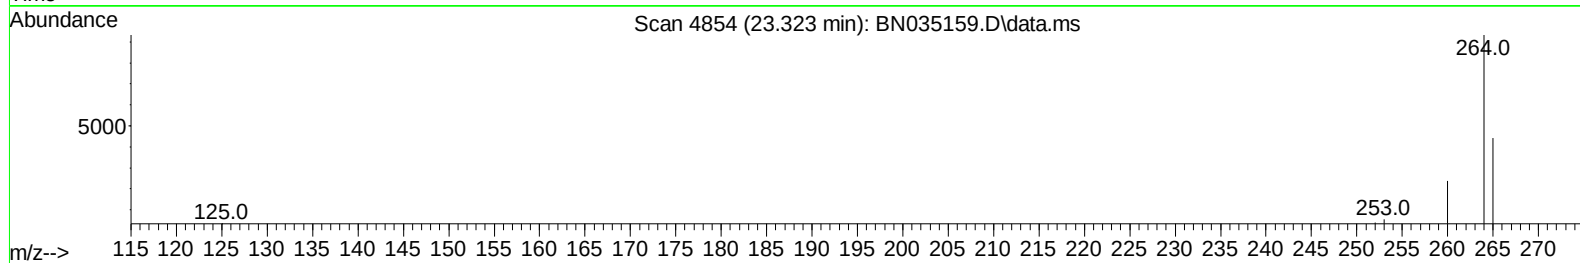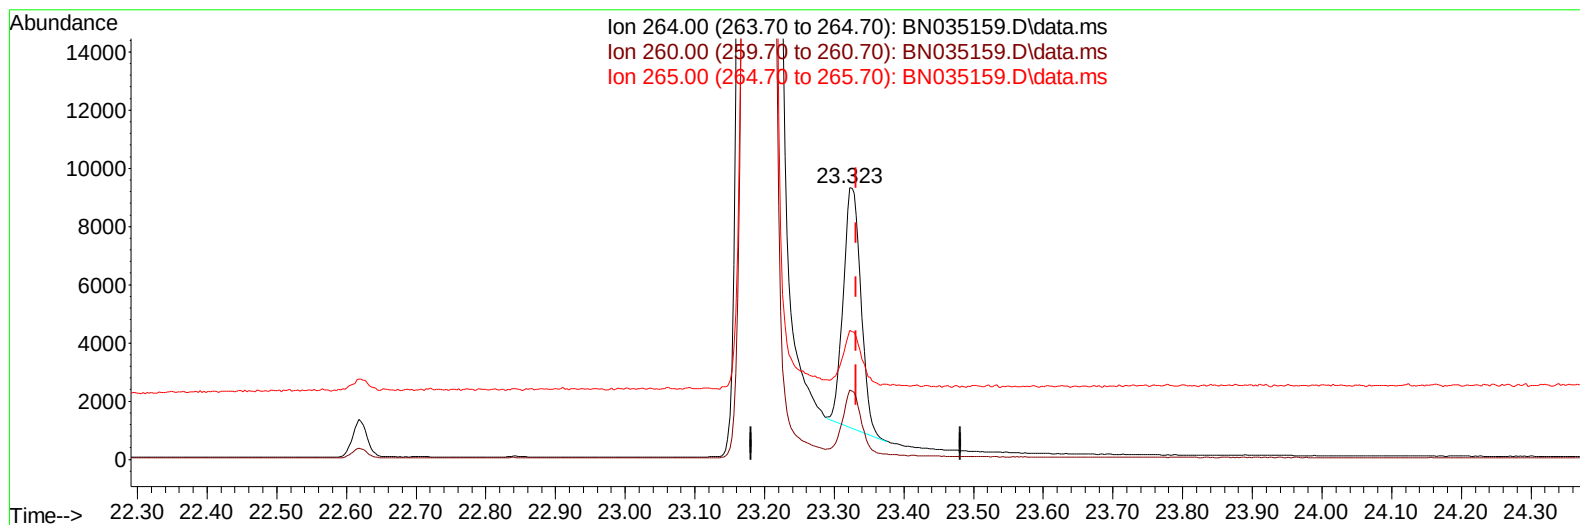

TIC: BN035159.D\data.ms

(23) Perylene-d12 (I)

23.323min (-0.009) 0.40 ng/ul m

response 14515

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.20	25.56
265.00	75.50	47.51#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111924\
 Data File : BN035159.D
 Acq On : 19 Nov 2024 13:17
 Operator : RC/JU
 Sample : PB165077BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK077

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/20/2024
 Supervised By :mohammad ahmed 11/22/2024

Quant Time: Nov 19 13:45:50 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 18 00:44:37 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.545	152	4785	0.400	ng/ul	0.00
4) Naphthalene-d8	10.306	136	12410	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.185	164	9341	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.941	188	21492m	0.400	ng/ul	0.00
17) Chrysene-d12	21.151	240	16488	0.400	ng/ul	0.00
23) Perylene-d12	23.323	264	14515m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.140	96	27451	6.277	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.906	152	7208	0.396	ng/ul	0.00
18) Fluoranthene-d10	18.977	212	20827	0.458	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111924\
Data File : BN035159.D
Acq On : 19 Nov 2024 13:17
Operator : RC/JU
Sample : PB165077BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK077

Manual IntegrationsAPPROVED

Quant Time: Nov 19 13:45:50 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 18 00:44:37 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/20/2024
Supervised By :mohammad ahmed 11/22/2024

