




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111924\
 Data File : BP023229.D
 Acq On : 19 Nov 2024 22:44
 Operator : RC/JU
 Sample : P4847-03
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK077

Manual IntegrationsAPPROVED

Quant Time: Nov 20 00:28:25 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 13 04:49:01 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/20/2024
 Supervised By :mohammad ahmed 11/22/2024

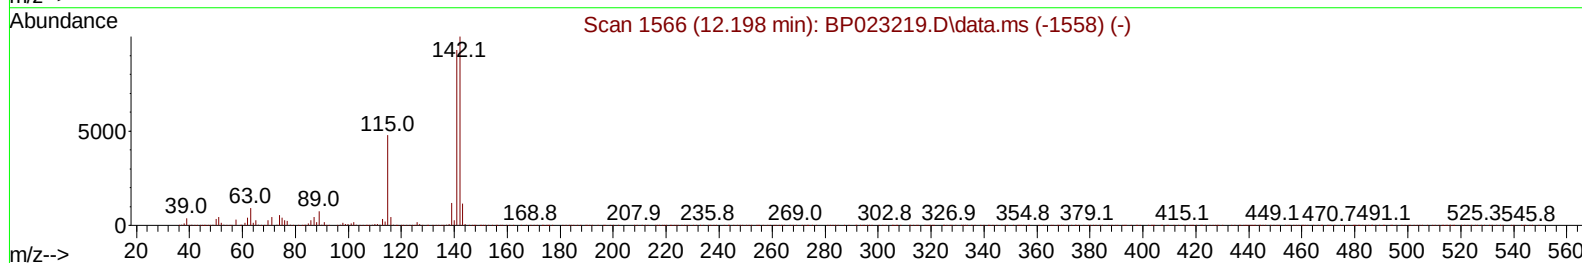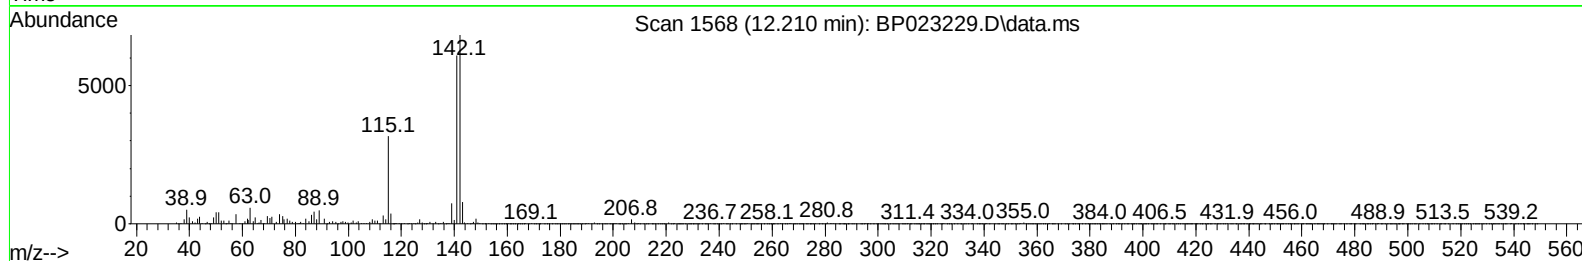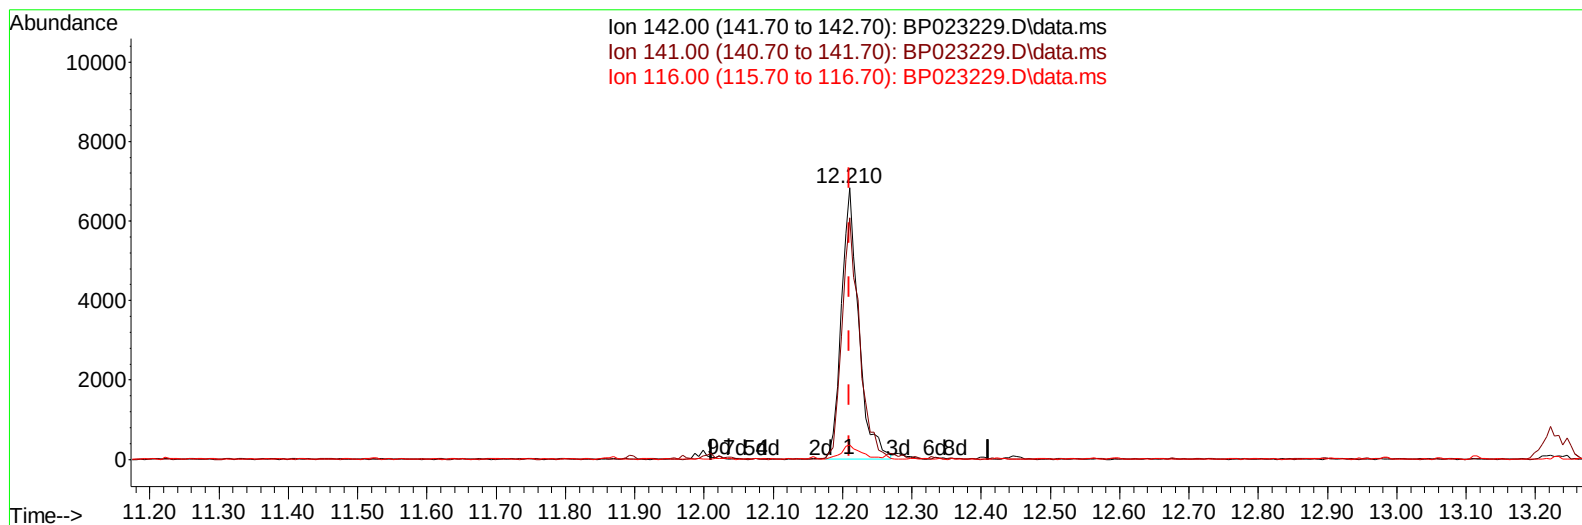

TIC: BP023229.D\data.ms

(37) 1-Methylnaphthalene

12.210min (-0.000) 1.16 ng/ul m

response 11821

Ion	Exp%	Act%
142.00	100.00	100.00
141.00	92.30	89.06
116.00	5.30	5.31
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111924\
Data File : BN035182.D
Acq On : 20 Nov 2024 03:52
Operator : RC/JU
Sample : PB165077BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK077

Manual IntegrationsAPPROVED

Quant Time: Nov 20 04:20:23 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 18 00:44:37 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/20/2024
Supervised By :mohammad ahmed 11/22/2024

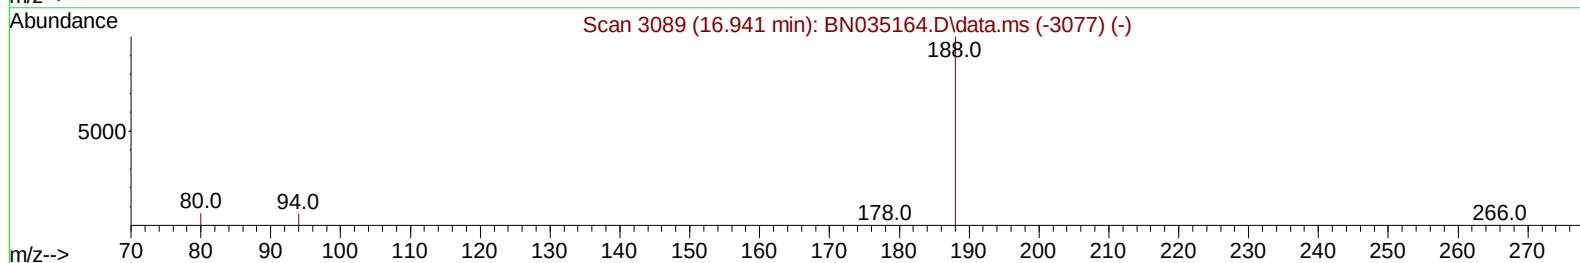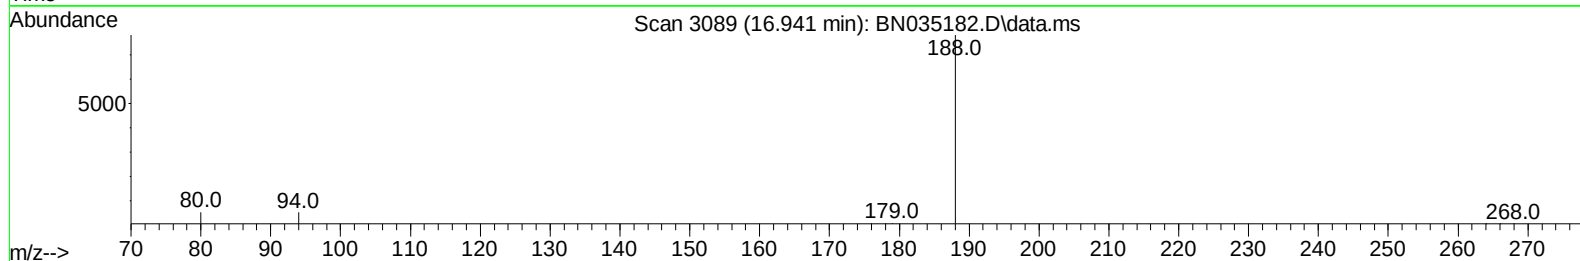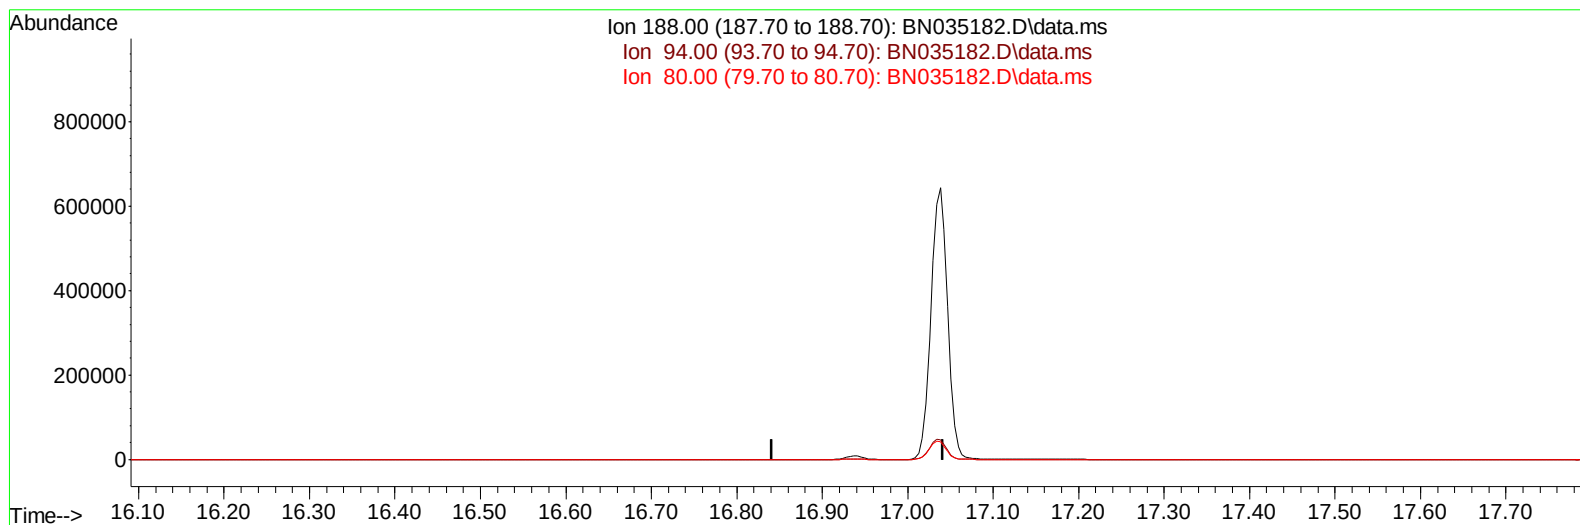

TIC: BN035182.D\data.ms

(13) Phenanthrene-d10 (I)

16.941min (-16.941) 0.00 ng/u1

response 0

Ion	Exp%	Act%
188.00	100.00	0.00
94.00	7.00	0.00#
80.00	7.60	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111924\
Data File : BN035182.D
Acq On : 20 Nov 2024 03:52
Operator : RC/JU
Sample : PB165077BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK077

Manual IntegrationsAPPROVED

Quant Time: Nov 20 04:20:23 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 18 00:44:37 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/20/2024
Supervised By :mohammad ahmed 11/22/2024

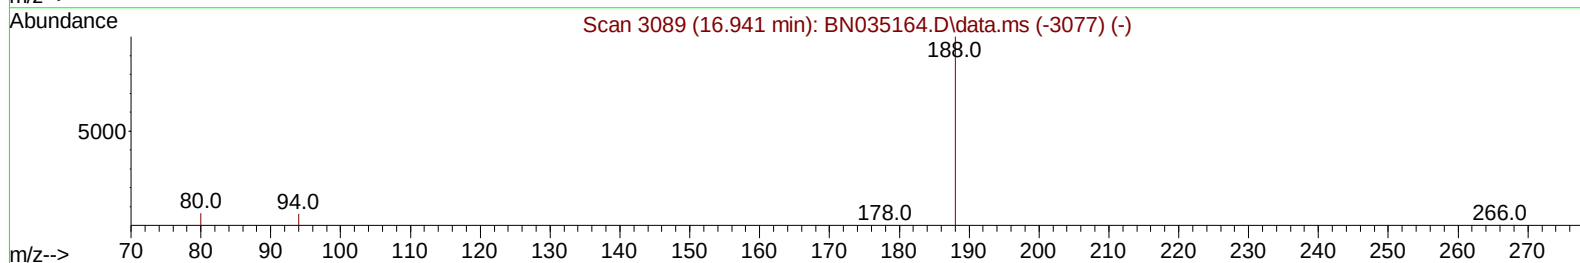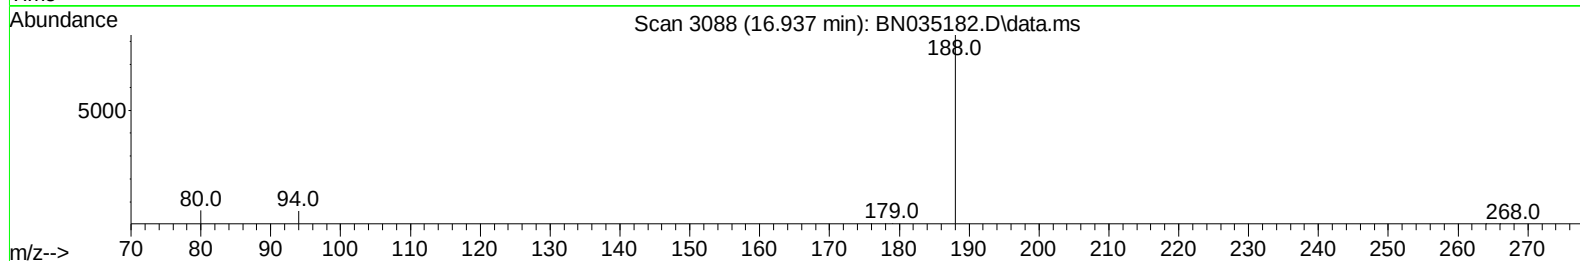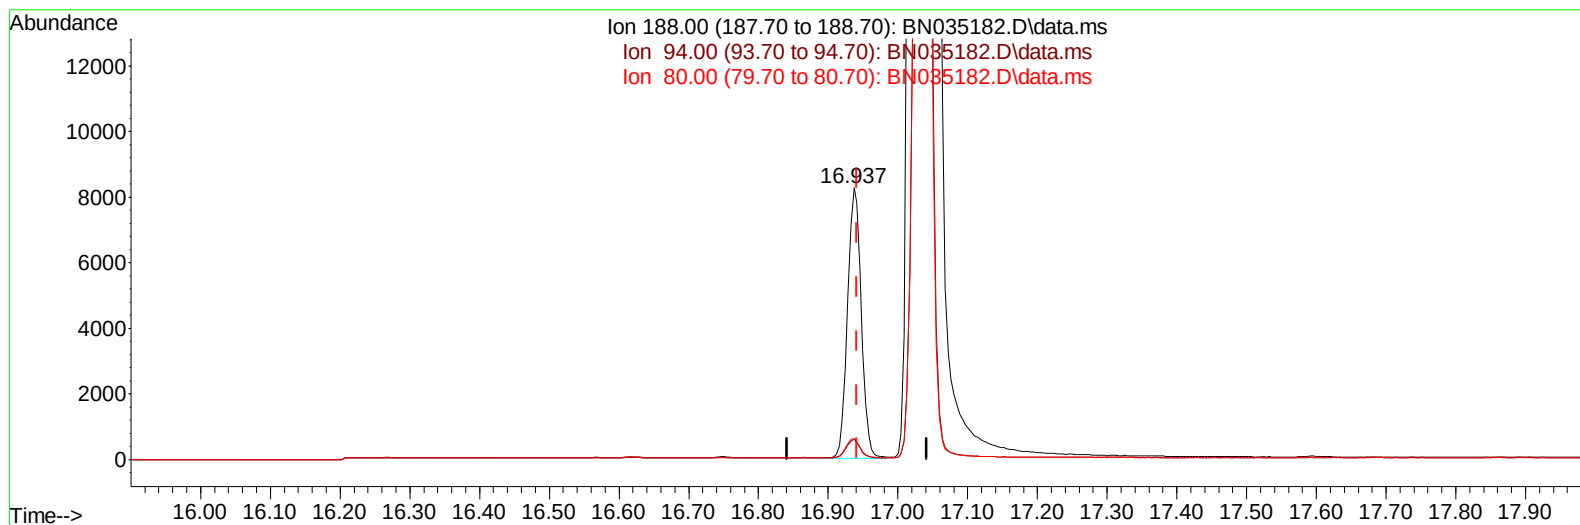

TIC: BN035182.D\data.ms

(13) Phenanthrene-d10 (I)

16.937min (-0.004) 0.40 ng/ul m

response 11261

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	7.00	7.38
80.00	7.60	7.62
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111924\
Data File : BN035182.D
Acq On : 20 Nov 2024 03:52
Operator : RC/JU
Sample : PB165077BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK077

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/20/2024
Supervised By :mohammad ahmed 11/22/2024

Quant Time: Nov 20 04:20:23 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 18 00:44:37 2024
Response via : Initial Calibration

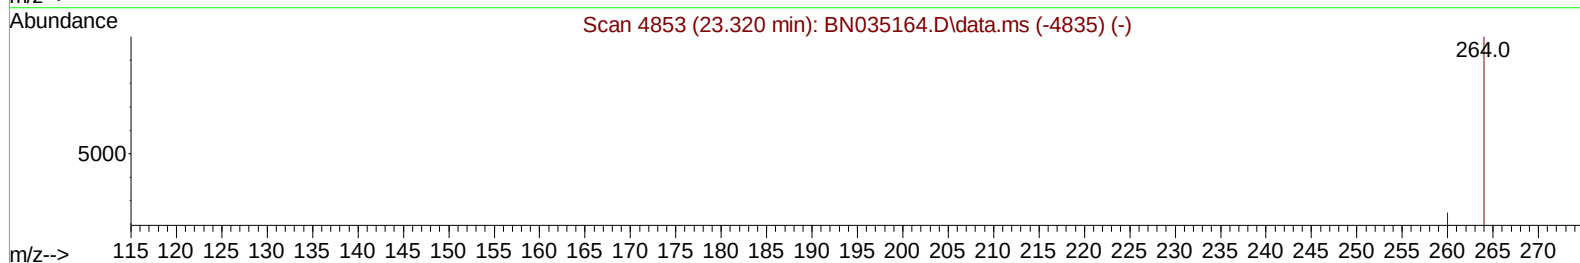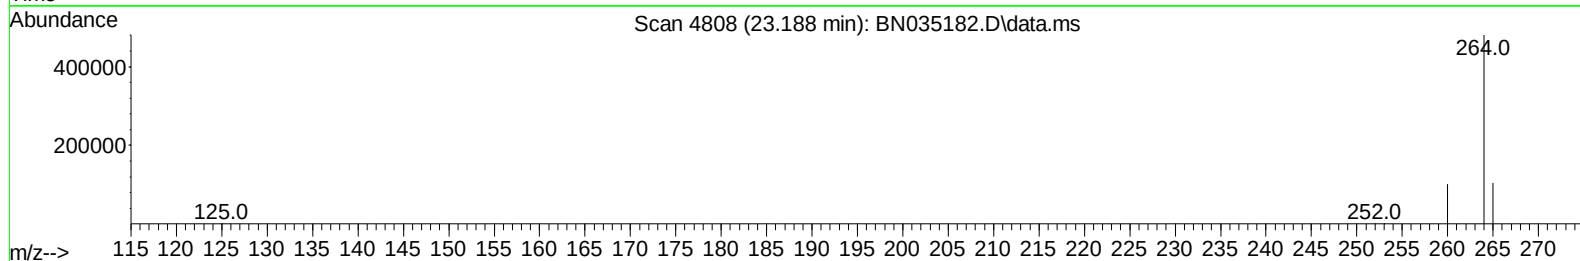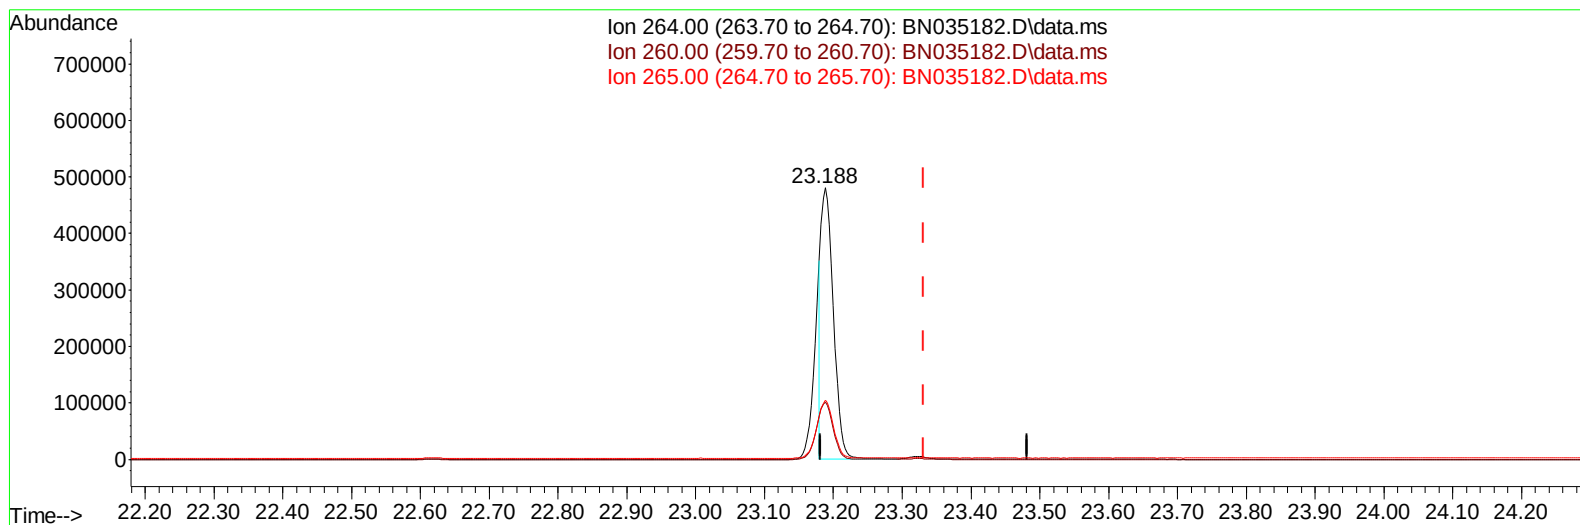

TIC: BN035182.D\data.ms

(23) Perylene-d12 (I)

23.188min (-0.143) 0.40 ng/u1

response 596381

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.20	21.02
265.00	75.50	21.76#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111924\
Data File : BN035182.D
Acq On : 20 Nov 2024 03:52
Operator : RC/JU
Sample : PB165077BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK077

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/20/2024
Supervised By :mohammad ahmed 11/22/2024

Quant Time: Nov 20 04:20:23 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 18 00:44:37 2024
Response via : Initial Calibration

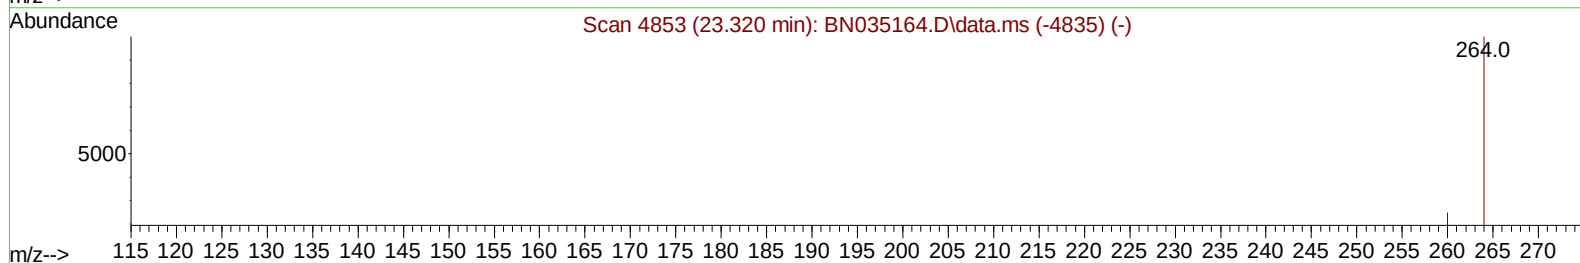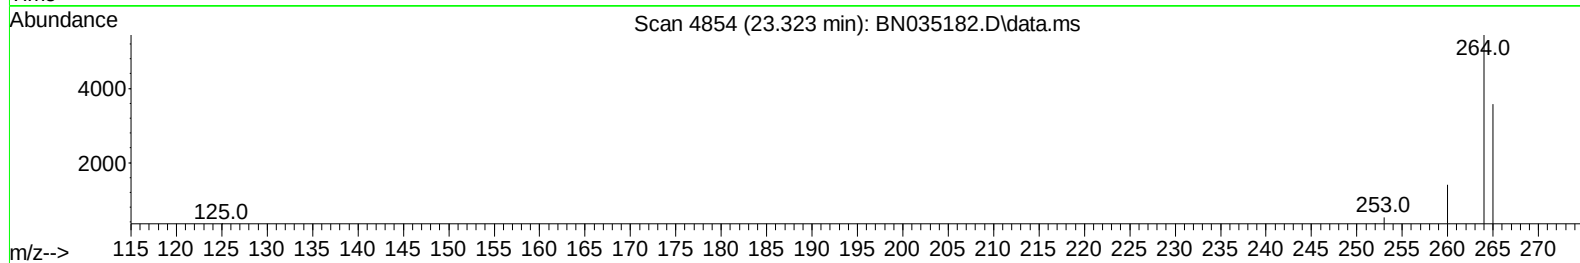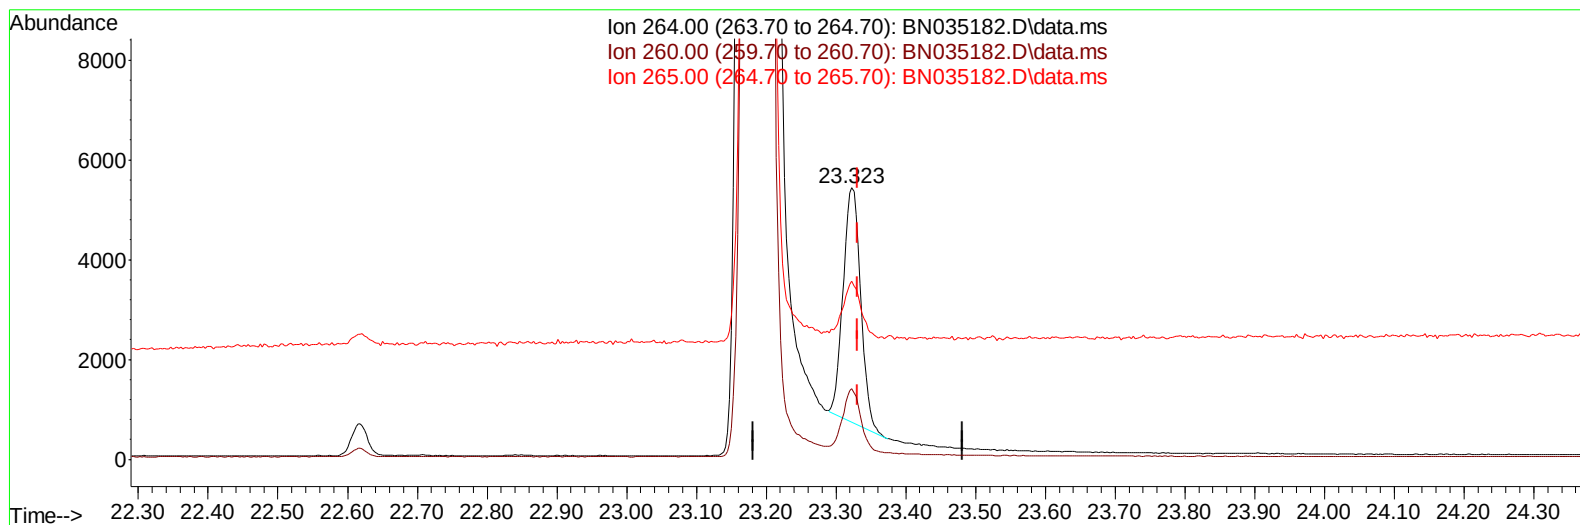

TIC: BN035182.D\data.ms

(23) Perylene-d12 (I)

23.323min (-0.009) 0.40 ng/ul m

response 8239

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.20	25.98
265.00	75.50	65.73
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111924\
 Data File : BN035182.D
 Acq On : 20 Nov 2024 03:52
 Operator : RC/JU
 Sample : PB165077BL
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK077

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/20/2024
 Supervised By :mohammad ahmed 11/22/2024

Quant Time: Nov 20 04:20:23 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 18 00:44:37 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.541	152	3181	0.400	ng/ul	0.00
4) Naphthalene-d8	10.306	136	7901	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.185	164	5542	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.937	188	11261m	0.400	ng/ul	0.00
17) Chrysene-d12	21.148	240	8223	0.400	ng/ul	0.00
23) Perylene-d12	23.323	264	8239m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.136	96	18584	6.392	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.901	152	4489	0.388	ng/ul	-0.01
18) Fluoranthene-d10	18.977	212	9984	0.440	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111924\
Data File : BN035182.D
Acq On : 20 Nov 2024 03:52
Operator : RC/JU
Sample : PB165077BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK077

Manual IntegrationsAPPROVED

Quant Time: Nov 20 04:20:23 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 18 00:44:37 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/20/2024
Supervised By :mohammad ahmed 11/22/2024

