




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111924\
Data File : BN035190.D
Acq On : 20 Nov 2024 09:05
Operator : RC/JU
Sample : PB164841BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK841

Manual IntegrationsAPPROVED

Quant Time: Nov 20 09:38:55 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 18 00:44:37 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/21/2024
Supervised By :mohammad ahmed 11/22/2024

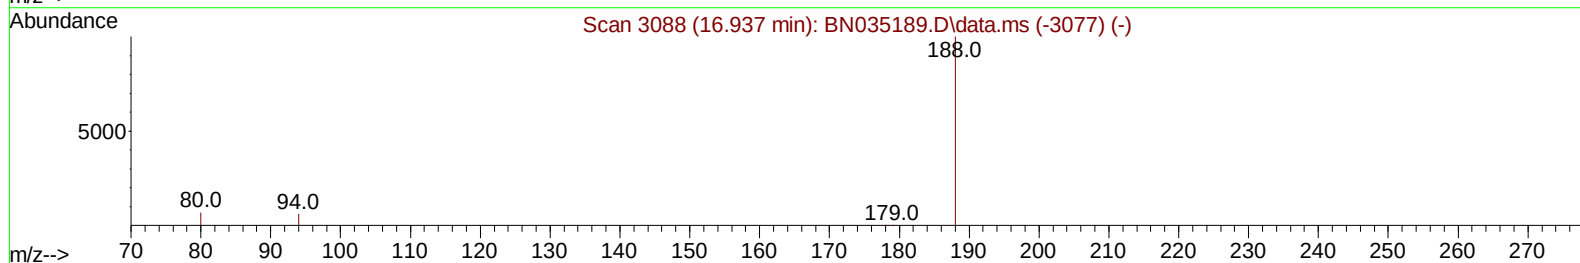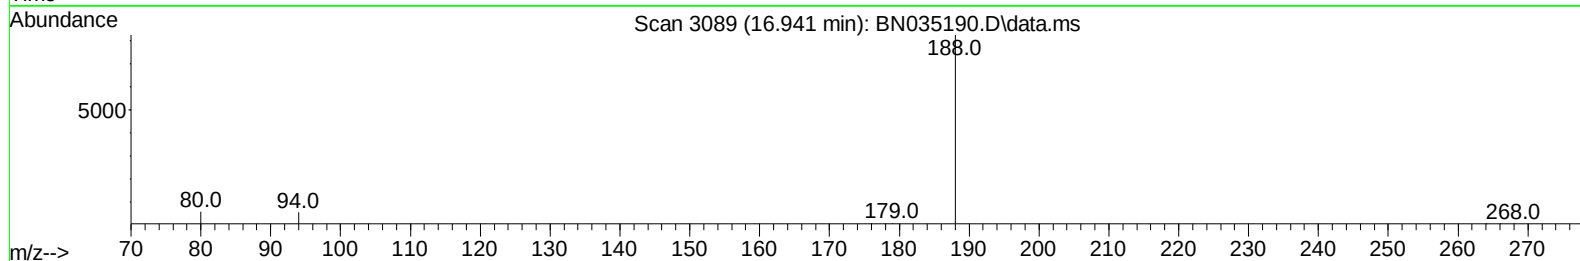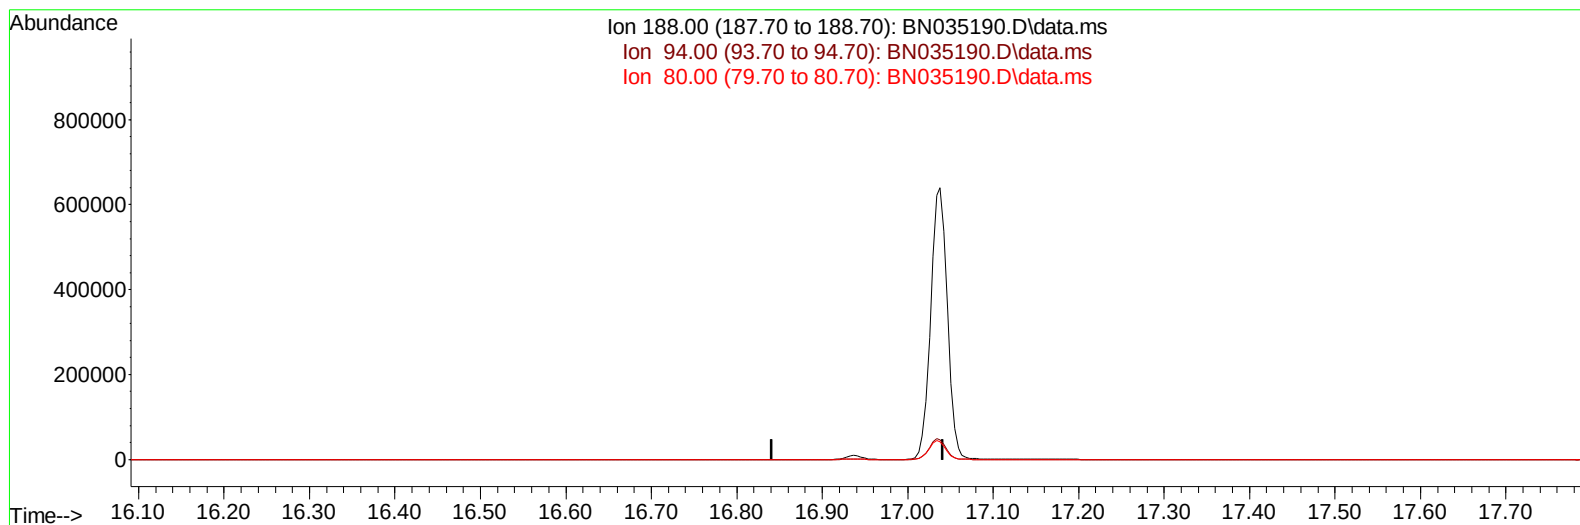

TIC: BN035190.D\data.ms

(13) Phenanthrene-d10 (I)

16.941min (-16.941) 0.00 ng/u1

response 0

Ion	Exp%	Act%
188.00	100.00	0.00
94.00	7.00	0.00#
80.00	7.60	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111924\
Data File : BN035190.D
Acq On : 20 Nov 2024 09:05
Operator : RC/JU
Sample : PB164841BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK841

Manual IntegrationsAPPROVED

Quant Time: Nov 20 09:38:55 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 18 00:44:37 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/21/2024
Supervised By :mohammad ahmed 11/22/2024

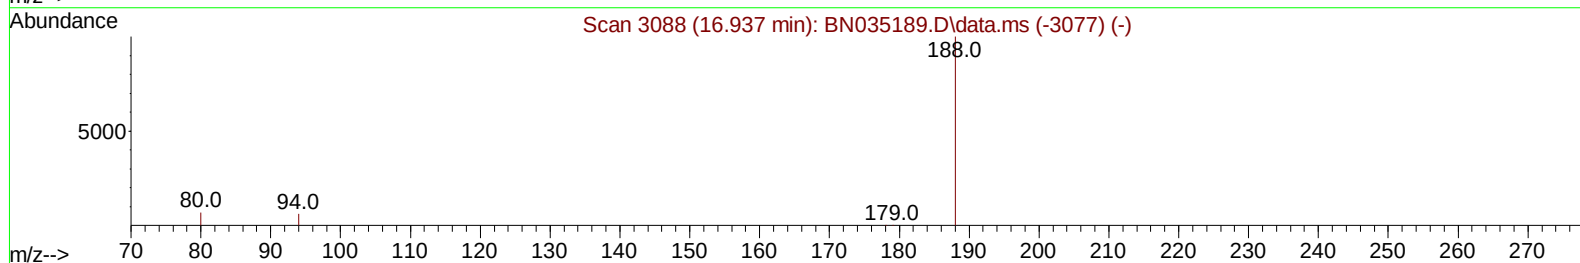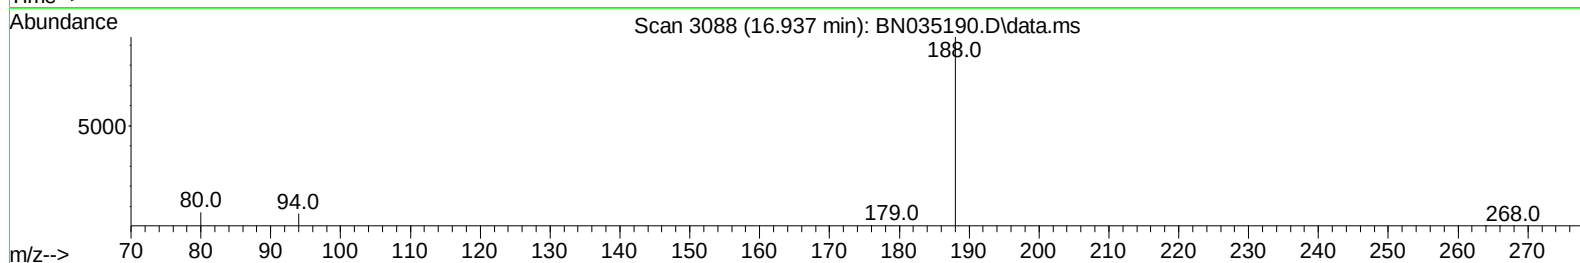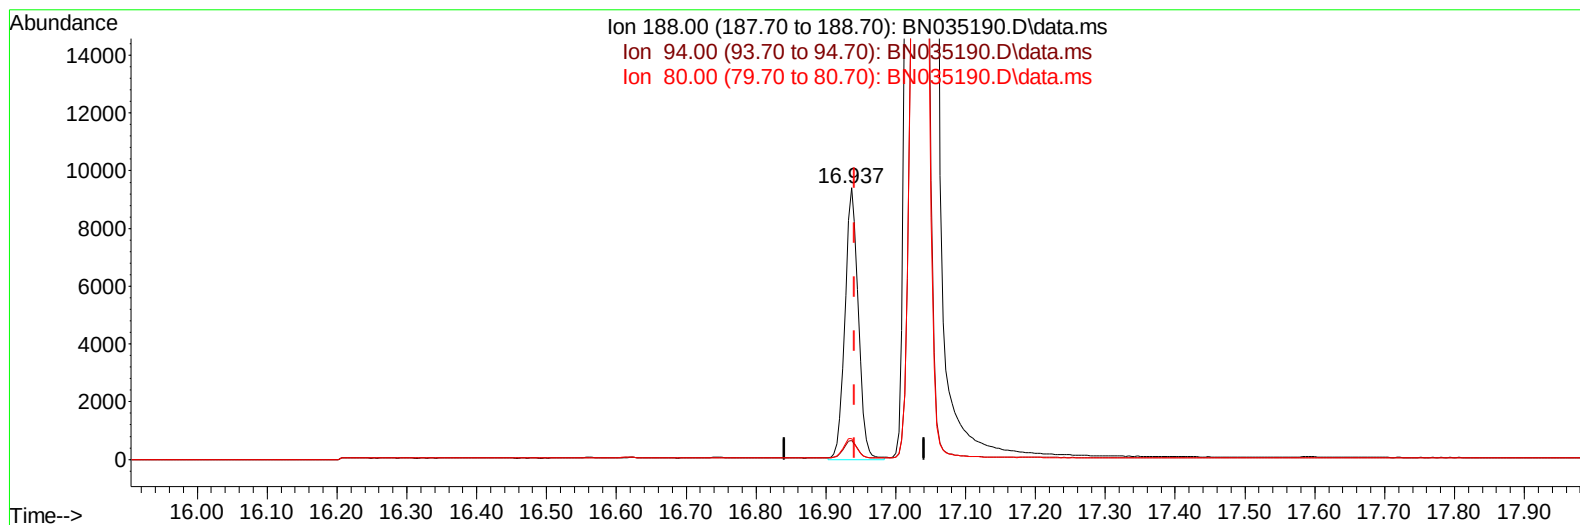

TIC: BN035190.D\data.ms

(13) Phenanthrene-d10 (I)

16.937min (-0.004) 0.40 ng/ul m

response 12500

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	7.00	6.92
80.00	7.60	7.61
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111924\
Data File : BN035190.D
Acq On : 20 Nov 2024 09:05
Operator : RC/JU
Sample : PB164841BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK841

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/21/2024
Supervised By :mohammad ahmed 11/22/2024

Quant Time: Nov 20 09:38:55 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 18 00:44:37 2024
Response via : Initial Calibration

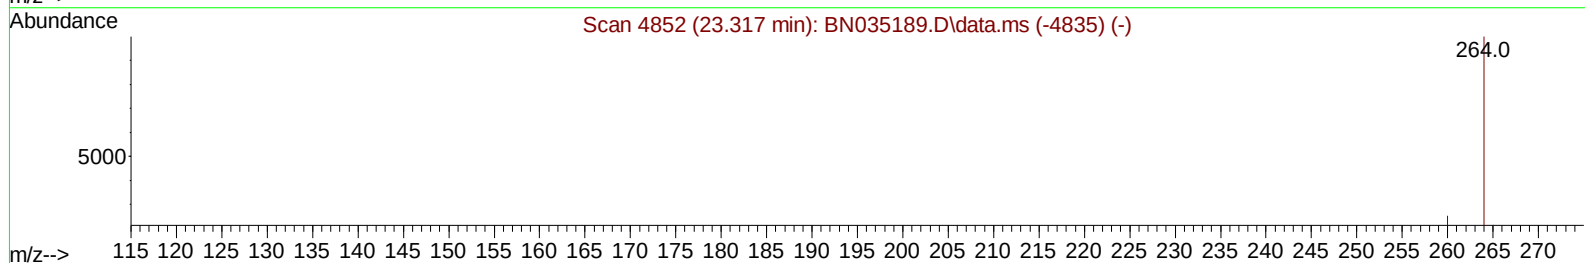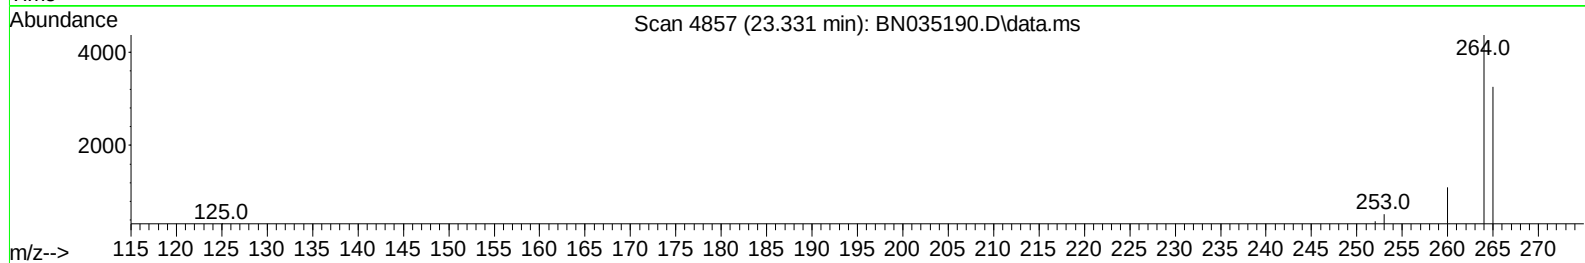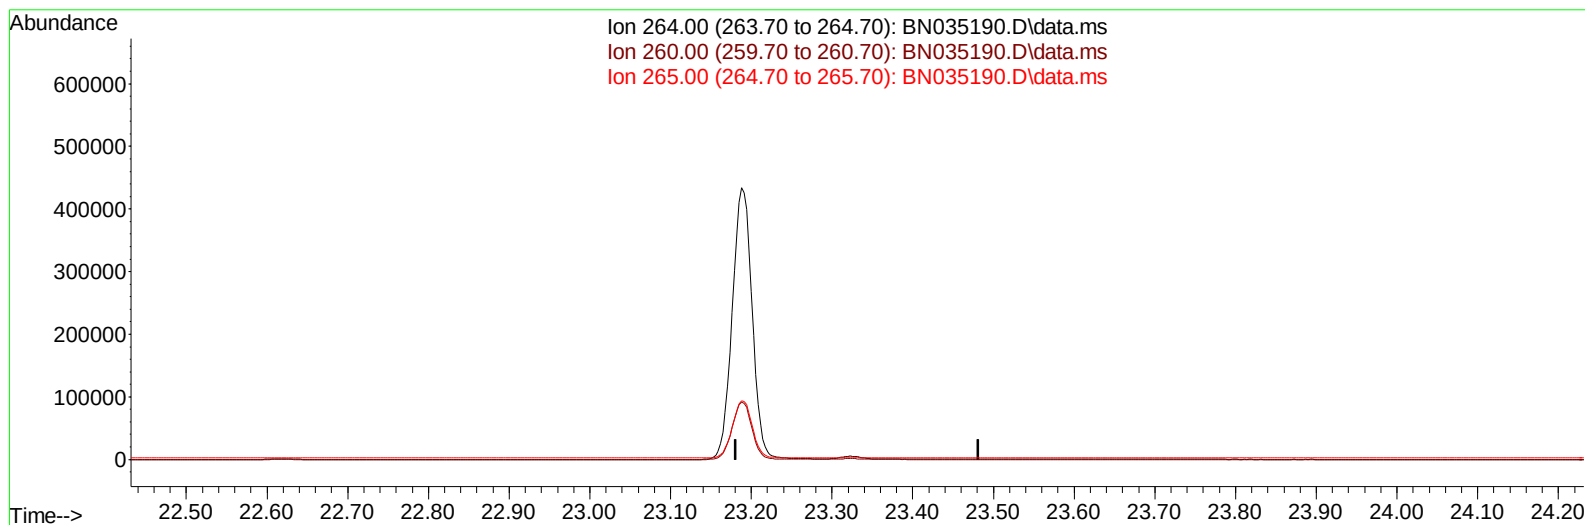

TIC: BN035190.D\data.ms

(23) Perylene-d12 (I)

23.331min (-23.331) 0.00 ng/ul

response 0

Ion	Exp%	Act%
264.00	100.00	0.00
260.00	26.20	0.00#
265.00	75.50	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111924\
Data File : BN035190.D
Acq On : 20 Nov 2024 09:05
Operator : RC/JU
Sample : PB164841BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK841

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/21/2024
Supervised By :mohammad ahmed 11/22/2024

Quant Time: Nov 20 09:38:55 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 18 00:44:37 2024
Response via : Initial Calibration

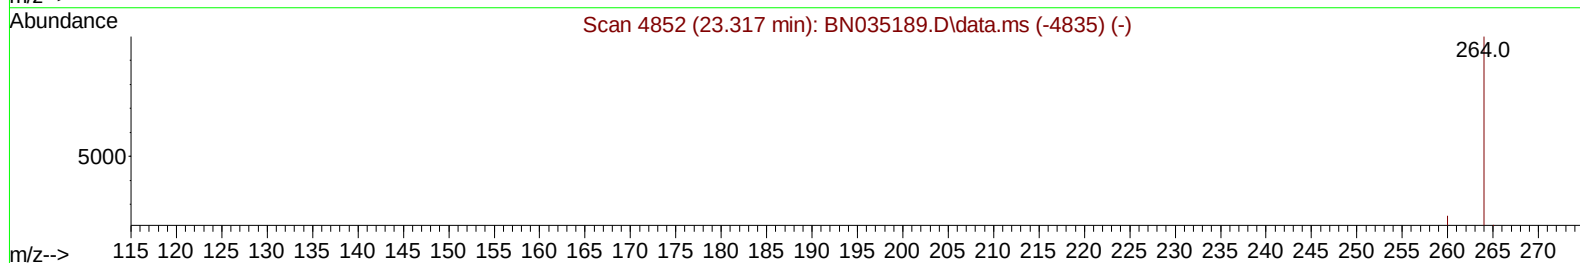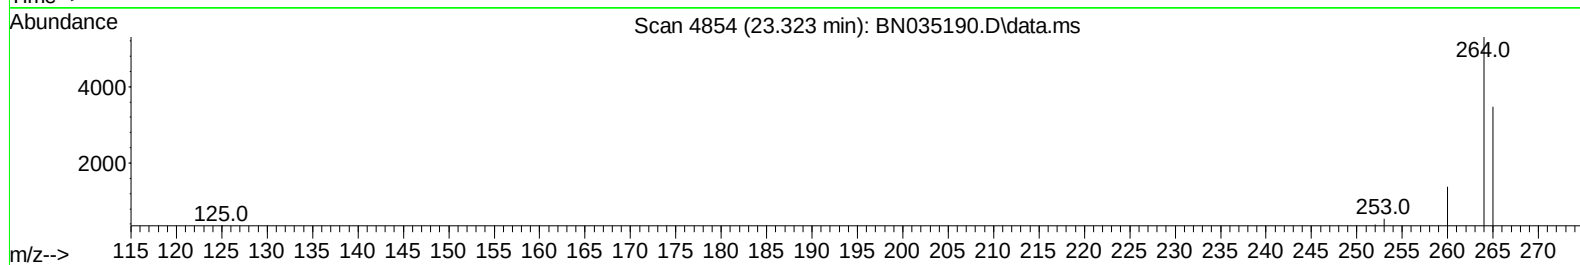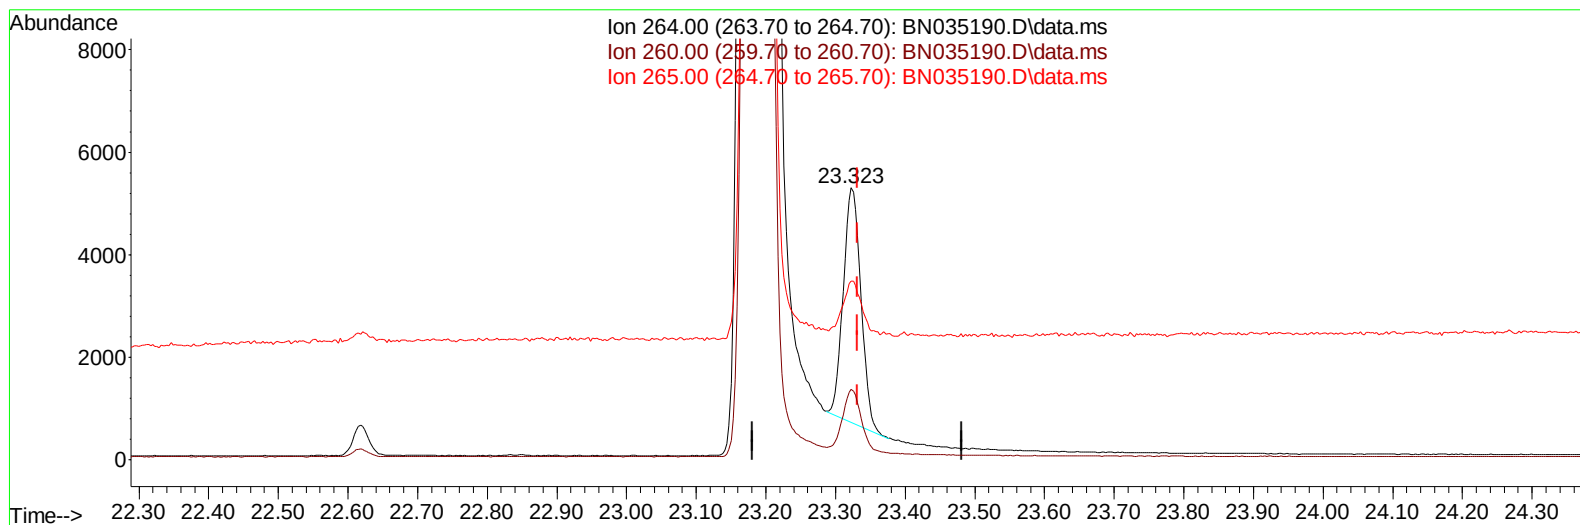

TIC: BN035190.D\data.ms

(23) Perylene-d12 (I)

23.323min (-0.009) 0.40 ng/ul m

response 8074

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.20	25.90
265.00	75.50	65.60
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111924\
 Data File : BN035190.D
 Acq On : 20 Nov 2024 09:05
 Operator : RC/JU
 Sample : PB164841BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK841

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/21/2024
 Supervised By :mohammad ahmed 11/22/2024

Quant Time: Nov 20 09:38:55 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 18 00:44:37 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.537	152	3236	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.300	136	8314	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.180	164	5881	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.937	188	12500m	0.400	ng/ul	0.00
17) Chrysene-d12	21.151	240	8471	0.400	ng/ul	0.00
23) Perylene-d12	23.323	264	8074m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.132	96	17971	6.076	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.901	152	4350	0.357	ng/ul	-0.01
18) Fluoranthene-d10	18.977	212	10073	0.431	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111924\
Data File : BN035190.D
Acq On : 20 Nov 2024 09:05
Operator : RC/JU
Sample : PB164841BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK841

Manual IntegrationsAPPROVED

Quant Time: Nov 20 09:38:55 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 18 00:44:37 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/21/2024
Supervised By :mohammad ahmed 11/22/2024

