

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111924\
 Data File : BN035184.D
 Acq On : 20 Nov 2024 05:04
 Operator : RC/JU
 Sample : P4875-08
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E2A22

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/20/2024
 Supervised By :mohammad ahmed 11/22/2024

Quant Time: Nov 20 05:32:24 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 18 00:44:37 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.541	152	3561	0.400	ng/ul	0.00
4) Naphthalene-d8	10.306	136	8518	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.185	164	5678	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.937	188	11743m	0.400	ng/ul	0.00
17) Chrysene-d12	21.148	240	10233	0.400	ng/ul	0.00
23) Perylene-d12	23.320	264	10784m	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.136	96	15346	4.715	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.901	152	4452	0.357	ng/ul	-0.01
18) Fluoranthene-d10	18.977	212	12363	0.438	ng/ul	0.00
Target Compounds						
					Qvalue	
5) Naphthalene	10.350	128	432	0.020	ng/ul#	64

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111924\
Data File : BN035184.D
Acq On : 20 Nov 2024 05:04
Operator : RC/JU
Sample : P4875-08
Misc :
ALS Vial : 29 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
E2A22

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/20/2024
Supervised By :mohammad ahmed 11/22/2024


Quant Time: Nov 20 05:32:24 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 18 00:44:37 2024
Response via : Initial Calibration

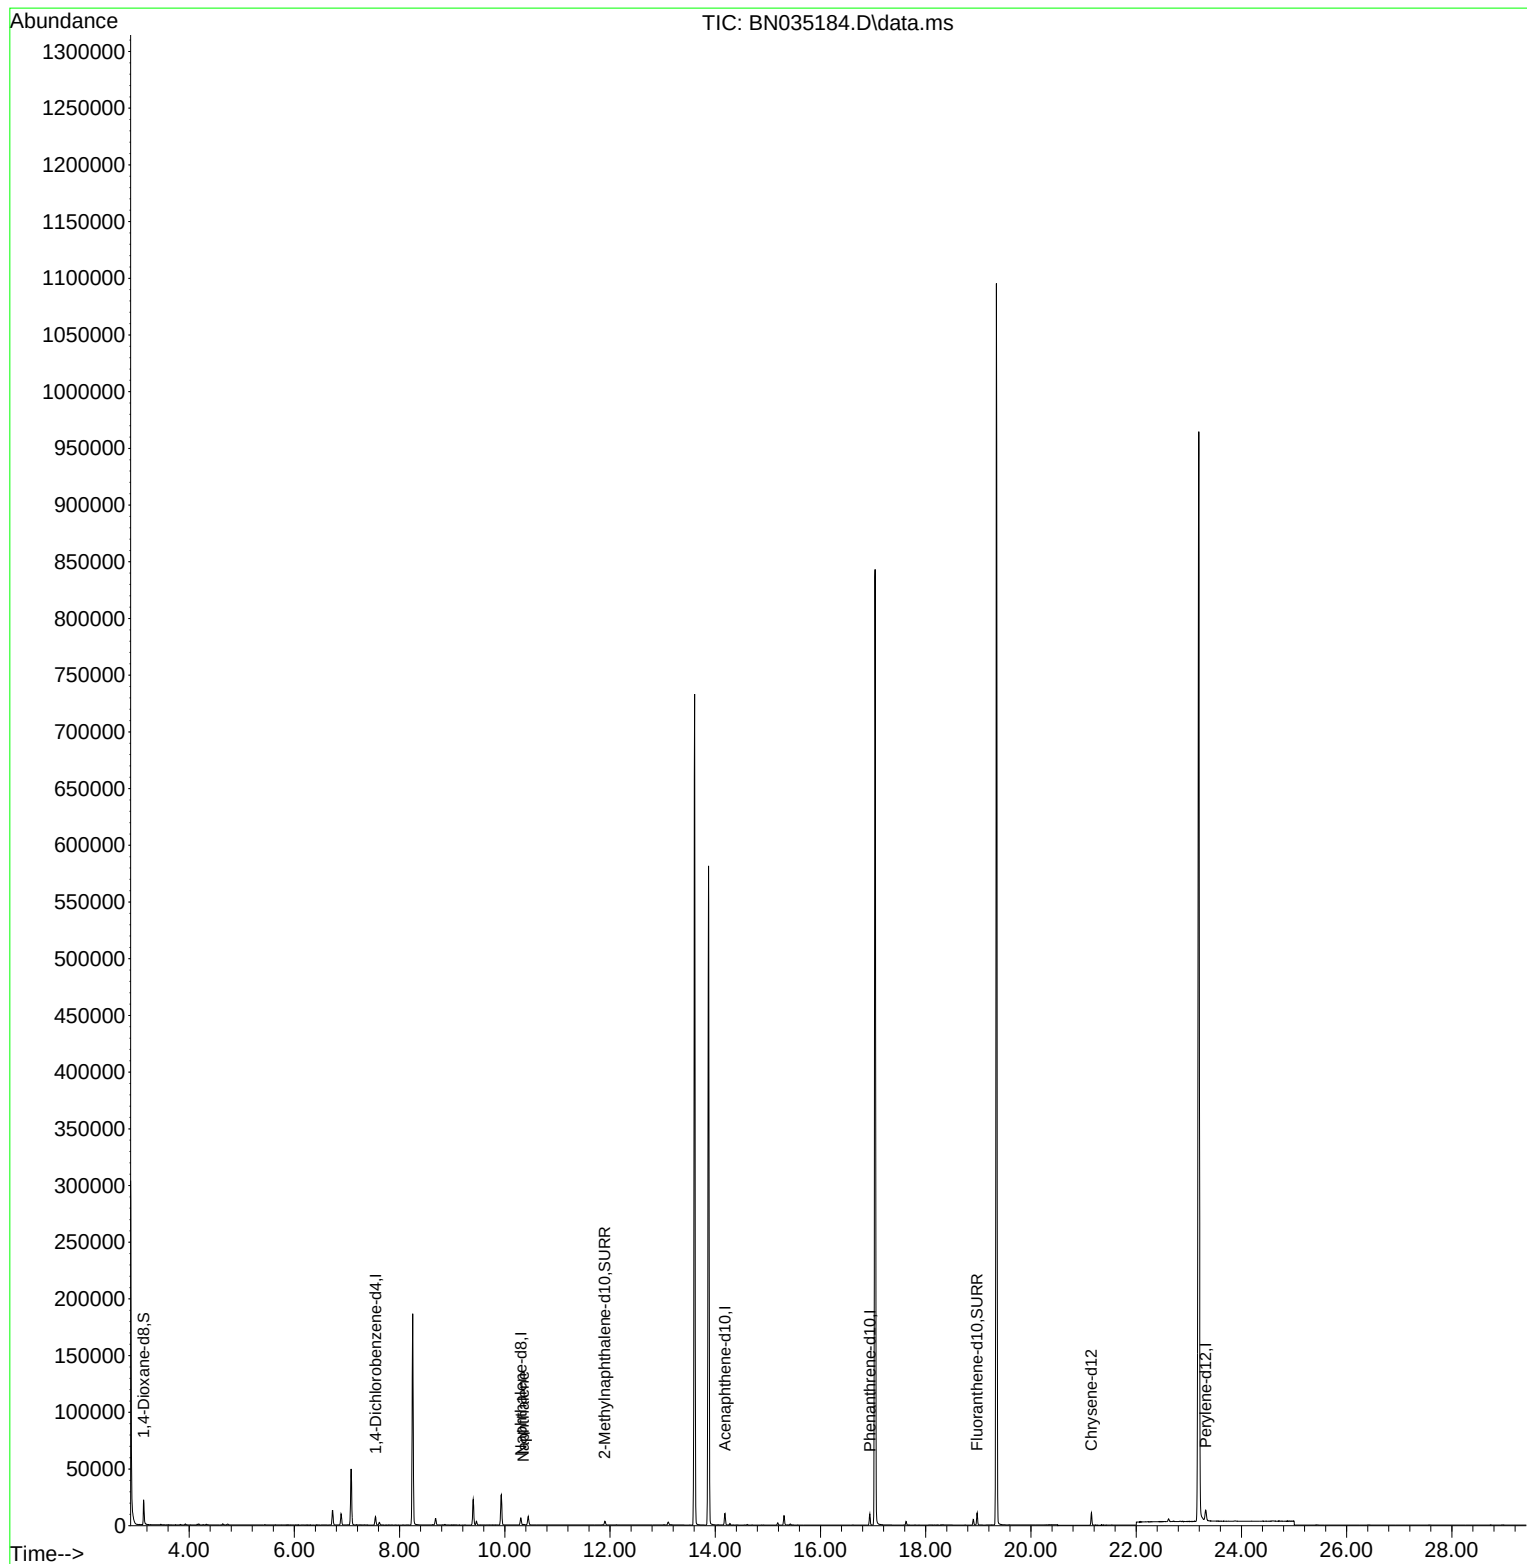

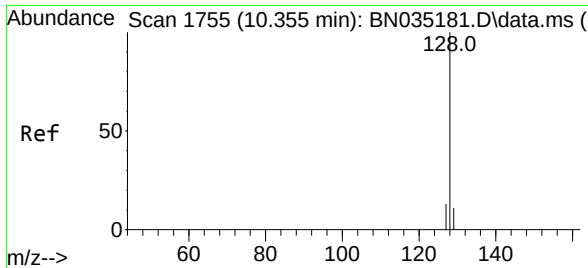

#5
Naphthalene
Concen: 0.020 ng/ul
RT: 10.350 min Scan# 11
Delta R.T. -0.011 min
Lab File: BN035184.D
Acq: 20 Nov 2024 05:04

Instrument :
BNA_N
ClientSampleId :
E2A22

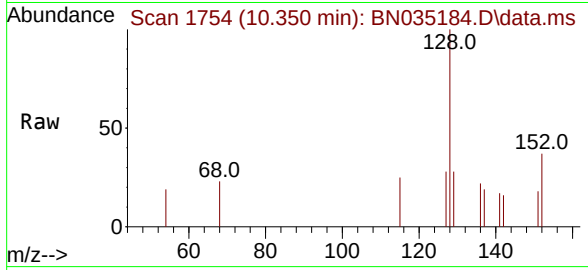

Tgt Ion:128 Resp: 432
Ion Ratio Lower Upper
128 100
129 27.6 9.9 14.9
127 28.3 11.4 17.2

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/20/2024
Supervised By :mohammad ahmed 11/22/2024

