


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112019\
Data File : BN008655.D
Acq On : 20 Nov 2019 11:44
Operator : JU
Sample : PB124751BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK51

Manual Integrations
APPROVED

mohammad
11/21/2019 1:05:50 PM

Quant Time: Nov 20 13:00:45 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 20 04:45:41 2019
Response via : Initial Calibration

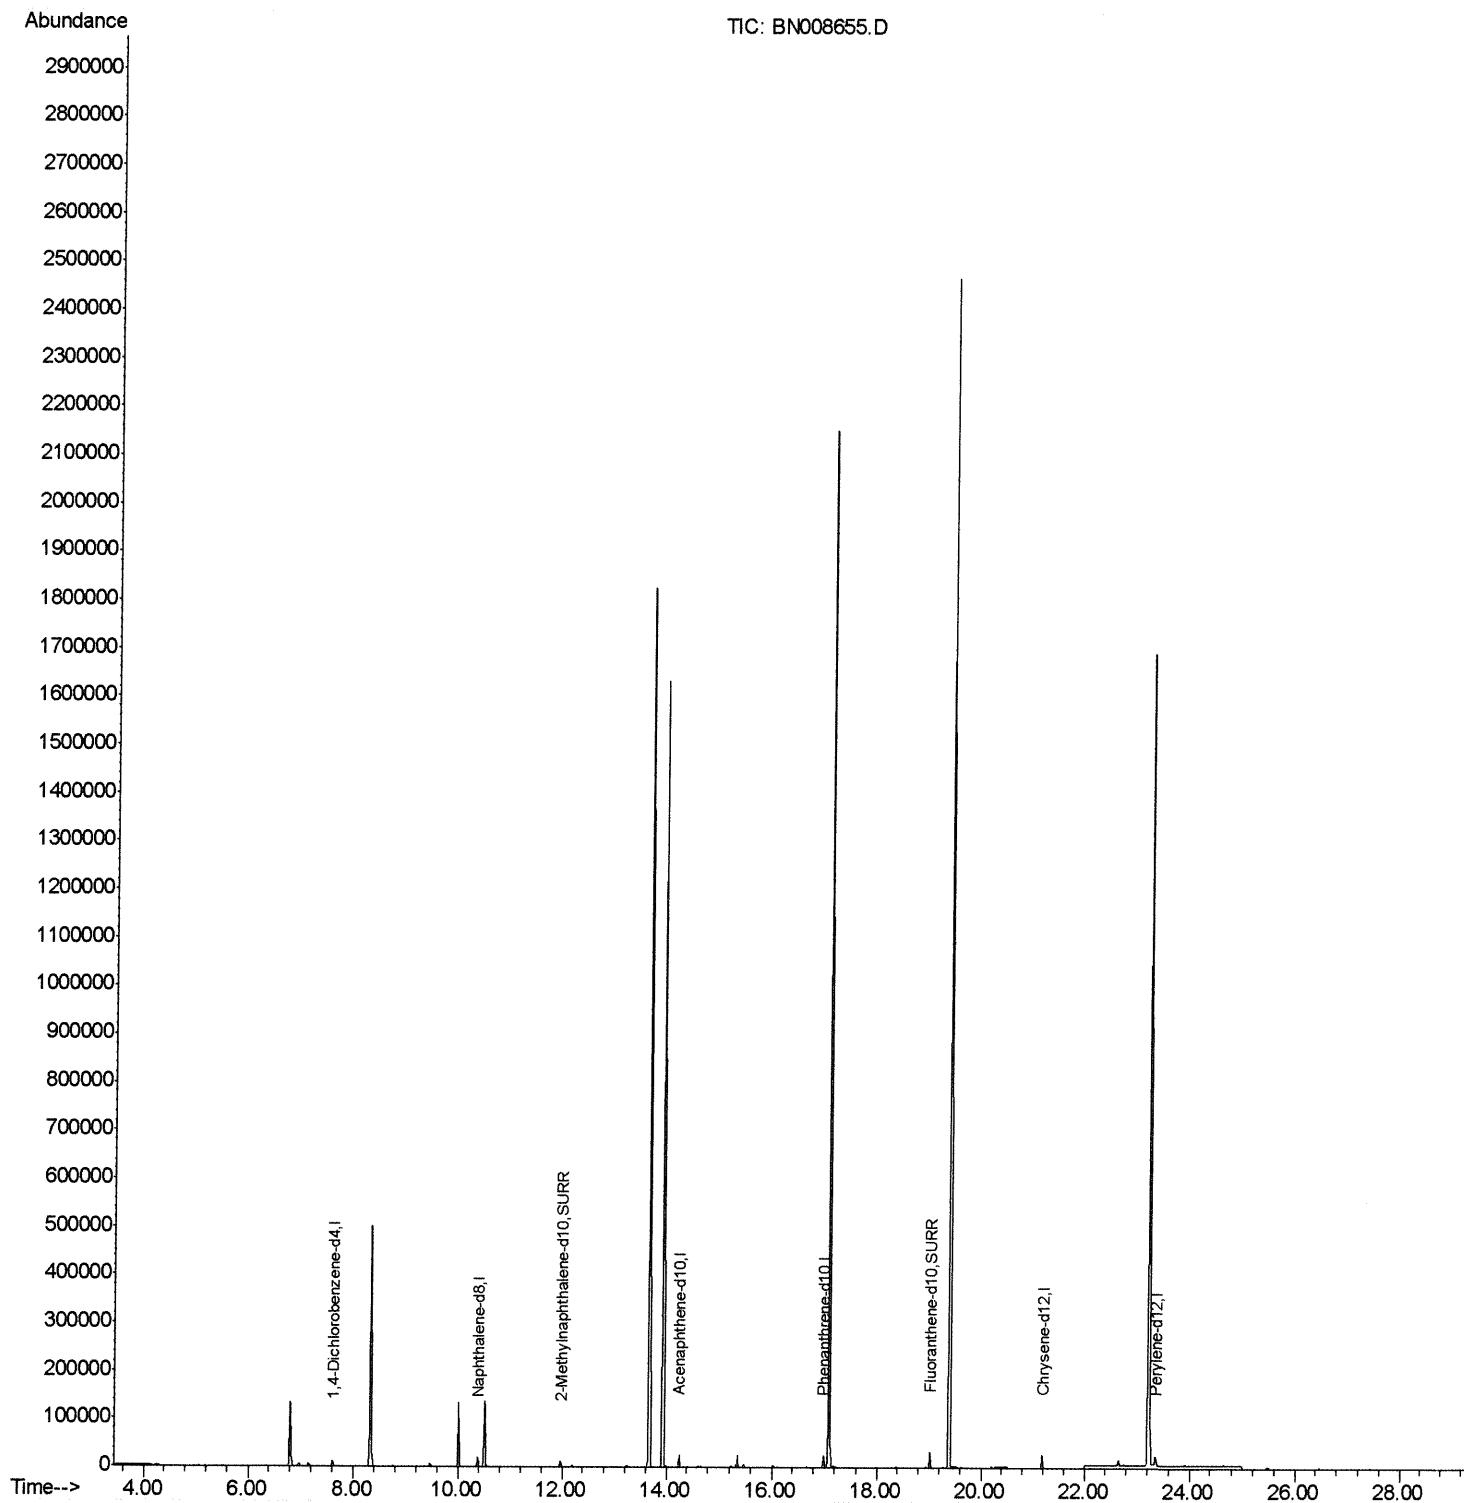


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112019\
Data File : BN008655.D
Acq On : 20 Nov 2019 11:44
Operator : JU
Sample : PB124751BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK51

Manual Integrations
APPROVED

mohammad
11/21/2019 1:05:50 PM

Quant Time: Nov 20 12:58:35 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 20 04:45:41 2019
Response via : Initial Calibration

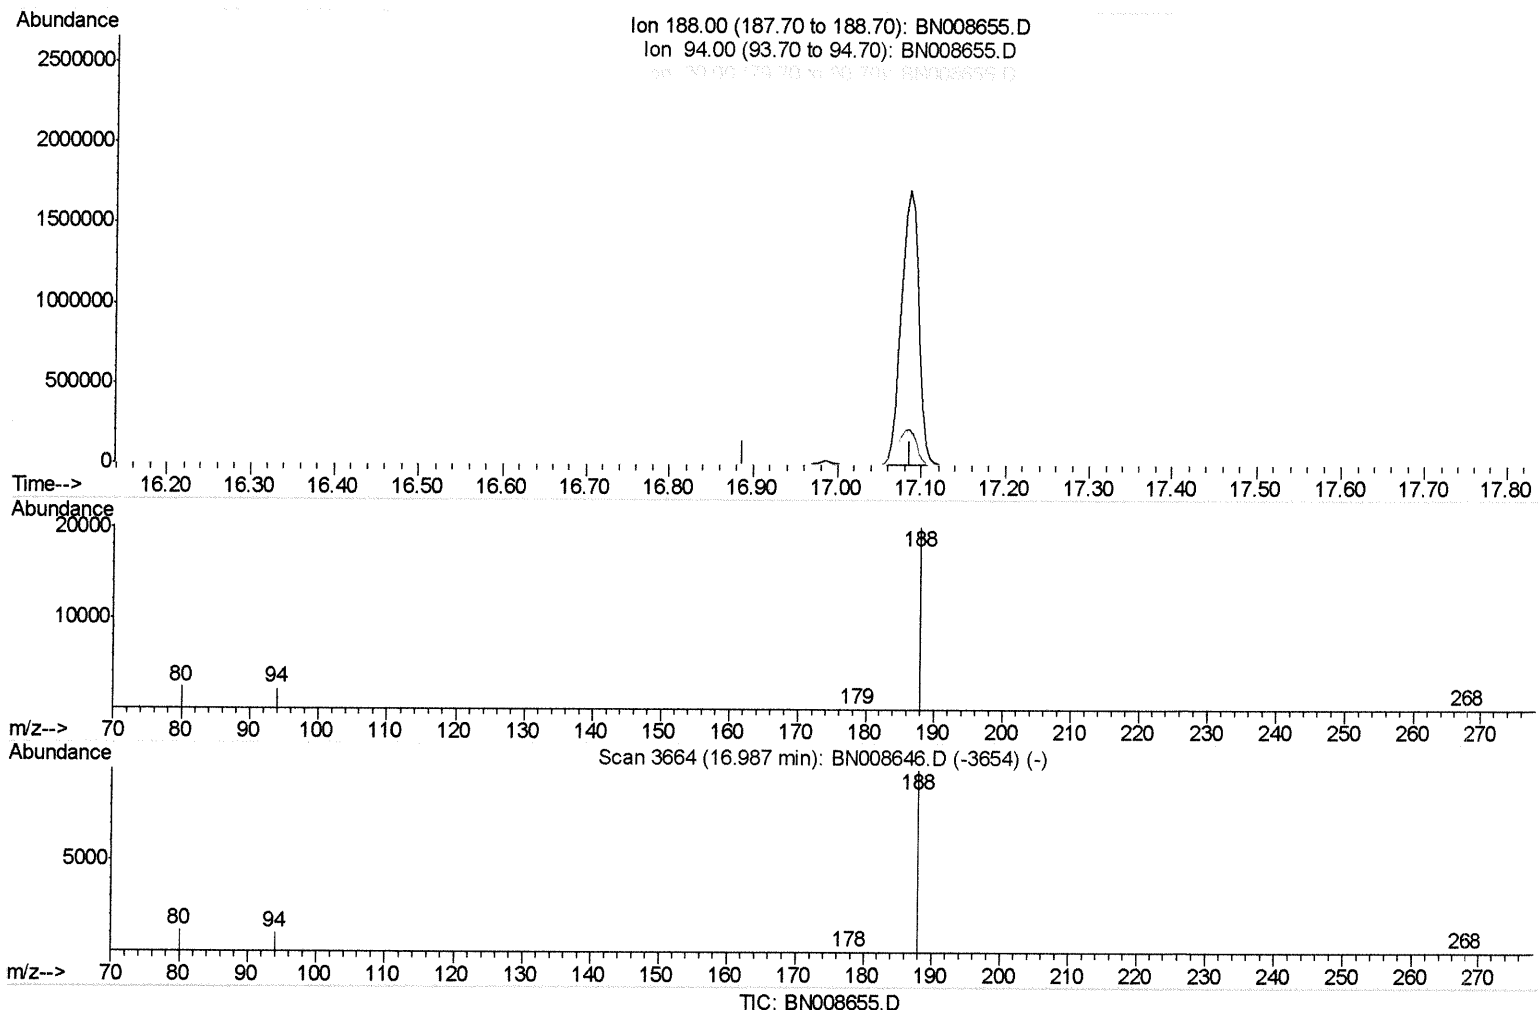

(10) Phenanthrene-d10 (I)

16.987min (-16.987) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	10.60	0.00#
80.00	11.80	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112019\
Data File : BN008655.D
Acq On : 20 Nov 2019 11:44
Operator : JU
Sample : PB124751BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK51

Manual Integrations
APPROVED

mohammad
11/21/2019 1:05:50 PM

Quant Time: Nov 20 12:58:35 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 20 04:45:41 2019
Response via : Initial Calibration

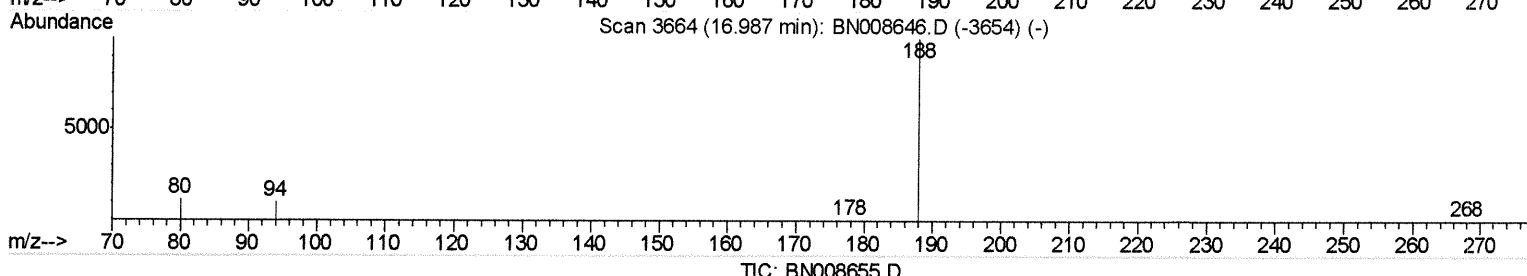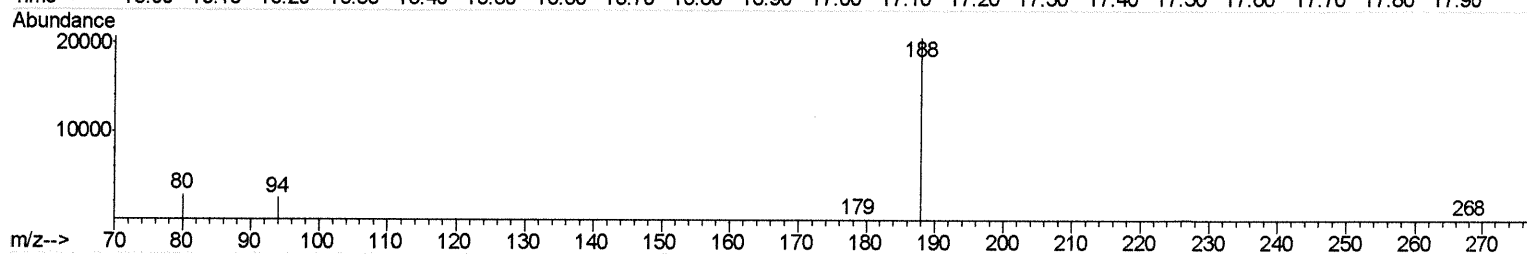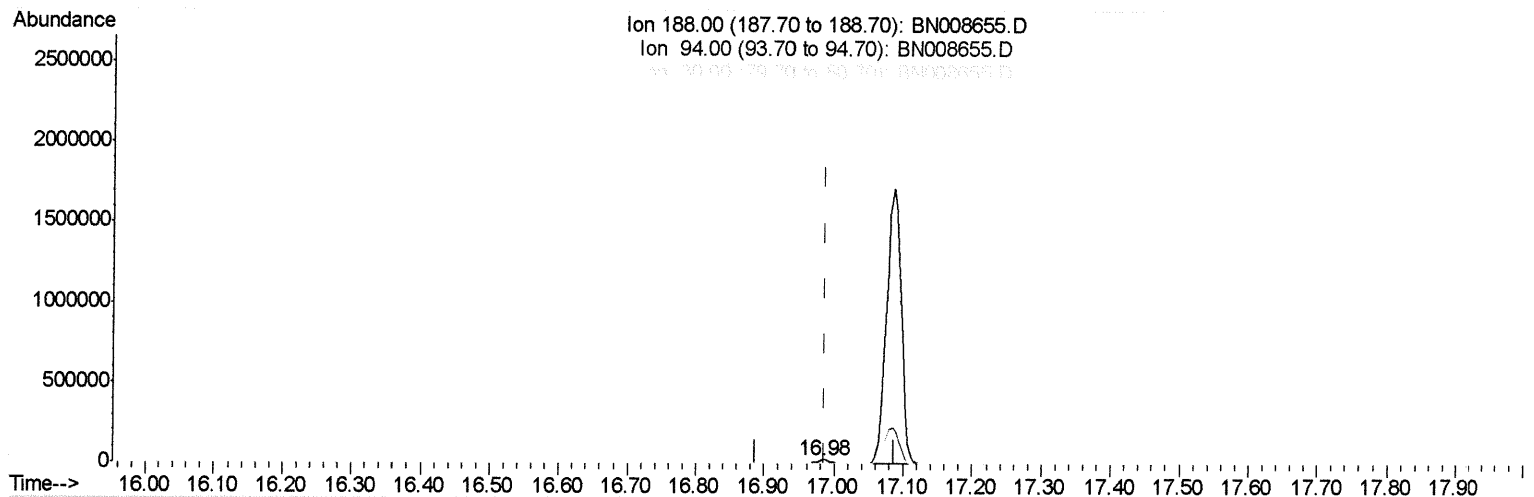

(10) Phenanthrene-d10 (I)

16.983min (-0.004) 0.40ng/ul m JU 11/23/19

response 28422

Ion	Exp%	Act%
188.00	100	100
94.00	10.60	11.63
80.00	11.80	13.37
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112019\
Data File : BN008655.D
Acq On : 20 Nov 2019 11:44
Operator : JU
Sample : PB124751BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK51

Manual Integrations
APPROVED

mohammad
11/21/2019 1:05:50 PM

Quant Time: Nov 20 13:00:45 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 20 04:45:41 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.61	152	6442	0.40	ng/ul	0.00
2) Naphthalene-d8	10.37	136	23935	0.40	ng/ul	-0.01
6) Acenaphthene-d10	14.24	164	13637	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.98	188	28422m >	0.40	ng/ul >	0.00
16) Chrysene-d12	21.18	240	23650	0.40	ng/ul	0.00
20) Perylene-d12	23.35	264	23939	0.40	ng/ul	0.00

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	11.97	152	15002	0.38	ng/ul	0.00
14) Fluoranthene-d10	19.02	212	34199	0.39	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed