


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN112019\
Data File : BN008663.D
Acq On : 20 Nov 2019 16:44
Operator : JU
Sample : PB124765BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK65

Manual Integrations
APPROVED

mohammad
11/21/2019 1:06:10 PM

Quant Time: Nov 21 00:46:44 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 20 04:45:41 2019
Response via : Initial Calibration

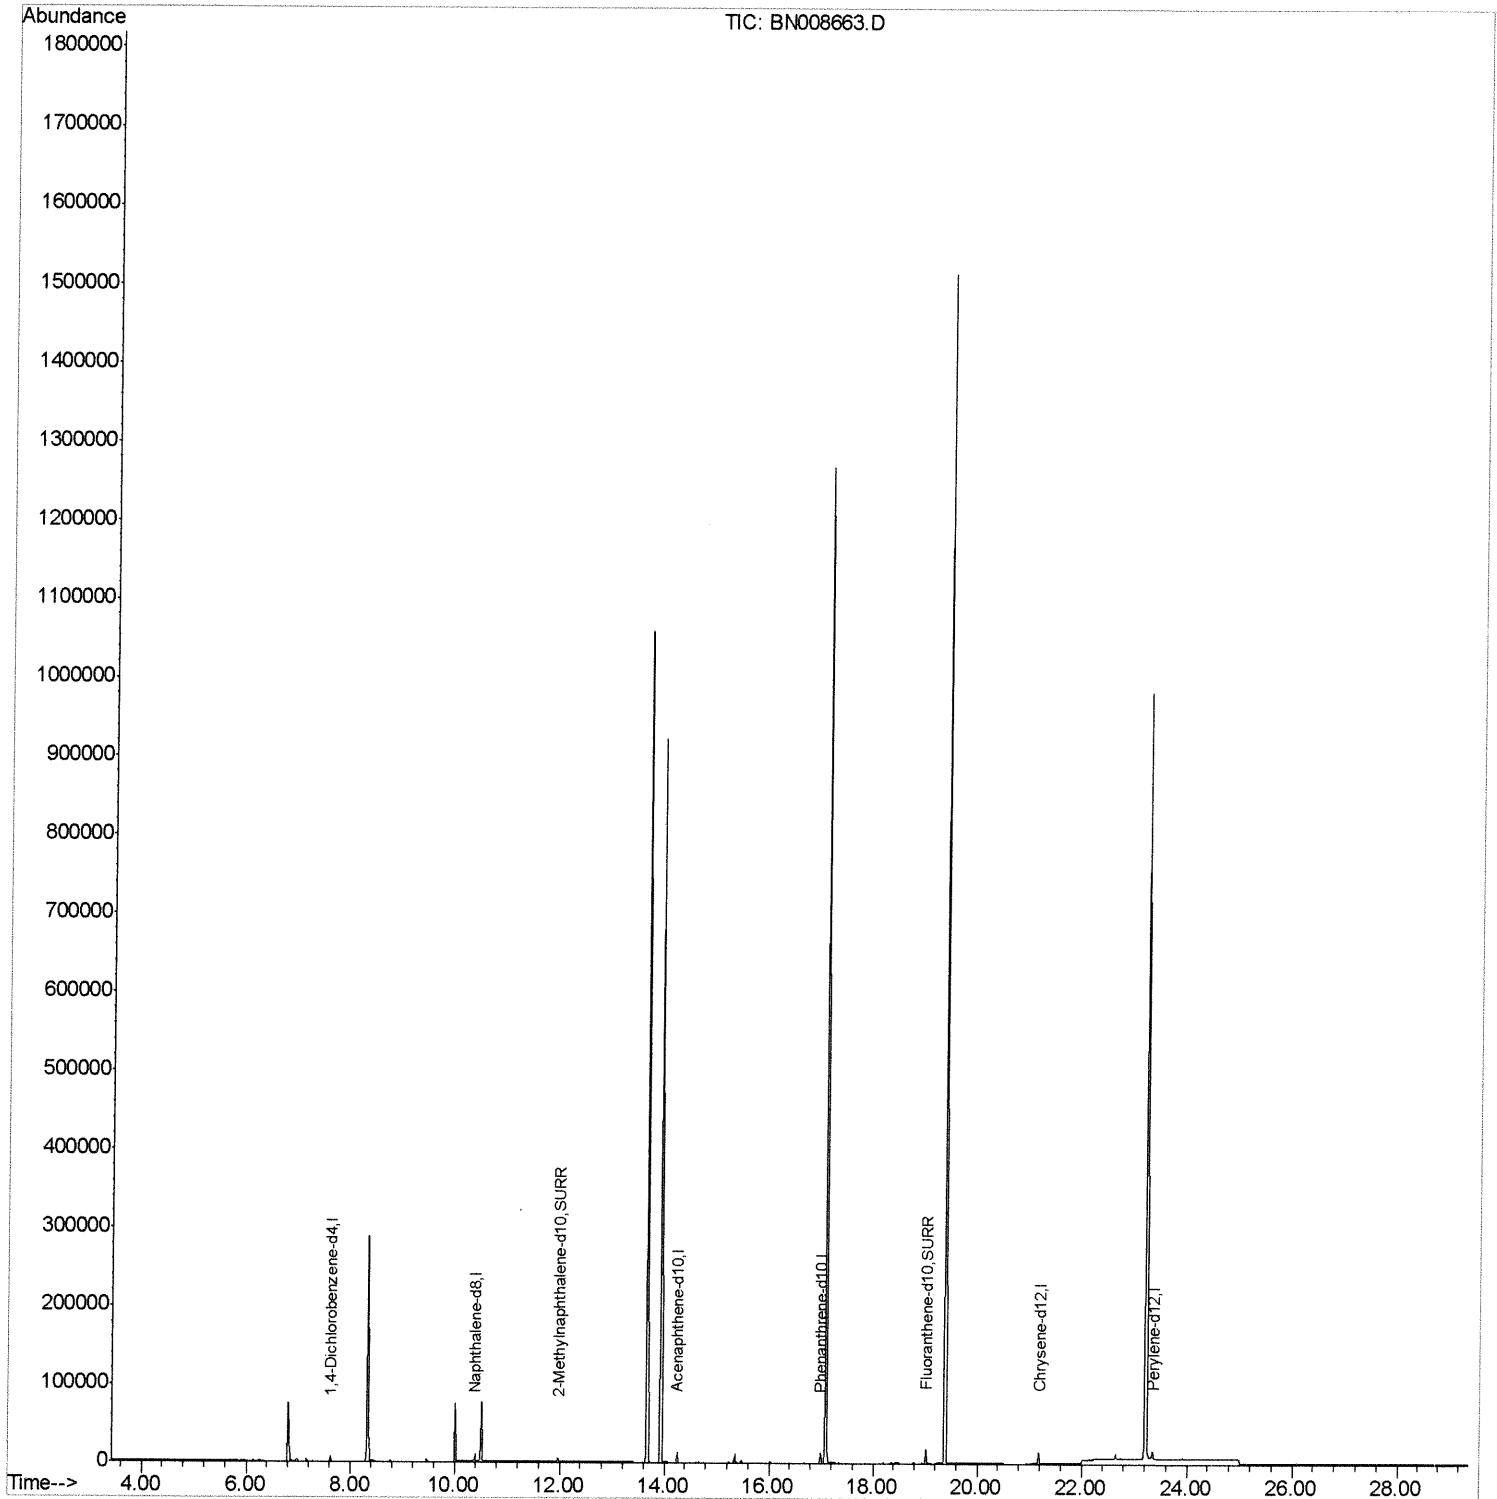




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN112019\
Data File : BN008663.D
Acq On : 20 Nov 2019 16:44
Operator : JU
Sample : PB124765BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK65

Manual Integrations
APPROVED

mohammad
11/21/2019 1:06:10 PM

Quant Time: Nov 21 00:42:54 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 20 04:45:41 2019
Response via : Initial Calibration

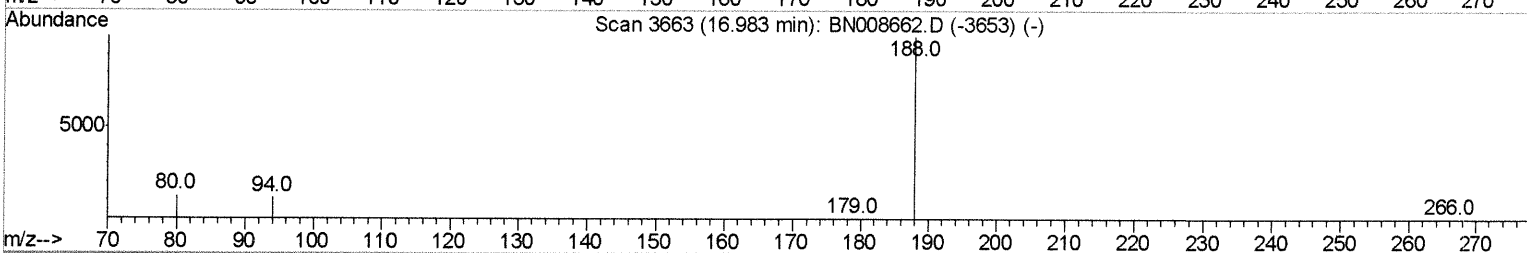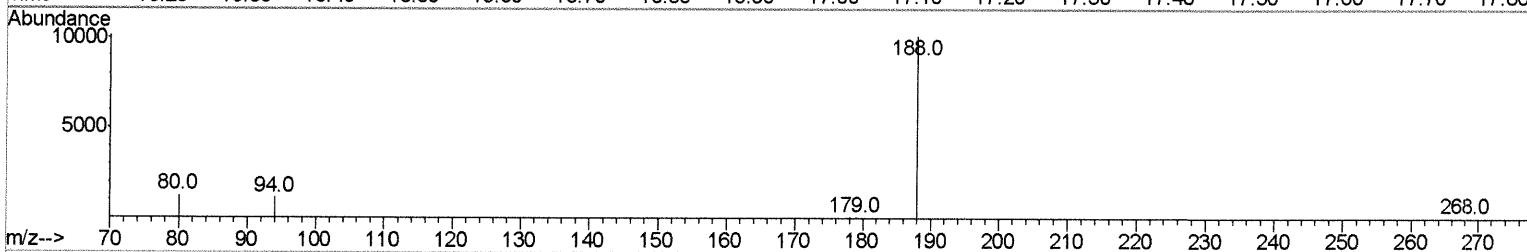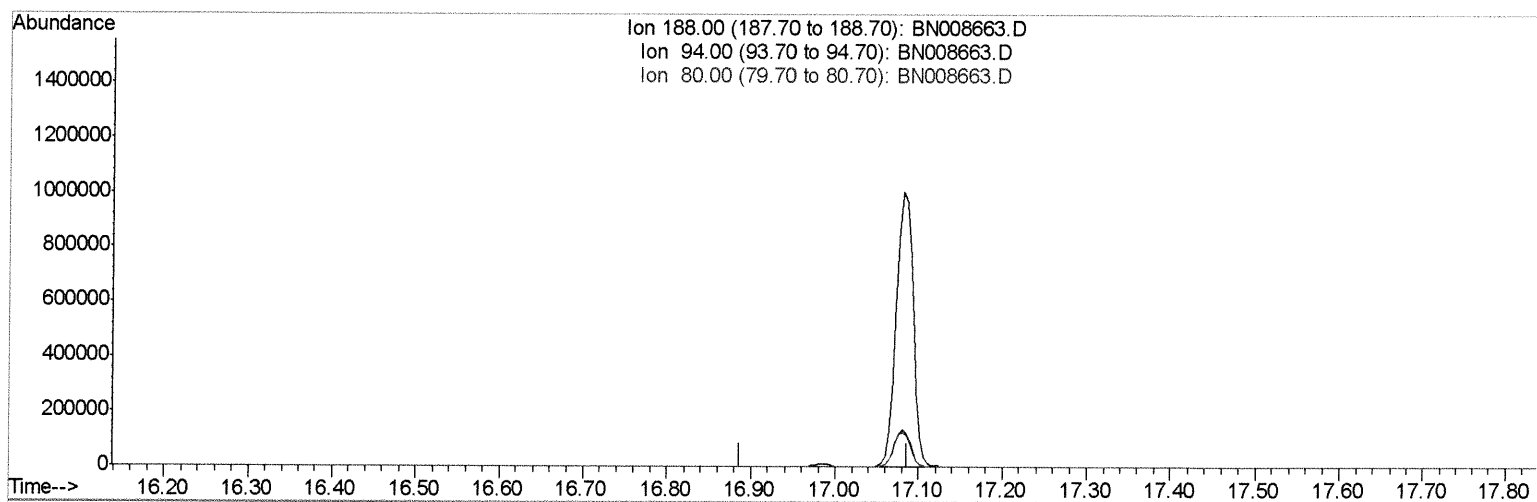

TIC: BN008663.D

(10) Phenanthrene-d10 (l)

16.987min (-16.987) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	10.60	0.00#
80.00	11.80	0.00#
0.00	0.00	0.00


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN112019\
Data File : BN008663.D
Acq On : 20 Nov 2019 16:44
Operator : JU
Sample : PB124765BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK65

Manual Integrations
APPROVED

mohammad
11/21/2019 1:06:10 PM

Quant Time: Nov 21 00:42:54 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 20 04:45:41 2019
Response via : Initial Calibration

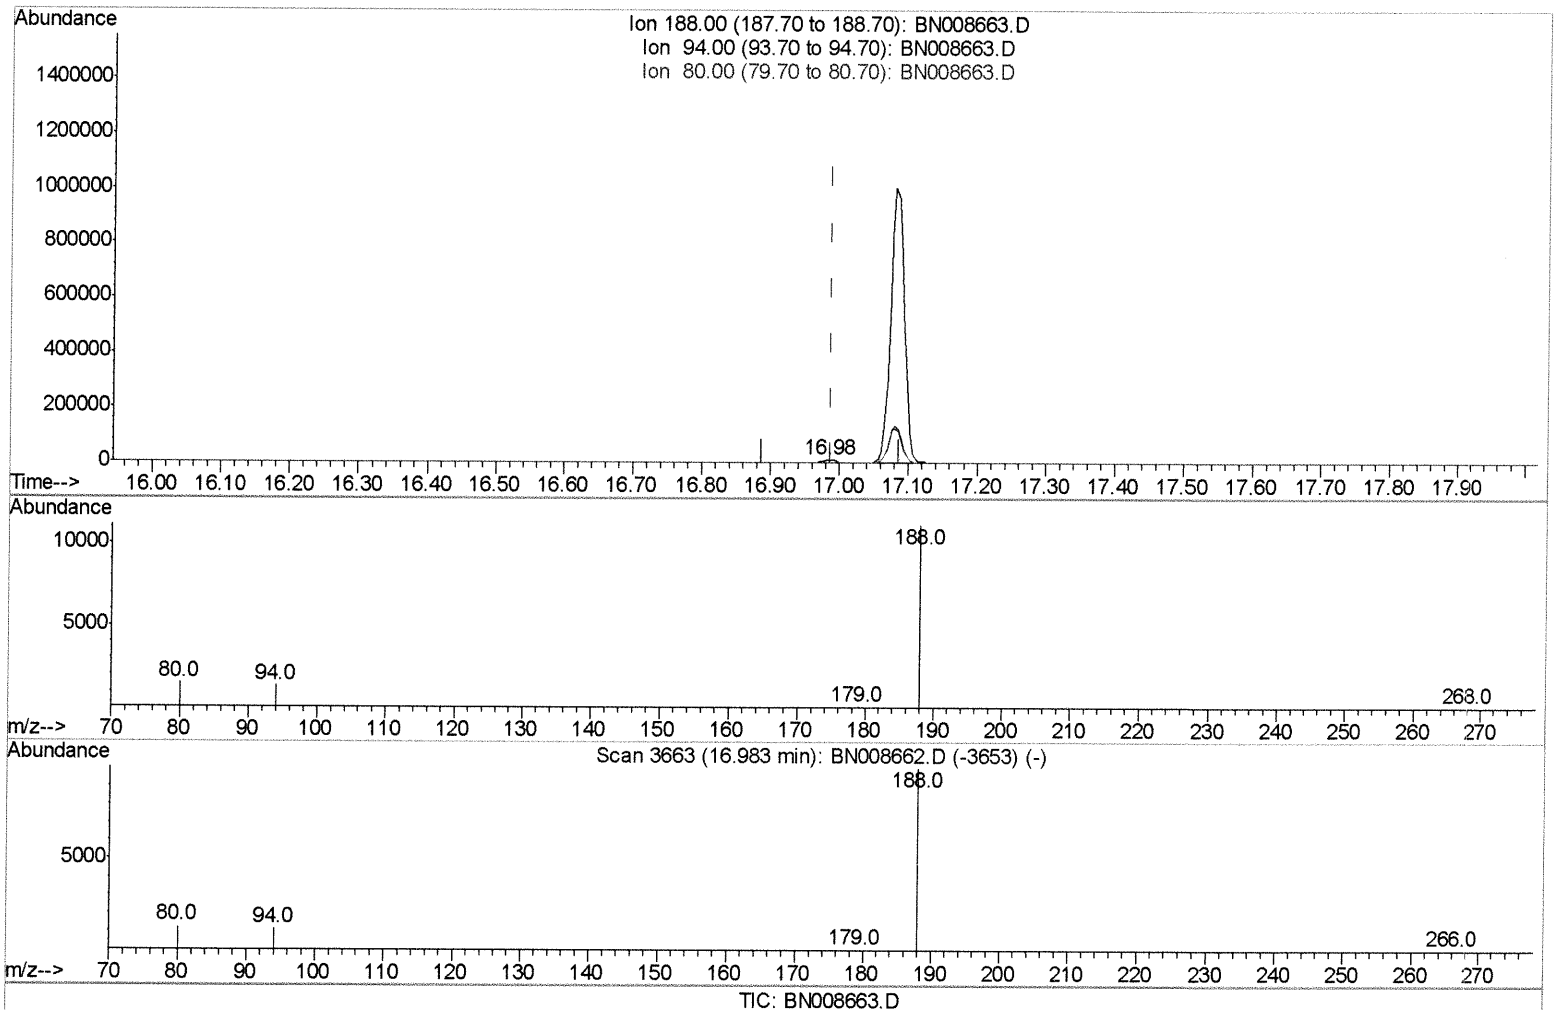

(10) Phenanthrene-d10 (l)

16.983min (-0.004) 0.40ng/ul m JU 11/25/19

response 14935

Ion	Exp%	Act%
188.00	100	100
94.00	10.60	11.76
80.00	11.80	13.32
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN112019\
 Data File : BN008663.D
 Acq On : 20 Nov 2019 16:44
 Operator : JU
 Sample : PB124765BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK65

Manual Integrations
 APPROVED

mohammad
 11/21/2019 1:06:10 PM

Quant Time: Nov 21 00:46:44 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111519.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 20 04:45:41 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.62	152	3538	0.40	ng/ul	0.00
2) Naphthalene-d8	10.38	136	13097	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.24	164	7289	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.98	188	14935m >	0.40	ng/ul >	0.00
16) Chrysene-d12	21.18	240	12605	0.40	ng/ul	0.00
20) Perylene-d12	23.35	264	12797	0.40	ng/ul	0.00

ju 11/25/19

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	11.97	152	8080	0.38	ng/ul	0.00
14) Fluoranthene-d10	19.01	212	18076	0.40	ng/ul	0.00

Target Compounds	Ovalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed