


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN112019\
Data File : BN008673.D
Acq On : 20 Nov 2019 22:44
Operator : JU
Sample : K5851-12
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AB0

Manual Integrations
APPROVED

mohammad
11/21/2019 1:06:36 PM

Quant Time: Nov 21 01:24:37 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 20 04:45:41 2019
Response via : Initial Calibration

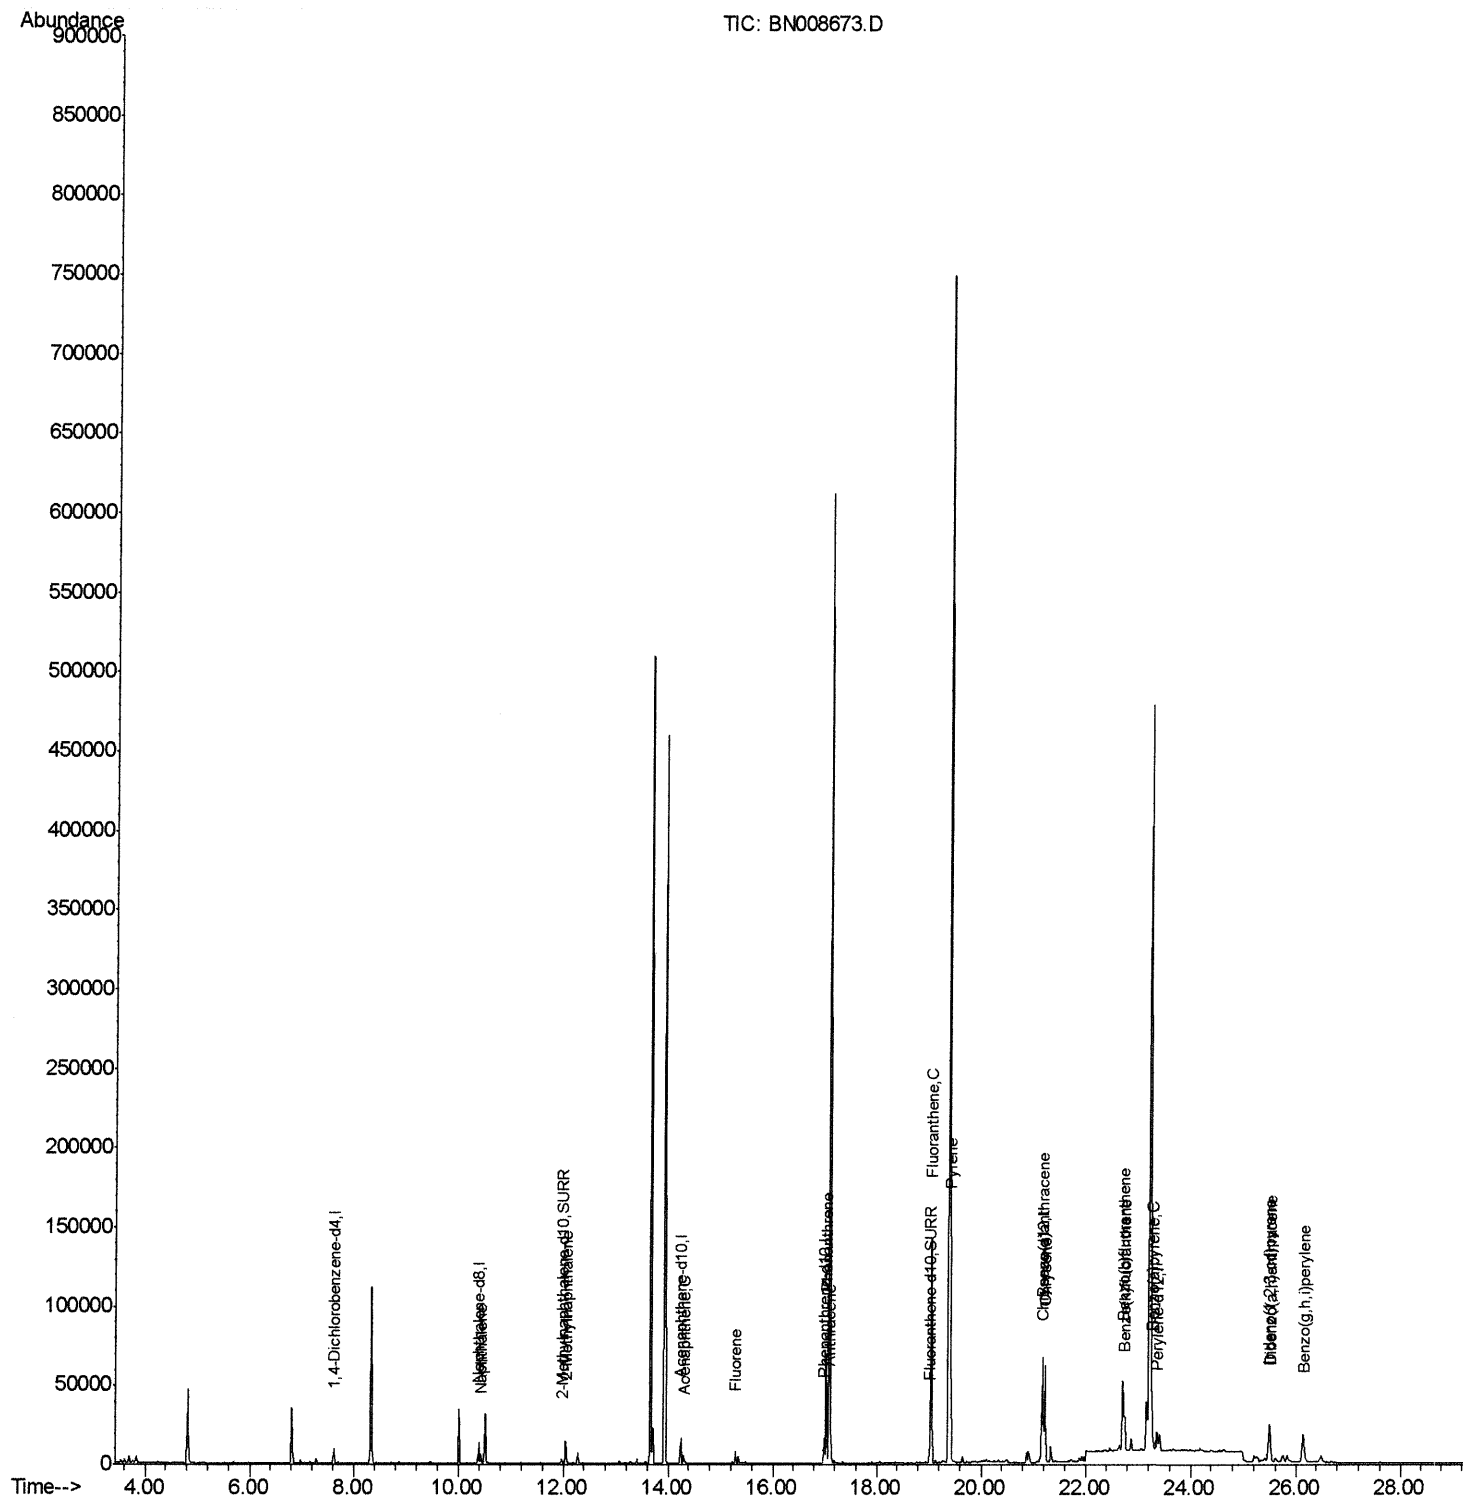




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN112019\
Data File : BN008673.D
Acq On : 20 Nov 2019 22:44
Operator : JU
Sample : K5851-12
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AB0

Manual Integrations
APPROVED

mohammad
11/21/2019 1:06:36 PM

Quant Time: Nov 21 00:43:40 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 20 04:45:41 2019
Response via : Initial Calibration

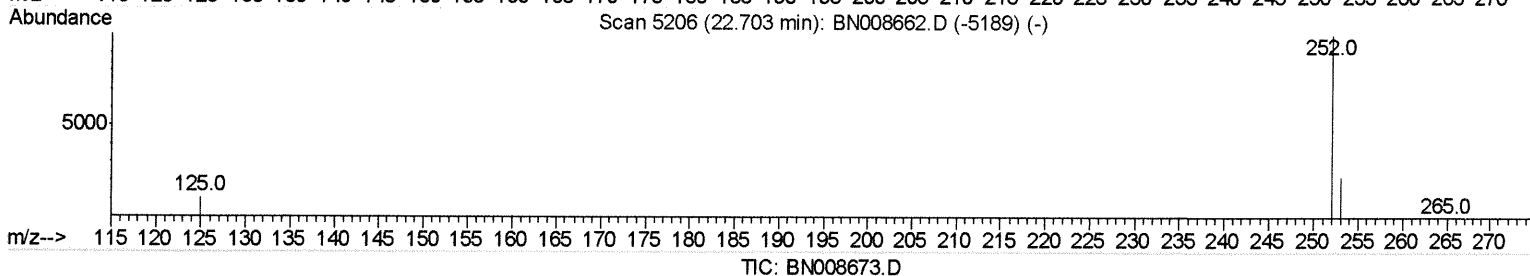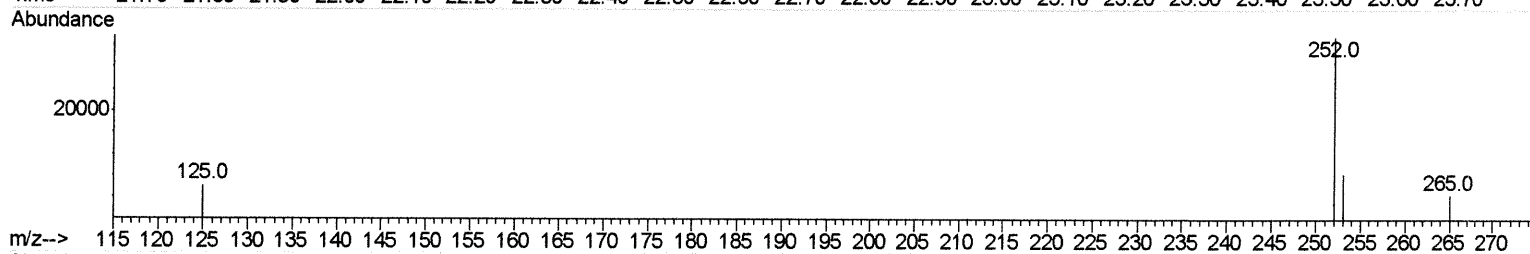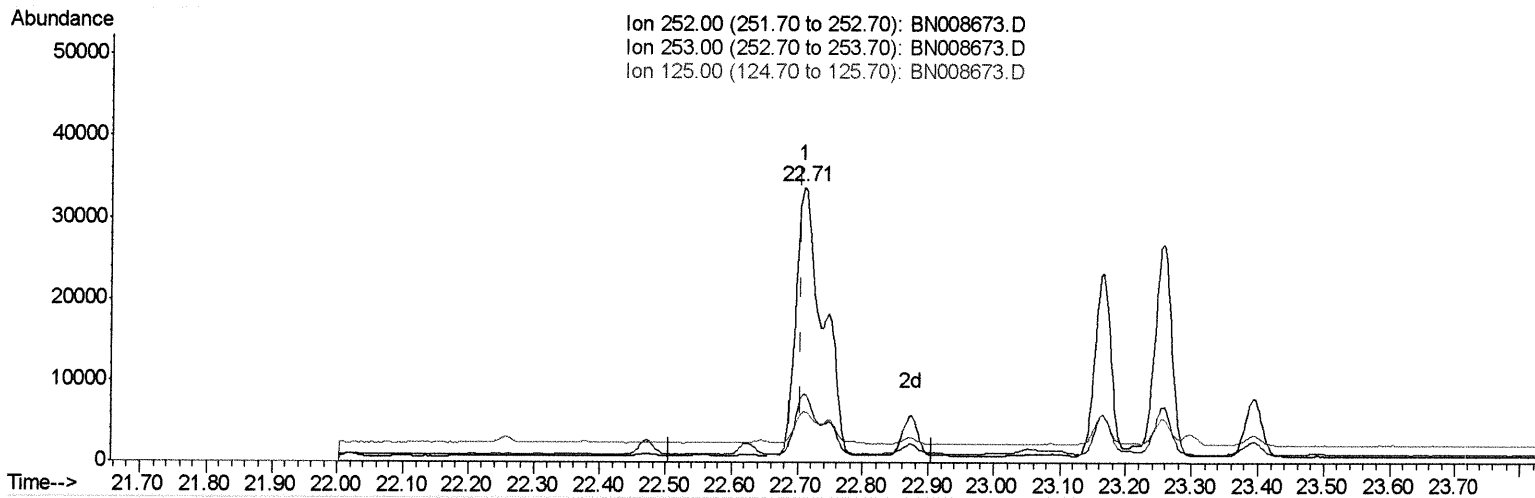

(21) Benzo(b)fluoranthene

22.709min (+0.003) 1.60ng/ul

response 94388

Ion	Exp%	Act%
252.00	100	100
253.00	25.10	24.88
125.00	15.00	18.61
0.00	0.00	0.00




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN112019\
Data File : BN008673.D
Acq On : 20 Nov 2019 22:44
Operator : JU
Sample : K5851-12
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AB0

Manual Integrations
APPROVED

mohammad
11/21/2019 1:06:36 PM

Quant Time: Nov 21 00:43:40 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 20 04:45:41 2019
Response via : Initial Calibration

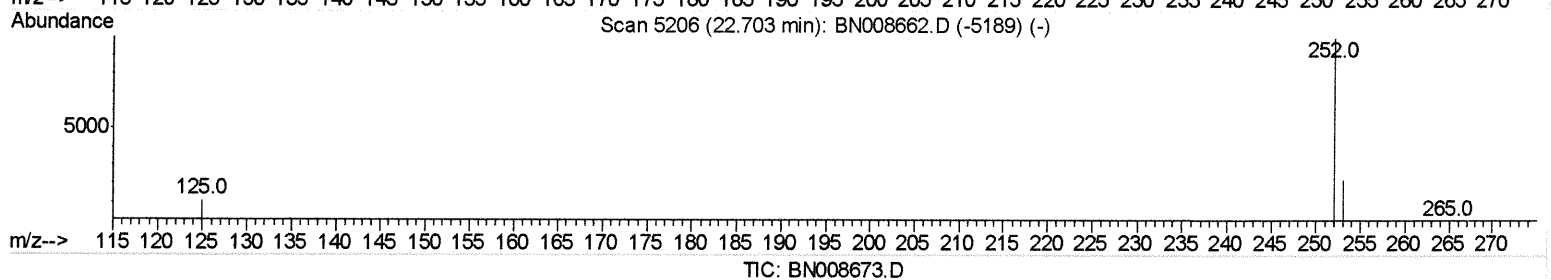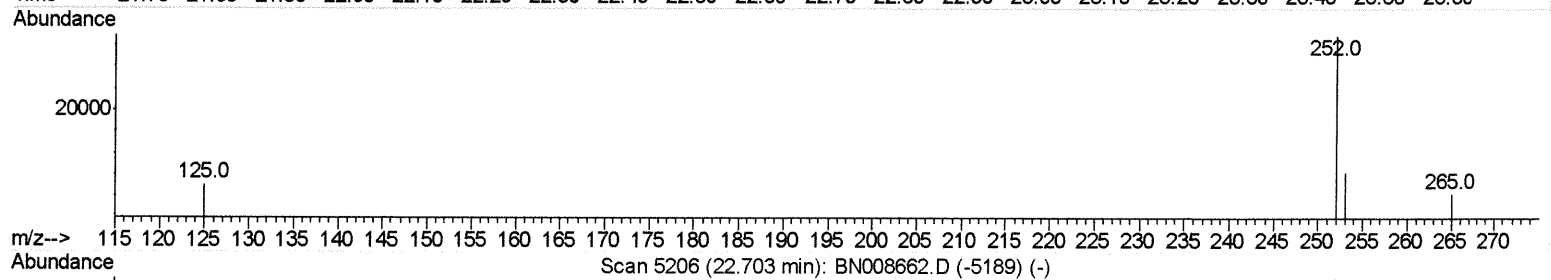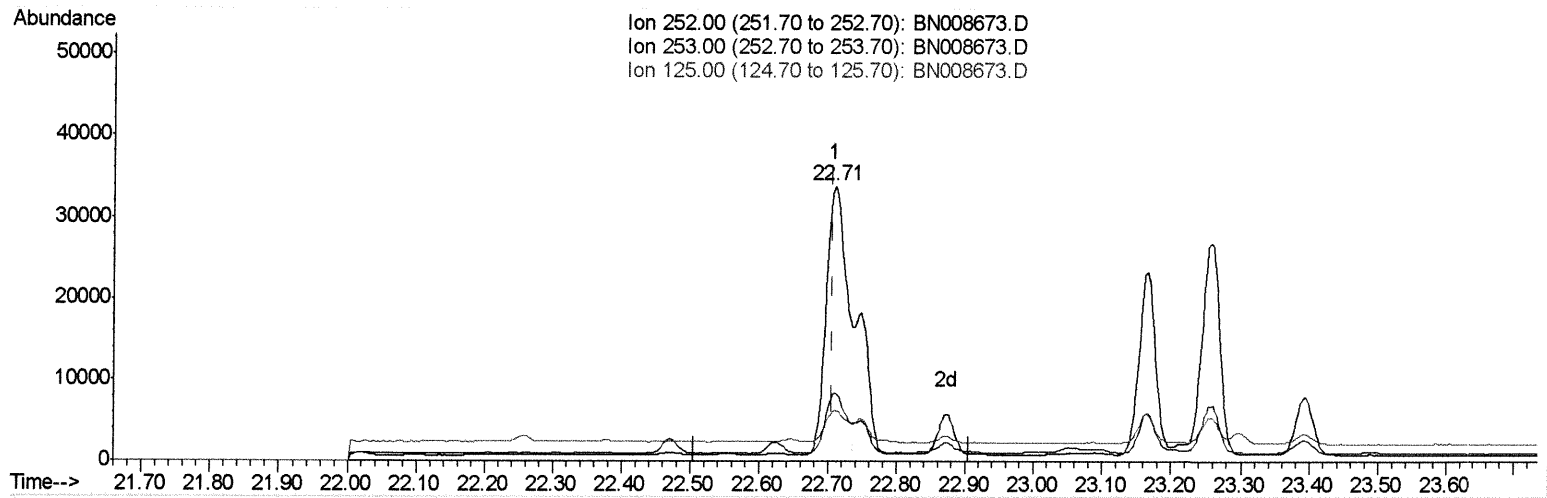

(21) Benzo(b)fluoranthene

22.709min (+0.003) 1.18ng/ul m JU 11/25/19

response 69290

Ion	Exp%	Act%
252.00	100	100
253.00	25.10	24.88
125.00	15.00	18.61
0.00	0.00	0.00




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN112019\
Data File : BN008673.D
Acq On : 20 Nov 2019 22:44
Operator : JU
Sample : K5851-12
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AB0

Manual Integrations
APPROVED

mohammad
11/21/2019 1:06:36 PM

Quant Time: Nov 21 00:43:40 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 20 04:45:41 2019
Response via : Initial Calibration

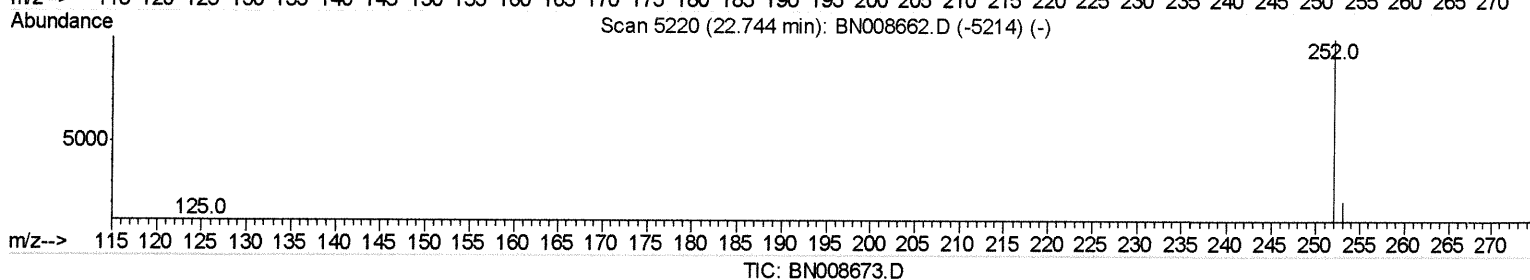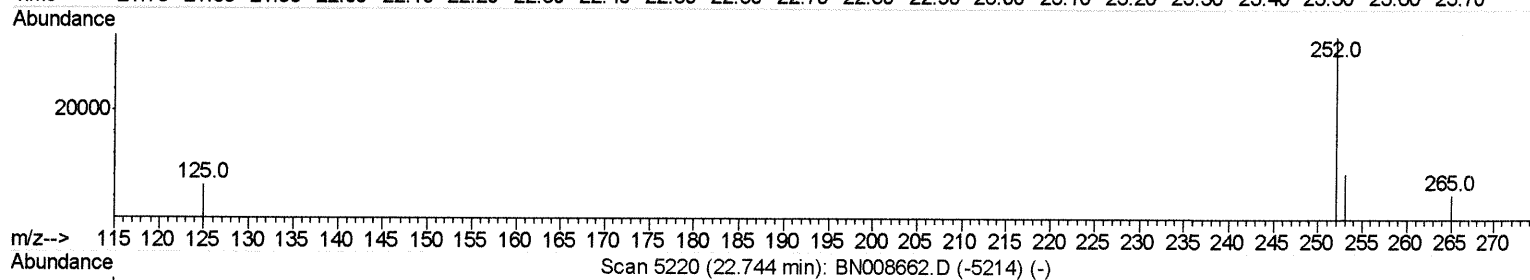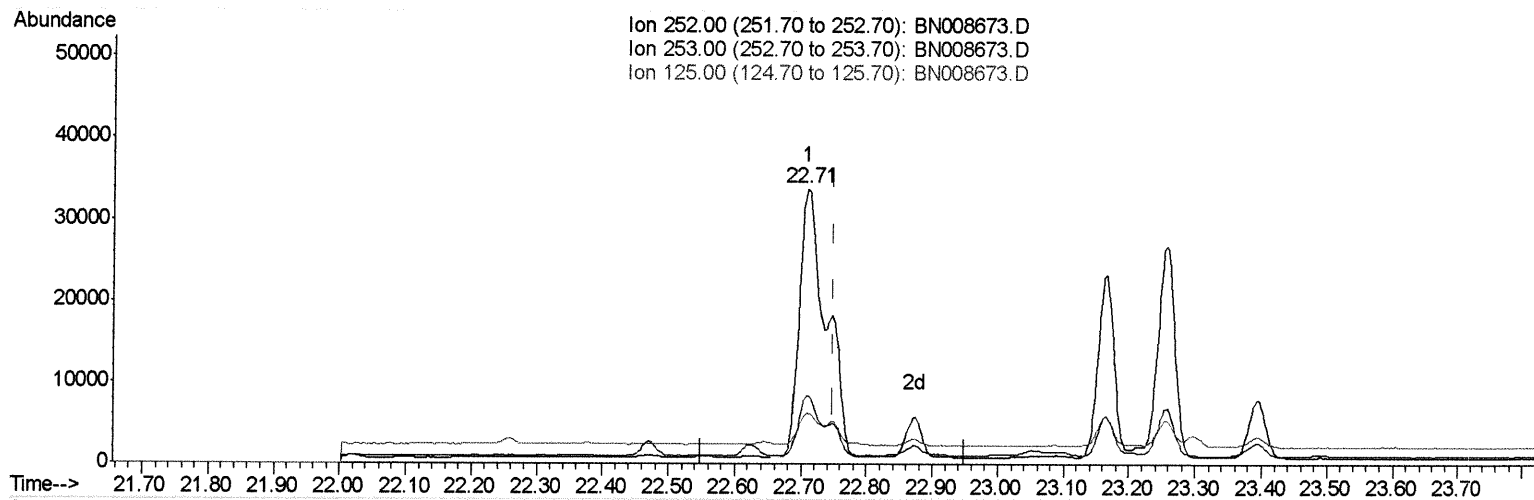

(22) Benzo(k)fluoranthene

22.709min (-0.041) 1.62ng/ui

response 94388

Ion	Exp%	Act%
252.00	100	100
253.00	25.60	24.88
125.00	18.70	18.61
0.00	0.00	0.00



Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN112019\
Data File : BN008673.D
Acq On : 20 Nov 2019 22:44
Operator : JU
Sample : K5851-12
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AB0


Manual Integrations
APPROVED

mohammad
11/21/2019 1:06:36 PM

Quant Time: Nov 21 00:43:40 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 20 04:45:41 2019
Response via : Initial Calibration

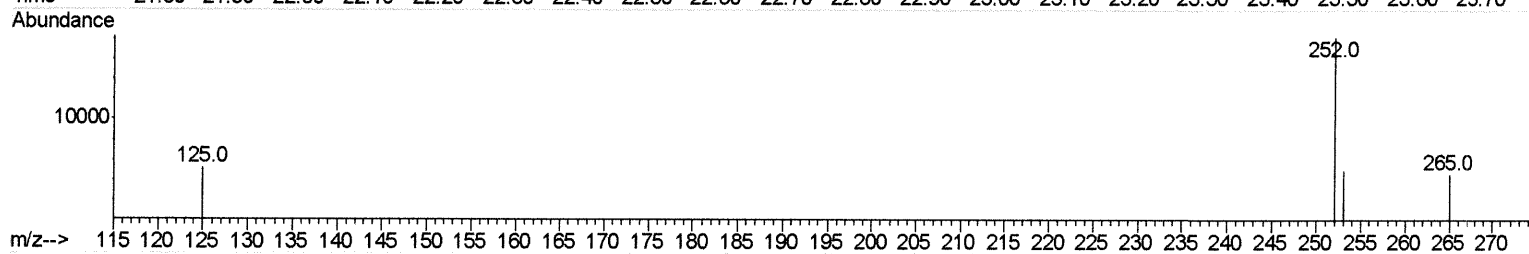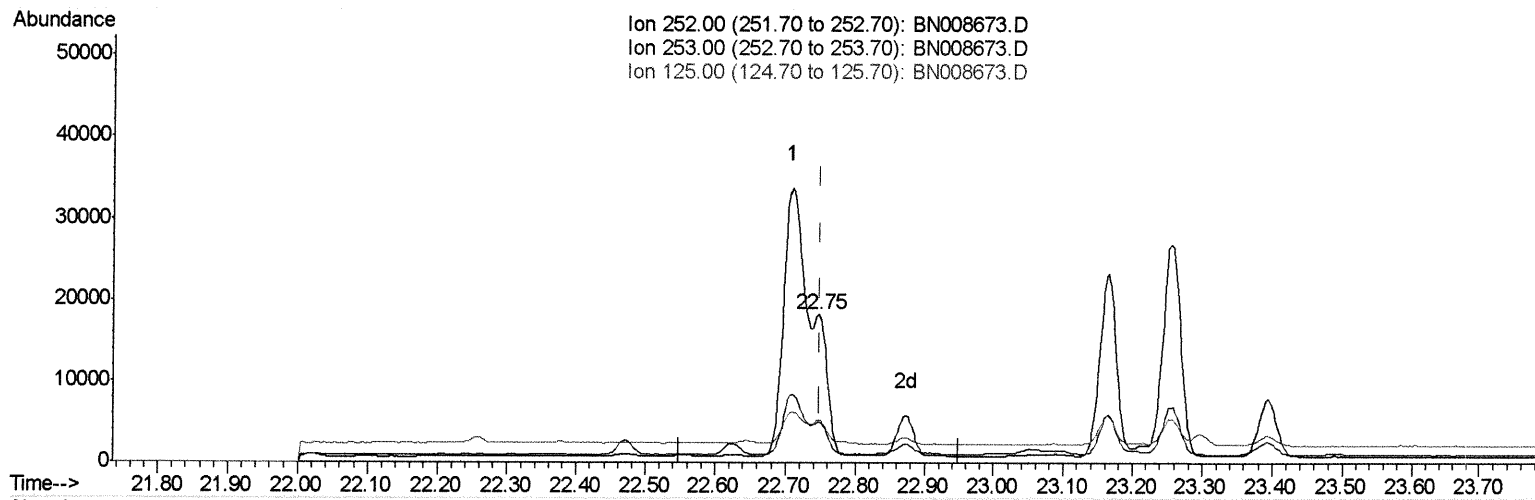

Scan 5220 (22.744 min): BN008662.D (-5214) (-)

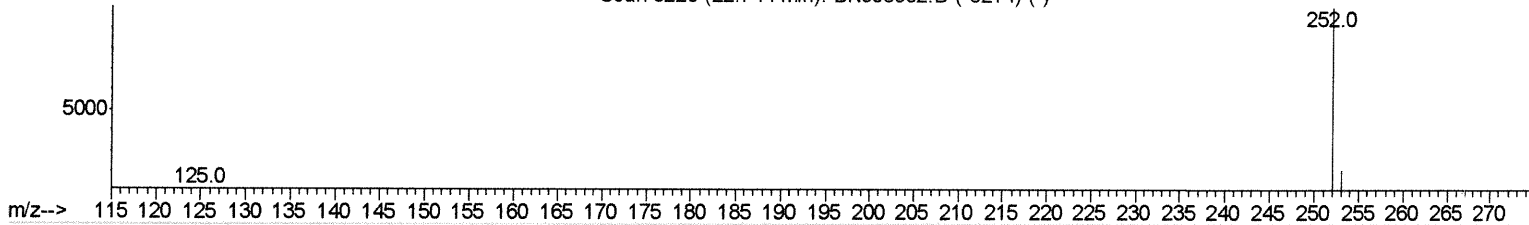

TIC: BN008673.D

(22) Benzo(k)fluoranthene

22.747min (-0.003) 0.43ng/ul m JU 11/25/19

response 24945

Ion	Exp%	Act%
252.00	100	100
253.00	25.60	27.64
125.00	18.70	28.68#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN112019\
 Data File : BN008673.D
 Acq On : 20 Nov 2019 22:44
 Operator : JU
 Sample : K5851-12
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AB0

Manual Integrations
 APPROVED

mohammad
 11/21/2019 1:06:36 PM

Quant Time: Nov 21 01:24:37 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111519.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 20 04:45:41 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.62	152	4166	0.40	ng/ul	0.00
2) Naphthalene-d8	10.38	136	15703	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.24	164	8725	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.98	188	17710	0.40	ng/ul	0.00
16) Chrysene-d12	21.18	240	14371	0.40	ng/ul	0.00
20) Perylene-d12	23.35	264	14281	0.40	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	11.97	152	3910	0.15	ng/ul	0.00
14) Fluoranthene-d10	19.01	212	8895	0.16	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
3) Naphthalene	10.42	128	7942	0.168	ng/ul	99
5) 2-Methylnaphthalene	12.04	142	10106	0.306	ng/ul	100
8) Acenaphthene	14.30	153	3294	0.092	ng/ul	97
9) Fluorene	15.29	166	4482	0.107	ng/ul#	98
12) Phenanthrene	17.02	178	73000	1.222	ng/ul	98
13) Anthracene	17.11	178	14328	0.254	ng/ul	99
15) Fluoranthene	19.04	202	120151	1.637	ng/ul	93
17) Pyrene	19.41	202	106070	1.840	ng/ul	99
18) Benzo(a)anthracene	21.16	228	53653	0.928	ng/ul	98
19) Chrysene	21.22	228	58210	1.025	ng/ul	97
21) Benzo(b)fluoranthene	22.71	252	69290m	1.177	ng/ul	> JU 11/25/19
22) Benzo(k)fluoranthene	22.75	252	24945m	0.427	ng/ul	
23) Benzo(a)pyrene	23.26	252	47296	0.856	ng/ul	96
24) Indeno(1,2,3-cd)pyrene	25.49	276	34068	0.527	ng/ul#	97
25) Dibenzo(a,h)anthracene	25.50	278	8217	0.157	ng/ul#	72
26) Benzo(a,h,i)perylene	26.14	276	34675	0.641	ng/ul	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed