


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN112020\
Data File : BN012663.D
Acq On : 20 Nov 2020 17:39
Operator : CG/JU
Sample : PB133127BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK27

Manual Integrations
APPROVED

mohammad
11/24/2020 8:55:57 AM

Quant Time: Nov 20 18:15:53 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN112020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 20 18:13:27 2020
Response via : Initial Calibration

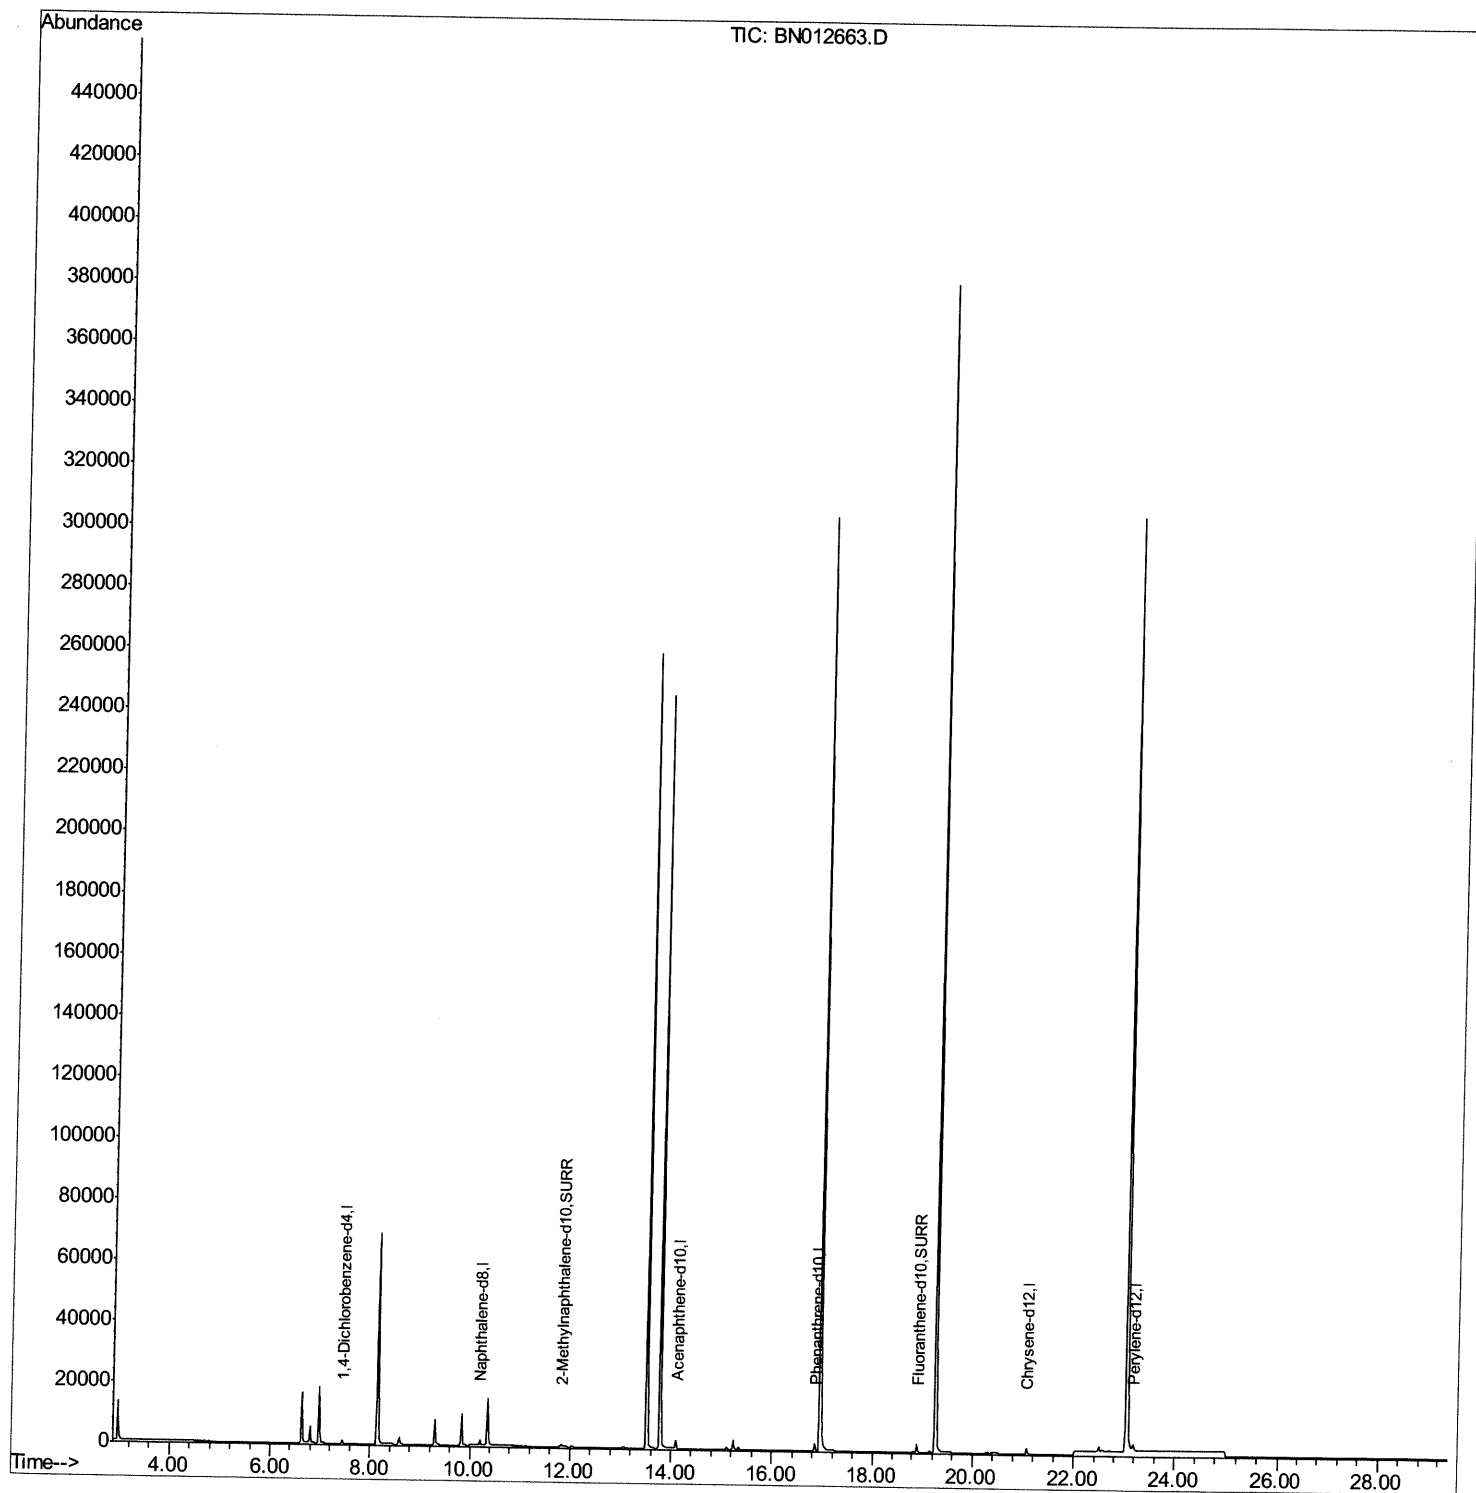

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN112020\
Data File : BN012663.D
Acq On : 20 Nov 2020 17:39
Operator : CG/JU
Sample : PB133127BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK27

Manual Integrations
APPROVED

mohammad
11/24/2020 8:55:57 AM

Quant Time: Nov 20 18:08:10 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN112020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 20 15:24:34 2020
Response via : Initial Calibration

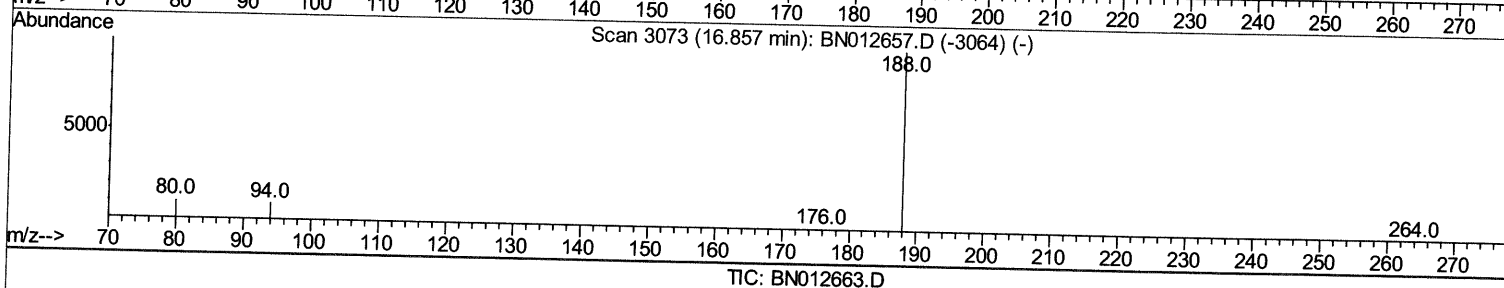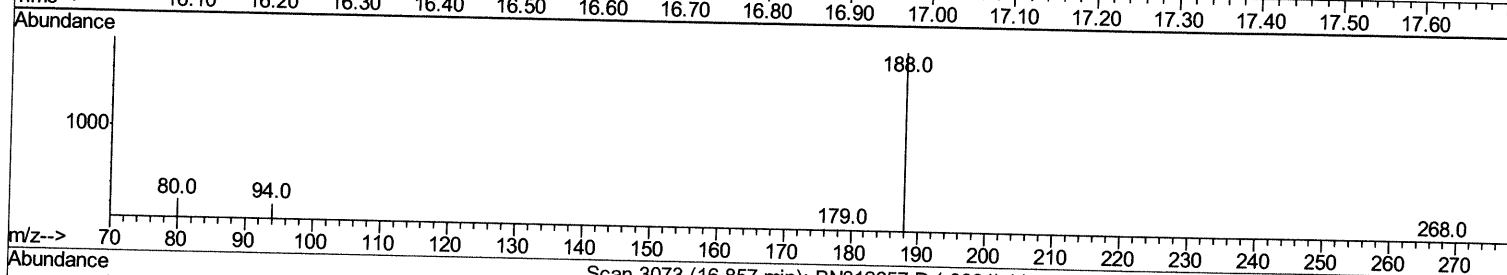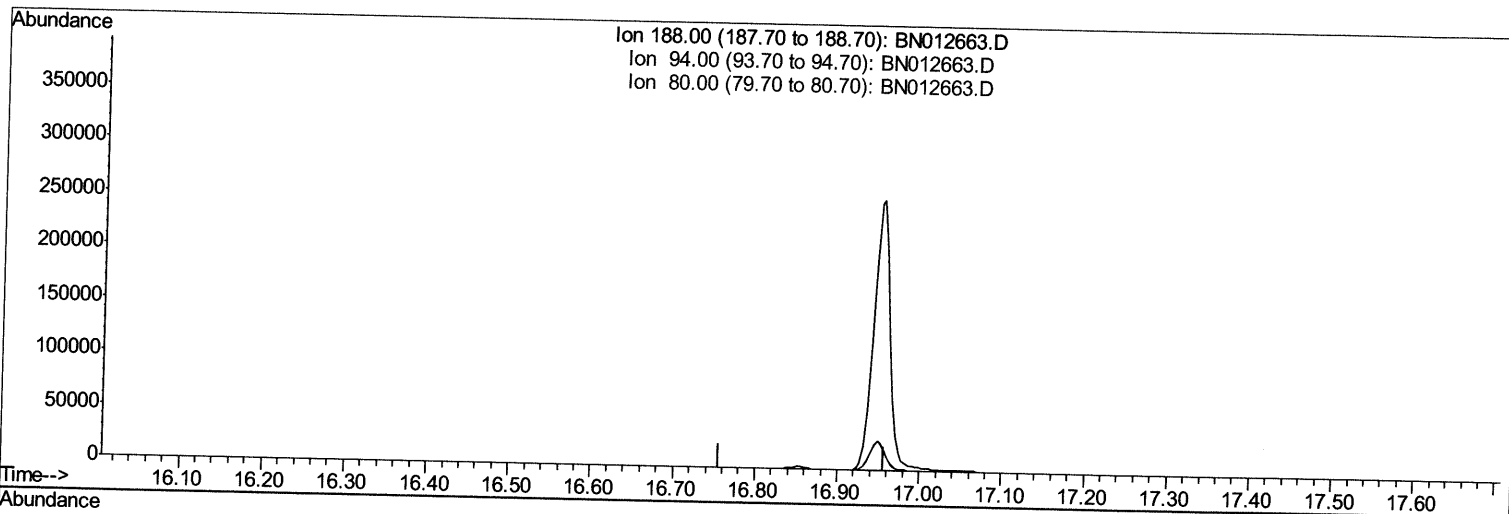

(10) Phenanthrene-d10 (I)

16.857min (-16.857) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	11.60	0.00#
80.00	12.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN112020\
 Data File : BN012663.D
 Acq On : 20 Nov 2020 17:39
 Operator : CG/JU
 Sample : PB133127BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
ClientSampleId :
 SBLK27

Manual Integrations
APPROVED

mohammad
 11/24/2020 8:55:57 AM

Quant Time: Nov 20 18:14:57 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN112020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 20 18:13:27 2020
 Response via : Initial Calibration

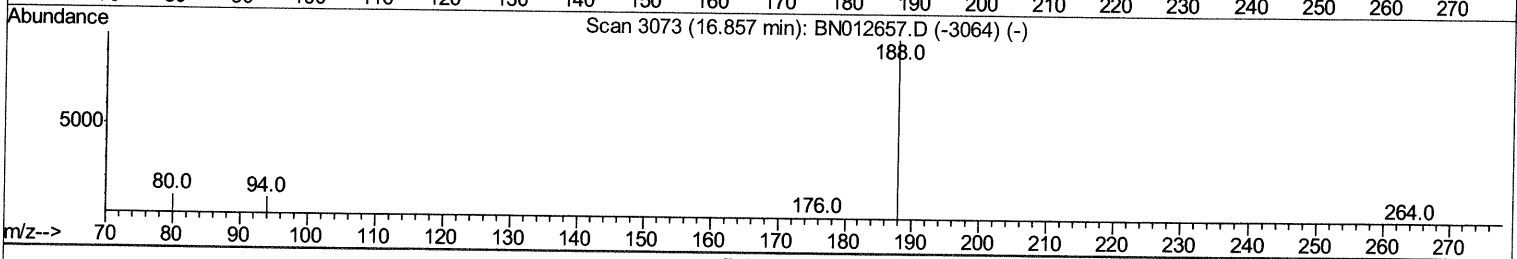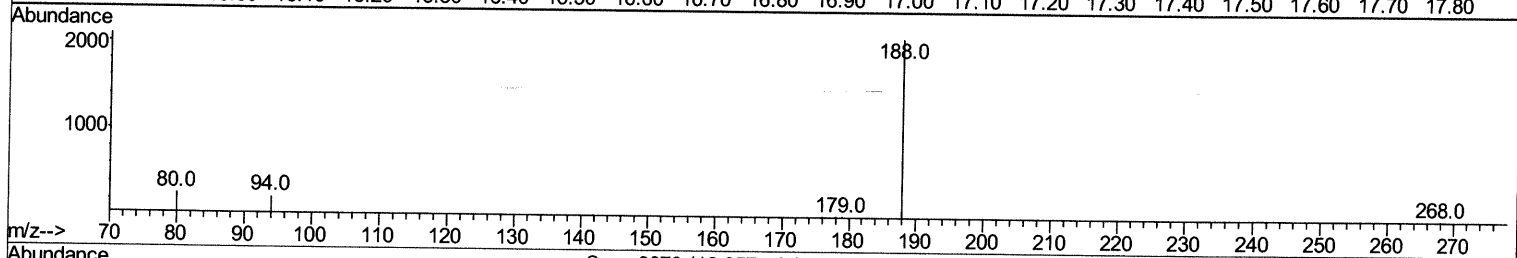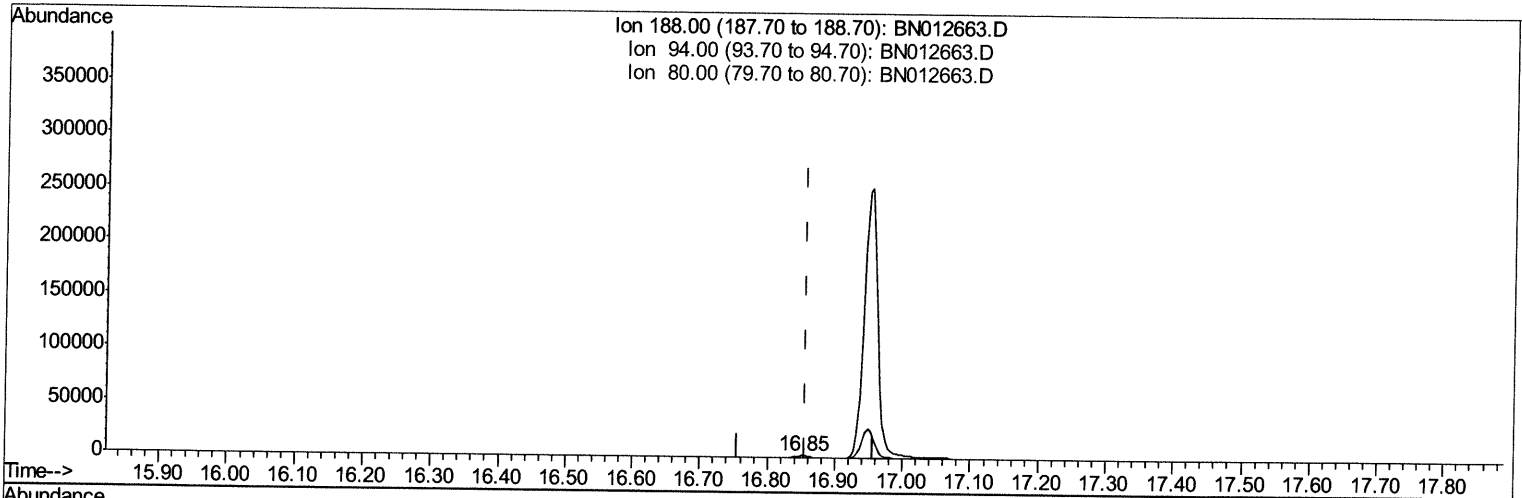

TIC: BN012663.D

(10) Phenanthrene-d10 (I)

16.851min (-0.005) 0.40ng/ul m 11/27/20 JU

response 3084

Ion	Exp%	Act%
188.00	100	100
94.00	11.60	11.22
80.00	12.60	12.66
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN112020\
 Data File : BN012663.D
 Acq On : 20 Nov 2020 17:39
 Operator : CG/JU
 Sample : PB133127BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK27

Manual Integrations
 APPROVED

mohammad
 11/24/2020 8:55:57 AM

Quant Time: Nov 20 18:15:53 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN112020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 20 18:13:27 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.44	152	650	0.40	ng/ul	0.00
2) Naphthalene-d8	10.21	136	2397	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.10	164	1491	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.85	188	3084m	0.40	ng/ul	0.00
16) Chrysene-d12	21.07	240	2470	0.40	ng/ul	0.00
20) Perylene-d12	23.18	264	2992	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.82	152	1528	0.44	ng/ul	0.00
14) Fluoranthene-d10	18.89	212	3337	0.41	ng/ul	0.00

Target Compounds

Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed