


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN112020\
Data File : BN012664.D
Acq On : 20 Nov 2020 18:15
Operator : CG/JU
Sample : PB133053BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK53

Manual Integrations
APPROVED

mohammad
11/24/2020 8:56:00 AM

Quant Time: Nov 21 01:47:44 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN112020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Nov 21 00:16:07 2020
Response via : Initial Calibration

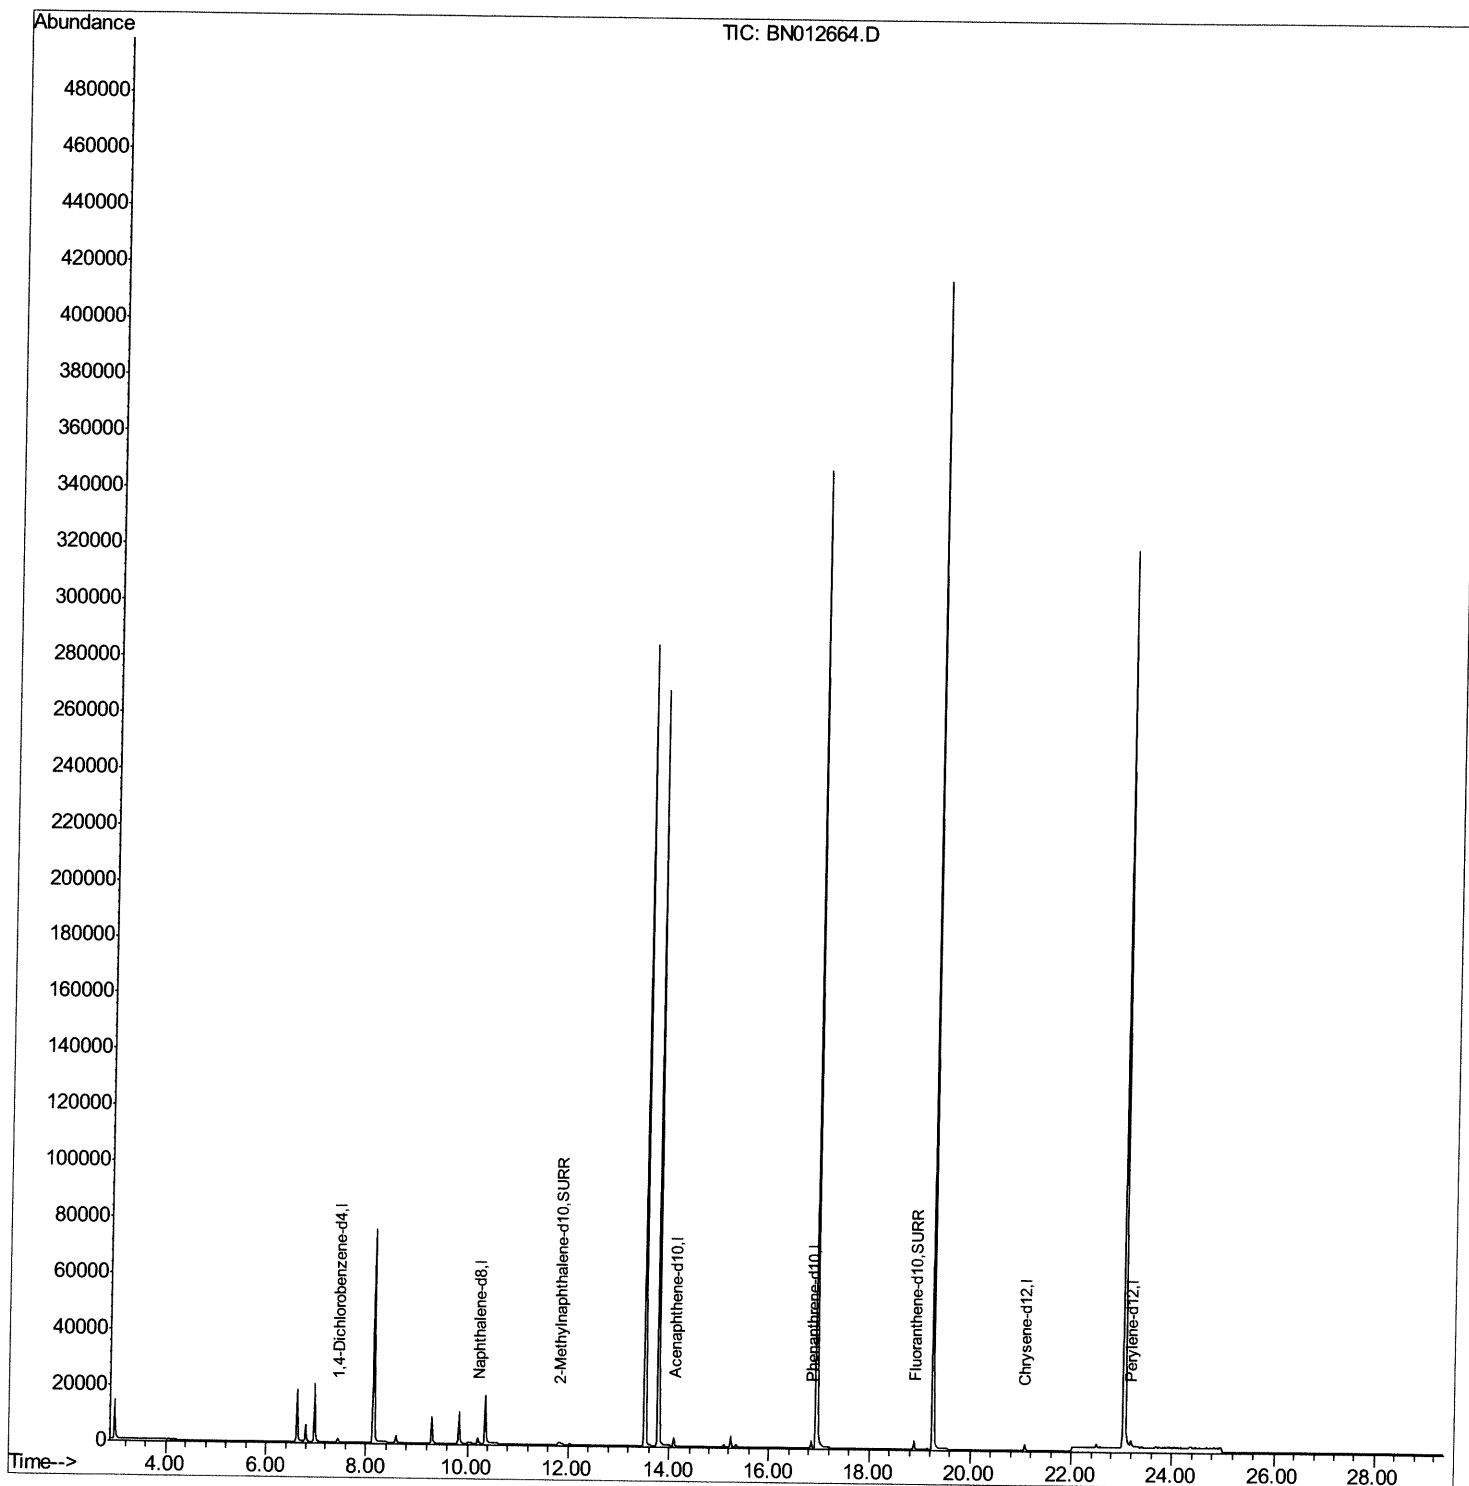

Quantitation Report (Qedit)


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN112020\
 Data File : BN012664.D
 Acq On : 20 Nov 2020 18:15
 Operator : CG/JU
 Sample : PB133053BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK53

Manual Integrations
 APPROVED

mohammad
 11/24/2020 8:56:00 AM

Quant Time: Nov 21 01:46:14 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN112020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Nov 21 00:16:07 2020
 Response via : Initial Calibration

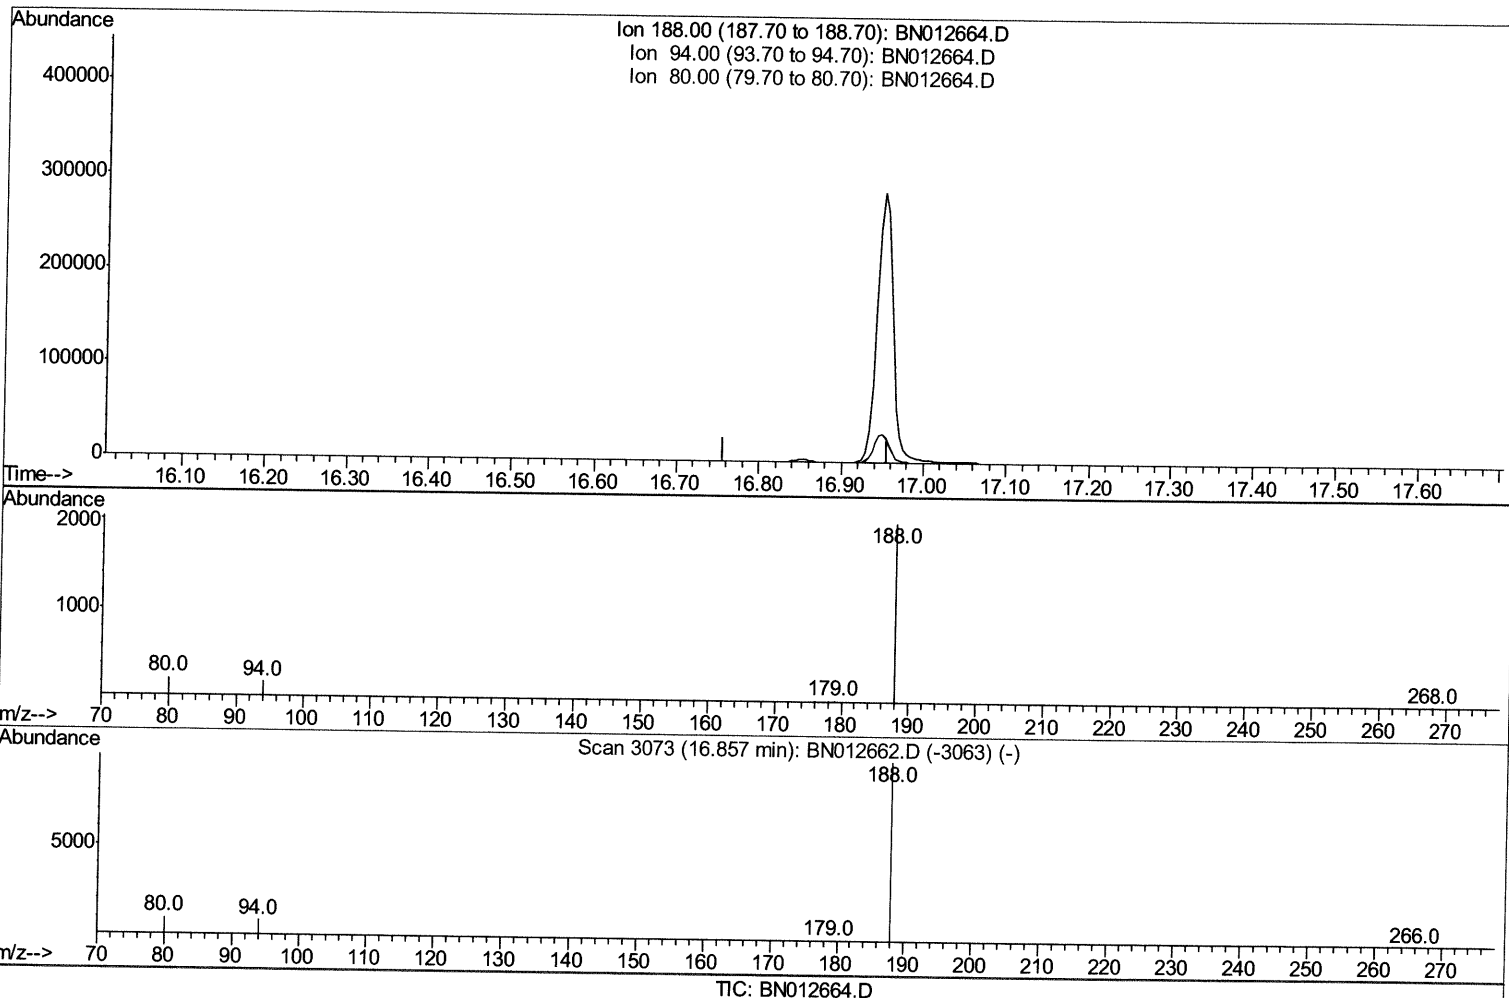

(10) Phenanthrene-d10 (I)

16.857min (-16.857) 0.00ng/ui

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	11.60	0.00#
80.00	12.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN112020\
Data File : BN012664.D
Acq On : 20 Nov 2020 18:15
Operator : CG/JU
Sample : PB133053BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK53

Manual Integrations
APPROVED

mohammad
11/24/2020 8:56:00 AM

Quant Time: Nov 21 01:46:14 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN112020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Nov 21 00:16:07 2020
Response via : Initial Calibration

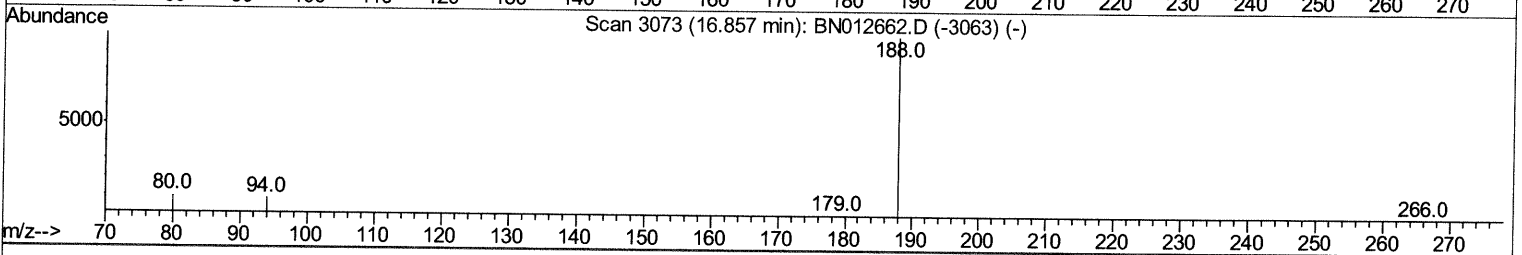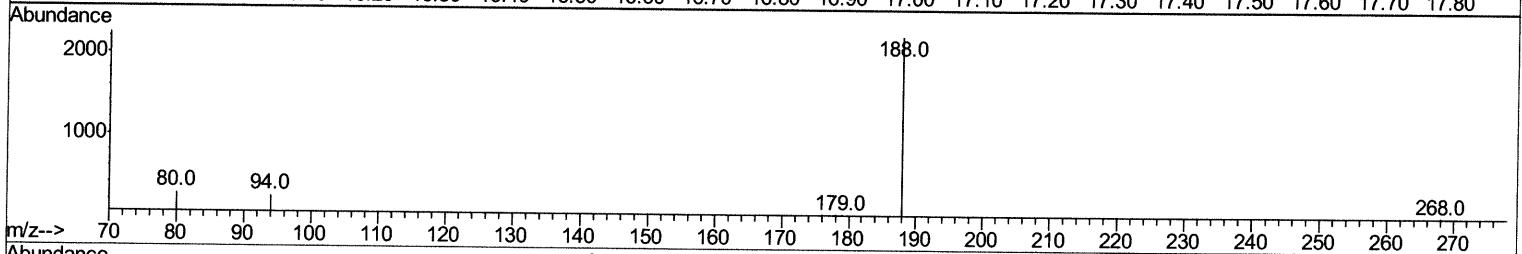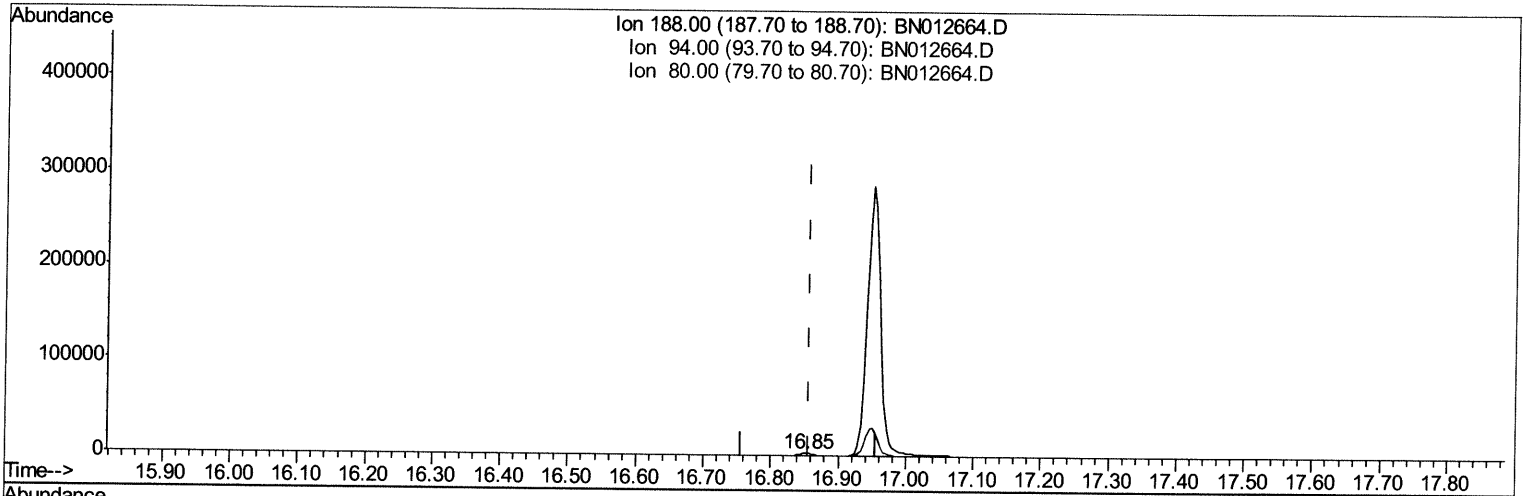

TIC: BN012664.D

(10) Phenanthrene-d10 (I)

16.853min (-0.004) 0.40ng/ul m 11/27/2024

response 3234

Ion	Exp%	Act%
188.00	100	100
94.00	11.60	10.75
80.00	12.60	12.36
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN112020\
 Data File : BN012664.D
 Acq On : 20 Nov 2020 18:15
 Operator : CG/JU
 Sample : PB133053BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK53

Manual Integrations
 APPROVED

mohammad
 11/24/2020 8:56:00 AM

Quant Time: Nov 21 01:47:44 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN112020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Nov 21 00:16:07 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.44	152	706	0.40	ng/ul	0.00
2) Naphthalene-d8	10.21	136	2733	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.10	164	1657	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.85	188	3234m >	0.40	ng/ul >	0.00
16) Chrysene-d12	21.07	240	2729	0.40	ng/ul	0.00
20) Perylene-d12	23.19	264	3197	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.82	152	1681	0.43	ng/ul	0.00
14) Fluoranthene-d10	18.89	212	3642	0.43	ng/ul	0.00

Target Compounds

Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed