


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN112020\
Data File : BN012673.D
Acq On : 20 Nov 2020 23:40
Operator : CG/JU
Sample : L4793-09
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0BG3

Manual Integrations
APPROVED

mohammad
11/24/2020 8:56:29 AM

Quant Time: Nov 21 01:30:20 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN112020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Nov 21 00:16:07 2020
Response via : Initial Calibration

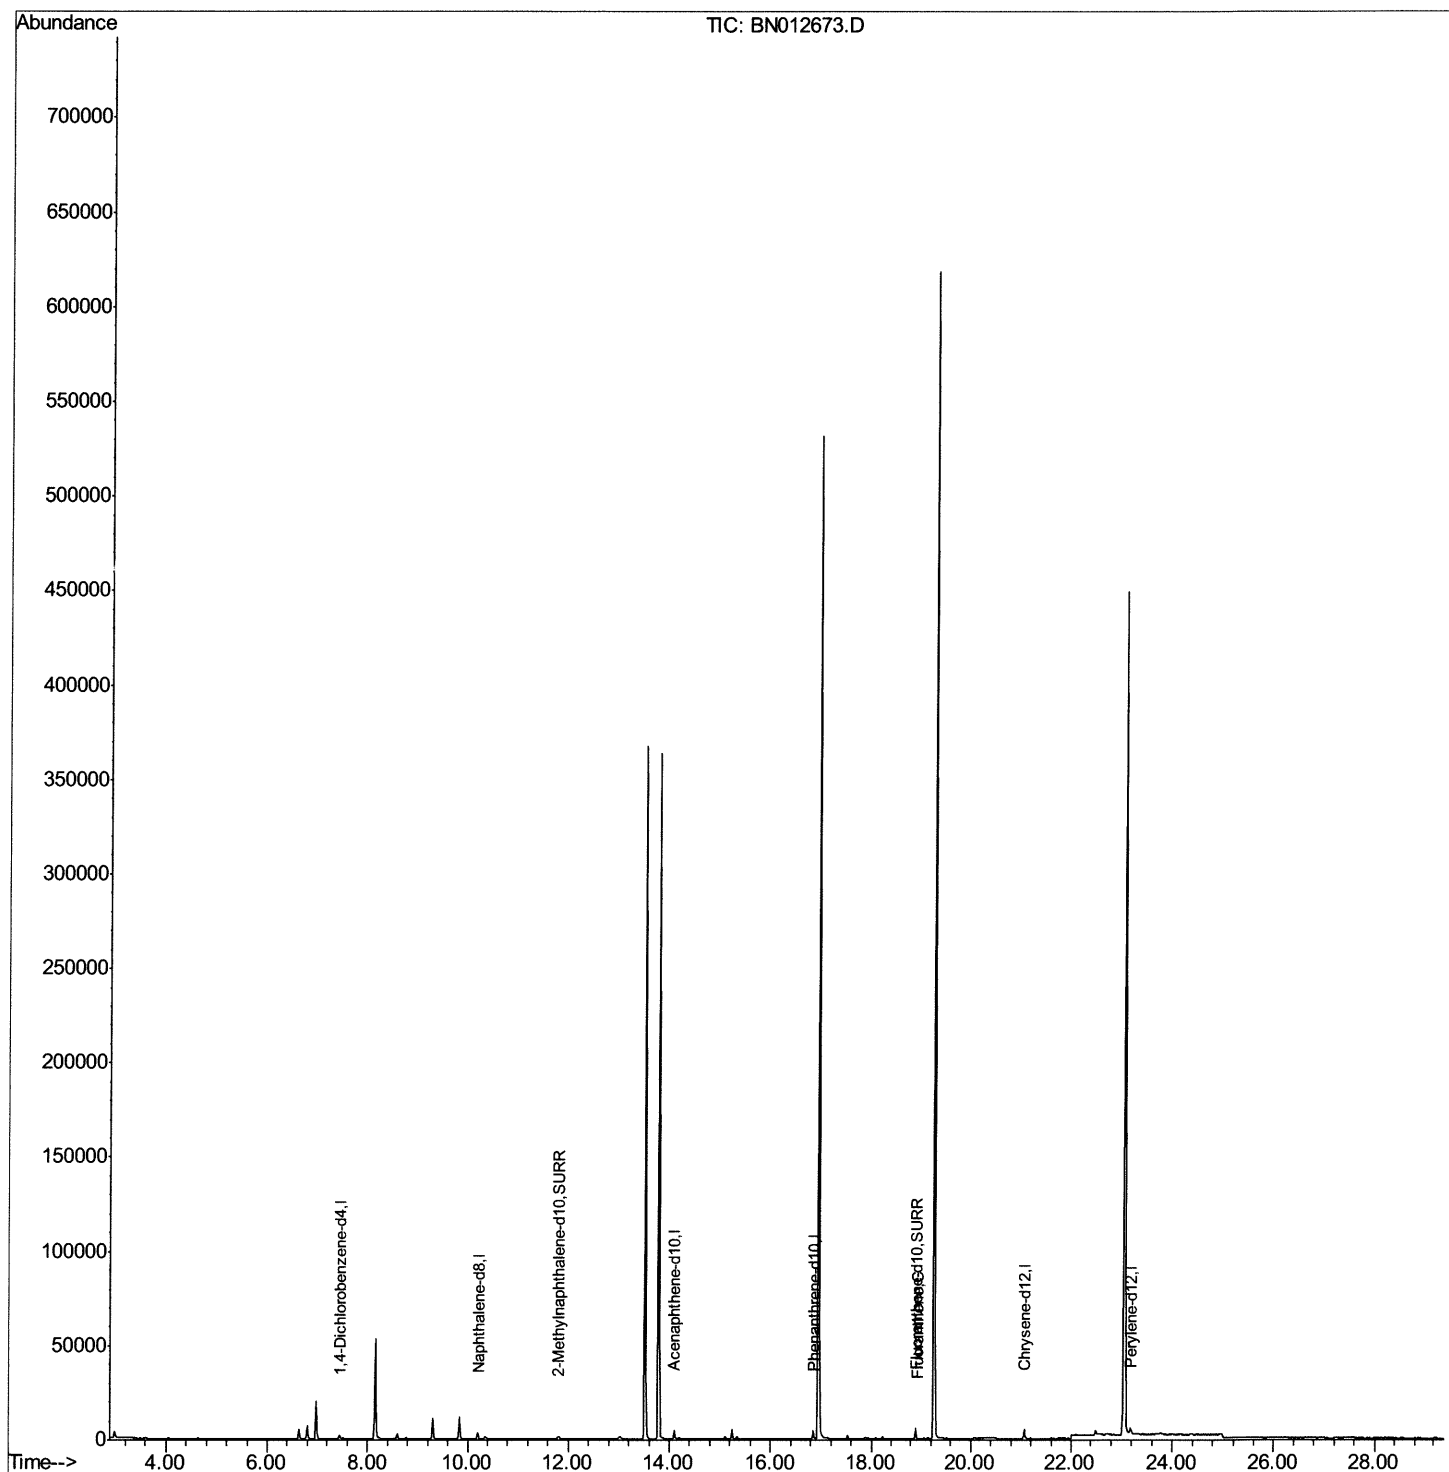

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN112020\
Data File : BN012673.D
Acq On : 20 Nov 2020 23:40
Operator : CG/JU
Sample : L4793-09
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0BG3

Manual Integrations
APPROVED

mohammad
11/24/2020 8:56:29 AM

Quant Time: Nov 21 01:28:10 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN112020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Nov 21 00:16:07 2020
Response via : Initial Calibration

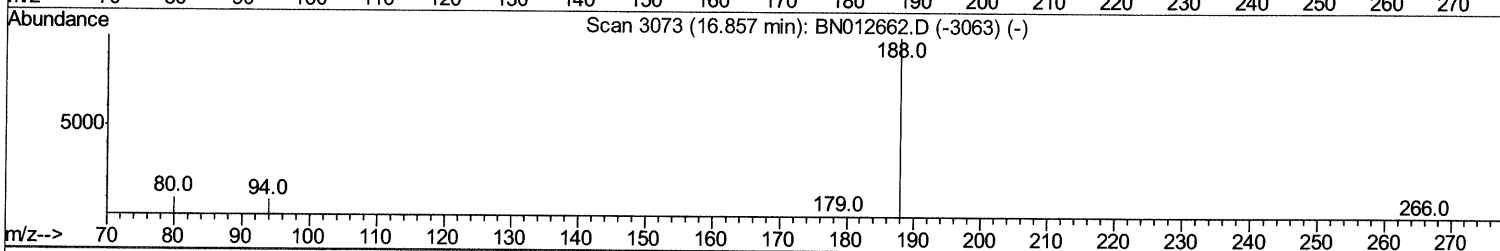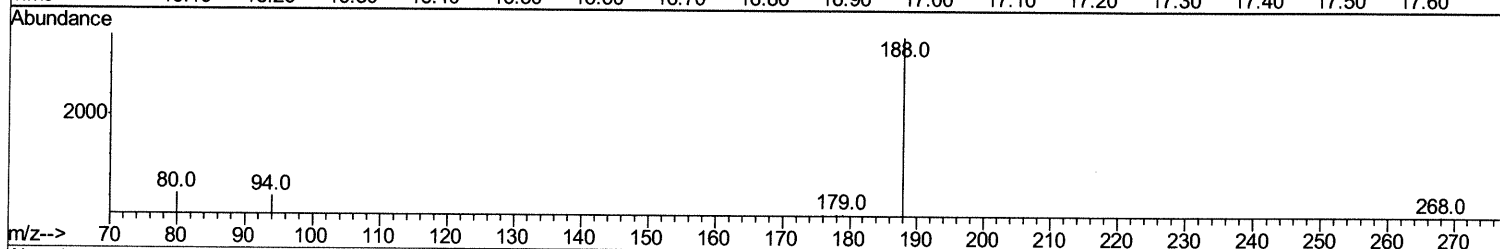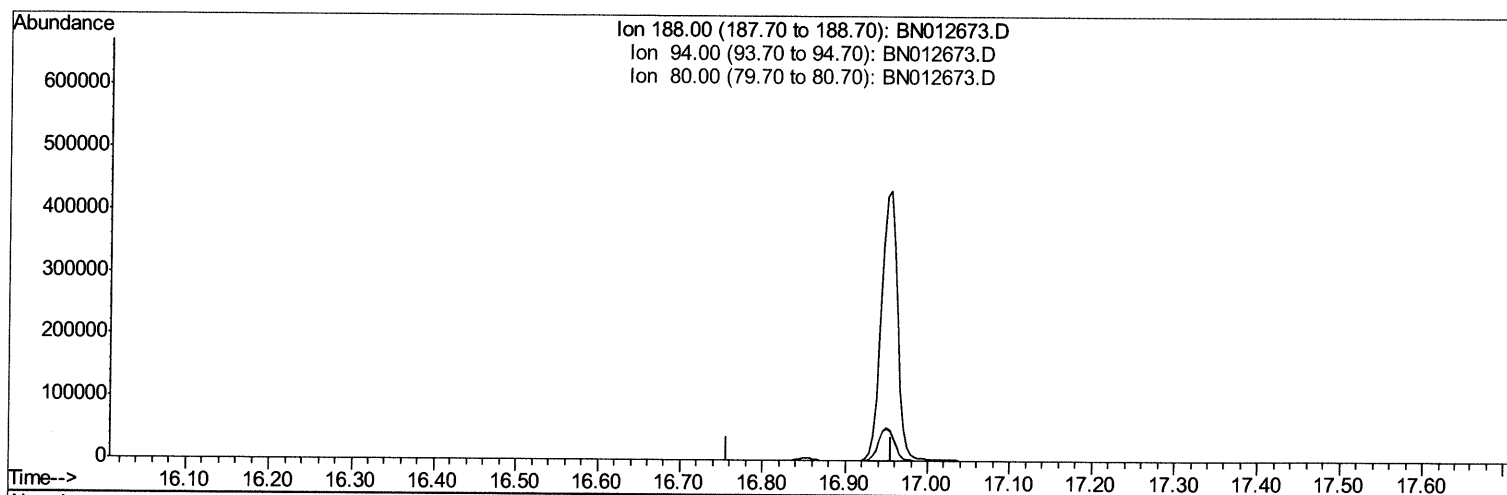

TIC: BN012673.D

(10) Phenanthrene-d10 (I)

16.857min (-16.857) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	11.60	0.00#
80.00	12.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN112020\
Data File : BN012673.D
Acq On : 20 Nov 2020 23:40
Operator : CG/JU
Sample : L4793-09
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0BG3

Manual Integrations
APPROVED

mohammad
11/24/2020 8:56:29 AM

Quant Time: Nov 21 01:28:10 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN112020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Nov 21 00:16:07 2020
Response via : Initial Calibration

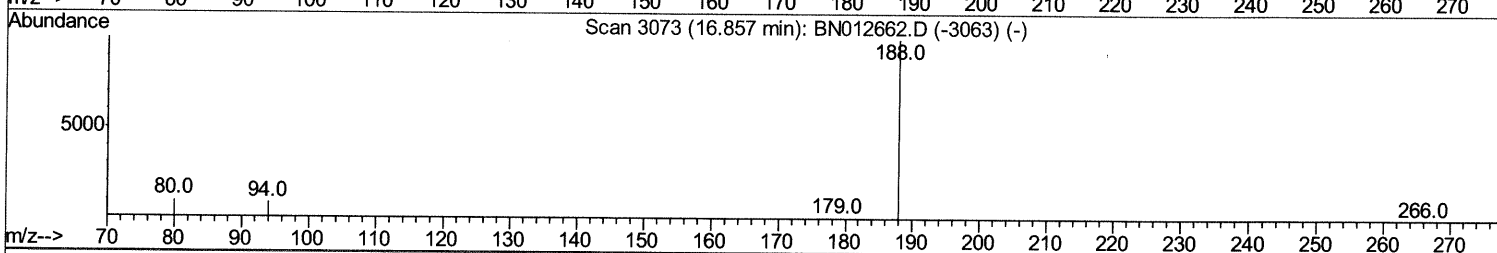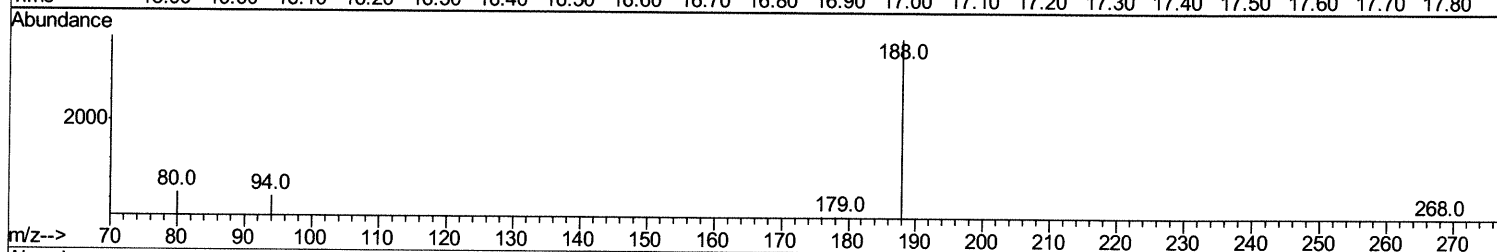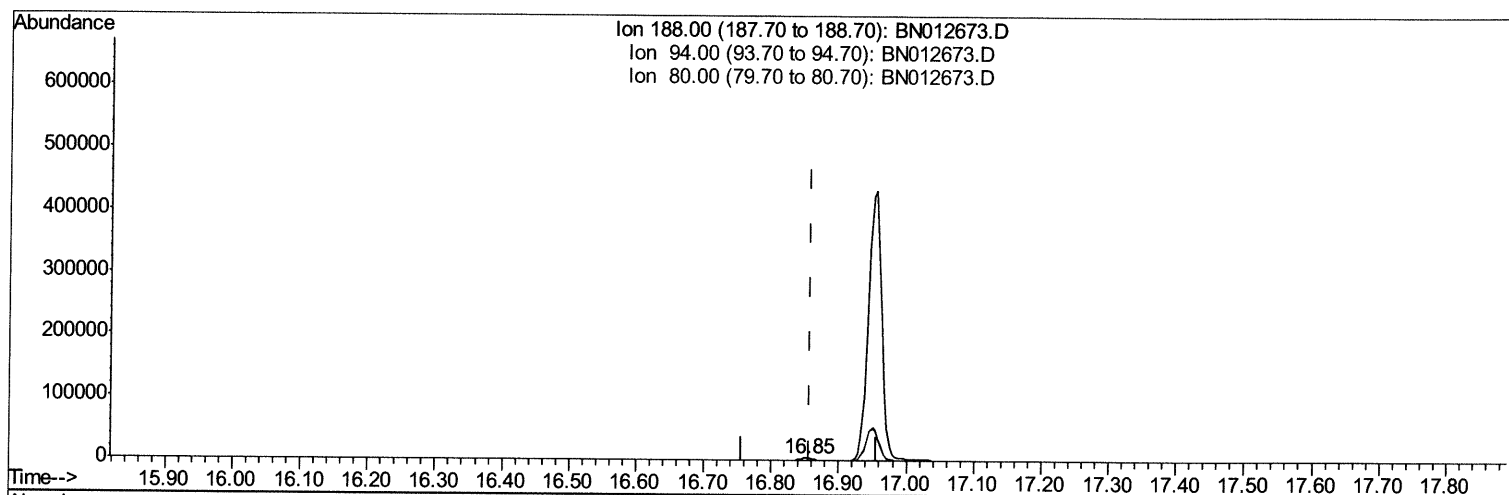

TIC: BN012673.D

(10) Phenanthrene-d10 (I)

16.852min (-0.004) 0.40ng/ul m

11/21/2024

response 5116

Ion	Exp%	Act%
188.00	100	100
94.00	11.60	12.22
80.00	12.60	14.51
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN112020\
 Data File : BN012673.D
 Acq On : 20 Nov 2020 23:40
 Operator : CG/JU
 Sample : L4793-09
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0BG3

Manual Integrations
 APPROVED

mohammad
 11/24/2020 8:56:29 AM

Quant Time: Nov 21 01:30:20 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN112020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Nov 21 00:16:07 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.44	152	1066	0.40	ng/ul	0.00
2) Naphthalene-d8	10.21	136	4432	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.10	164	2712	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.85	188	5116m >	0.40	ng/ul >	0.00
16) Chrysene-d12	21.07	240	4495	0.40	ng/ul	0.00
20) Perylene-d12	23.18	264	4629	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.81	152	2507	0.39	ng/ul	0.00
14) Fluoranthene-d10	18.89	212	6407	0.48	ng/ul	0.00
Target Compounds						
15) Fluoranthene	18.93	202	432	0.021	ng/ul	Ovalue 51

(#) = qualifier out of range (m) = manual integration (+) = signals summed