


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN112020\
Data File : BN012674.D
Acq On : 21 Nov 2020 00:16
Operator : CG/JU
Sample : L4794-22
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0BH0

Manual Integrations
APPROVED

mohammad
11/24/2020 8:56:31 AM

Quant Time: Nov 21 01:33:12 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN112020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Nov 21 00:16:07 2020
Response via : Initial Calibration

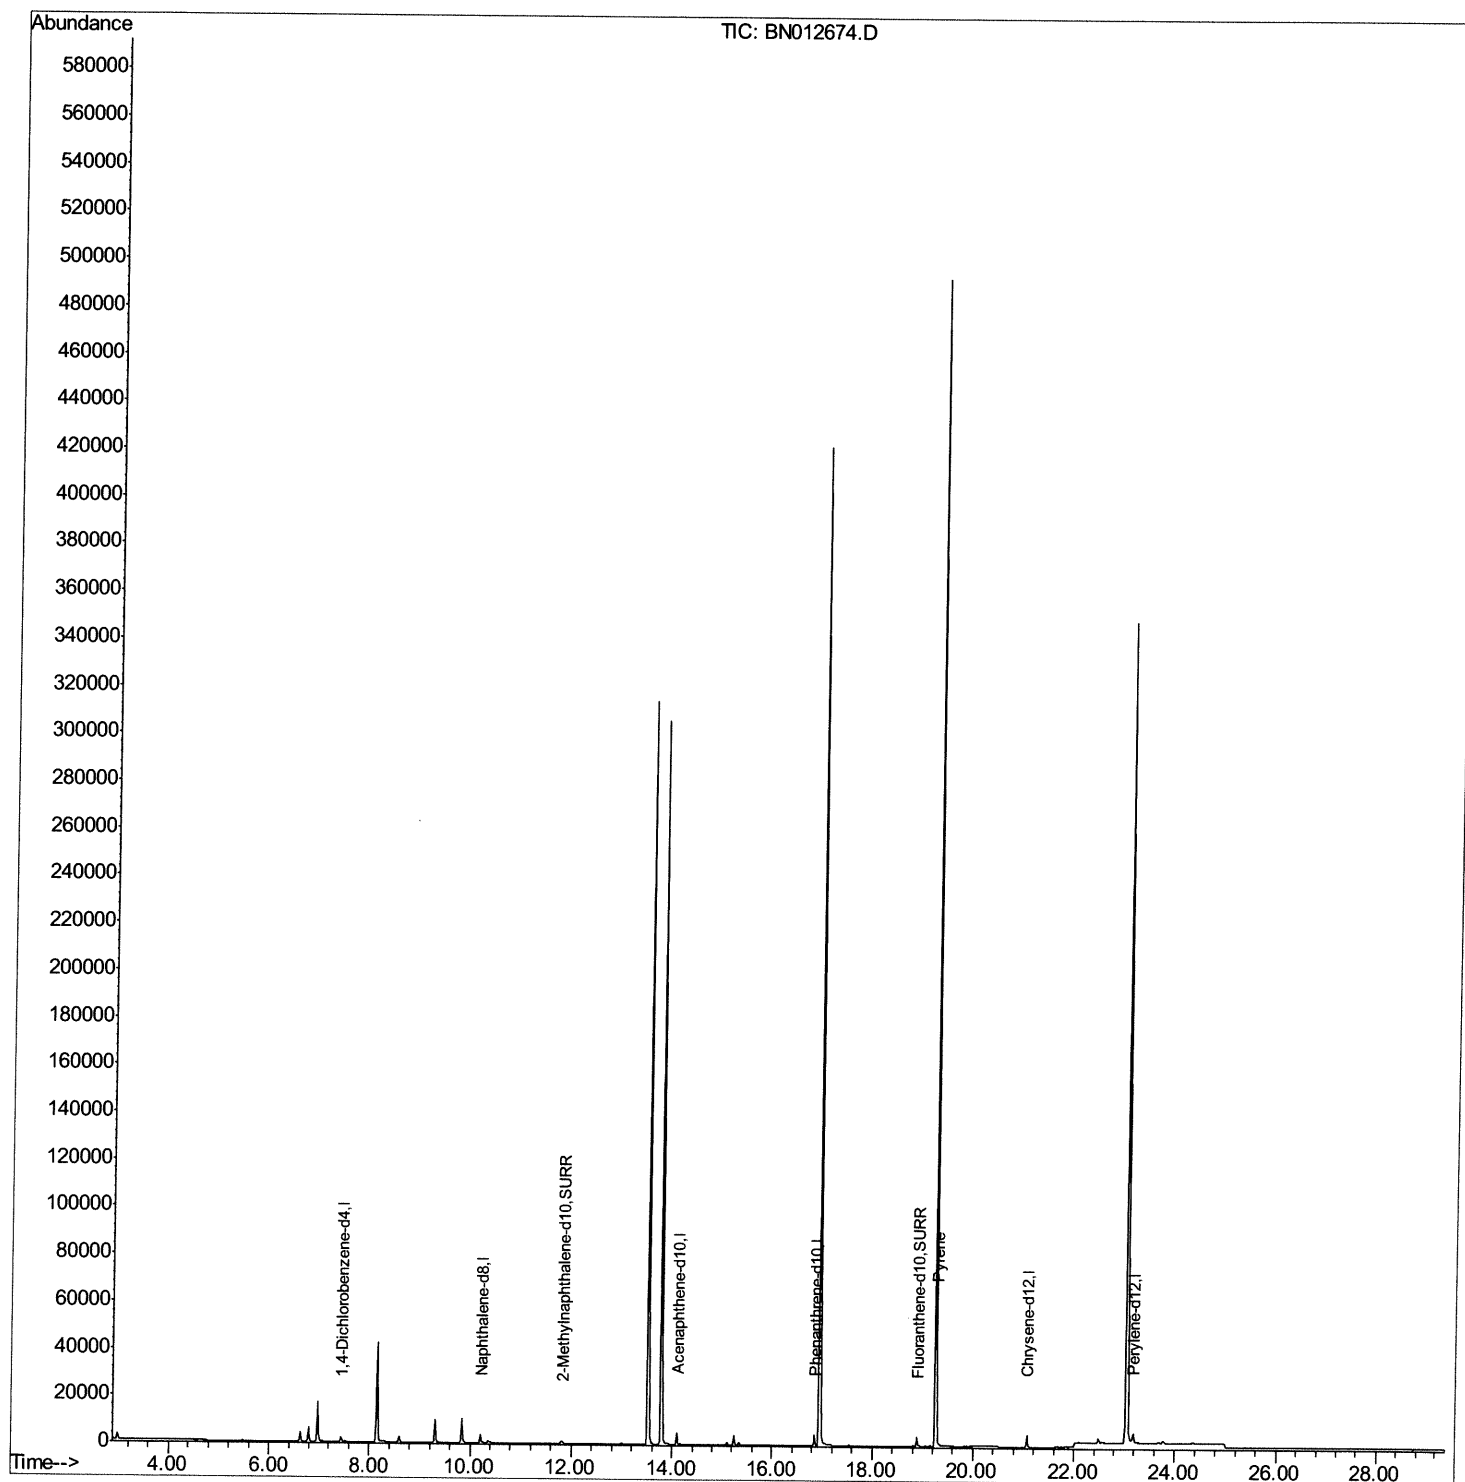

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN112020\
Data File : BN012674.D
Acq On : 21 Nov 2020 00:16
Operator : CG/JU
Sample : L4794-22
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0BH0

Manual Integrations
APPROVED

mohammad
11/24/2020 8:56:31 AM

Quant Time: Nov 21 01:31:47 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN112020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Nov 21 00:16:07 2020
Response via : Initial Calibration

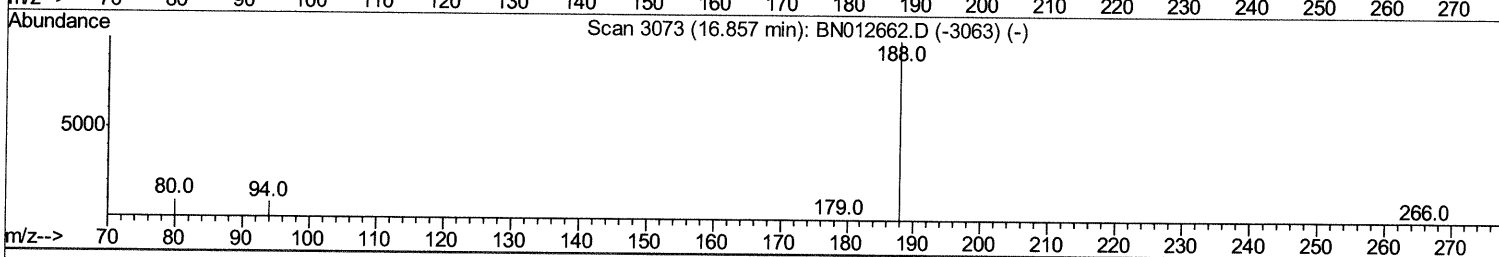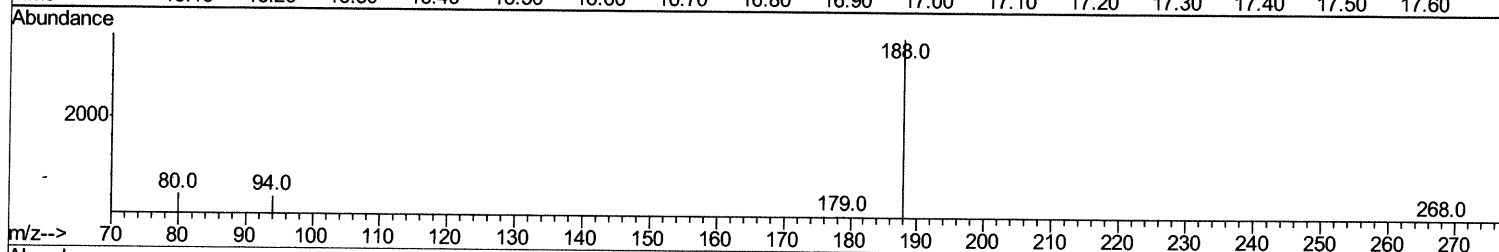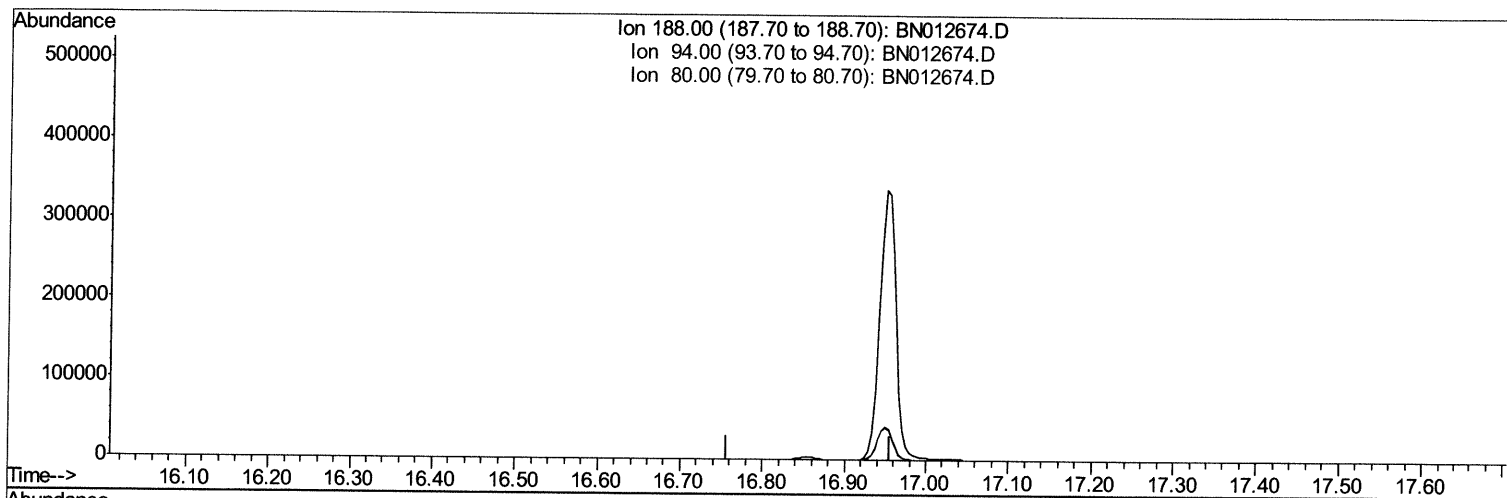

TIC: BN012674.D

(10) Phenanthrene-d10 (I)

16.857min (-16.857) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	11.60	0.00#
80.00	12.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN112020\
Data File : BN012674.D
Acq On : 21 Nov 2020 00:16
Operator : CG/JU
Sample : L4794-22
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0BH0

Manual Integrations
APPROVED

mohammad
11/24/2020 8:56:31 AM

Quant Time: Nov 21 01:31:47 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN112020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Nov 21 00:16:07 2020
Response via : Initial Calibration

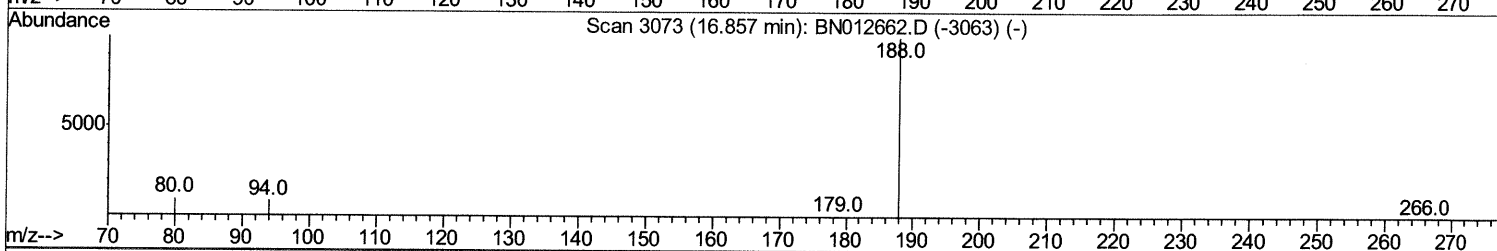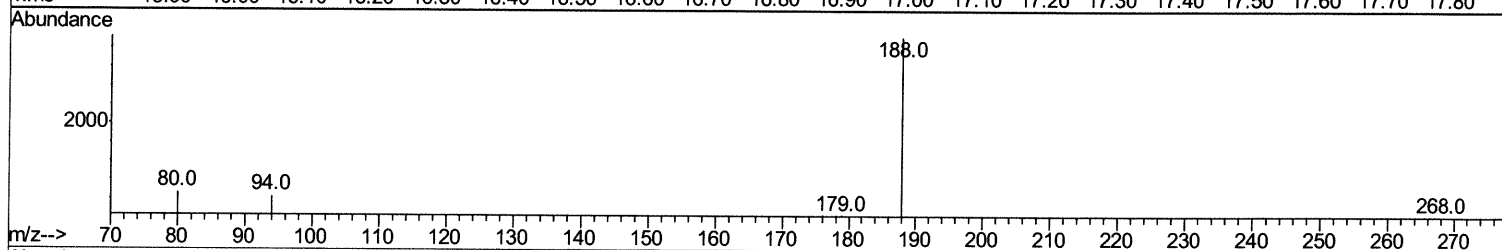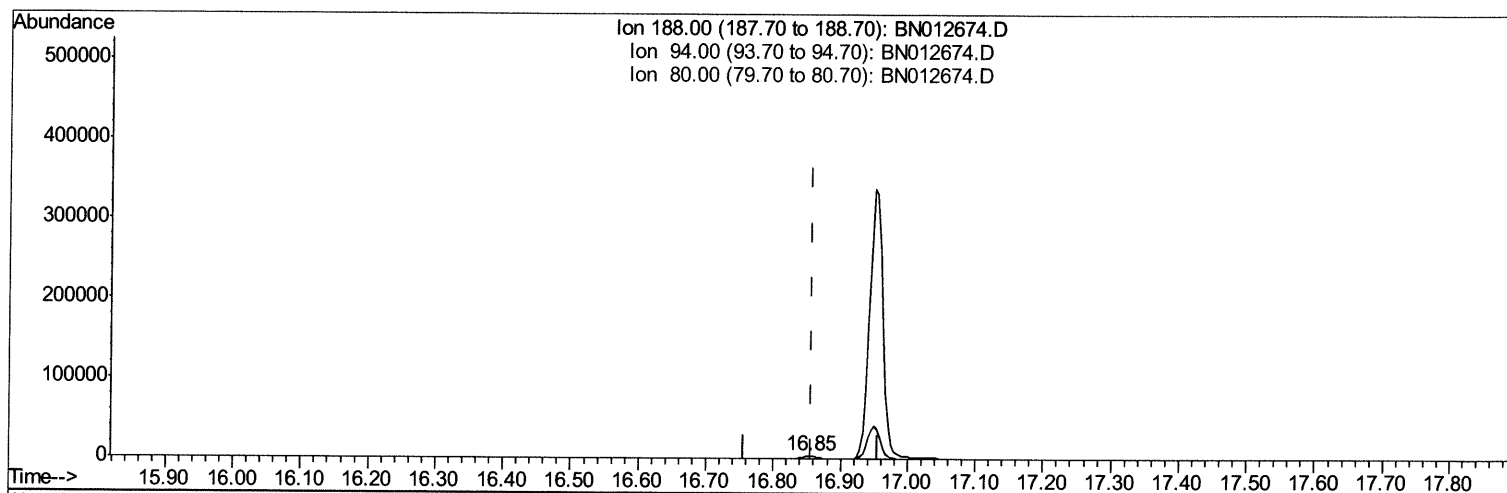

TIC: BN012674.D

(10) Phenanthrene-d10 (I)

16.853min (-0.004) 0.40ng/ul m 11/21/2024

response 5280

Ion	Exp%	Act%
188.00	100	100
94.00	11.60	11.67
80.00	12.60	13.59
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN112020\
 Data File : BN012674.D
 Acq On : 21 Nov 2020 00:16
 Operator : CG/JU
 Sample : L4794-22
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 COBH0

Manual Integrations
 APPROVED

mohammad
 11/24/2020 8:56:31 AM

Quant Time: Nov 21 01:33:12 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN112020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Nov 21 00:16:07 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.44	152	1089	0.40	ng/ul	0.00
2) Naphthalene-d8	10.21	136	4591	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.10	164	2697	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.85	188	5280m>	0.40	ng/ul>	0.00 11/21/2020
16) Chrysene-d12	21.07	240	4531	0.40	ng/ul	0.00
20) Perylene-d12	23.18	264	4862	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.81	152	1892	0.28	ng/ul	0.00
14) Fluoranthene-d10	18.89	212	4354	0.32	ng/ul	0.00
Target Compounds						
17) Pvrene	19.29	202	463	0.023	ng/ul#	Ovalue 39

(#) = qualifier out of range (m) = manual integration (+) = signals summed