


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN112020\
Data File : BN012687.D
Acq On : 21 Nov 2020 15:26
Operator : CG/JU
Sample : L4794-22RE
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0BH0

Manual Integrations
APPROVED

mohammad
11/24/2020 8:57:03 AM

Quant Time: Nov 23 02:33:37 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN112020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 23 01:22:42 2020
Response via : Initial Calibration

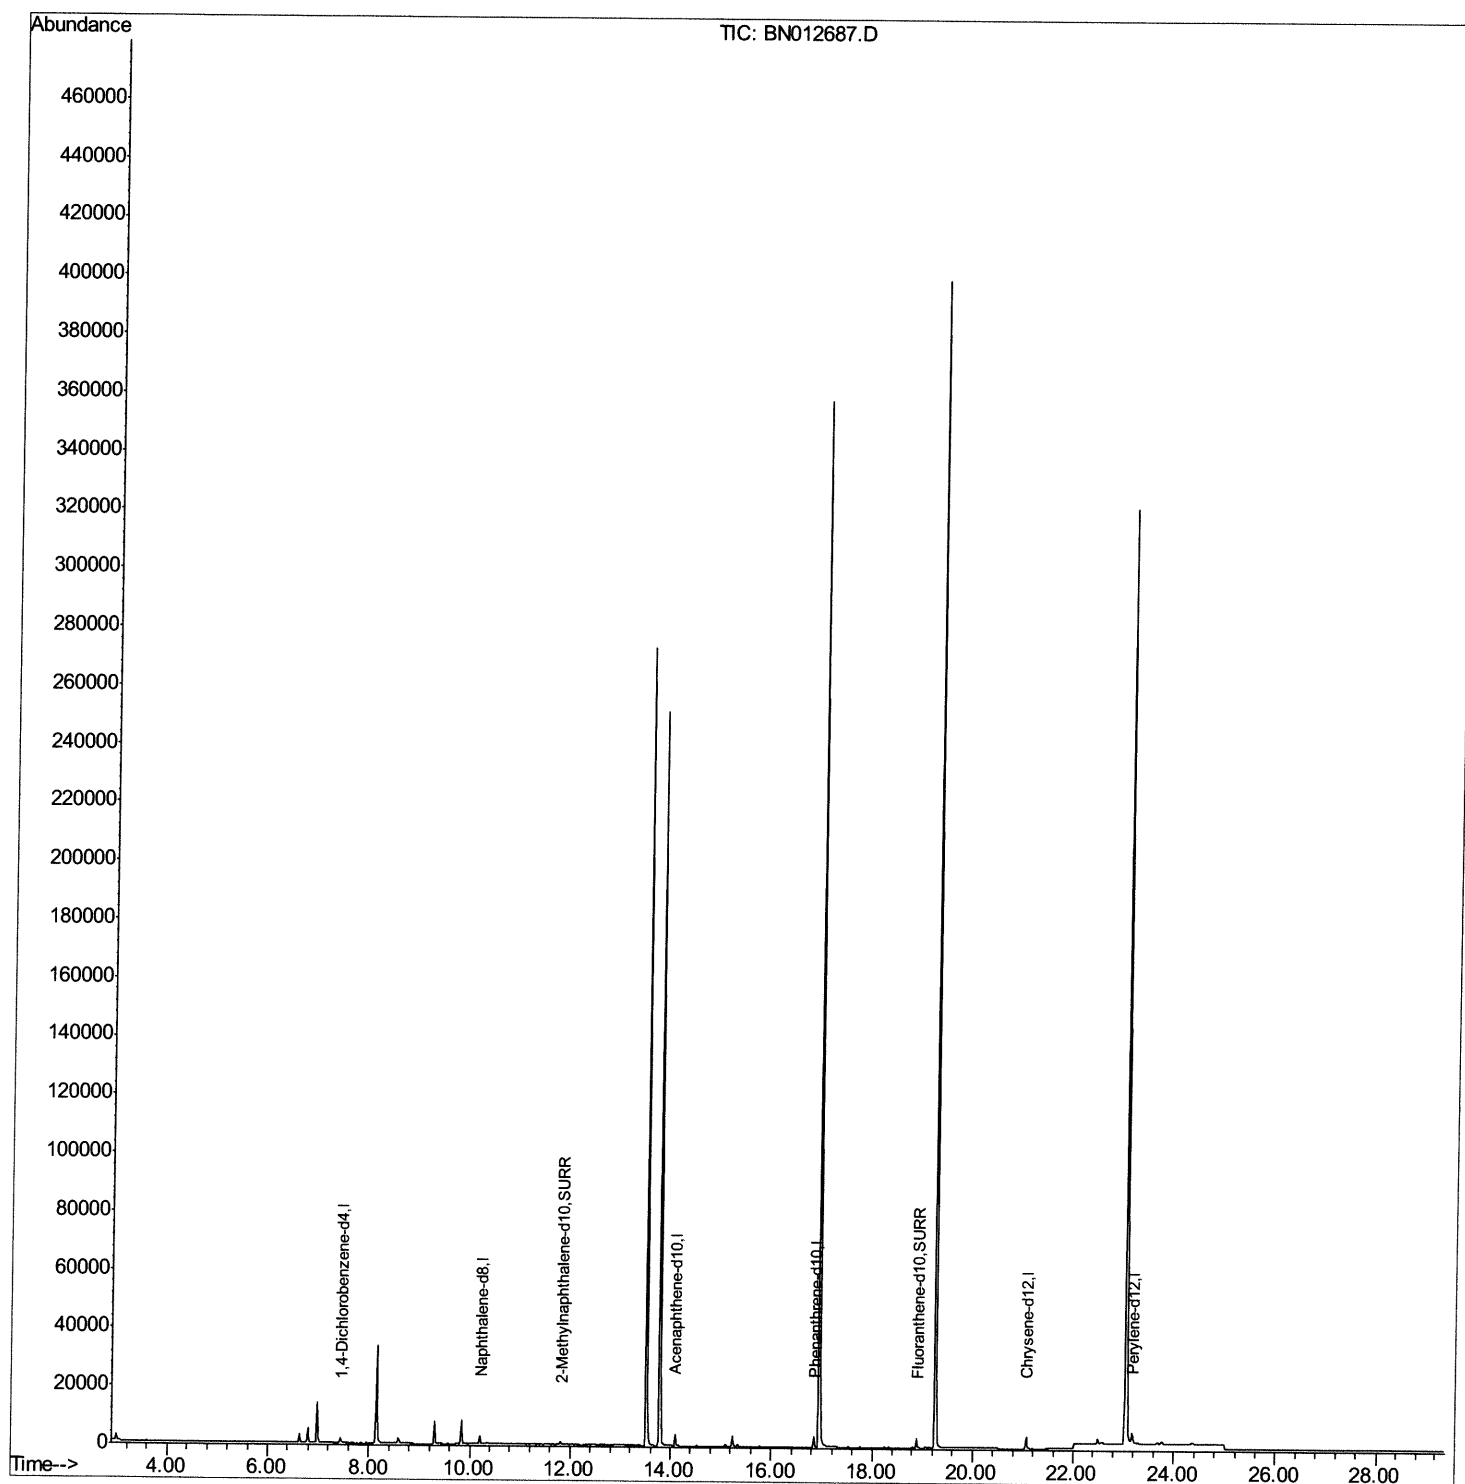

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN112020\
Data File : BN012687.D
Acq On : 21 Nov 2020 15:26
Operator : CG/JU
Sample : L4794-22RE
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0BH0

Manual Integrations
APPROVED

mohammad
11/24/2020 8:57:03 AM

Quant Time: Nov 23 01:25:11 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN112020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 23 01:22:42 2020
Response via : Initial Calibration

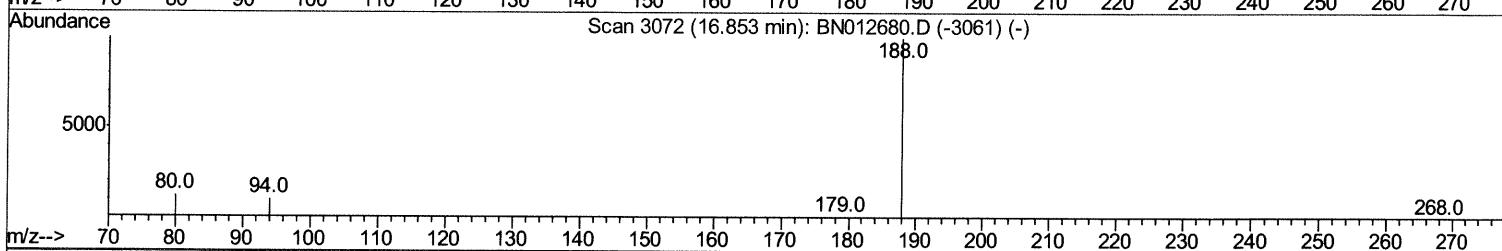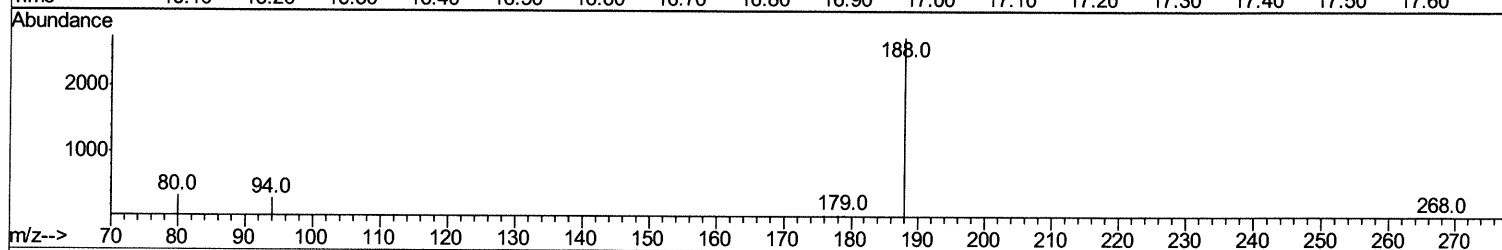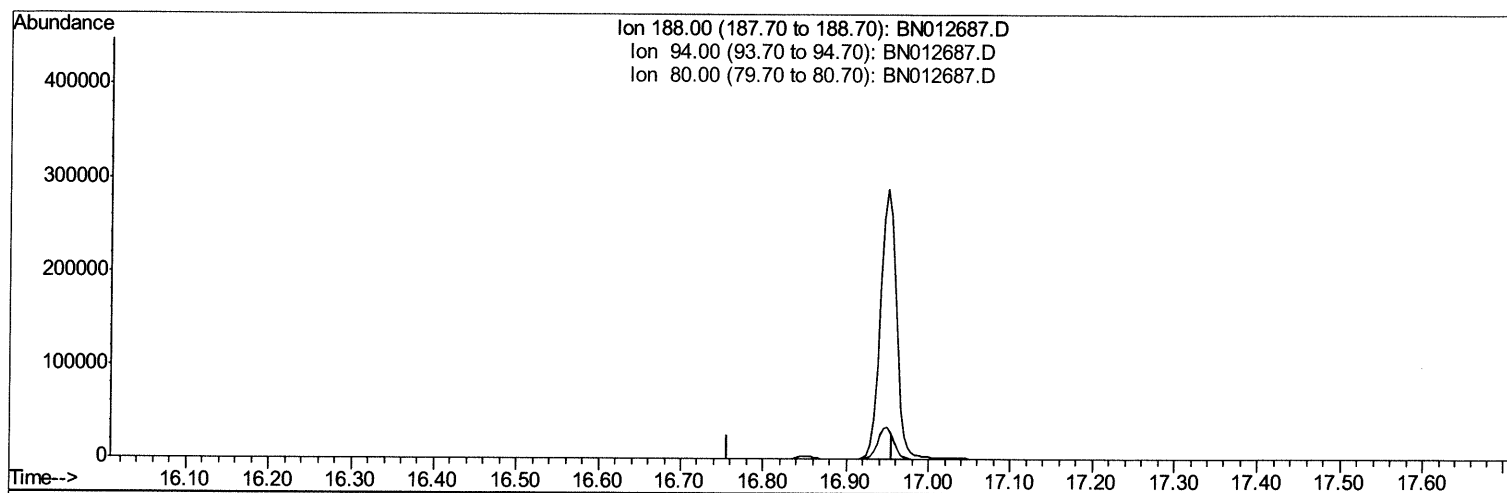

TIC: BN012687.D

(10) Phenanthrene-d10 (I)

16.857min (-16.857) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	11.60	0.00#
80.00	12.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN112020\
 Data File : BN012687.D
 Acq On : 21 Nov 2020 15:26
 Operator : CG/JU
 Sample : L4794-22RE
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0BH0

Manual Integrations
 APPROVED

mohammad
 11/24/2020 8:57:03 AM

Quant Time: Nov 23 01:25:11 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN112020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 23 01:22:42 2020
 Response via : Initial Calibration

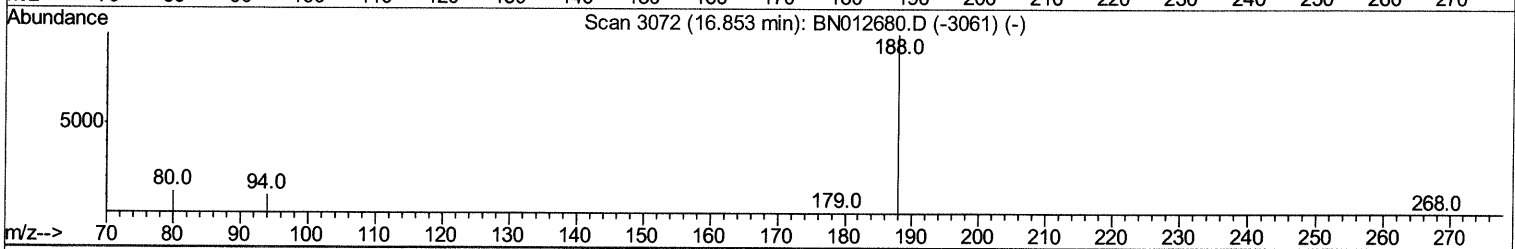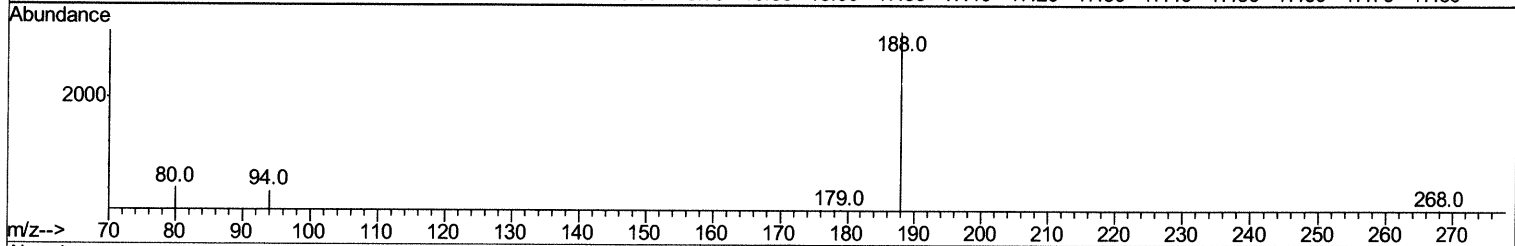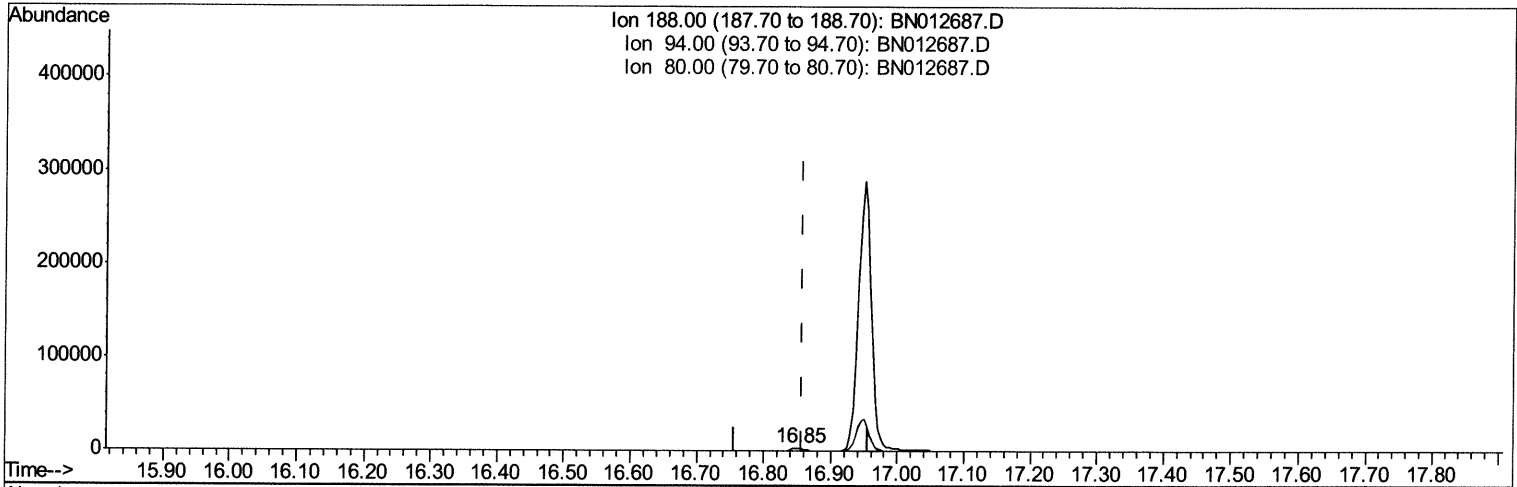

TIC: BN012687.D

(10) Phenanthrene-d10 (I)

16.852min (-0.004) 0.40ng/ul m 11/21/2024

response 4457

Ion	Exp%	Act%
188.00	100	100
94.00	11.60	11.63
80.00	12.60	13.61
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN112020\
 Data File : BN012687.D
 Acq On : 21 Nov 2020 15:26
 Operator : CG/JU
 Sample : L4794-22RE
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 COBH0

Manual Integrations
 APPROVED

mohammad
 11/24/2020 8:57:03 AM

Quant Time: Nov 23 02:33:37 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN112020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 23 01:22:42 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.44	152	925	0.40	ng/ul	0.00
2) Naphthalene-d8	10.21	136	3812	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.10	164	2287	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.85	188	4457m >	0.40	ng/ul >	0.00
16) Chrysene-d12	21.07	240	3821	0.40	ng/ul	0.00
20) Perylene-d12	23.18	264	4361	0.40	ng/ul	0.00

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	11.81	152	1548	0.28	ng/ul	0.00
14) Fluoranthene-d10	18.89	212	3697	0.32	ng/ul	0.00

Target Compounds

Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed