

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112122\
 Data File : BN022790.D
 Acq On : 21 Nov 2022 16:59
 Operator : CG/JU
 Sample : PB149195BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK195

Quant Time: Nov 21 21:42:46 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Nov 19 05:51:00 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.852	152	50852	20.000	ng/ul	0.00
20) Naphthalene-d8	10.669	136	244812	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.522	164	161971	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.275	188	340304	20.000	ng/ul	0.00
79) Chrysene-d12	21.475	240	328815	20.000	ng/ul	0.00
88) Perylene-d12	23.874	264	327591	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.175	96	9021	6.057	ng/uL	0.00
4) Pyridine-d5	3.611	84	124449	29.545	ng/ul	0.00
7) Phenol-d5	7.016	99	153110	31.879	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.181	67	101200	35.143	ng/ul	0.00
11) 2-Chlorophenol-d4	7.375	132	113372	32.232	ng/ul	0.00
15) 4-Methylphenol-d8	8.575	113	126955	33.483	ng/ul	0.00
21) Nitrobenzene-d5	9.028	128	61680	32.550	ng/ul	0.00
24) 2-Nitrophenol-d4	9.752	143	67596	31.970	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.293	165	111619	30.966	ng/ul	0.00
31) 4-Chloroaniline-d4	10.816	131	178089	32.435	ng/ul	0.00
46) Dimethylphthalate-d6	13.940	166	415200	35.243	ng/ul	0.00
49) Acenaphthylene-d8	14.216	160	446267	34.379	ng/ul	0.00
54) 4-Nitrophenol-d4	14.740	143	69591	29.631	ng/ul	0.00
60) Fluorene-d10	15.516	176	340135	35.202	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.651	200	58670	27.124	ng/ul	0.00
73) Anthracene-d10	17.375	188	530335	35.590	ng/ul	0.00
81) Pyrene-d10	19.675	212	587379	34.470	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.716	264	570777	34.661	ng/ul	0.00


Target Compounds					Qvalue
17) N-Nitroso-di-n-propyla...	8.575	70	3507	1.087 ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112122\
Data File : BN022790.D
Acq On : 21 Nov 2022 16:59
Operator : CG/JU
Sample : PB149195BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK195


Quant Time: Nov 21 21:42:46 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Nov 19 05:51:00 2022
Response via : Initial Calibration

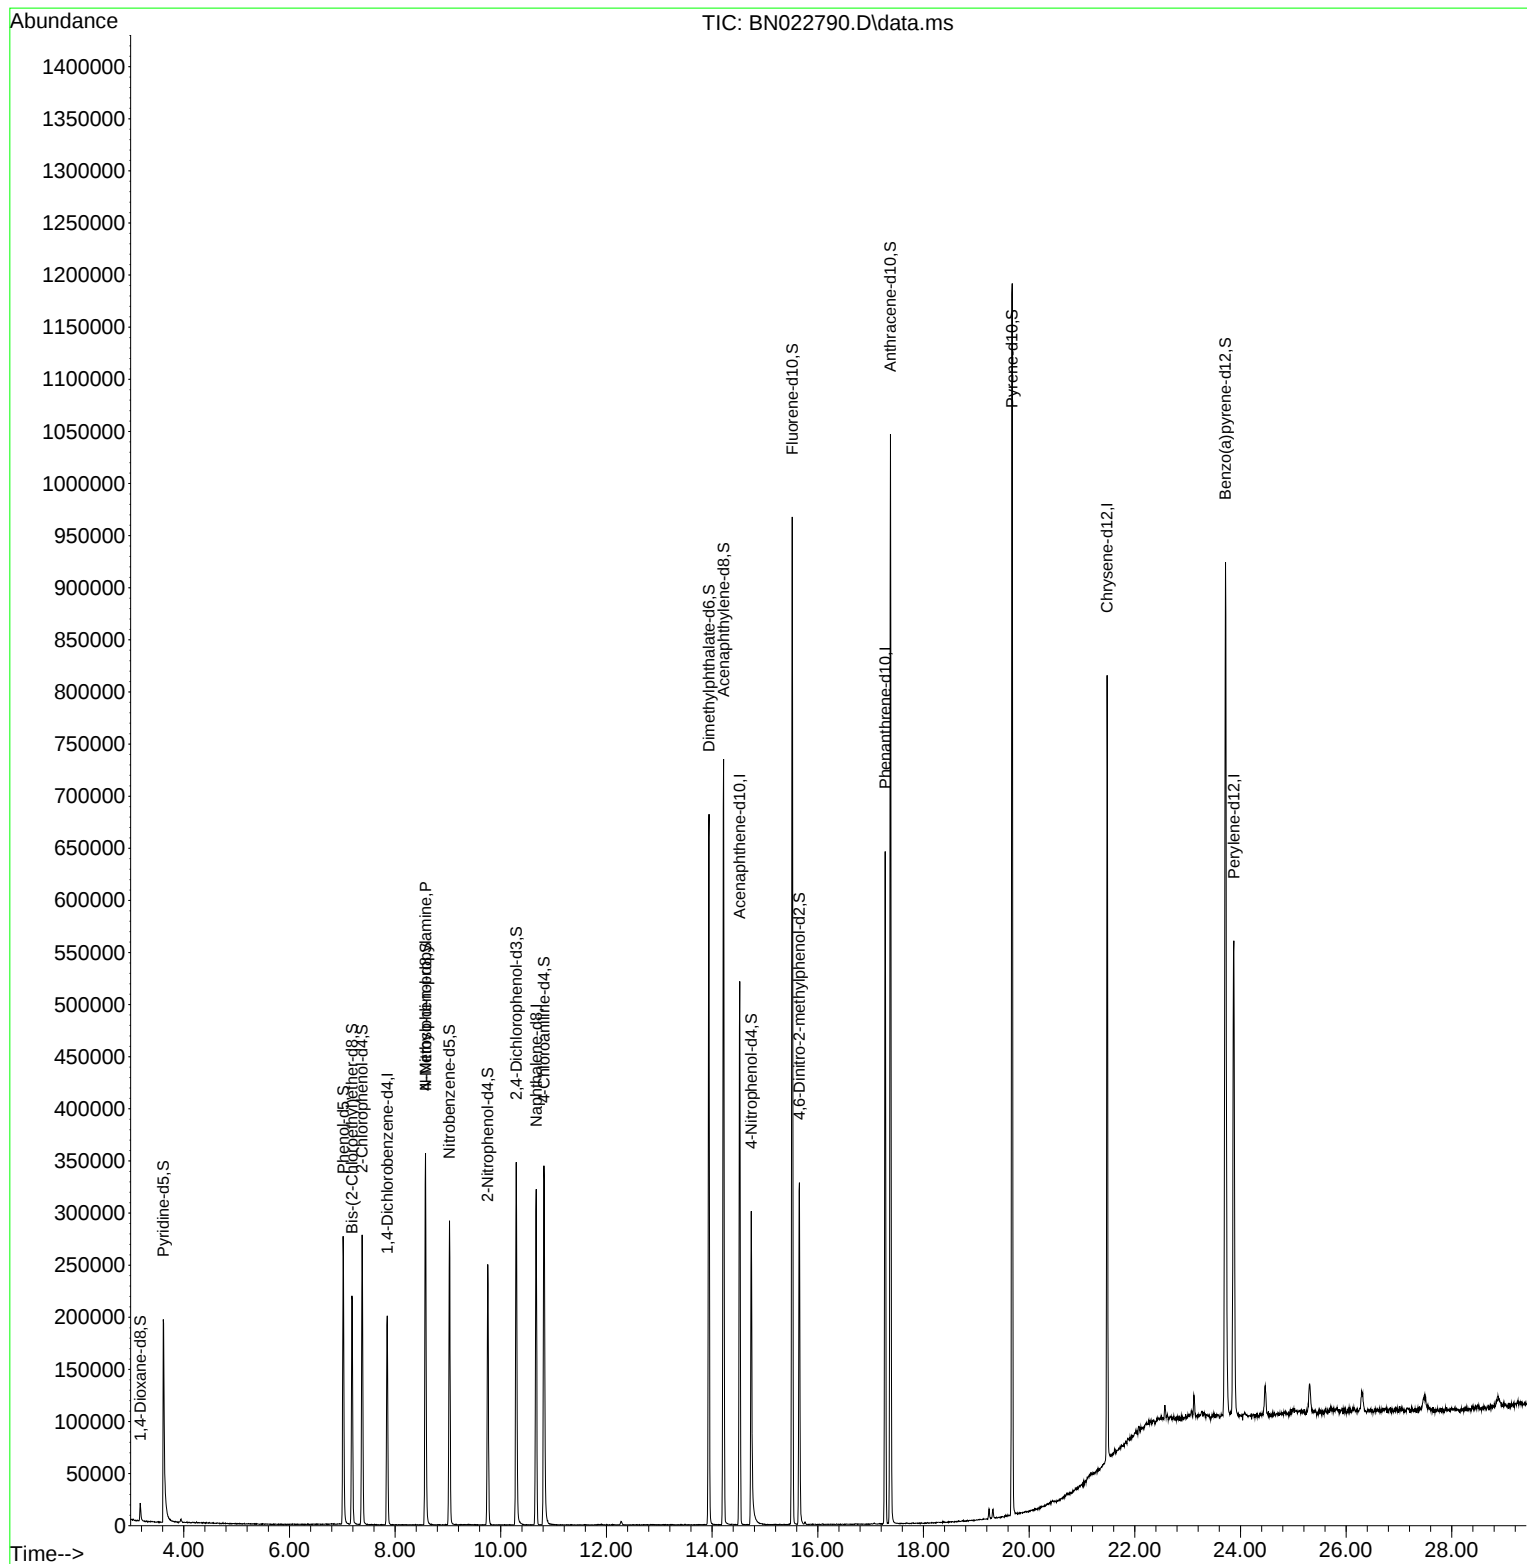

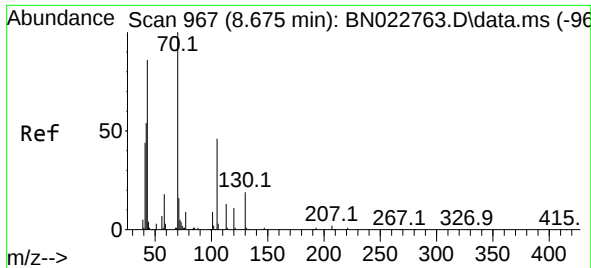

#17
N-Nitroso-di-n-propylamine
Concen: 1.087 ng/ul
RT: 8.575 min Scan# 91
Delta R.T. -0.100 min
Lab File: BN022790.D
Acq: 21 Nov 2022 16:59

Instrument :
BNA_N
ClientSampleId :
SBLK195

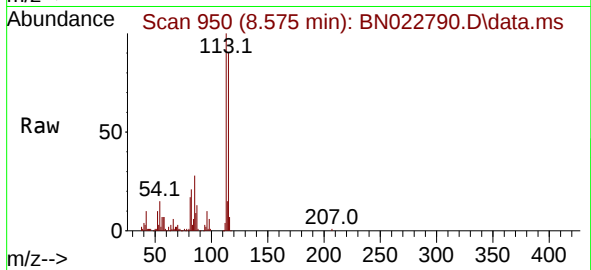

Tgt Ion:	70	Resp:	3507
Ion	Ratio	Lower	Upper
70	100		
42	309.0	43.4	65.2#
101	0.0	8.0	12.0#
130	0.0	16.2	24.4#

