

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112122\
 Data File : BN022830.D
 Acq On : 22 Nov 2022 18:29
 Operator : CG/JU
 Sample : PB149044BL
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK044

Quant Time: Nov 22 21:53:31 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 22 05:15:51 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.846	152	50395	20.000	ng/ul	0.00
20) Naphthalene-d8	10.663	136	243007	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.516	164	161841	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.269	188	330539	20.000	ng/ul	0.00
79) Chrysene-d12	21.475	240	315333	20.000	ng/ul	0.00
88) Perylene-d12	23.863	264	313232	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.176	96	9911	6.714	ng/uL	0.00
4) Pyridine-d5	3.611	84	128532	30.791	ng/ul	0.00
7) Phenol-d5	7.011	99	164983	34.663	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.181	67	110554	38.739	ng/ul	0.00
11) 2-Chlorophenol-d4	7.369	132	125450	35.990	ng/ul	0.00
15) 4-Methylphenol-d8	8.569	113	136641	36.364	ng/ul	0.00
21) Nitrobenzene-d5	9.028	128	66574	35.393	ng/ul	0.00
24) 2-Nitrophenol-d4	9.752	143	73515	35.027	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.287	165	119563	33.416	ng/ul	0.00
31) 4-Chloroaniline-d4	10.816	131	189641	34.796	ng/ul	0.00
46) Dimethylphthalate-d6	13.934	166	433184	36.799	ng/ul	0.00
49) Acenaphthylene-d8	14.210	160	467142	36.016	ng/ul	0.00
54) 4-Nitrophenol-d4	14.734	143	73698	31.405	ng/ul	0.00
60) Fluorene-d10	15.516	176	356504	36.926	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.645	200	58974	28.070	ng/ul	0.00
73) Anthracene-d10	17.369	188	556538	38.452	ng/ul	0.00
81) Pyrene-d10	19.675	212	606602	37.120	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.710	264	594088	37.730	ng/ul	0.00


Target Compounds					Qvalue
17) N-Nitroso-di-n-propyla...	8.569	70	3681	1.152 ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112122\
Data File : BN022830.D
Acq On : 22 Nov 2022 18:29
Operator : CG/JU
Sample : PB149044BL
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK044

Quant Time: Nov 22 21:53:31 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN11522.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 22 05:15:51 2022
Response via : Initial Calibration

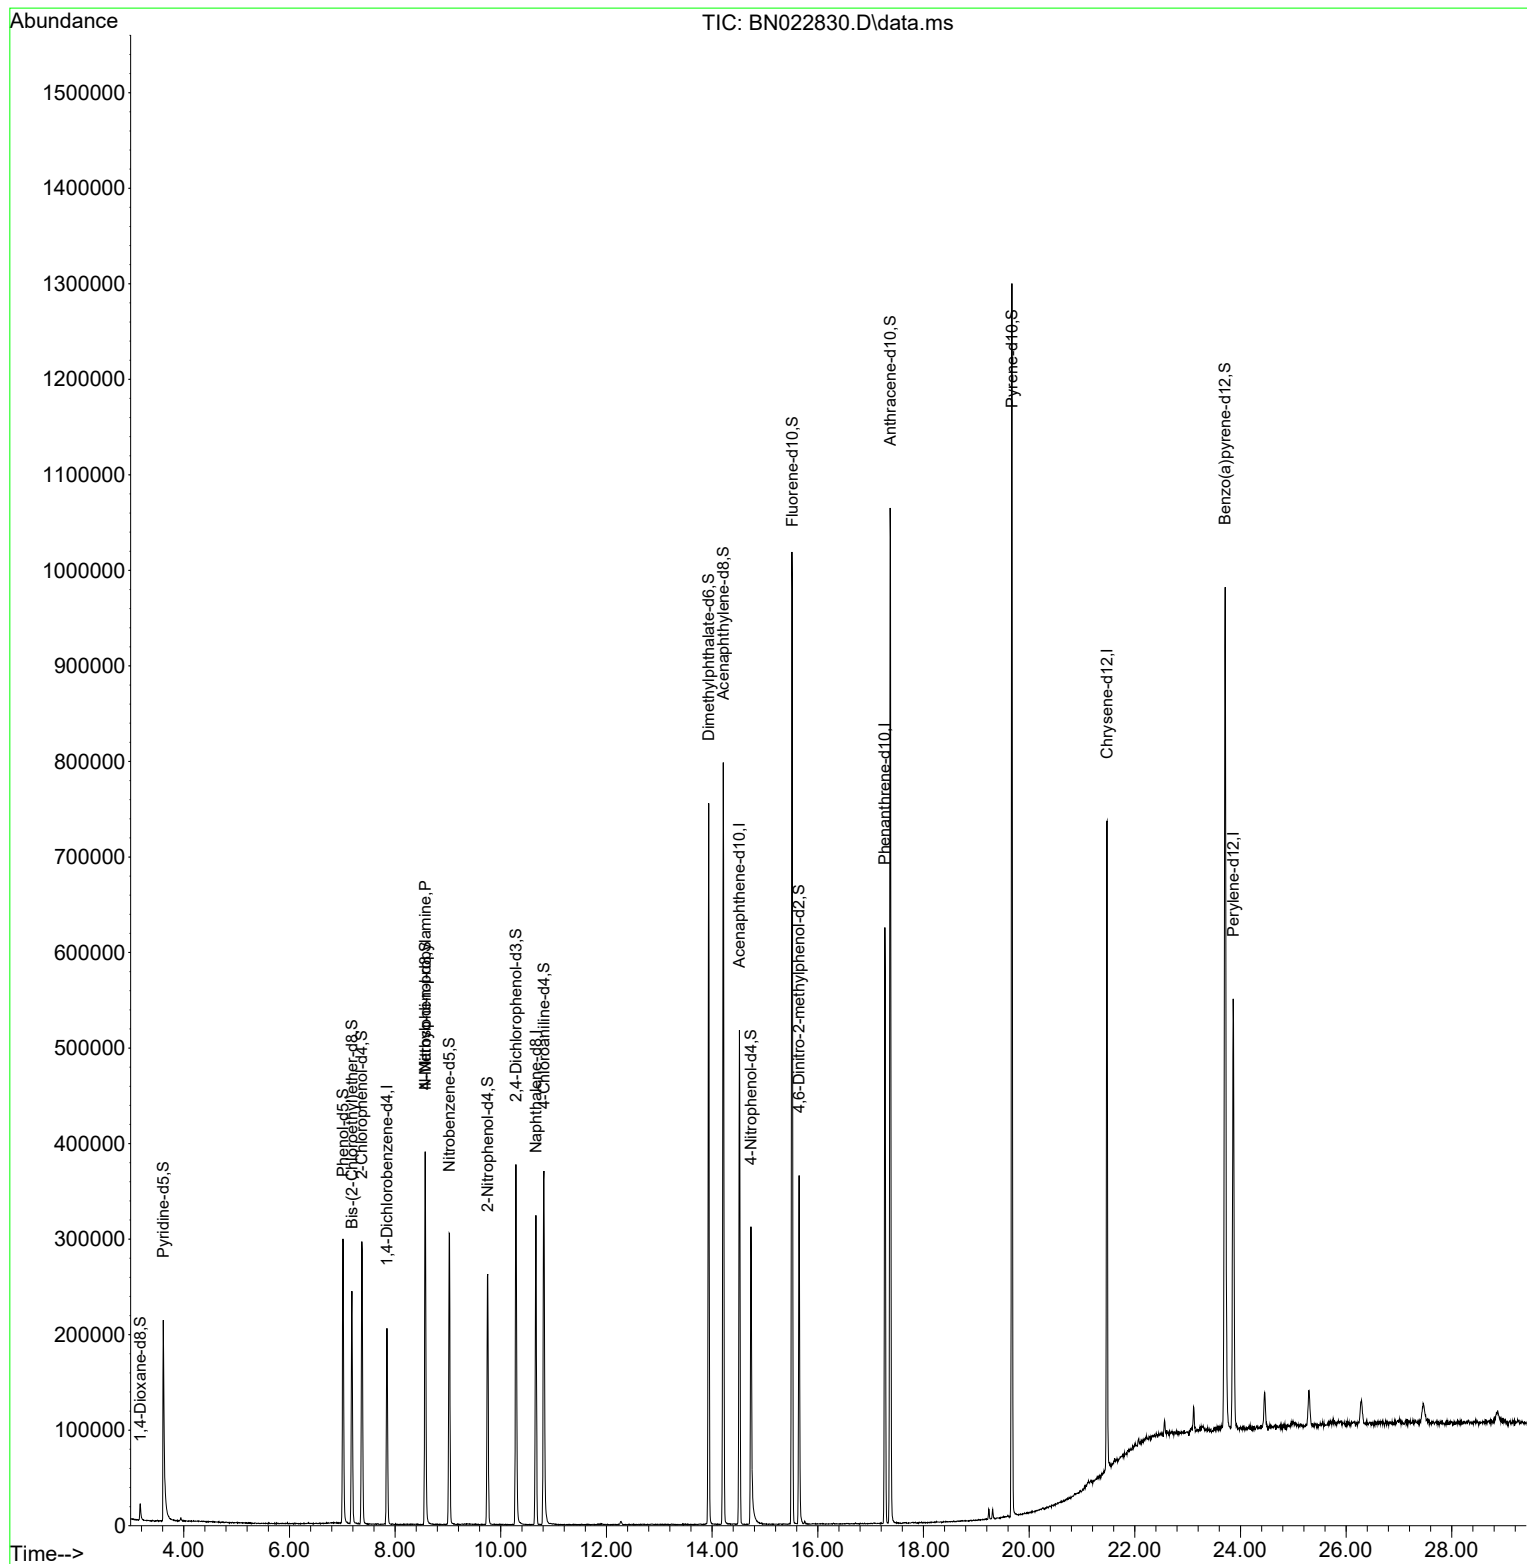

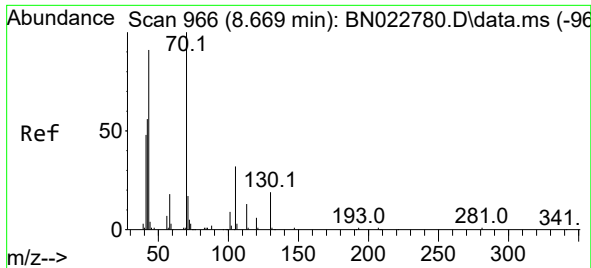

#17
 N-Nitroso-di-n-propylamine
 Concen: 1.152 ng/ul
 RT: 8.569 min Scan# 949
 Delta R.T. -0.100 min
 Lab File: BN022830.D
 Acq: 22 Nov 2022 18:29

Instrument :
 BNA_N
 ClientSampleId :
 SBLK044

Tgt Ion: 70 Resp: 3681
 Ion Ratio Lower Upper
 70 100
 42 385.7 43.4 65.2#
 101 0.0 8.0 12.0#
 130 0.0 16.2 24.4#

