

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112122\
 Data File : BN022832.D
 Acq On : 22 Nov 2022 19:44
 Operator : CG/JU
 Sample : PB149040BL
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK040

Quant Time: Nov 22 21:54:08 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 22 05:15:51 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.846	152	69666	20.000	ng/ul	0.00
20) Naphthalene-d8	10.663	136	334080	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.516	164	220871	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.269	188	443185	20.000	ng/ul	0.00
79) Chrysene-d12	21.474	240	434052	20.000	ng/ul	0.00
88) Perylene-d12	23.868	264	410219	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.175	96	11770	5.768	ng/uL	0.00
4) Pyridine-d5	3.611	84	149244	25.863	ng/ul	0.00
7) Phenol-d5	7.011	99	195380	29.694	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.181	67	128932	32.682	ng/ul	0.00
11) 2-Chlorophenol-d4	7.369	132	143506	29.781	ng/ul	0.00
15) 4-Methylphenol-d8	8.569	113	158795	30.570	ng/ul	0.00
21) Nitrobenzene-d5	9.028	128	78215	30.247	ng/ul	0.00
24) 2-Nitrophenol-d4	9.752	143	87573	30.351	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.287	165	142512	28.972	ng/ul	0.00
31) 4-Chloroaniline-d4	10.816	131	225430	30.087	ng/ul	0.00
46) Dimethylphthalate-d6	13.934	166	523875	32.609	ng/ul	0.00
49) Acenaphthylene-d8	14.210	160	559631	31.615	ng/ul	0.00
54) 4-Nitrophenol-d4	14.734	143	87272	27.250	ng/ul	0.00
60) Fluorene-d10	15.510	176	425910	32.324	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.645	200	72282	25.659	ng/ul	0.00
73) Anthracene-d10	17.369	188	661445	34.084	ng/ul	0.00
81) Pyrene-d10	19.675	212	738272	32.821	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.710	264	695334	33.719	ng/ul	0.00


Target Compounds					Qvalue
17) N-Nitroso-di-n-propyla...	8.563	70	4491	1.016 ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112122\
Data File : BN022832.D
Acq On : 22 Nov 2022 19:44
Operator : CG/JU
Sample : PB149040BL
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK040

Quant Time: Nov 22 21:54:08 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN11522.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 22 05:15:51 2022
Response via : Initial Calibration

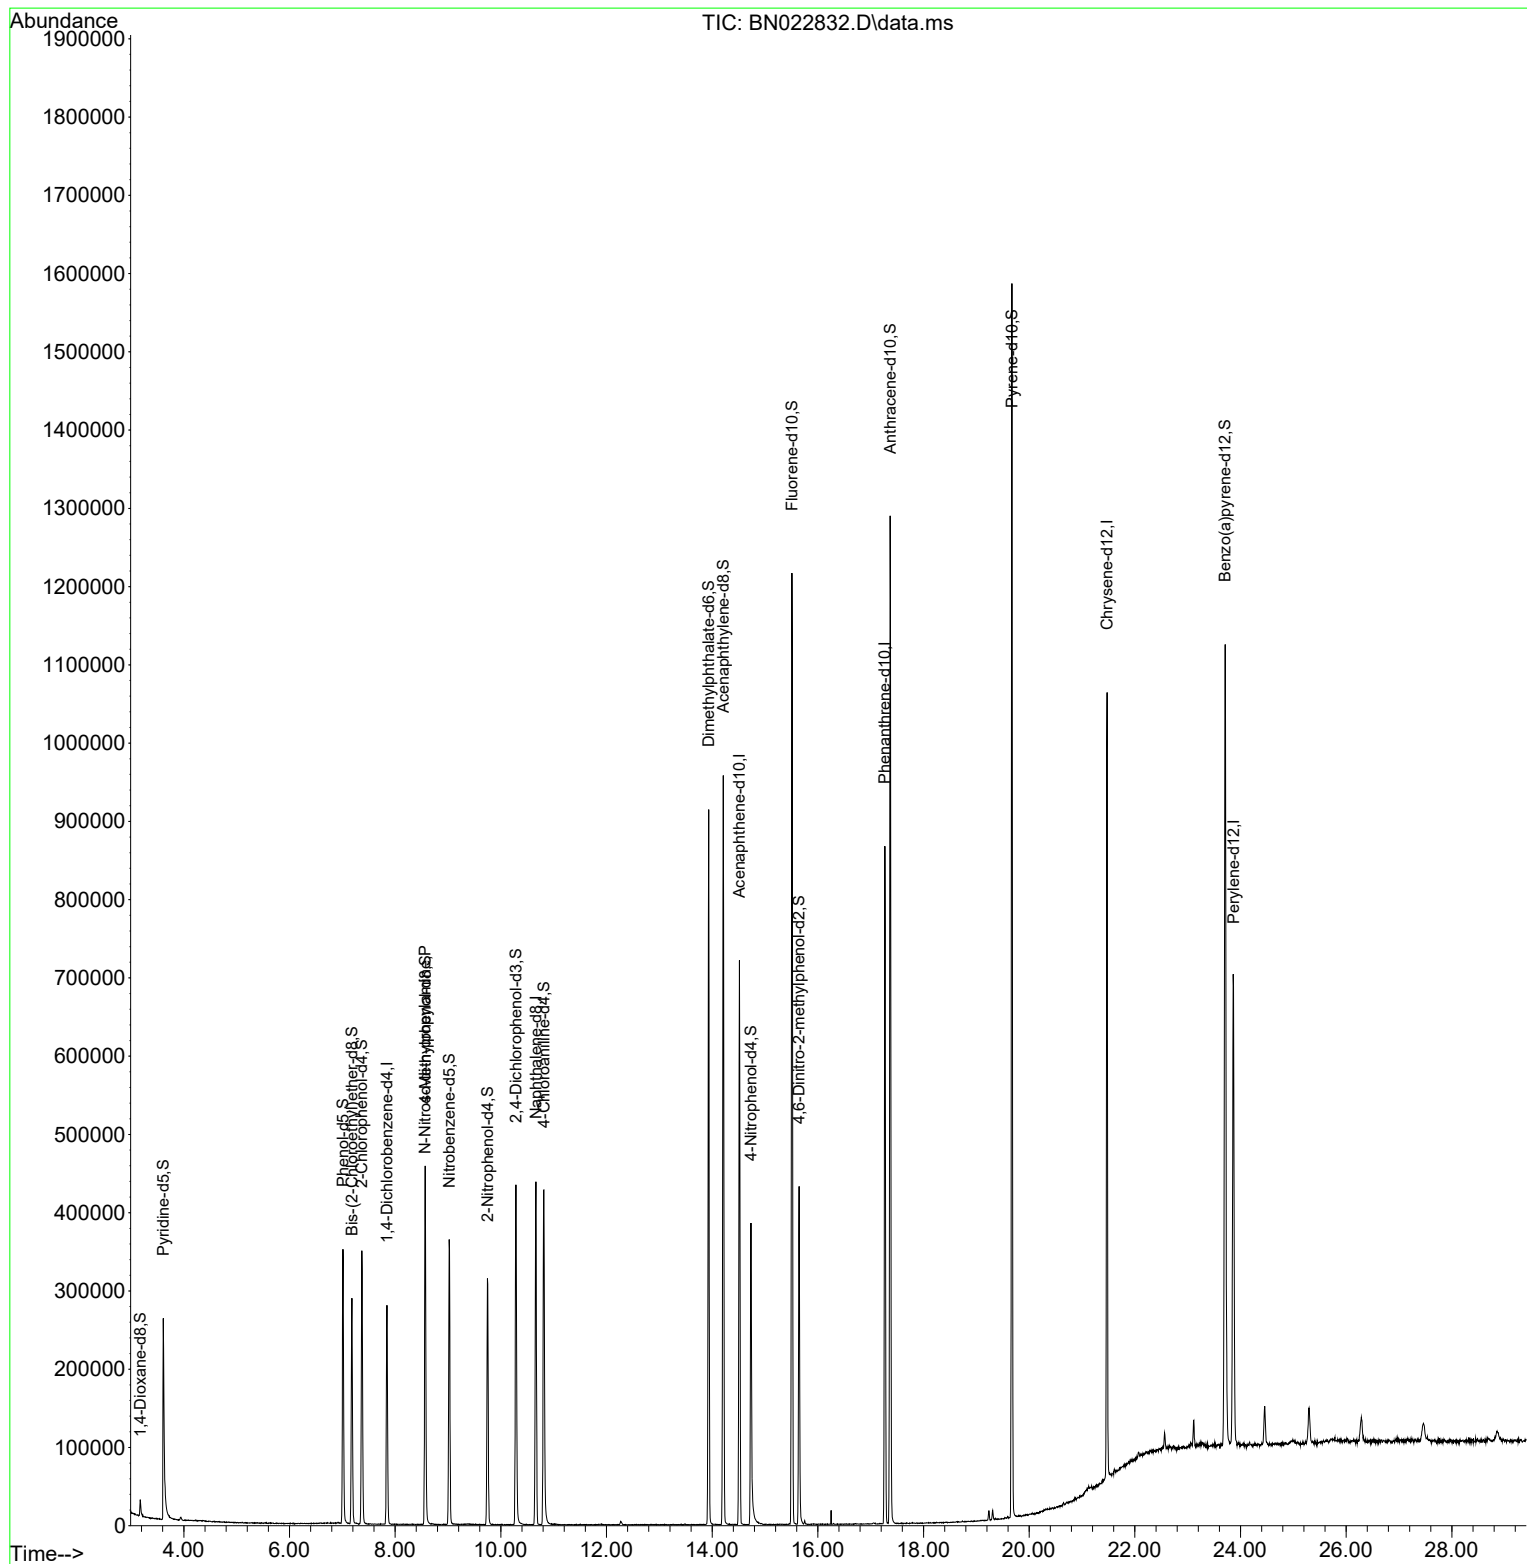

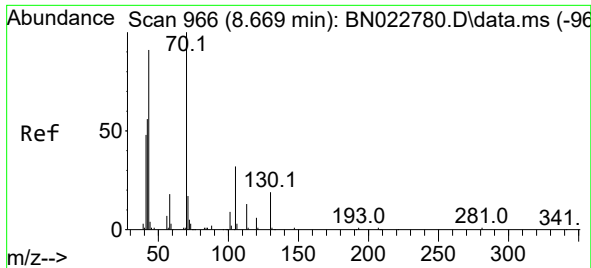

#17
 N-Nitroso-di-n-propylamine
 Concen: 1.016 ng/ul
 RT: 8.563 min Scan# 94
 Delta R.T. -0.106 min
 Lab File: BN022832.D
 Acq: 22 Nov 2022 19:44

Instrument :
 BNA_N
 ClientSampleId :
 SBLK040

Tgt Ion: 70 Resp: 4491
 Ion Ratio Lower Upper
 70 100
 42 349.0 43.4 65.2#
 101 0.0 8.0 12.0#
 130 0.0 16.2 24.4#

