

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112122\
 Data File : BN022833.D
 Acq On : 22 Nov 2022 20:21
 Operator : CG/JU
 Sample : N5593-10
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 H0AD9

Quant Time: Nov 22 21:54:16 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 22 05:15:51 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.846	152	60962	20.000	ng/u1	0.00
20) Naphthalene-d8	10.663	136	285057	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.516	164	183674	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.269	188	395375	20.000	ng/u1	0.00
79) Chrysene-d12	21.469	240	376646	20.000	ng/u1	0.00
88) Perylene-d12	23.863	264	367212	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.175	96	7660	4.290	ng/uL	0.00
4) Pyridine-d5	3.617	84	62856	12.448	ng/u1	0.00
7) Phenol-d5	7.016	99	53412	9.277	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.181	67	146162	42.339	ng/u1	0.00
11) 2-Chlorophenol-d4	7.369	132	133128	31.572	ng/u1	0.00
15) 4-Methylphenol-d8	8.569	113	98463	21.662	ng/u1	0.00
21) Nitrobenzene-d5	9.022	128	87900	39.838	ng/u1	0.00
24) 2-Nitrophenol-d4	9.746	143	94024	38.190	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.287	165	151379	36.067	ng/u1	0.00
31) 4-Chloroaniline-d4	10.816	131	204053	31.917	ng/u1	0.00
46) Dimethylphthalate-d6	13.934	166	571673	42.791	ng/u1	0.00
49) Acenaphthylene-d8	14.210	160	623472	42.355	ng/u1	0.00
54) 4-Nitrophenol-d4	14.740	143	21956	8.244	ng/u1	0.00
60) Fluorene-d10	15.510	176	474882	43.340	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.645	200	90549	36.031	ng/u1	0.00
73) Anthracene-d10	17.369	188	767589	44.337	ng/u1	0.00
81) Pyrene-d10	19.675	212	901219	46.171	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.710	264	887745	48.092	ng/u1	0.00


Target Compounds					Qvalue
2) 1,4-Dioxane	3.217	88	7826	4.119 ng/uL#	87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112122\
Data File : BN022833.D
Acq On : 22 Nov 2022 20:21
Operator : CG/JU
Sample : N5593-10
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
H0AD9


Quant Time: Nov 22 21:54:16 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN11522.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 22 05:15:51 2022
Response via : Initial Calibration

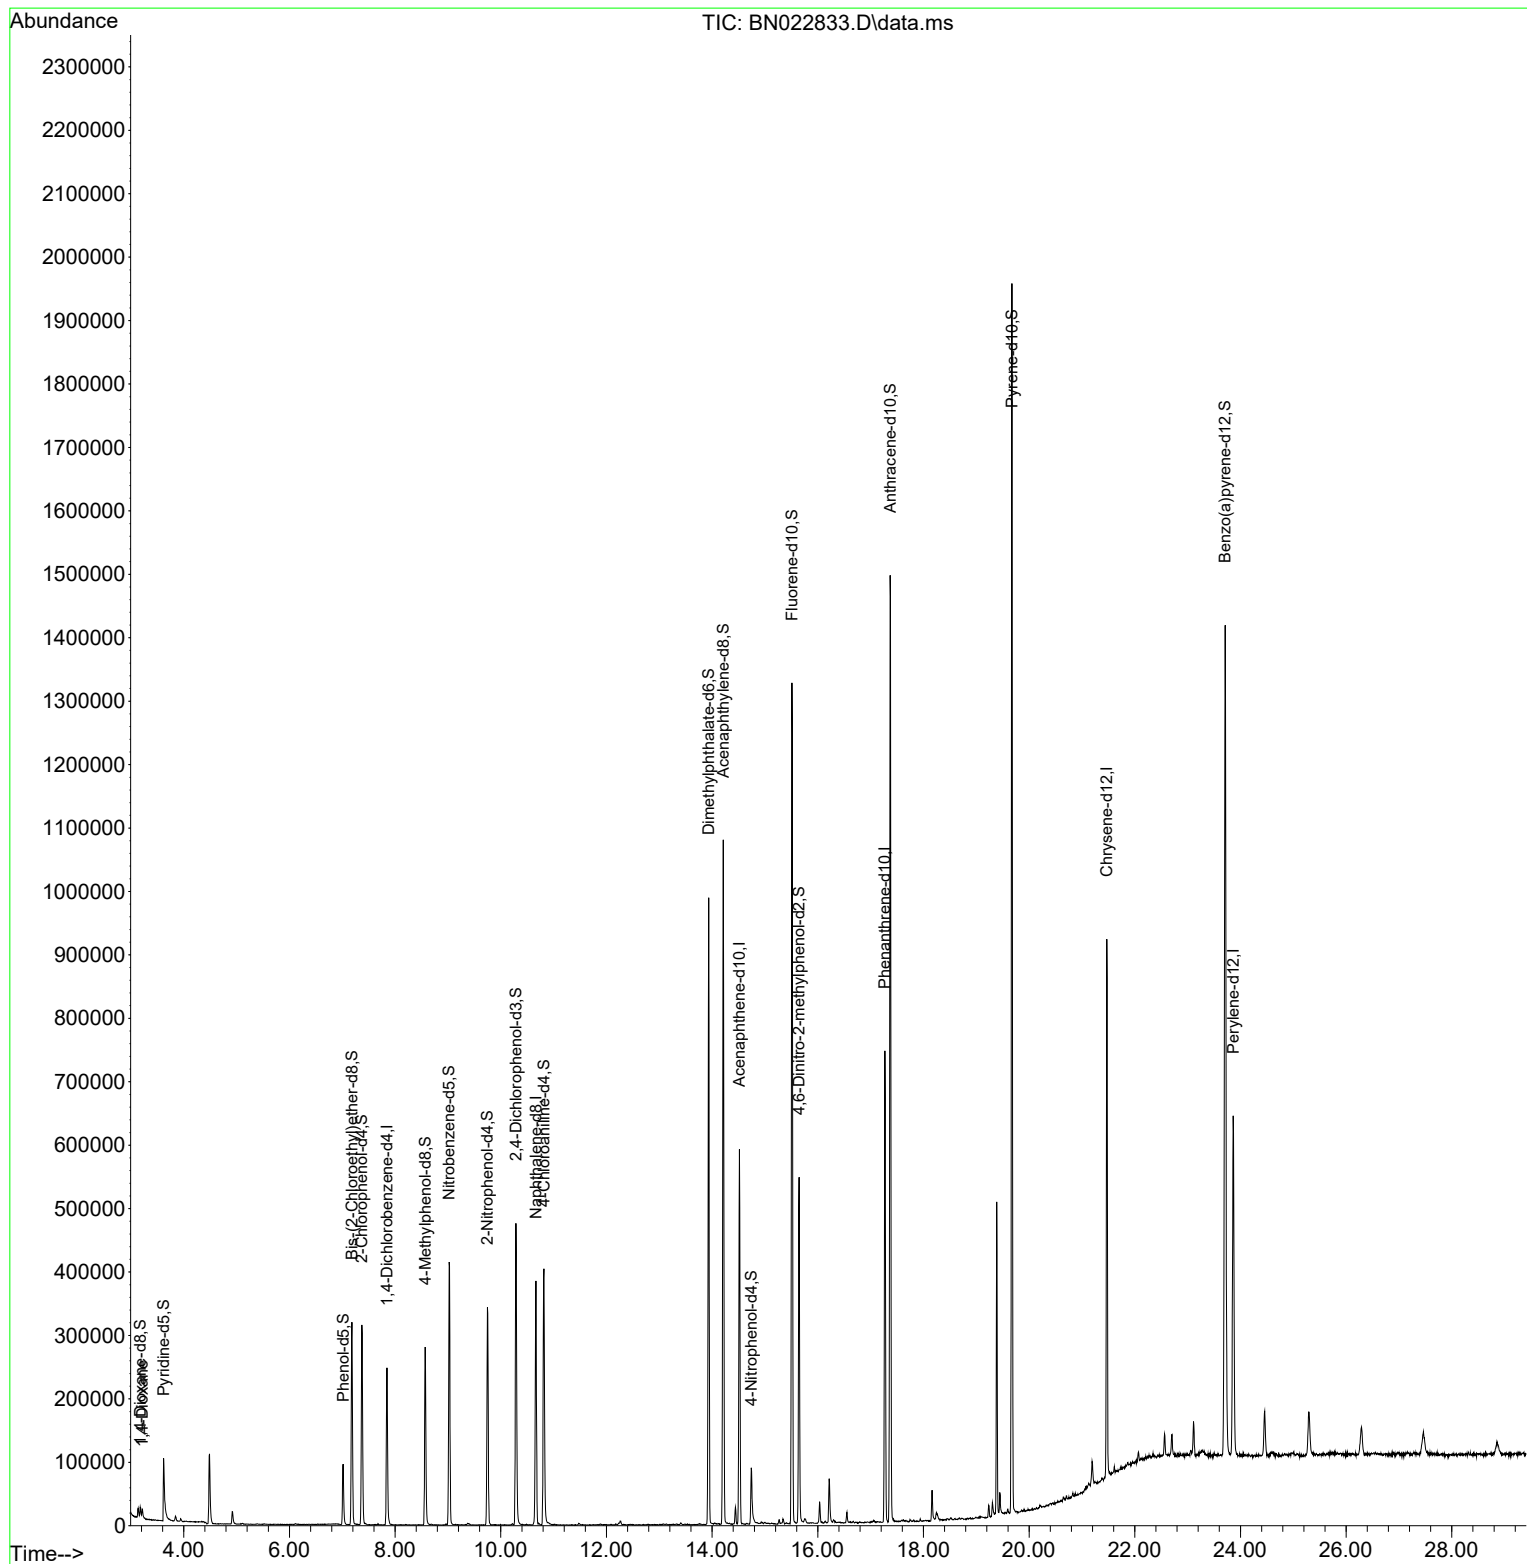

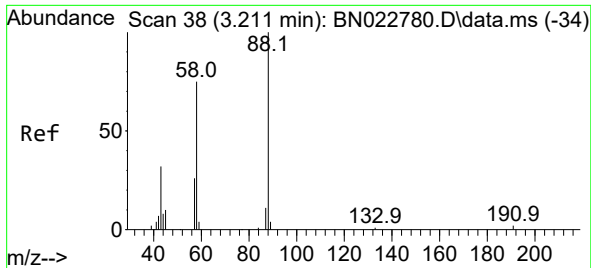

#2
 1,4-Dioxane
 Concen: 4.119 ng/uL
 RT: 3.217 min Scan# 39
 Delta R.T. 0.006 min
 Lab File: BN022833.D
 Acq: 22 Nov 2022 20:21

Instrument :
 BNA_N
 ClientSampleId :
 H0AD9

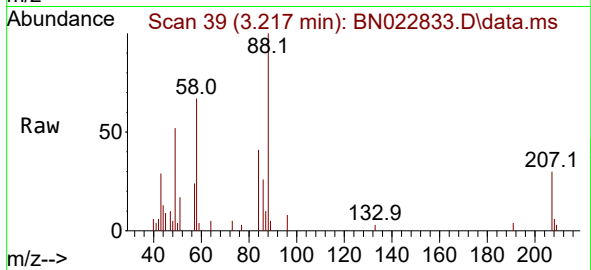

Tgt Ion: 88 Resp: 7826
 Ion Ratio Lower Upper
 88 100
 43 29.1 30.8 46.2#
 58 67.0 61.7 92.5

