




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112122\
Data File : BN022801.D
Acq On : 21 Nov 2022 23:45
Operator : CG/JU
Sample : N5690-04
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGCE8

Manual IntegrationsAPPROVED

Quant Time: Nov 22 00:15:43 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN11522.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Nov 19 05:51:00 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/22/2022
Supervised By :mohammad ahmed 11/25/2022

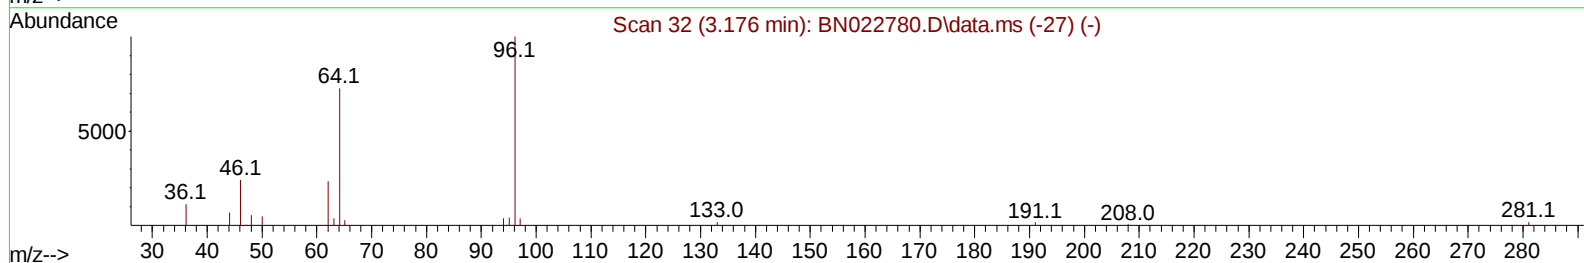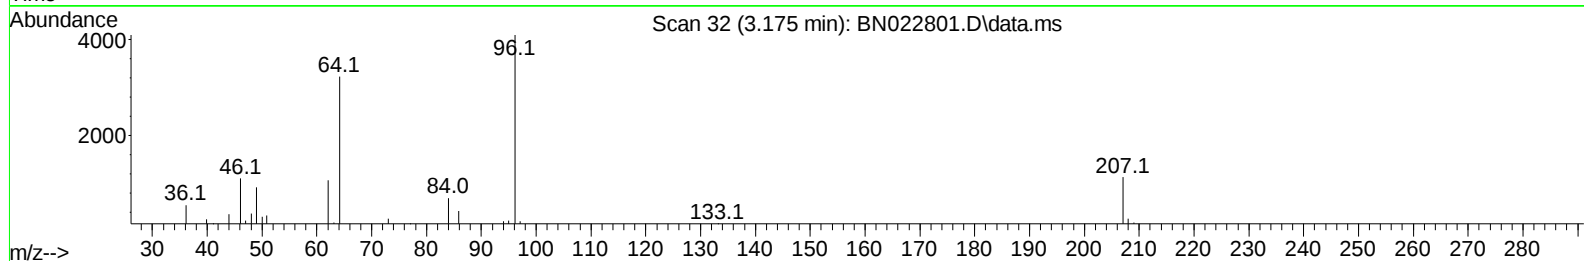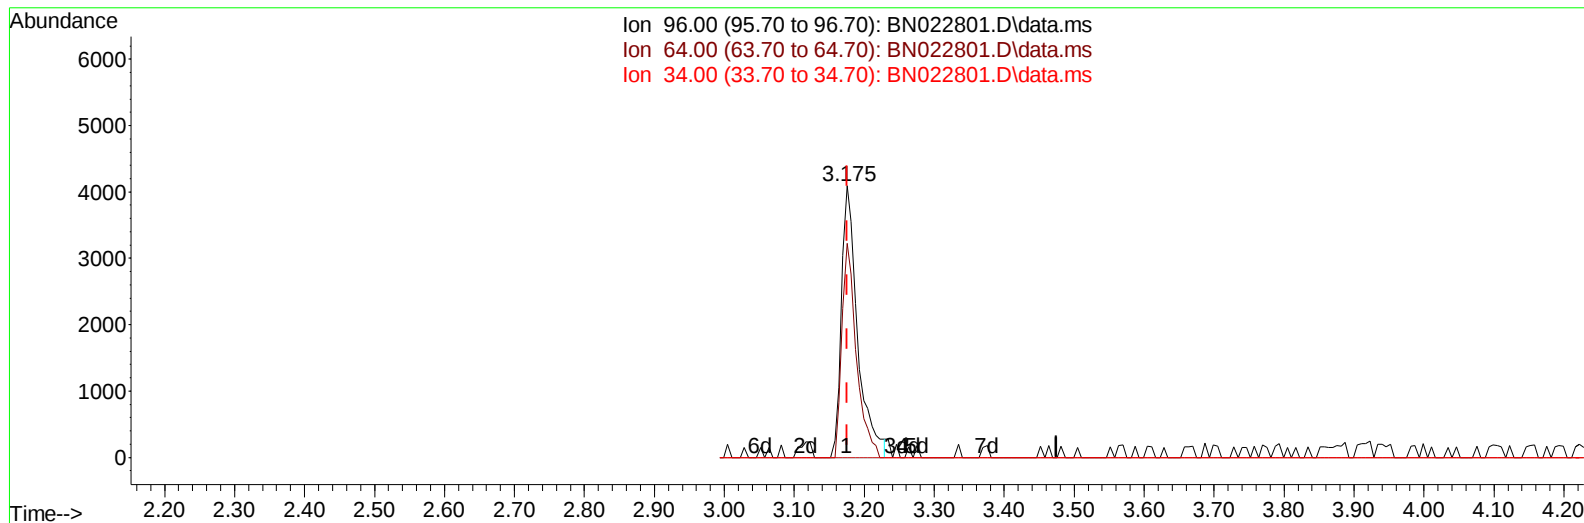

TIC: BN022801.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.175min (-0.000) 4.09 ng/uL

response 6557

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	77.50	78.78
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112122\
 Data File : BN022801.D
 Acq On : 21 Nov 2022 23:45
 Operator : CG/JU
 Sample : N5690-04
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BGCE8

Manual IntegrationsAPPROVED

Quant Time: Nov 22 00:15:43 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN11522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Nov 19 05:51:00 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/22/2022
 Supervised By :mohammad ahmed 11/25/2022

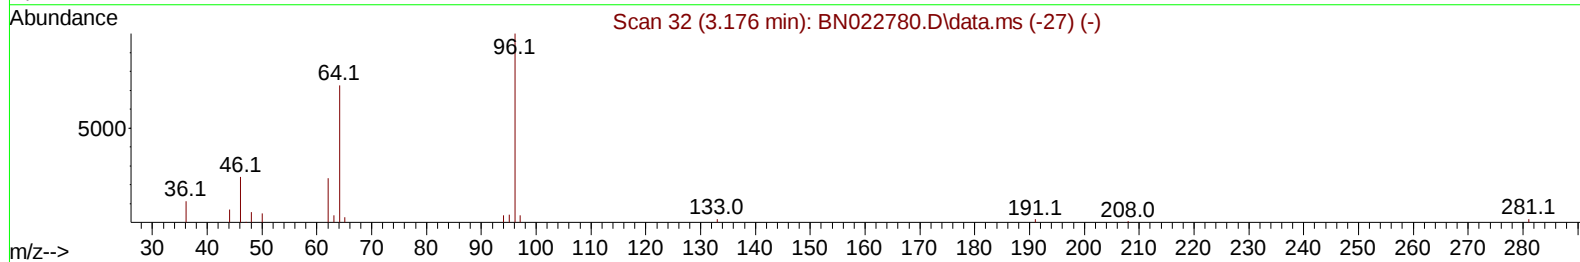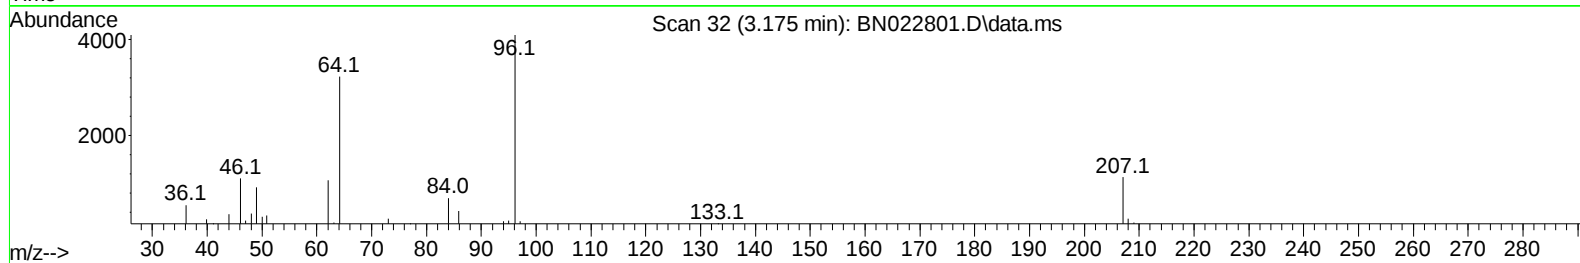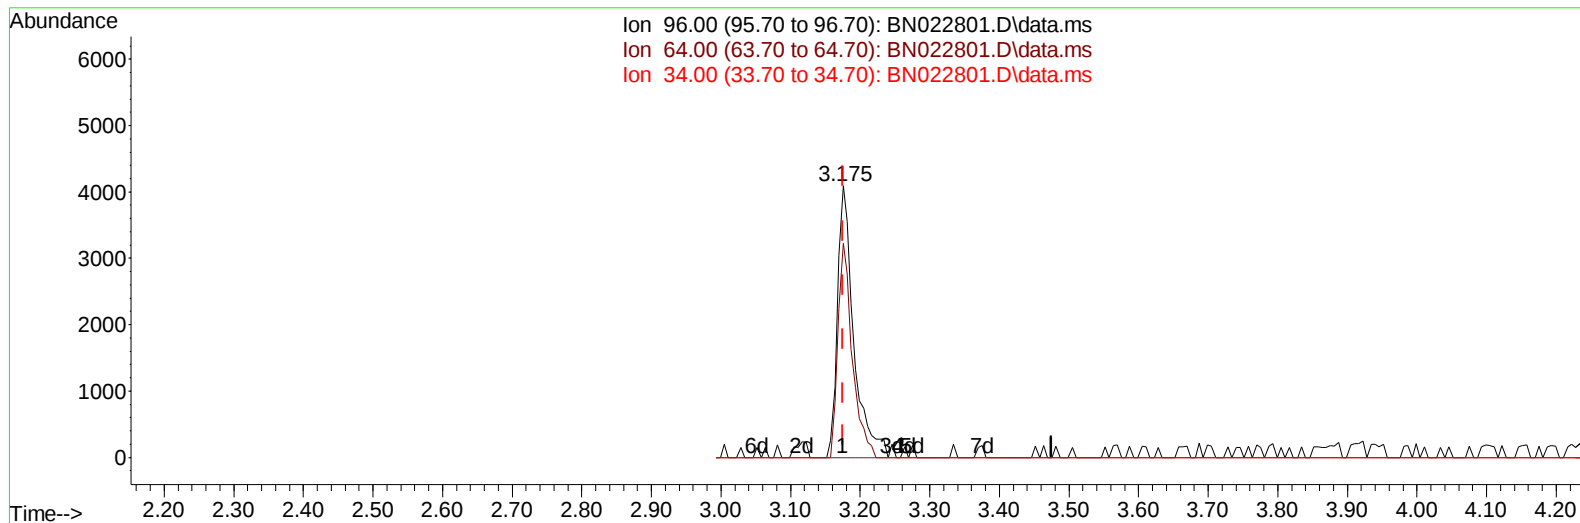

TIC: BN022801.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.175min (-0.000) 4.14 ng/uL m

response 6652

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	77.50	78.78
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112122\
 Data File : BN022801.D
 Acq On : 21 Nov 2022 23:45
 Operator : CG/JU
 Sample : N5690-04
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BGCE8

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 11/22/2022
 Supervised By :mohammad ahmed 11/25/2022

Quant Time: Nov 22 00:15:43 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN11522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Nov 19 05:51:00 2022
 Response via : Initial Calibration

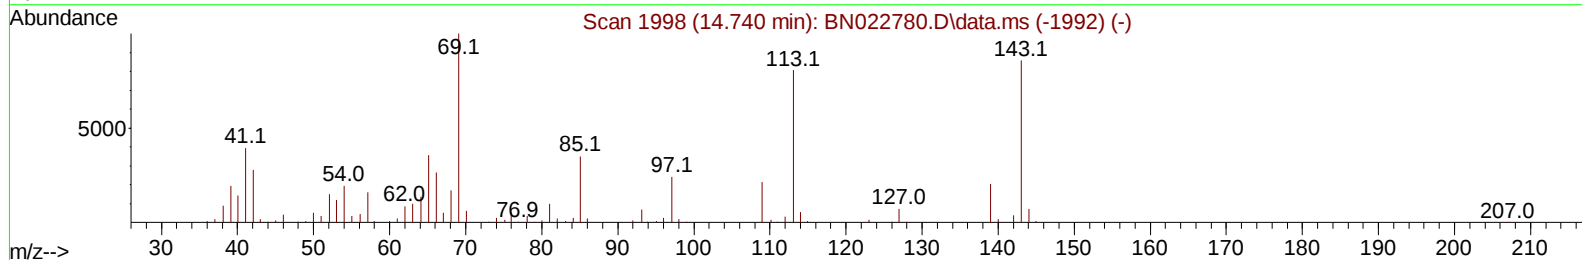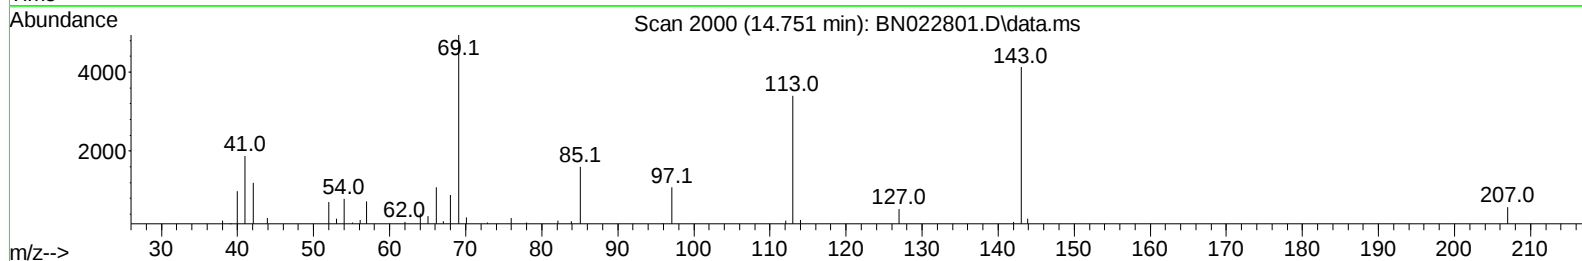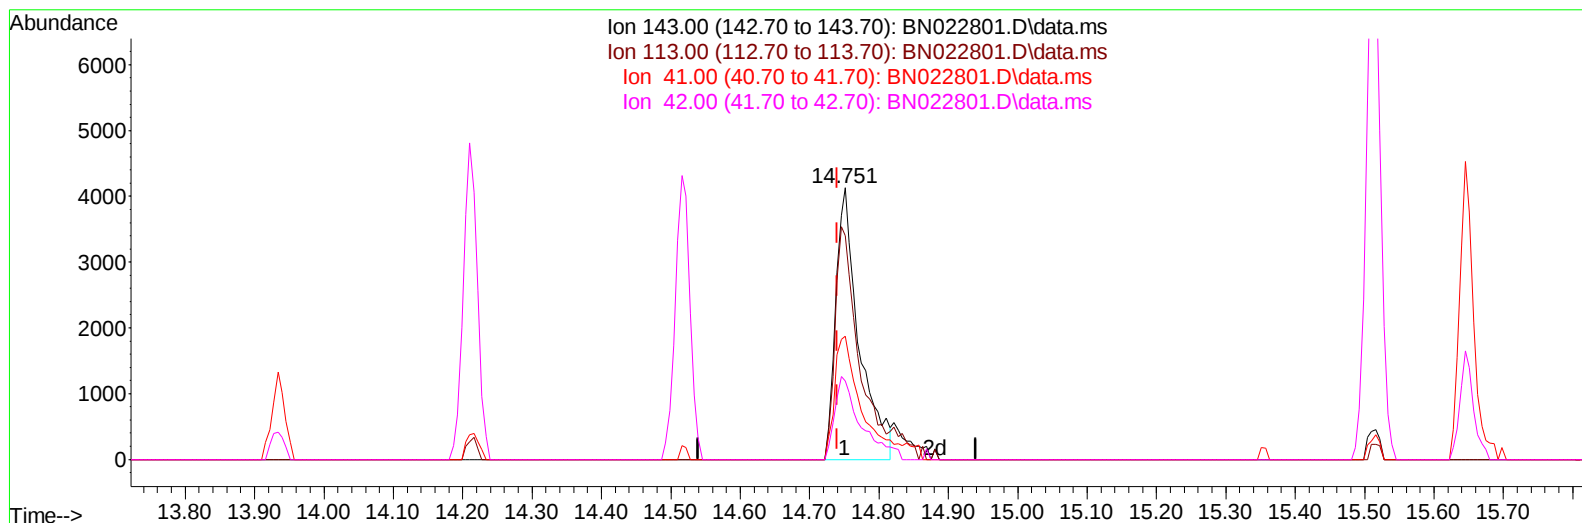

TIC: BN022801.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.751min (+ 0.012) 3.86 ng/u1

response 9636

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	95.00	82.41
41.00	46.30	45.49
42.00	31.30	28.90




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112122\
Data File : BN022801.D
Acq On : 21 Nov 2022 23:45
Operator : CG/JU
Sample : N5690-04
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGCE8

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 11/22/2022
Supervised By :mohammad ahmed 11/25/2022

Quant Time: Nov 22 00:15:43 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN11522.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Nov 19 05:51:00 2022
Response via : Initial Calibration

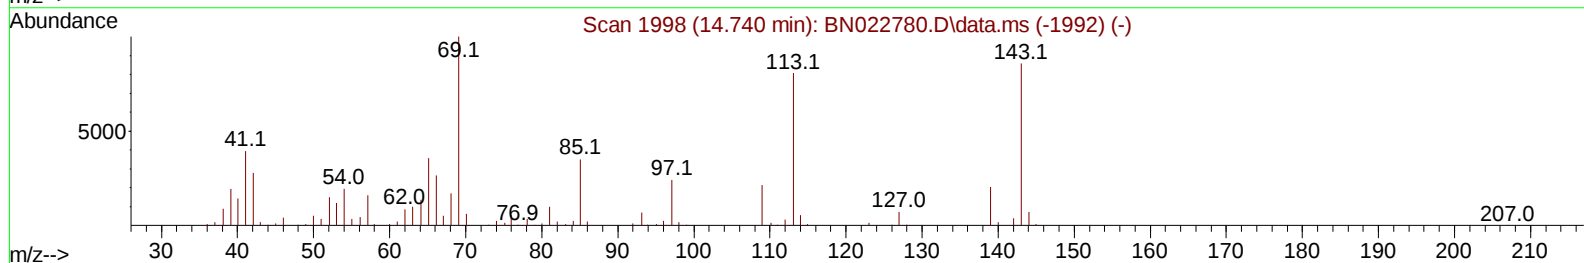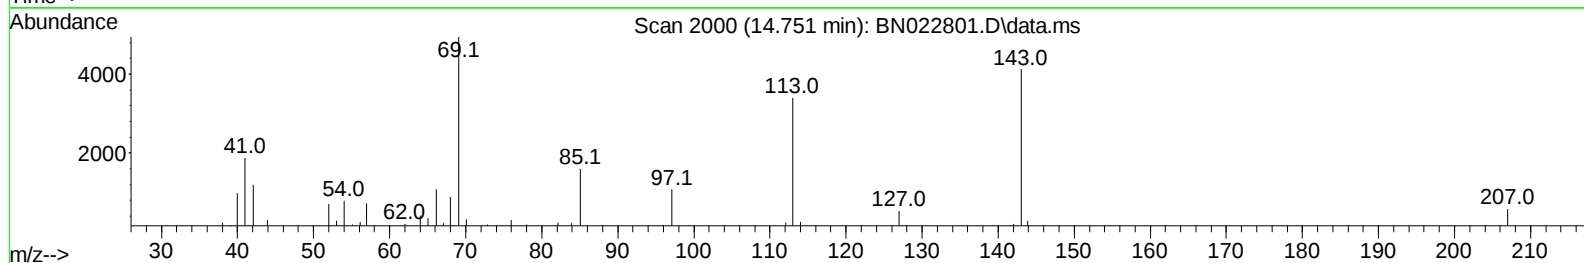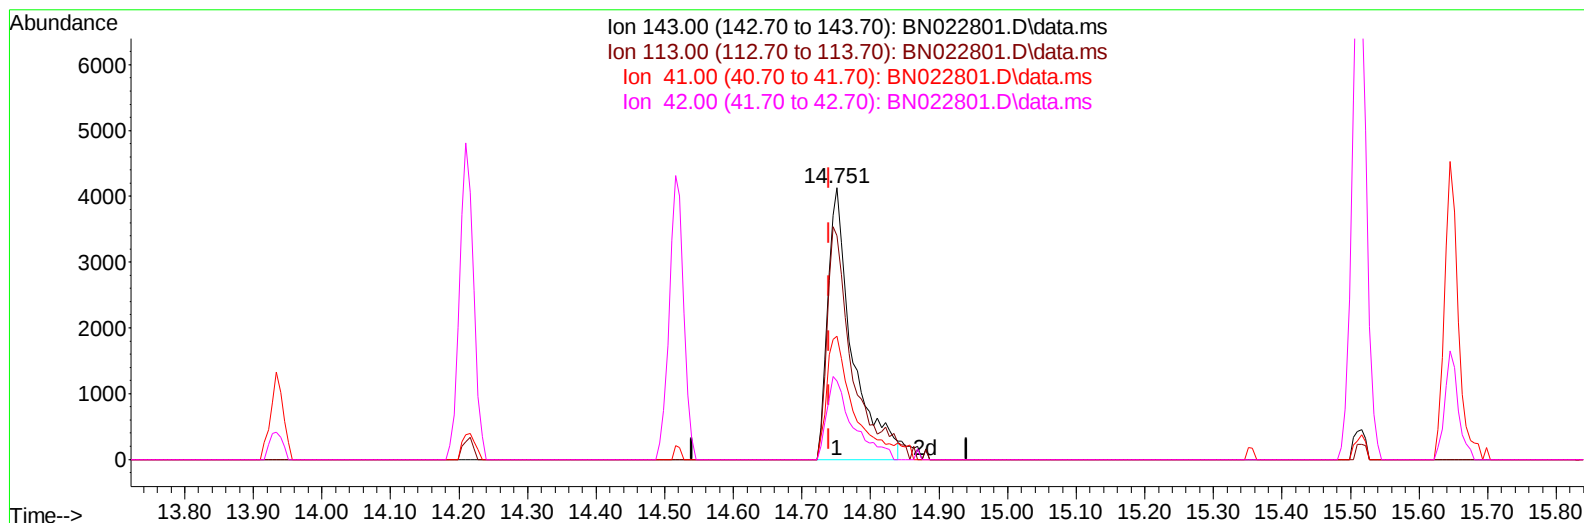

TIC: BN022801.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.751min (+ 0.012) 4.09 ng/ul m

response 10203

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	95.00	82.41
41.00	46.30	45.49
42.00	31.30	28.90

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112122\
 Data File : BN022801.D
 Acq On : 21 Nov 2022 23:45
 Operator : CG/JU
 Sample : N5690-04
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BGCE8

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 11/22/2022
 Supervised By :mohammad ahmed 11/25/2022

Quant Time: Nov 22 00:15:43 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Nov 19 05:51:00 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.846	152	54791	20.000	ng/ul	0.00
20) Naphthalene-d8	10.663	136	259607	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.516	164	172241	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.275	188	357087	20.000	ng/ul	0.00
79) Chrysene-d12	21.474	240	340135	20.000	ng/ul	0.00
88) Perylene-d12	23.868	264	343899	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.175	96	6652m	4.145	ng/uL	0.00
4) Pyridine-d5	3.622	84	27763	6.117	ng/ul	0.01
7) Phenol-d5	7.016	99	28321	5.473	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.181	67	98304	31.683	ng/ul	0.00
11) 2-Chlorophenol-d4	7.375	132	83087	21.924	ng/ul	0.00
15) 4-Methylphenol-d8	8.569	113	56669	13.871	ng/ul	0.00
21) Nitrobenzene-d5	9.028	128	59348	29.534	ng/ul	0.00
24) 2-Nitrophenol-d4	9.752	143	61260	27.322	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.293	165	95226	24.912	ng/ul	0.00
31) 4-Chloroaniline-d4	10.816	131	133806	22.981	ng/ul	0.00
46) Dimethylphthalate-d6	13.934	166	429367	34.272	ng/ul	0.00
49) Acenaphthylene-d8	14.210	160	444033	32.167	ng/ul	0.00
54) 4-Nitrophenol-d4	14.751	143	10203m	4.085	ng/ul	0.01
60) Fluorene-d10	15.516	176	357072	34.751	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.645	200	58905	25.953	ng/ul	0.00
73) Anthracene-d10	17.375	188	599407	38.335	ng/ul	0.00
81) Pyrene-d10	19.675	212	663414	37.636	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.715	264	636697	36.830	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112122\
Data File : BN022801.D
Acq On : 21 Nov 2022 23:45
Operator : CG/JU
Sample : N5690-04
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGCE8

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 11/22/2022
Supervised By :mohammad ahmed 11/25/2022

Quant Time: Nov 22 00:15:43 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN11522.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Nov 19 05:51:00 2022
Response via : Initial Calibration

