

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112122\
 Data File : BN022784.D
 Acq On : 21 Nov 2022 13:18
 Operator : CG/JU
 Sample : N5713-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BGC74

Quant Time: Nov 21 14:21:16 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Nov 19 05:51:00 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.852	152	68261	20.000	ng/u1	0.00
20) Naphthalene-d8	10.669	136	319787	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.522	164	210955	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.275	188	440275	20.000	ng/u1	0.00
79) Chrysene-d12	21.475	240	439989	20.000	ng/u1	0.00
88) Perylene-d12	23.874	264	448219	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.176	96	7395	3.699	ng/uL	0.00
4) Pyridine-d5	0.000	84	0d	0.000	ng/u1	
7) Phenol-d5	7.017	99	126792	19.667	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.181	67	91393	23.643	ng/u1	0.00
11) 2-Chlorophenol-d4	7.375	132	95821	20.295	ng/u1	0.00
15) 4-Methylphenol-d8	8.575	113	107777	21.175	ng/u1	0.00
21) Nitrobenzene-d5	9.028	128	54209	21.900	ng/u1	0.00
24) 2-Nitrophenol-d4	9.752	143	58108	21.039	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.293	165	91456	19.423	ng/u1	0.00
31) 4-Chloroaniline-d4	10.822	131	49573	6.912	ng/u1	0.00
46) Dimethylphthalate-d6	13.934	166	362531	23.627	ng/u1	0.00
49) Acenaphthylene-d8	14.210	160	352013	20.821	ng/u1	0.00
54) 4-Nitrophenol-d4	14.740	143	56234	18.384	ng/u1	0.00
60) Fluorene-d10	15.516	176	288421	22.919	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.645	200	51429	18.377	ng/u1	0.00
73) Anthracene-d10	17.375	188	438287	22.734	ng/u1	0.00
81) Pyrene-d10	19.675	212	466389	20.454	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.716	264	428075	18.999	ng/u1	0.00
Target Compounds						
					Qvalue	
16) Acetophenone	8.693	105	17378	2.139	ng/u1	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112122\
Data File : BN022784.D
Acq On : 21 Nov 2022 13:18
Operator : CG/JU
Sample : N5713-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGC74


Quant Time: Nov 21 14:21:16 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN11522.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Nov 19 05:51:00 2022
Response via : Initial Calibration

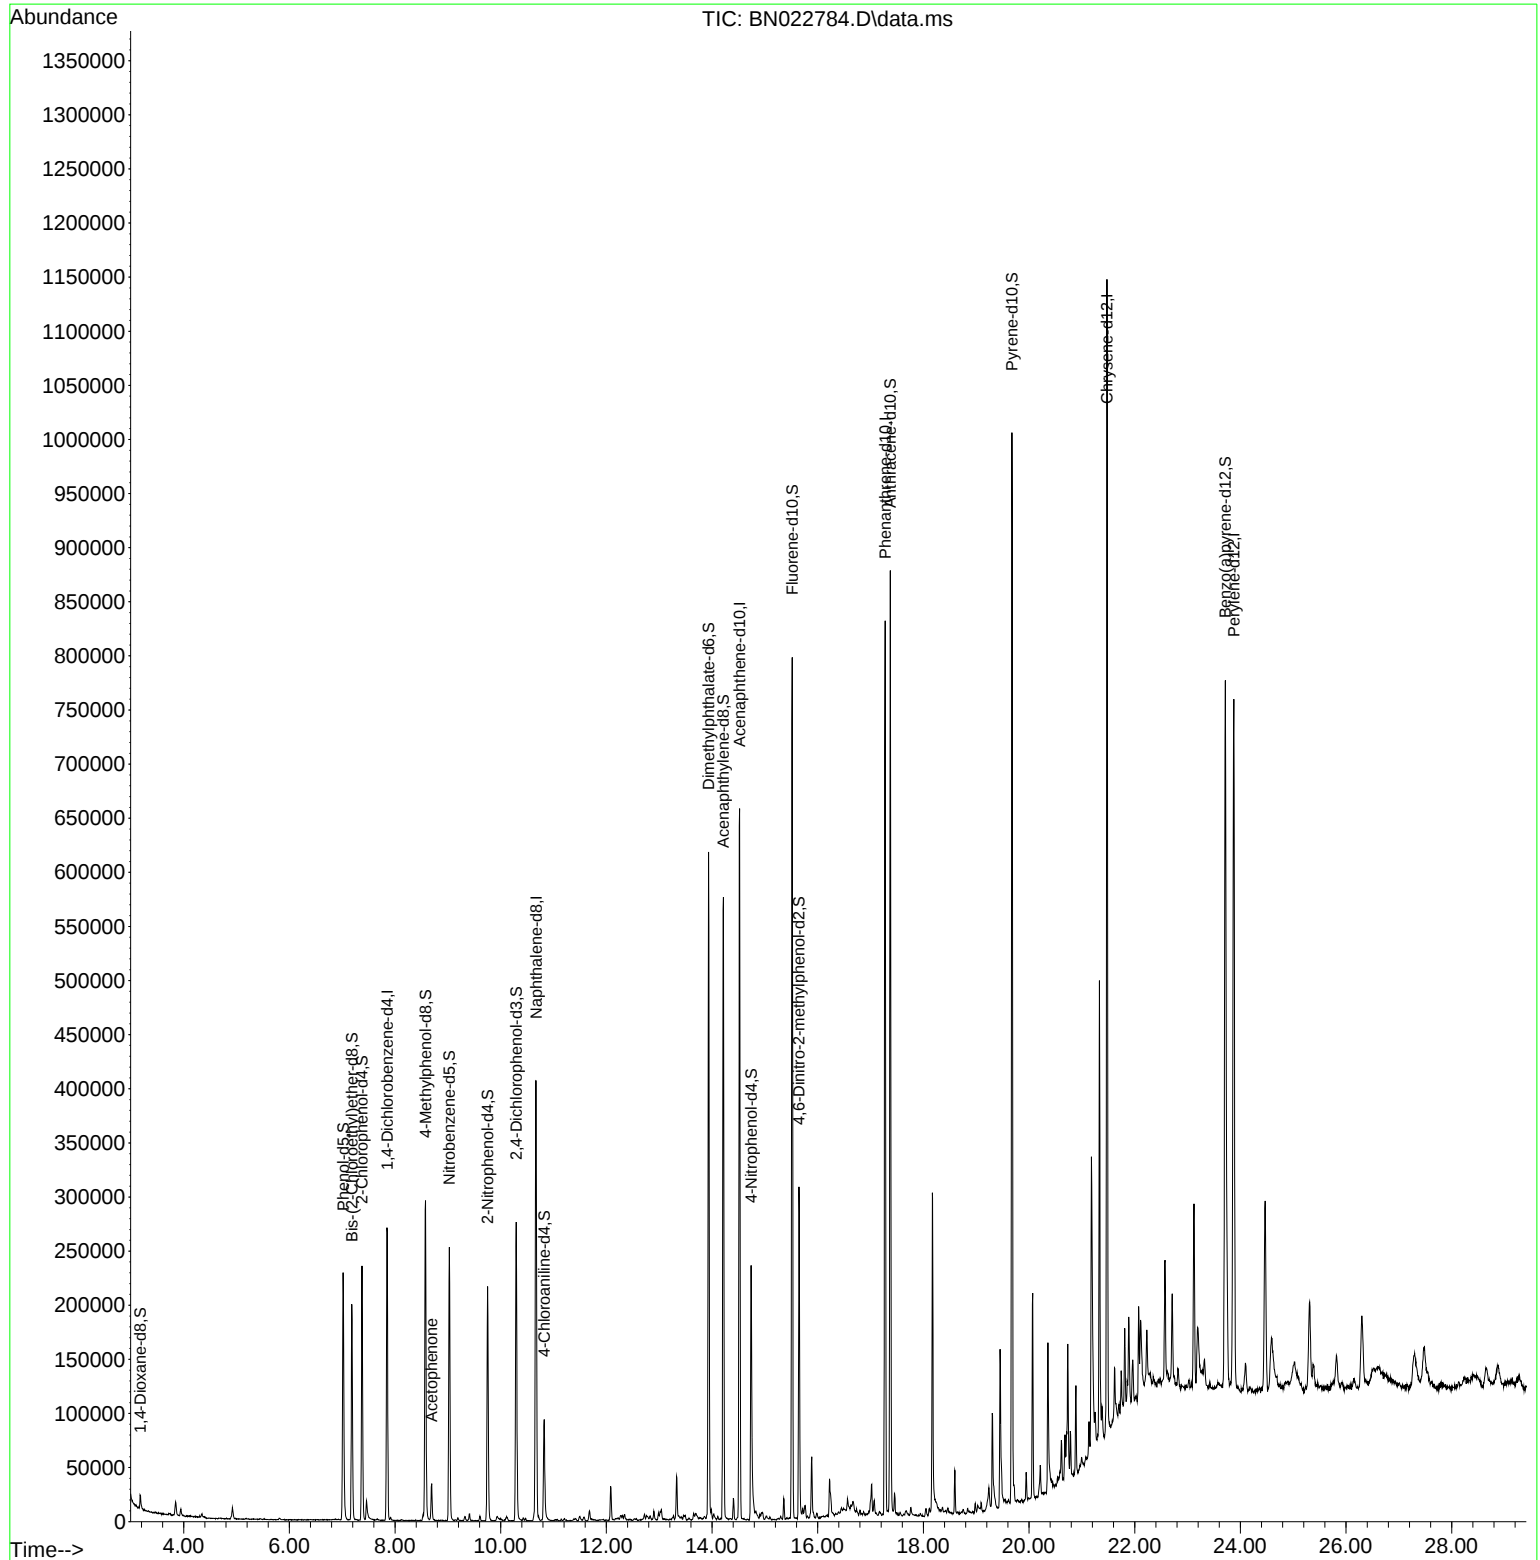

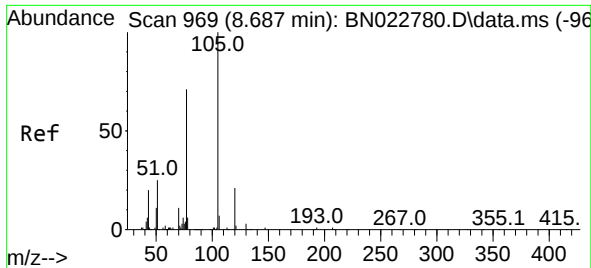

#16
 Acetophenone
 Concen: 2.139 ng/ul
 RT: 8.693 min Scan# 91
 Delta R.T. 0.006 min
 Lab File: BN022784.D
 Acq: 21 Nov 2022 13:18

Instrument :
 BNA_N
 ClientSampleId :
 BGC74

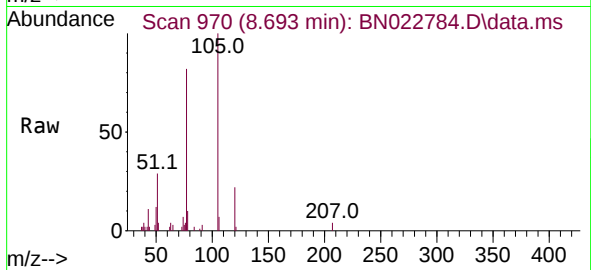

Tgt Ion:	105	Resp:	17378
Ion	Ratio	Lower	Upper
105	100		
77	82.3	64.0	96.0
51	29.5	20.8	31.2

