

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112122\
 Data File : BN022785.D
 Acq On : 21 Nov 2022 13:54
 Operator : CG/JU
 Sample : N5713-04
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BGC75

Quant Time: Nov 21 15:23:49 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Nov 19 05:51:00 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc Units	Dev(Min)


Internal Standards					
1) 1,4-Dichlorobenzene-d4	7.851	152	58986	20.000 ng/u1	0.00
20) Naphthalene-d8	10.669	136	281471	20.000 ng/u1	0.00
38) Acenaphthene-d10	14.522	164	185148	20.000 ng/u1	0.00
64) Phenanthrene-d10	17.274	188	389115	20.000 ng/u1	0.00
79) Chrysene-d12	21.474	240	390630	20.000 ng/u1	0.00
88) Perylene-d12	23.868	264	391730	20.000 ng/u1	0.00
System Monitoring Compounds					
3) 1,4-Dioxane-d8	3.175	96	5799	3.356 ng/uL	0.00
4) Pyridine-d5	3.628	84	24146	4.942 ng/u1	0.02
7) Phenol-d5	7.016	99	110671	19.865 ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.181	67	73883	22.119 ng/u1	0.00
11) 2-Chlorophenol-d4	7.375	132	82870	20.312 ng/u1	0.00
15) 4-Methylphenol-d8	8.575	113	94301	21.441 ng/u1	0.00
21) Nitrobenzene-d5	9.028	128	44026	20.207 ng/u1	0.00
24) 2-Nitrophenol-d4	9.751	143	47787	19.657 ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.293	165	82619	19.935 ng/u1	0.00
31) 4-Chloroaniline-d4	10.822	131	36493	5.781 ng/u1	0.00
46) Dimethylphthalate-d6	13.933	166	315196	23.405 ng/u1	0.00
49) Acenaphthylene-d8	14.216	160	320066	21.570 ng/u1	0.00
54) 4-Nitrophenol-d4	14.739	143	52770	19.656 ng/u1	0.00
60) Fluorene-d10	15.516	176	255950	23.173 ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.651	200	46828	18.933 ng/u1	0.00
73) Anthracene-d10	17.374	188	417213	24.486 ng/u1	0.00
81) Pyrene-d10	19.674	212	471695	23.301 ng/u1	0.00
92) Benzo(a)pyrene-d12	23.715	264	457625	23.239 ng/u1	0.00
Target Compounds					
16) Acetophenone	8.693	105	26994	3.845 ng/u1	Qvalue 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112122\
Data File : BN022785.D
Acq On : 21 Nov 2022 13:54
Operator : CG/JU
Sample : N5713-04
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGC75

Quant Time: Nov 21 15:23:49 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN11522.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Nov 19 05:51:00 2022
Response via : Initial Calibration

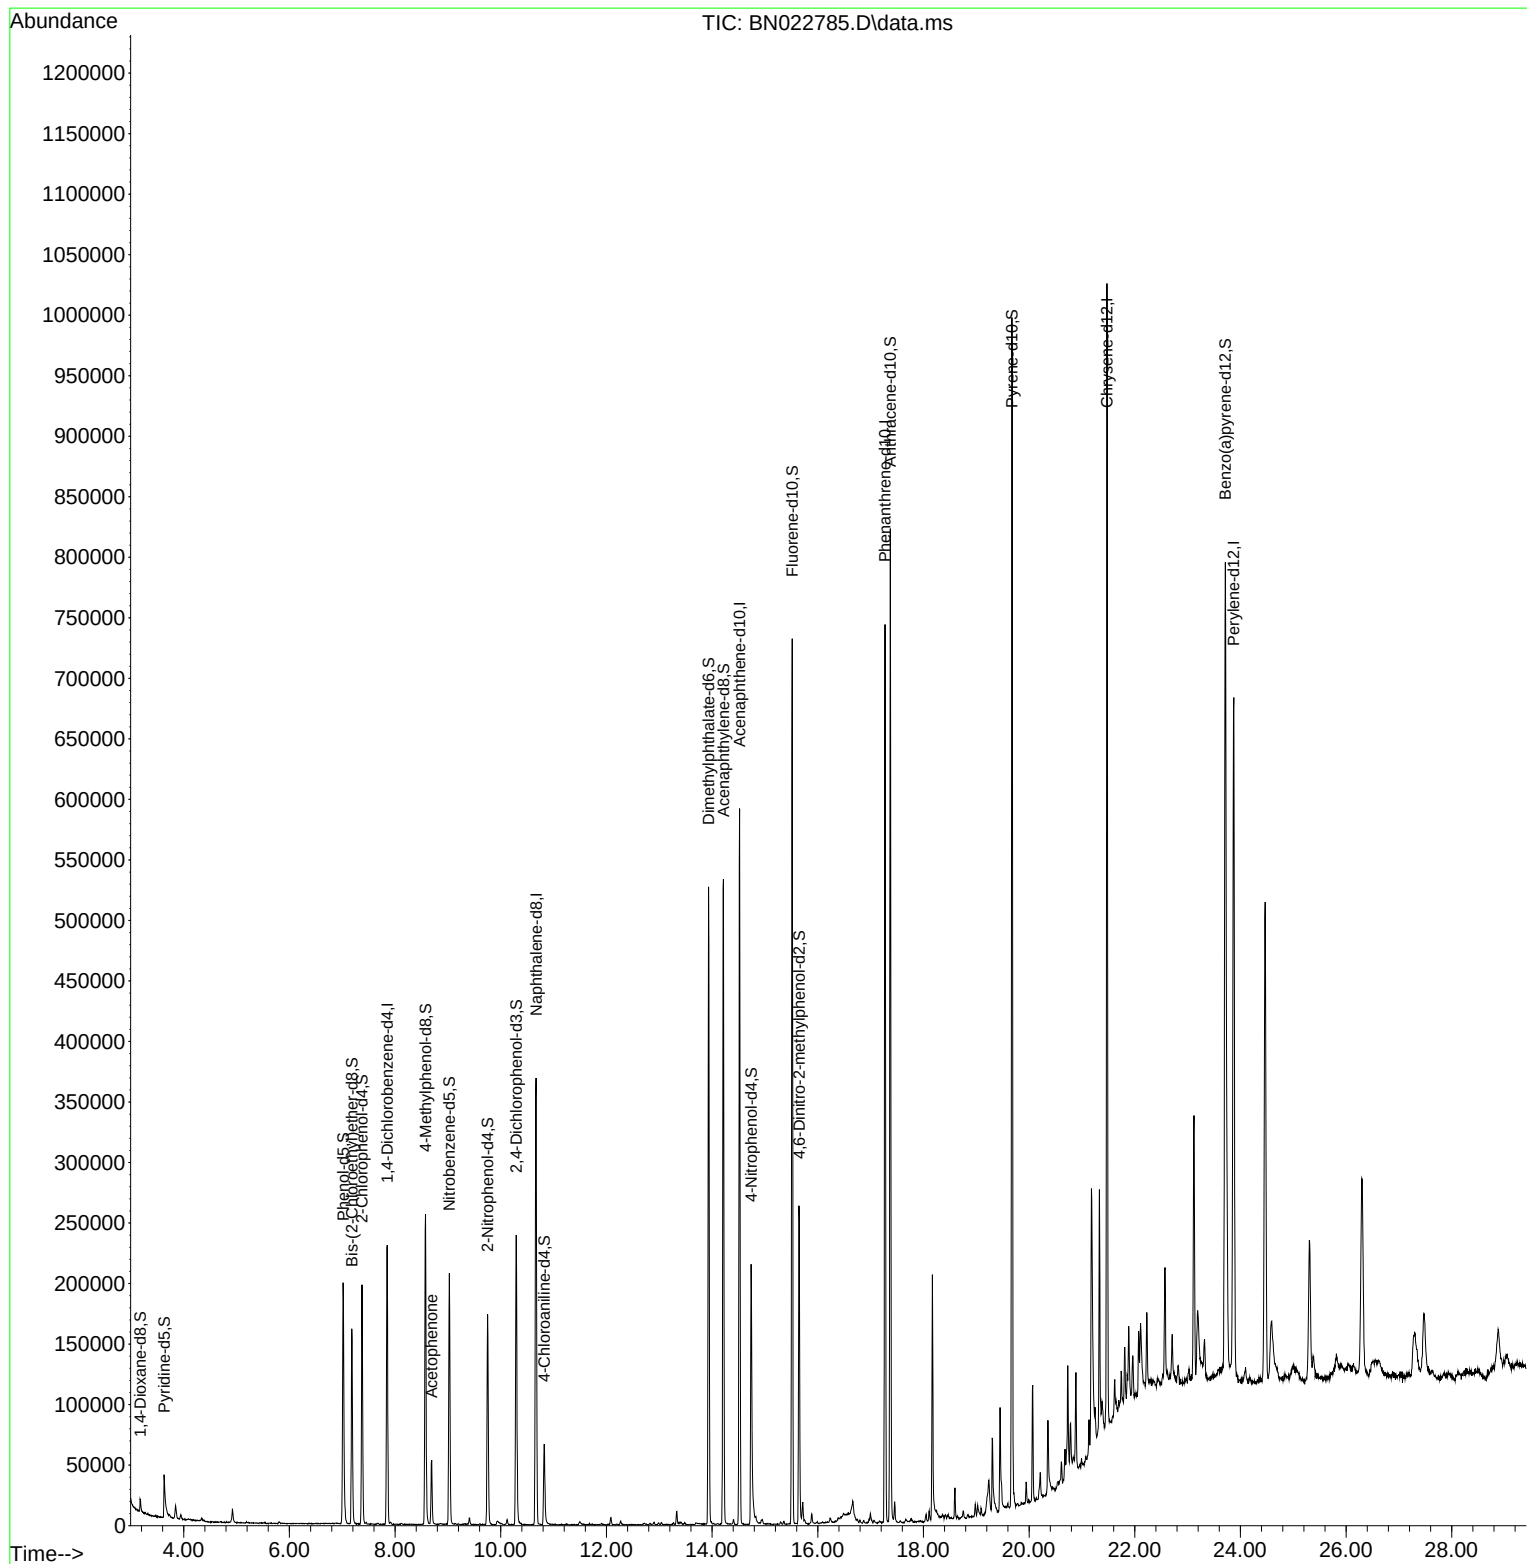

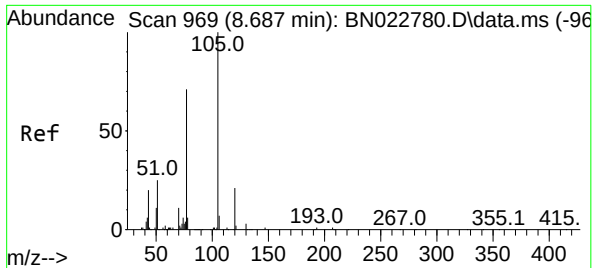

#16
 Acetophenone
 Concen: 3.845 ng/ul
 RT: 8.693 min Scan# 91
 Delta R.T. 0.006 min
 Lab File: BN022785.D
 Acq: 21 Nov 2022 13:54

Instrument :
 BNA_N
 ClientSampleId :
 BGC75

Tgt Ion:	105	Resp:	26994
Ion	Ratio	Lower	Upper
105	100		
77	82.9	64.0	96.0
51	30.1	20.8	31.2

