

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112122\
 Data File : BN022812.D
 Acq On : 22 Nov 2022 07:03
 Operator : CG/JU
 Sample : N5652-01
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH1K4

Quant Time: Nov 22 07:34:00 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN11522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 22 05:15:51 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.846	152	74109	20.000	ng/u1	0.00
20) Naphthalene-d8	10.663	136	351210	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.516	164	231235	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.269	188	481161	20.000	ng/u1	0.00
79) Chrysene-d12	21.474	240	470226	20.000	ng/u1	0.00
88) Perylene-d12	23.868	264	455491	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.175	96	9753	4.493	ng/uL	0.00
4) Pyridine-d5	3.622	84	42318	6.894	ng/u1	0.01
7) Phenol-d5	7.016	99	51253	7.322	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.181	67	144256	34.374	ng/u1	0.00
11) 2-Chlorophenol-d4	7.369	132	130635	25.485	ng/u1	0.00
15) 4-Methylphenol-d8	8.569	113	96969	17.548	ng/u1	0.00
21) Nitrobenzene-d5	9.022	128	89580	32.952	ng/u1	0.00
24) 2-Nitrophenol-d4	9.751	143	96361	31.767	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.287	165	150837	29.169	ng/u1	0.00
31) 4-Chloroaniline-d4	10.810	131	214376	27.216	ng/u1	0.00
46) Dimethylphthalate-d6	13.934	166	603557	35.885	ng/u1	0.00
49) Acenaphthylene-d8	14.210	160	654848	35.336	ng/u1	0.00
54) 4-Nitrophenol-d4	14.739	143	19960	5.953	ng/u1	0.00
60) Fluorene-d10	15.510	176	499106	36.182	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.645	200	87434	28.589	ng/u1	0.00
73) Anthracene-d10	17.369	188	799899	37.966	ng/u1	0.00
81) Pyrene-d10	19.674	212	886100	36.362	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.710	264	873548	38.151	ng/u1	0.00
Target Compounds						
2) 1,4-Dioxane	3.217	88	2322	1.005	ng/uL	Qvalue 94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112122\
Data File : BN022812.D
Acq On : 22 Nov 2022 07:03
Operator : CG/JU
Sample : N5652-01
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH1K4

Quant Time: Nov 22 07:34:00 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN11522.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 22 05:15:51 2022
Response via : Initial Calibration

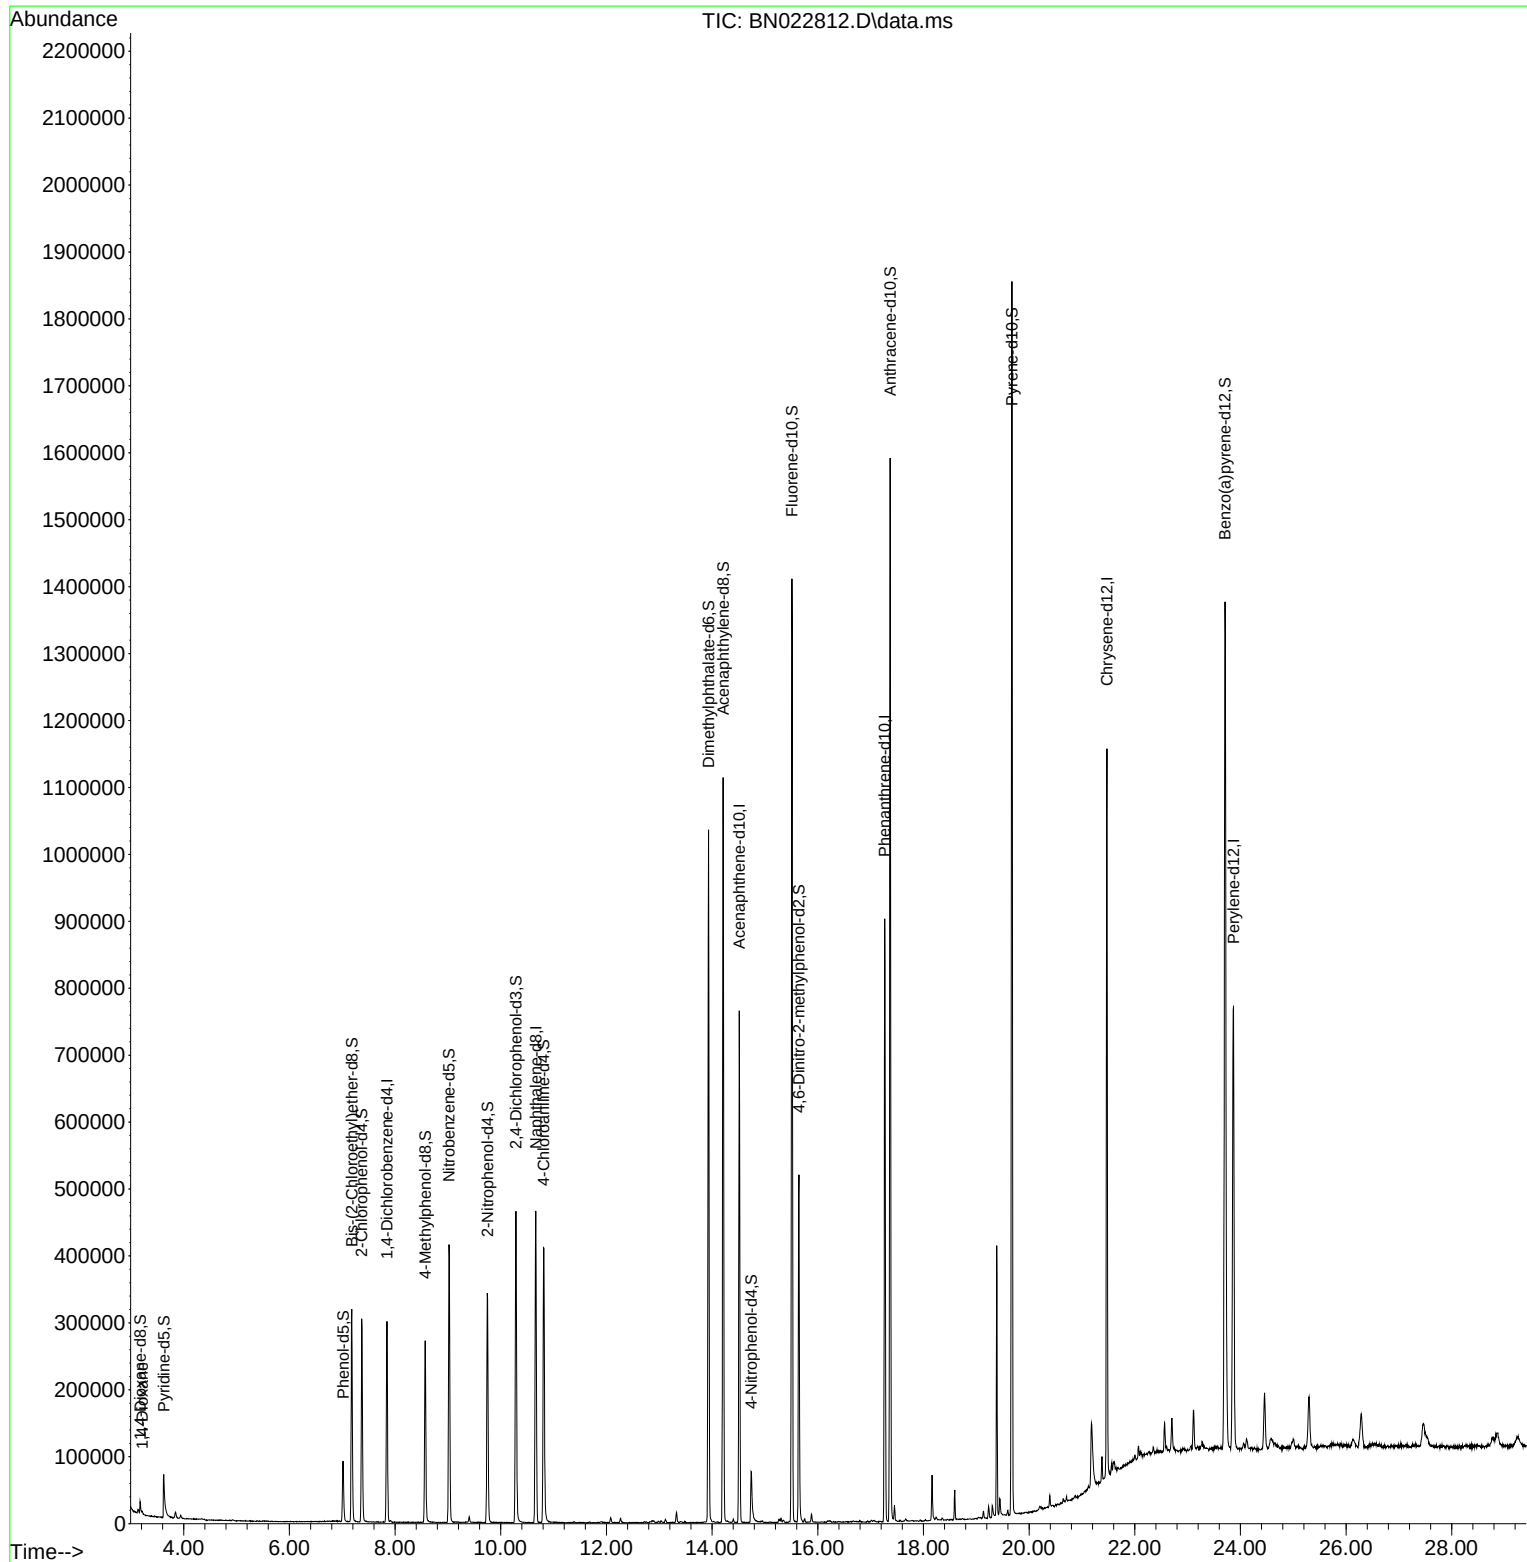

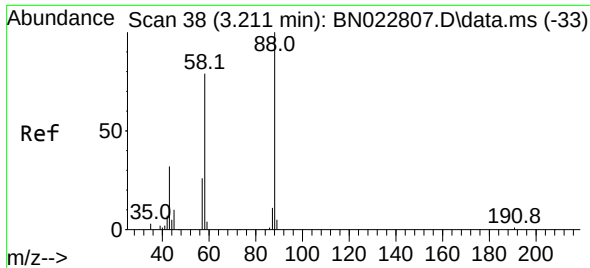

#2
 1,4-Dioxane
 Concen: 1.005 ng/uL
 RT: 3.217 min Scan# 39
 Delta R.T. 0.006 min
 Lab File: BN022812.D
 Acq: 22 Nov 2022 07:03

Instrument :
 BNA_N
 ClientSampleId :
 BH1K4

Tgt Ion: 88 Resp: 2322
 Ion Ratio Lower Upper
 88 100
 43 32.4 30.8 46.2
 58 73.1 61.7 92.5

