

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112122\
 Data File : BN022824.D
 Acq On : 22 Nov 2022 14:46
 Operator : CG/JU
 Sample : N5593-06
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 H0AD4

Quant Time: Nov 22 17:17:21 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 22 05:15:51 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.846	152	64233	20.000	ng/u1	0.00
20) Naphthalene-d8	10.663	136	304512	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.516	164	199557	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.269	188	405661	20.000	ng/u1	0.00
79) Chrysene-d12	21.469	240	393702	20.000	ng/u1	0.00
88) Perylene-d12	23.863	264	382494	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.176	96	9372	4.981	ng/uL	0.00
4) Pyridine-d5	3.617	84	63403	11.917	ng/u1	0.00
7) Phenol-d5	7.016	99	50713	8.359	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.181	67	152239	41.854	ng/u1	0.00
11) 2-Chlorophenol-d4	7.369	132	133352	30.015	ng/u1	0.00
15) 4-Methylphenol-d8	8.569	113	95309	19.900	ng/u1	0.00
21) Nitrobenzene-d5	9.028	128	94281	40.000	ng/u1	0.00
24) 2-Nitrophenol-d4	9.746	143	91480	34.783	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.287	165	151222	33.728	ng/u1	0.00
31) 4-Chloroaniline-d4	10.810	131	236465	34.624	ng/u1	0.00
46) Dimethylphthalate-d6	13.934	166	619186	42.659	ng/u1	0.00
49) Acenaphthylene-d8	14.210	160	665800	41.630	ng/u1	0.00
54) 4-Nitrophenol-d4	14.740	143	16758	5.791	ng/u1	0.00
60) Fluorene-d10	15.510	176	511725	42.986	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.645	200	71019	27.543	ng/u1	0.00
73) Anthracene-d10	17.369	188	854009	48.078	ng/u1	0.00
81) Pyrene-d10	19.675	212	925552	45.364	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.710	264	904079	47.020	ng/u1	0.00


Target Compounds					Qvalue
2) 1,4-Dioxane	3.211	88	5368	2.681	ng/uL 92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112122\
Data File : BN022824.D
Acq On : 22 Nov 2022 14:46
Operator : CG/JU
Sample : N5593-06
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
H0AD4

Quant Time: Nov 22 17:17:21 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN11522.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 22 05:15:51 2022
Response via : Initial Calibration

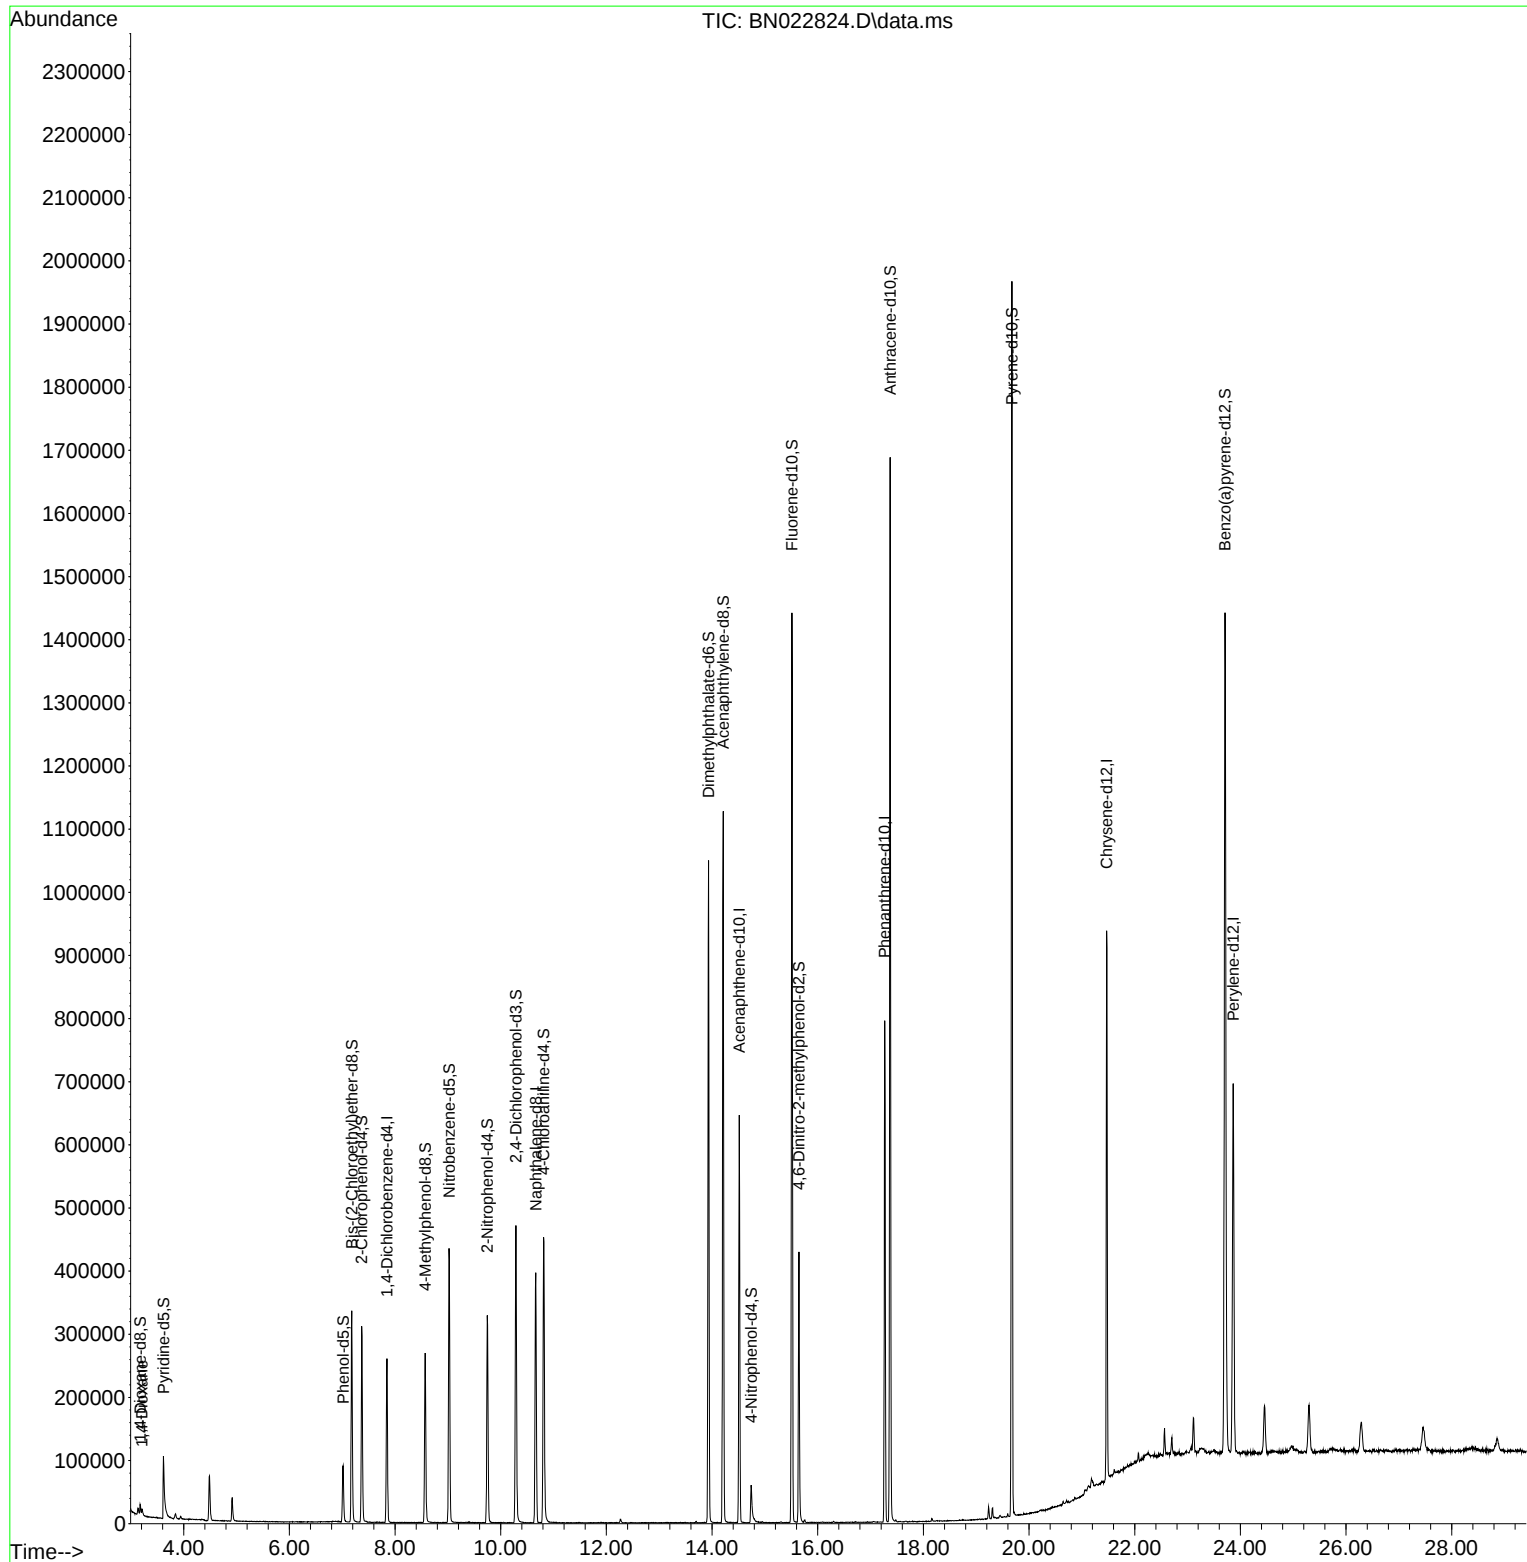

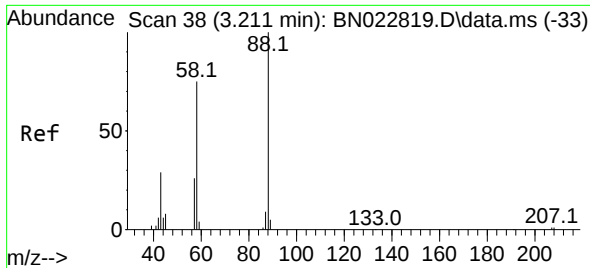

#2
 1,4-Dioxane
 Concen: 2.681 ng/uL
 RT: 3.211 min Scan# 38
 Delta R.T. 0.000 min
 Lab File: BN022824.D
 Acq: 22 Nov 2022 14:46

Instrument :
 BNA_N
 ClientSampleId :
 H0AD4

Tgt Ion: 88	Resp: 5368
Ion Ratio	Lower Upper
88	100
43	32.9 30.8 46.2
58	70.2 61.7 92.5

