

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112122\
 Data File : BN022825.D
 Acq On : 22 Nov 2022 15:23
 Operator : CG/JU
 Sample : N5593-07
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 H0AD5

Quant Time: Nov 22 17:31:59 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 22 05:15:51 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc Units	Dev(Min)


Internal Standards					
1) 1,4-Dichlorobenzene-d4	7.846	152	66719	20.000 ng/u1	0.00
20) Naphthalene-d8	10.663	136	317556	20.000 ng/u1	0.00
38) Acenaphthene-d10	14.516	164	208890	20.000 ng/u1	0.00
64) Phenanthrene-d10	17.269	188	437226	20.000 ng/u1	0.00
79) Chrysene-d12	21.474	240	422782	20.000 ng/u1	0.00
88) Perylene-d12	23.863	264	432622	20.000 ng/u1	0.00
System Monitoring Compounds					
3) 1,4-Dioxane-d8	3.175	96	8996	4.603 ng/uL	0.00
4) Pyridine-d5	3.622	84	45095	8.160 ng/u1	0.01
7) Phenol-d5	7.016	99	44622	7.081 ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.181	67	135761	35.933 ng/u1	0.00
11) 2-Chlorophenol-d4	7.369	132	117402	25.440 ng/u1	0.00
15) 4-Methylphenol-d8	8.569	113	85291	17.145 ng/u1	0.00
21) Nitrobenzene-d5	9.028	128	84185	34.249 ng/u1	0.00
24) 2-Nitrophenol-d4	9.752	143	84966	30.979 ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.287	165	135973	29.081 ng/u1	0.00
31) 4-Chloroaniline-d4	10.816	131	176273	24.750 ng/u1	0.00
46) Dimethylphthalate-d6	13.934	166	547096	36.008 ng/u1	0.00
49) Acenaphthylene-d8	14.210	160	610210	36.450 ng/u1	0.00
54) 4-Nitrophenol-d4	14.740	143	17168	5.668 ng/u1	0.00
60) Fluorene-d10	15.510	176	462087	37.082 ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.645	200	78297	28.174 ng/u1	0.00
73) Anthracene-d10	17.369	188	753675	39.366 ng/u1	0.00
81) Pyrene-d10	19.675	212	876739	40.016 ng/u1	0.00
92) Benzo(a)pyrene-d12	23.716	264	862960	39.681 ng/u1	0.01
Target Compounds				Qvalue	
2) 1,4-Dioxane	3.211	88	4435	2.133 ng/uL#	83


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112122\
Data File : BN022825.D
Acq On : 22 Nov 2022 15:23
Operator : CG/JU
Sample : N5593-07
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
H0AD5

Quant Time: Nov 22 17:31:59 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN11522.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 22 05:15:51 2022
Response via : Initial Calibration

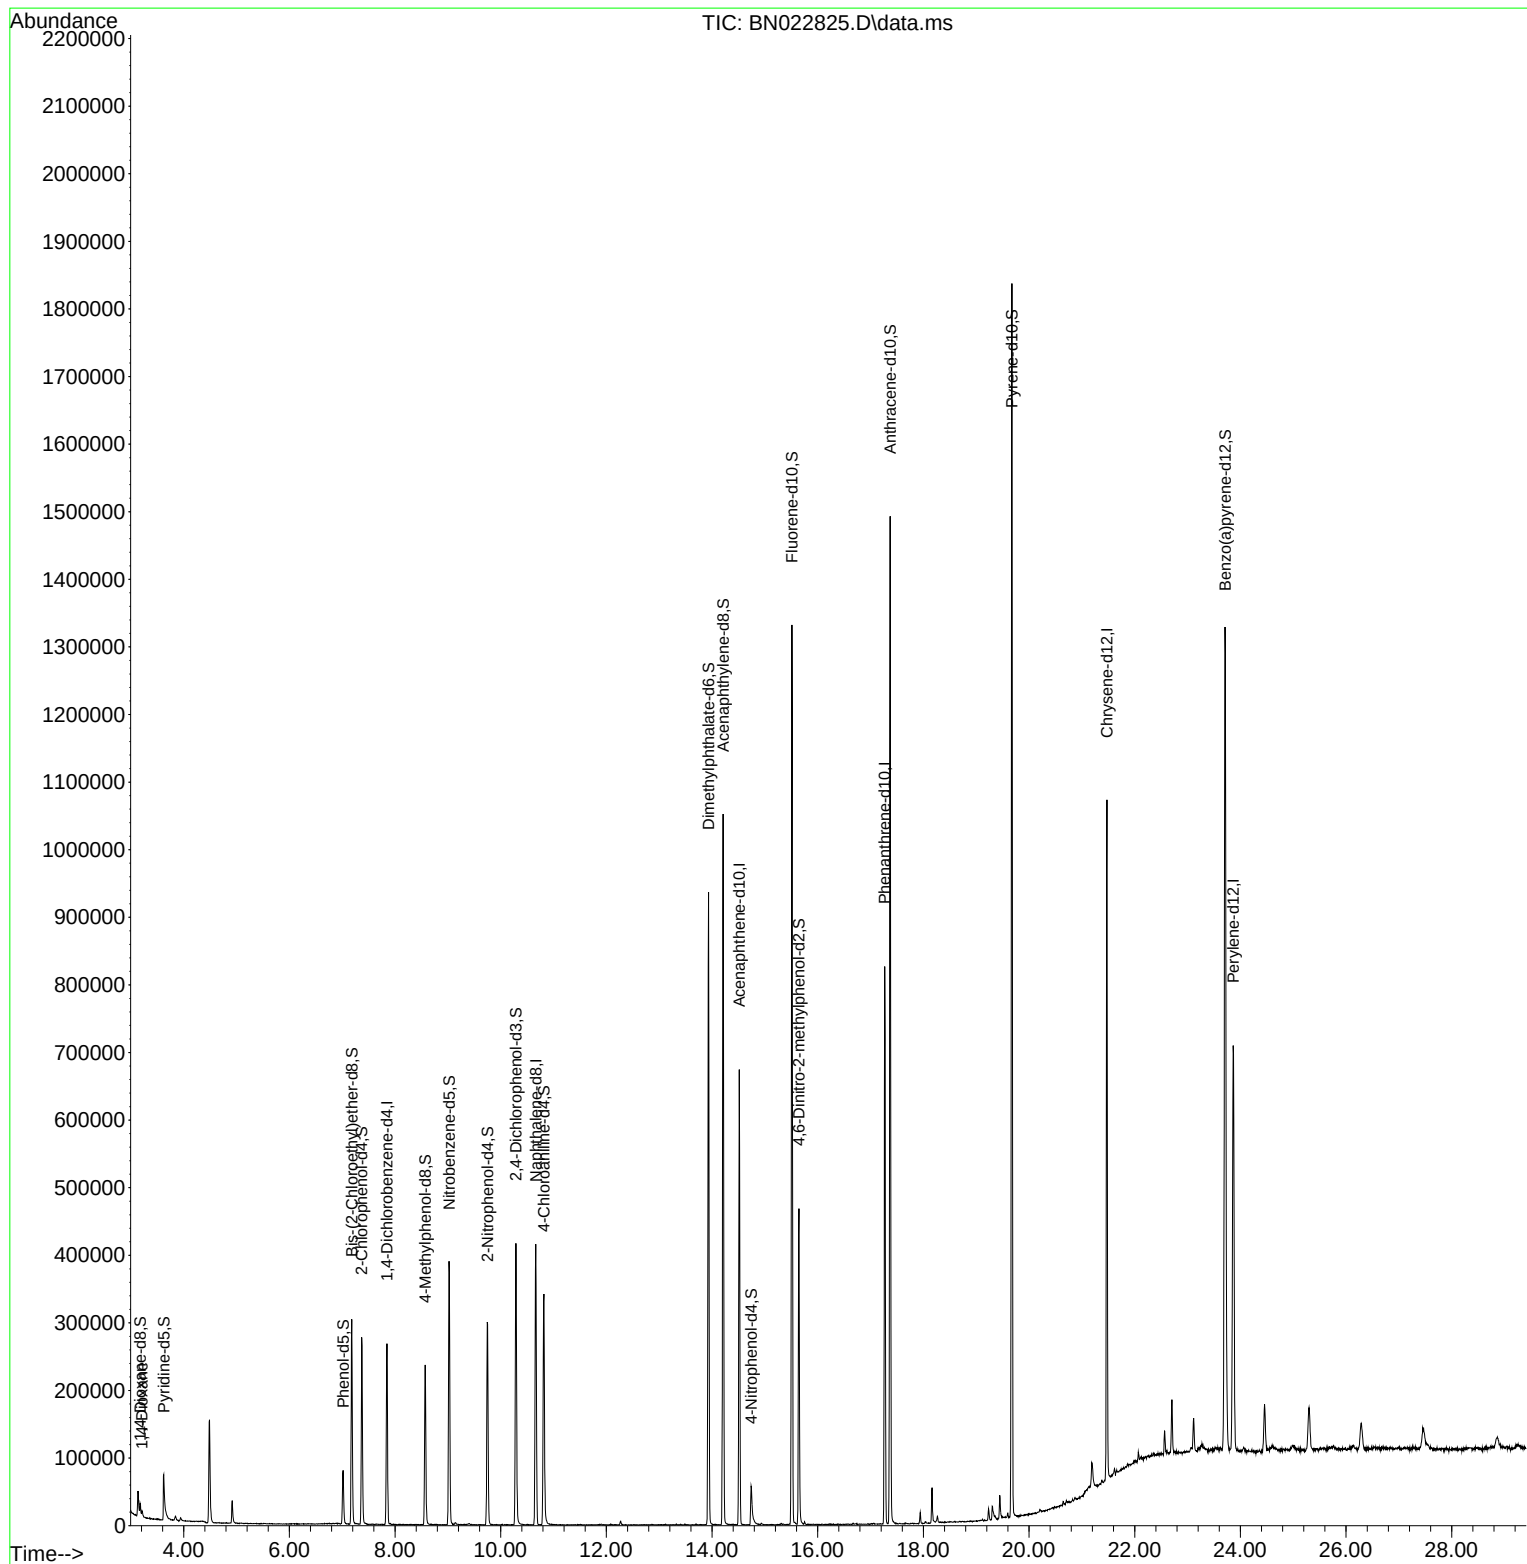

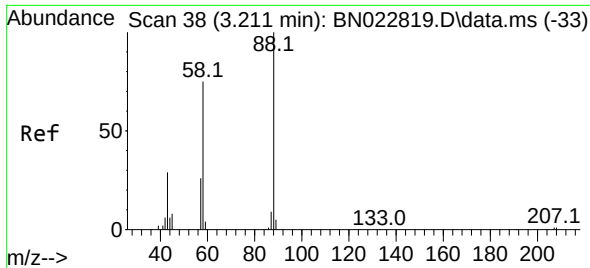

#2
 1,4-Dioxane
 Concen: 2.133 ng/uL
 RT: 3.211 min Scan# 38
 Delta R.T. 0.000 min
 Lab File: BN022825.D
 Acq: 22 Nov 2022 15:23

Instrument :
 BNA_N
 ClientSampleId :
 H0AD5

Tgt Ion: 88 Resp: 4435
 Ion Ratio Lower Upper
 88 100
 43 27.5 30.8 46.2#
 58 63.3 61.7 92.5

