

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112122\
 Data File : BN022843.D
 Acq On : 23 Nov 2022 02:30
 Operator : CG/JU
 Sample : N5593-03
 Misc :
 ALS Vial : 65 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 H0AD1

Quant Time: Nov 23 03:04:21 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 22 05:15:51 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.846	152	60643	20.000	ng/u1	0.00
20) Naphthalene-d8	10.663	136	292669	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.510	164	190192	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.269	188	402152	20.000	ng/u1	0.00
79) Chrysene-d12	21.474	240	387344	20.000	ng/u1	0.00
88) Perylene-d12	23.868	264	386109	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.170	96	15669	8.821	ng/uL	0.00
4) Pyridine-d5	3.617	84	52129	10.378	ng/u1	0.00
7) Phenol-d5	7.011	99	50003	8.730	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.175	67	137555	40.056	ng/u1	0.00
11) 2-Chlorophenol-d4	7.369	132	124642	29.715	ng/u1	0.00
15) 4-Methylphenol-d8	8.569	113	89500	19.793	ng/u1	0.00
21) Nitrobenzene-d5	9.022	128	84329	37.225	ng/u1	0.00
24) 2-Nitrophenol-d4	9.746	143	88822	35.139	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.287	165	144538	33.541	ng/u1	0.00
31) 4-Chloroaniline-d4	10.810	131	157850	24.048	ng/u1	0.00
46) Dimethylphthalate-d6	13.934	166	547528	39.579	ng/u1	0.00
49) Acenaphthylene-d8	14.210	160	606472	39.788	ng/u1	0.00
54) 4-Nitrophenol-d4	14.740	143	19989	7.248	ng/u1	0.00
60) Fluorene-d10	15.510	176	468917	41.329	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.645	200	85280	33.363	ng/u1	0.00
73) Anthracene-d10	17.369	188	719208	40.842	ng/u1	0.00
81) Pyrene-d10	19.675	212	851972	42.443	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.710	264	775871	39.974	ng/u1	0.00


Target Compounds					Qvalue	
2) 1,4-Dioxane	3.205	88	67992	35.970	ng/uL#	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112122\
Data File : BN022843.D
Acq On : 23 Nov 2022 02:30
Operator : CG/JU
Sample : N5593-03
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
H0AD1


Quant Time: Nov 23 03:04:21 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN11522.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 22 05:15:51 2022
Response via : Initial Calibration

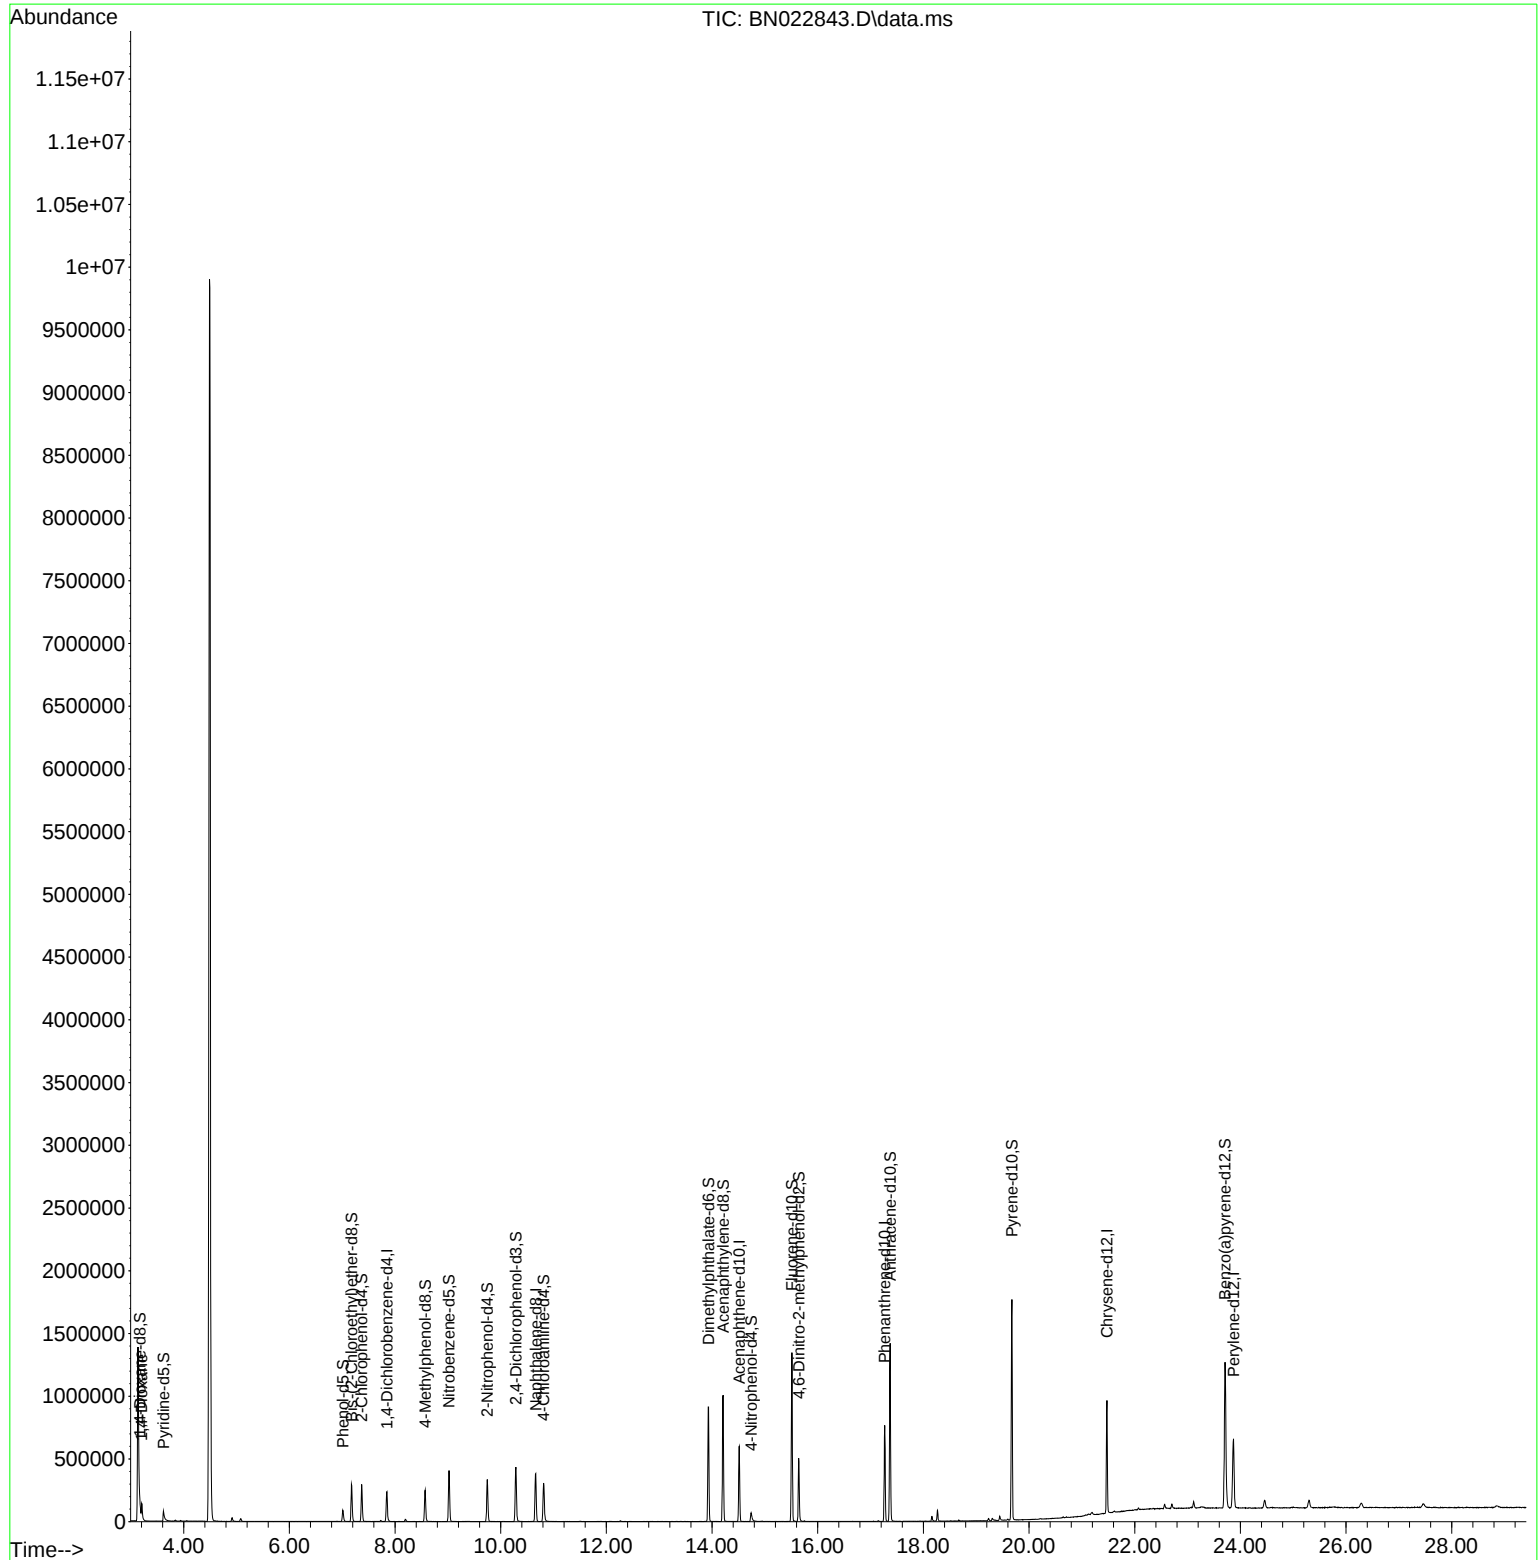

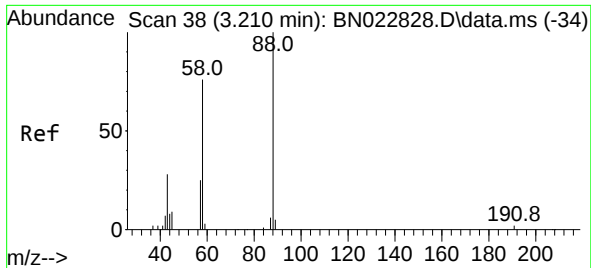

#2
 1,4-Dioxane
 Concen: 35.970 ng/uL
 RT: 3.205 min Scan# 31
 Delta R.T. -0.006 min
 Lab File: BN022843.D
 Acq: 23 Nov 2022 02:30

Instrument :
 BNA_N
 ClientSampleId :
 H0AD1

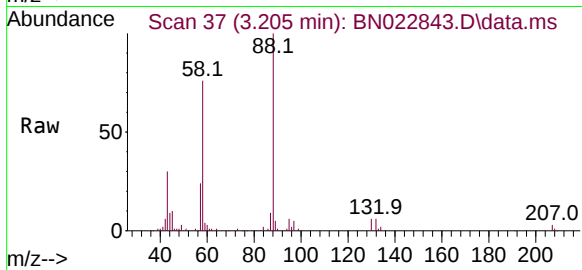

Tgt Ion: 88 Resp: 67992
 Ion Ratio Lower Upper
 88 100
 43 30.3 30.8 46.2#
 58 76.2 61.7 92.5

