

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112122\
 Data File : BN022781.D
 Acq On : 21 Nov 2022 11:29
 Operator : CG/JU
 Sample : PB149178BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK178

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
 Title : SVOA CALIBRATION

Signal : TIC: BN022781.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.181	29	33	44	rVB	17140	26632	1.48%	0.139%
2	3.616	103	107	133	rVB	196588	348605	19.42%	1.821%
3	3.946	159	163	168	rVB	4018	6631	0.37%	0.035%
4	7.016	679	685	699	rBV	274194	441563	24.60%	2.307%
5	7.181	707	713	726	rVB	224435	352952	19.66%	1.844%
6	7.375	740	746	761	rVB	275440	443540	24.71%	2.317%
7	7.851	820	827	837	rBV	255184	416067	23.18%	2.173%
8	8.575	943	950	964	rBV	350417	569872	31.75%	2.977%
9	9.028	1020	1027	1039	rBV	288475	466386	25.98%	2.436%
10	9.751	1144	1150	1160	rBV	237804	393310	21.91%	2.054%
11	10.292	1235	1242	1263	rBV	330236	575233	32.05%	3.005%
12	10.669	1298	1306	1316	rVB	394622	664653	37.03%	3.472%
13	10.816	1324	1331	1352	rBV	338548	617085	34.38%	3.223%
14	12.286	1574	1581	1587	rBV2	3356	6550	0.36%	0.034%
15	13.404	1767	1771	1776	rVB4	2099	3498	0.19%	0.018%
16	13.933	1855	1861	1873	rVB	668272	936430	52.17%	4.891%
17	14.216	1902	1909	1918	rBV	726537	1052755	58.65%	5.499%
18	14.522	1954	1961	1968	rBV	634993	932084	51.93%	4.869%
19	14.739	1991	1998	2021	rBV	279535	479130	26.69%	2.503%
20	15.516	2123	2130	2140	rVB	986013	1348706	75.14%	7.045%
21	15.651	2147	2153	2167	rBV	307611	448092	24.96%	2.341%
22	15.751	2167	2170	2175	rVB	3114	3841	0.21%	0.020%
23	17.063	2389	2393	2397	rBV2	1373	1897	0.11%	0.010%
24	17.274	2423	2429	2437	rBV	819127	1122681	62.55%	5.864%
25	17.374	2439	2446	2463	rVB	1093992	1501442	83.65%	7.843%
26	19.239	2759	2763	2767	rBV3	10009	13268	0.74%	0.069%
27	19.310	2771	2775	2779	rBV2	9591	12060	0.67%	0.063%
28	19.680	2832	2838	2849	rBV	1207478	1672726	93.19%	8.738%
29	21.474	3138	3143	3152	rBV2	968490	1264973	70.47%	6.608%
30	23.715	3517	3524	3539	rVB	897340	1794946	100.00%	9.376%
31	23.874	3544	3551	3560	rVB2	615138	1226484	68.33%	6.407%


Sum of corrected areas: 19144092

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112122\
Data File : BN022781.D
Acq On : 21 Nov 2022 11:29
Operator : CG/JU
Sample : PB149178BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK178

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

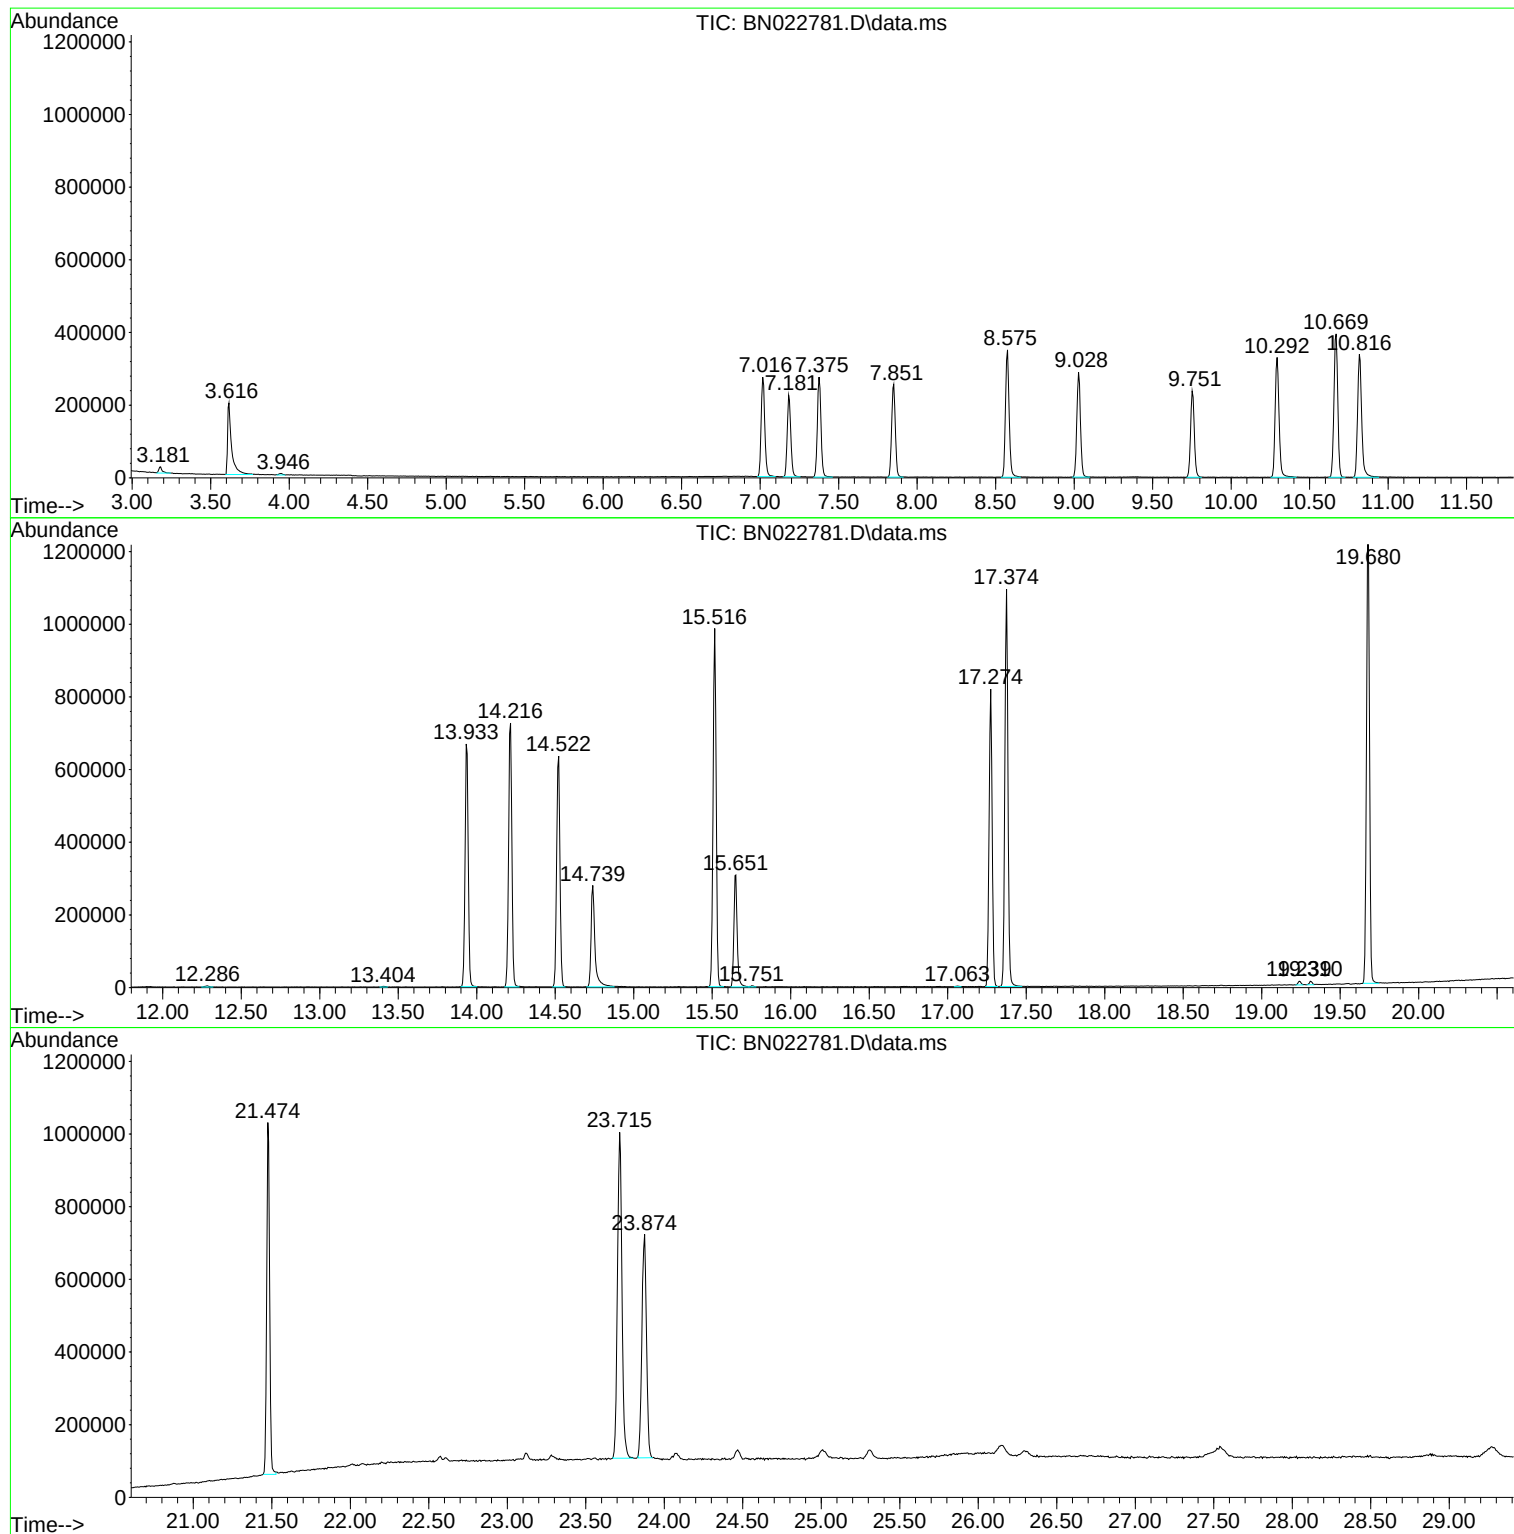

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112122\
Data File : BN022781.D
Acq On : 21 Nov 2022 11:29
Operator : CG/JU
Sample : PB149178BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK178

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112122\
Data File : BN022781.D
Acq On : 21 Nov 2022 11:29
Operator : CG/JU
Sample : PB149178BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK178

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc