

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112122\
 Data File : BN022790.D
 Acq On : 21 Nov 2022 16:59
 Operator : CG/JU
 Sample : PB149195BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK195

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
 Title : SVOA CALIBRATION

Signal : TIC: BN022790.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.175	28	32	45	rVB	17523	25216	1.49%	0.140%
2	3.611	103	106	127	rBV	194687	354207	20.97%	1.970%
3	3.946	159	163	169	rVB2	3382	5023	0.30%	0.028%
4	7.016	679	685	703	rVB	276210	447510	26.49%	2.489%
5	7.181	707	713	727	rVB	218965	351780	20.82%	1.957%
6	7.375	739	746	760	rBV	277997	437240	25.88%	2.432%
7	7.852	820	827	838	rVB	200684	326112	19.30%	1.814%
8	8.575	943	950	969	rBV	356645	578538	34.24%	3.218%
9	9.028	1019	1027	1038	rBV	291946	474779	28.10%	2.641%
10	9.752	1143	1150	1159	rBV	249706	404832	23.96%	2.252%
11	10.293	1233	1242	1263	rBV	348007	588701	34.85%	3.275%
12	10.669	1297	1306	1314	rBV	322048	533424	31.57%	2.967%
13	10.816	1324	1331	1349	rBV	344601	628516	37.20%	3.496%
14	12.275	1574	1579	1588	rVB2	3453	6674	0.40%	0.037%
15	13.940	1855	1862	1874	rVB	681484	966872	57.23%	5.378%
16	14.216	1902	1909	1931	rBV	734915	1084826	64.21%	6.034%
17	14.522	1954	1961	1972	rBV	521341	754006	44.63%	4.194%
18	14.740	1992	1998	2024	rBV	300713	512610	30.34%	2.851%
19	15.516	2123	2130	2146	rVB	966596	1358569	80.42%	7.557%
20	15.651	2146	2153	2167	rVV	327855	483184	28.60%	2.688%
21	15.757	2167	2171	2176	rVB	2479	3289	0.19%	0.018%
22	17.275	2423	2429	2436	rBV	644850	885624	52.42%	4.926%
23	17.375	2439	2446	2464	rBV2	1045296	1487118	88.03%	8.272%
24	19.239	2759	2763	2768	rBV3	10129	15064	0.89%	0.084%
25	19.316	2772	2776	2782	rVB2	8622	12263	0.73%	0.068%
26	19.680	2832	2838	2847	rBV	1180491	1649080	97.61%	9.173%
27	21.475	3138	3143	3153	rBV	753074	965046	57.12%	5.368%
28	23.716	3517	3524	3538	rVB2	817969	1689413	100.00%	9.398%
29	23.874	3544	3551	3565	rVB2	456242	947600	56.09%	5.271%




Sum of corrected areas: 17977116

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112122\
Data File : BN022790.D
Acq On : 21 Nov 2022 16:59
Operator : CG/JU
Sample : PB149195BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK195

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

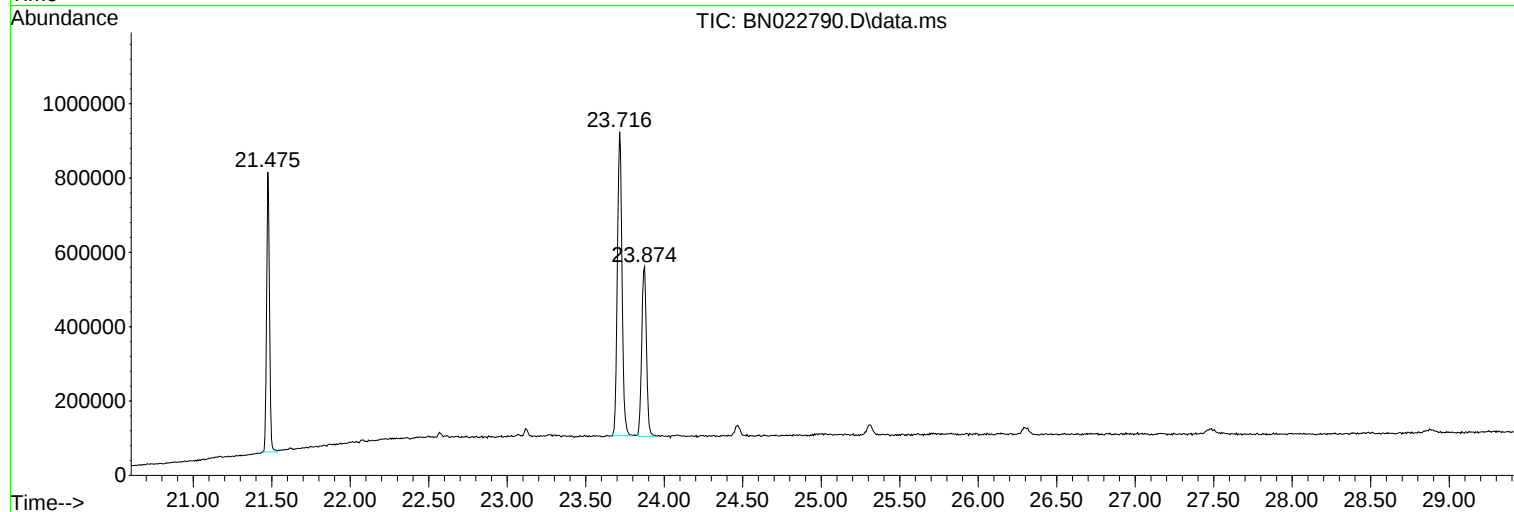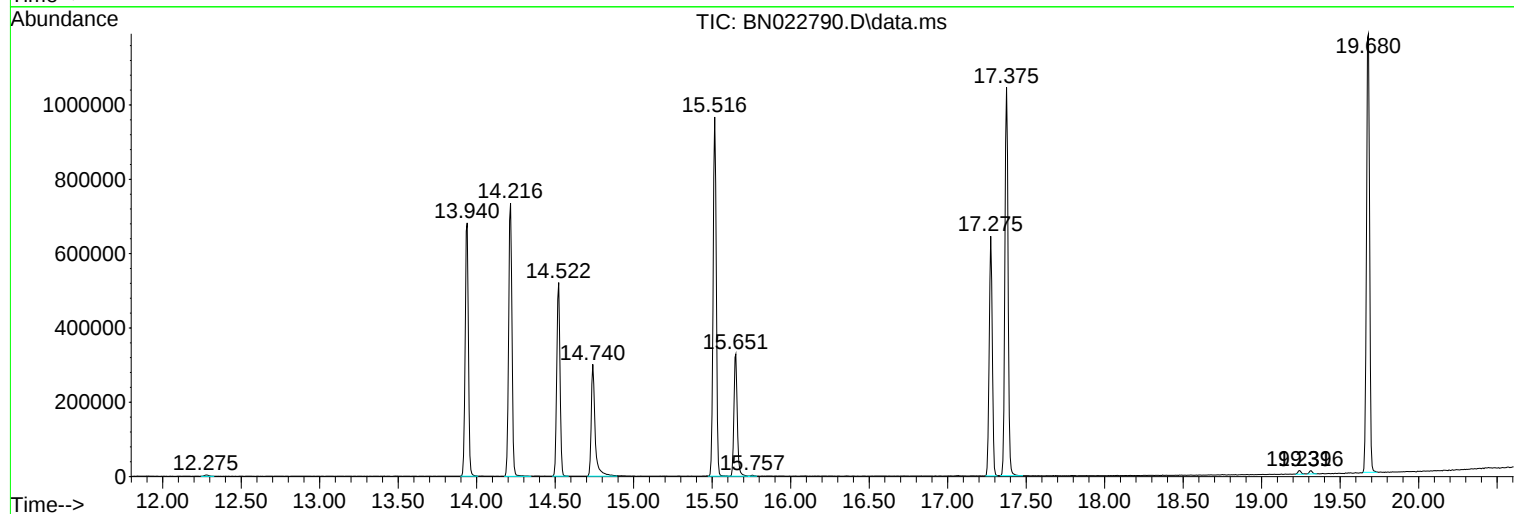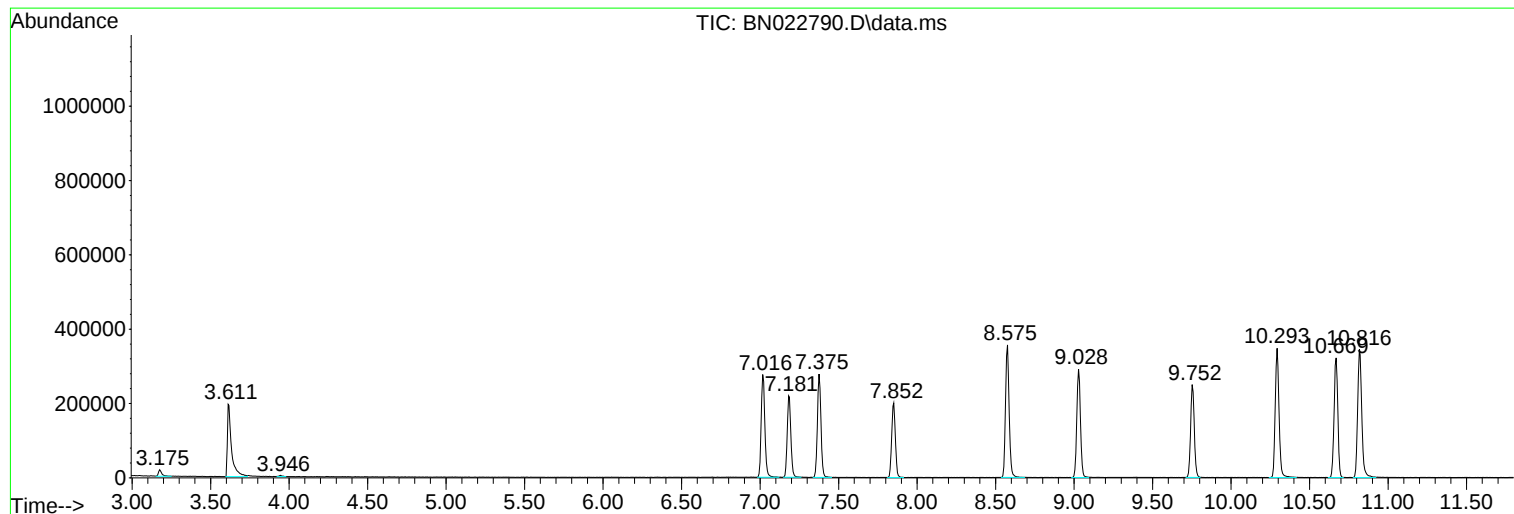

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112122\
Data File : BN022790.D
Acq On : 21 Nov 2022 16:59
Operator : CG/JU
Sample : PB149195BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK195

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112122\
Data File : BN022790.D
Acq On : 21 Nov 2022 16:59
Operator : CG/JU
Sample : PB149195BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK195

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc