

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112122\
 Data File : BN022795.D
 Acq On : 21 Nov 2022 20:04
 Operator : CG/JU
 Sample : N5690-13
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BGCF4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
 Title : SVOA CALIBRATION

Signal : TIC: BN022795.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.181	29	33	44	rVB	14406	26417	1.05%	0.117%
2	3.628	107	109	119	rBV	32647	56296	2.23%	0.250%
3	3.846	141	146	153	rVB3	7831	13295	0.53%	0.059%
4	3.946	159	163	166	rBV2	4367	5463	0.22%	0.024%
5	7.017	679	685	703	rVB	69813	115998	4.60%	0.514%
6	7.181	707	713	726	rBV	271172	423683	16.81%	1.878%
7	7.375	740	746	758	rBV	248688	398697	15.82%	1.767%
8	7.846	820	826	836	rBV	278127	449289	17.83%	1.992%
9	8.575	943	950	960	rBV	204817	345446	13.71%	1.531%
10	9.028	1019	1027	1041	rBV	359354	581009	23.06%	2.575%
11	9.146	1044	1047	1052	rVB4	3009	4426	0.18%	0.020%
12	9.411	1087	1092	1097	rVB	2627	4280	0.17%	0.019%
13	9.752	1143	1150	1161	rBV	289896	470792	18.68%	2.087%
14	10.293	1235	1242	1254	rBV	371426	635420	25.22%	2.817%
15	10.663	1298	1305	1316	rBV	424233	719465	28.55%	3.189%
16	10.816	1324	1331	1349	rBV	344554	616904	24.48%	2.734%
17	11.375	1420	1426	1428	rBV3	1378	2584	0.10%	0.011%
18	12.087	1543	1547	1556	rVB2	4730	7668	0.30%	0.034%
19	12.275	1571	1579	1585	rBV	4490	8483	0.34%	0.038%
20	13.328	1754	1758	1763	rBV	7731	10865	0.43%	0.048%
21	13.934	1855	1861	1873	rVB	879385	1225297	48.63%	5.431%
22	14.210	1902	1908	1919	rBV	936623	1377140	54.65%	6.104%
23	14.522	1954	1961	1967	rBV	676254	1000680	39.71%	4.436%
24	14.746	1994	1999	2017	rBV	59792	122851	4.88%	0.545%
25	14.951	2032	2034	2039	rVB4	2909	3347	0.13%	0.015%
26	15.516	2123	2130	2141	rBV	1250609	1778364	70.57%	7.883%
27	15.645	2147	2152	2165	rBV	511174	692368	27.48%	3.069%
28	15.757	2165	2171	2176	rVB2	4753	6712	0.27%	0.030%
29	15.887	2185	2193	2200	rBV	20189	28149	1.12%	0.125%
30	17.016	2382	2385	2390	rBV2	2682	3693	0.15%	0.016%
31	17.275	2422	2429	2436	rBV	861739	1187445	47.12%	5.263%
32	17.375	2439	2446	2456	rVV	1523549	2147615	85.23%	9.519%
33	17.457	2456	2460	2464	rVB3	10722	14426	0.57%	0.064%
34	17.681	2494	2498	2502	rVB6	2735	4083	0.16%	0.018%
35	17.763	2507	2512	2515	rBV2	3030	3983	0.16%	0.018%
36	17.945	2538	2543	2545	rVB4	2346	2904	0.12%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112122\
 Data File : BN022795.D
 Acq On : 21 Nov 2022 20:04
 Operator : CG/JU
 Sample : N5690-13
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BGCF4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
 Title : SVOA CALIBRATION

37	18.039	2555	2559	2562	rBV6	2500	3555	0.14%	0.016%
38	18.163	2576	2580	2587	rBV	46406	66156	2.63%	0.293%
39	18.245	2591	2594	2599	rVV3	1985	3264	0.13%	0.014%
40	18.457	2627	2630	2635	rVB5	3291	3841	0.15%	0.017%
41	18.539	2639	2644	2645	rBV4	4960	6532	0.26%	0.029%
42	18.592	2650	2653	2659	rVB2	22138	28395	1.13%	0.126%
43	19.092	2735	2738	2742	rBV4	2733	3940	0.16%	0.017%
44	19.239	2759	2763	2769	rVB3	17967	23503	0.93%	0.104%
45	19.310	2769	2775	2782	rBV	19449	32929	1.31%	0.146%
46	19.451	2795	2799	2808	rBV2	24412	37051	1.47%	0.164%
47	19.598	2821	2824	2827	rVB4	5369	6549	0.26%	0.029%
48	19.681	2831	2838	2849	rBV	1732771	2416047	95.88%	10.709%
49	20.651	3001	3003	3008	rVB5	5904	5007	0.20%	0.022%
50	21.180	3089	3093	3105	rBV4	41407	105757	4.20%	0.469%
51	21.475	3138	3143	3151	rBV	1014215	1283872	50.95%	5.691%
52	22.569	3326	3329	3334	rVB2	33688	44425	1.76%	0.197%
53	23.116	3419	3422	3429	rVB	55112	84595	3.36%	0.375%
54	23.716	3516	3524	3540	rBV2	1205350	2519827	100.00%	11.169%
55	23.869	3543	3550	3563	rVB2	626617	1227688	48.72%	5.442%
56	24.463	3647	3651	3660	rVB	77083	161768	6.42%	0.717%




Sum of corrected areas: 22560238

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112122\
Data File : BN022795.D
Acq On : 21 Nov 2022 20:04
Operator : CG/JU
Sample : N5690-13
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGCF4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

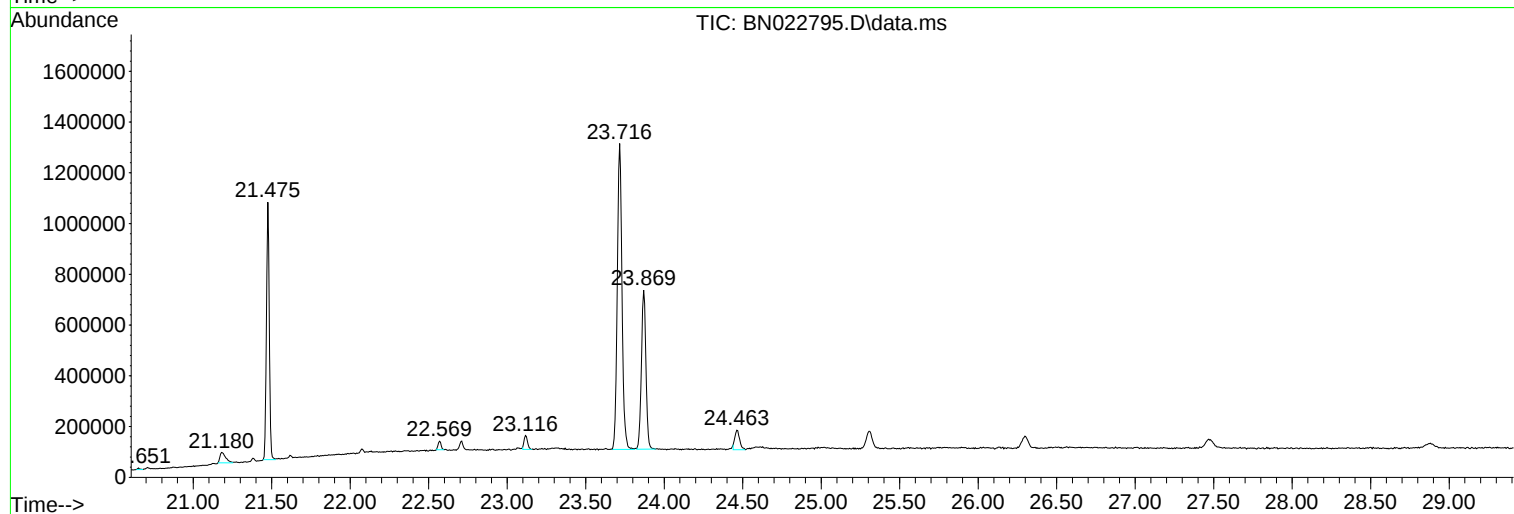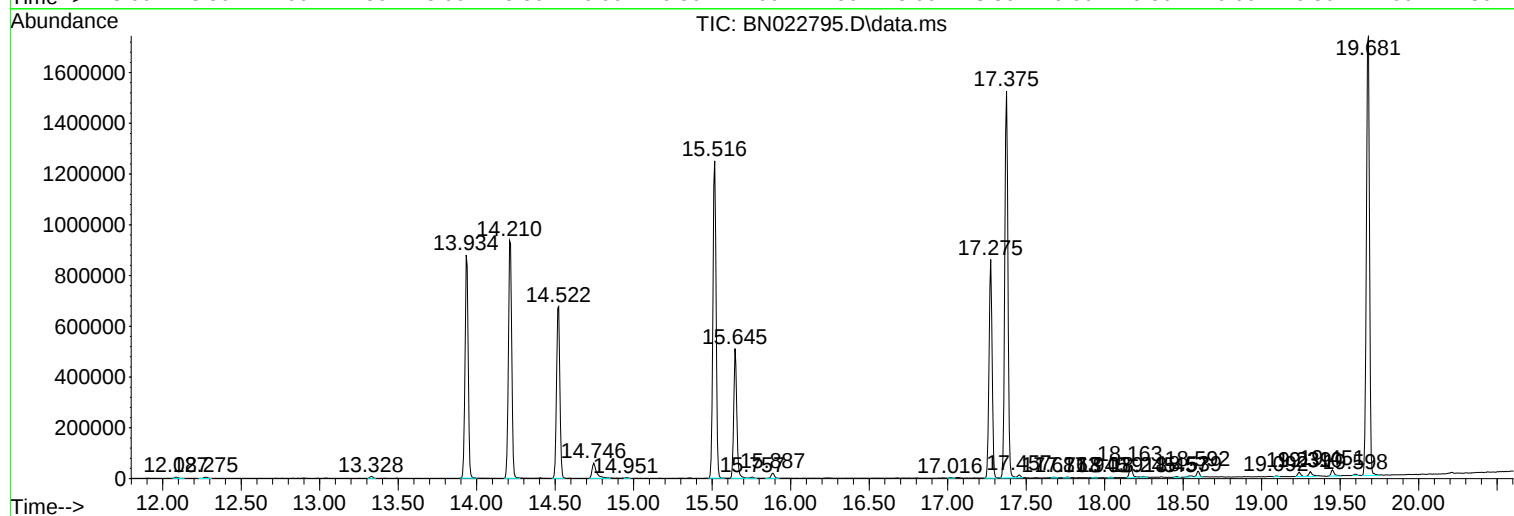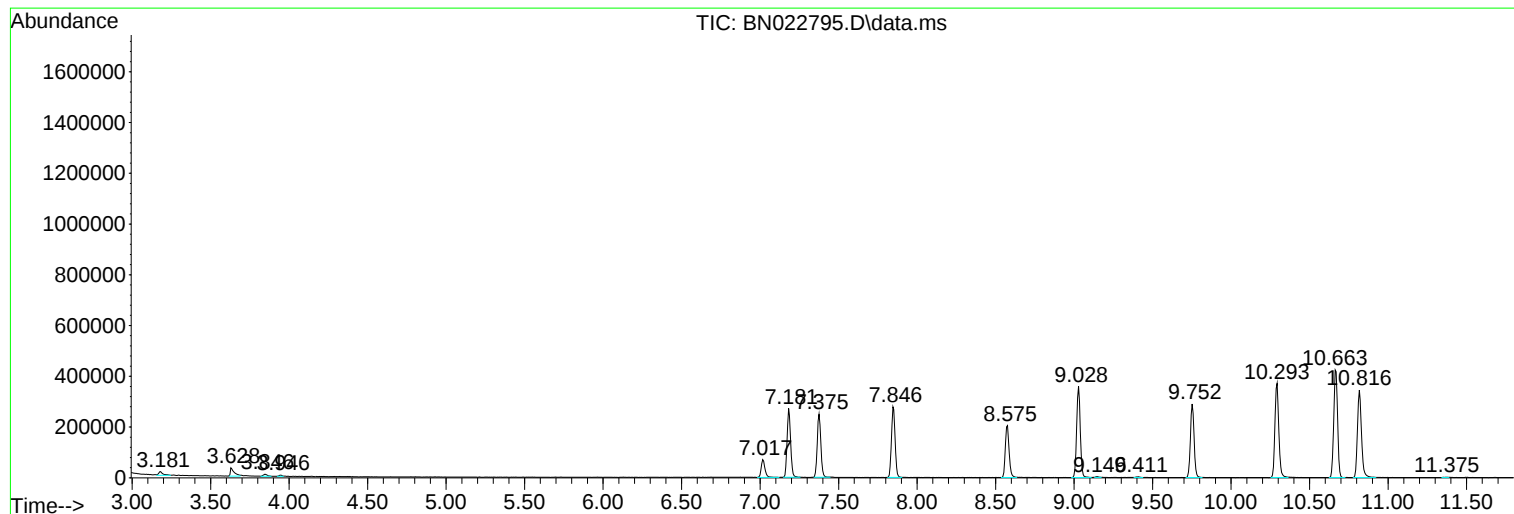

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112122\
Data File : BN022795.D
Acq On : 21 Nov 2022 20:04
Operator : CG/JU
Sample : N5690-13
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGCF4










Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
24.463	2.64 ng/ul	161768	Perylene-d12	23.869

Hit#	of 5	Tentative ID	MW	MolForm	CAS#	Qual
1		Tetratetracontane	619	C44H90	007098-22-8	90
2		Hexacosane	366	C26H54	000630-01-3	90
3		4-Methylheneicosane	310	C22H46	025117-29-7	90
4		Docosane	310	C22H46	000629-97-0	90
5		Docosane, 1-iodo-	436	C22H45I	1000406-31-9	90

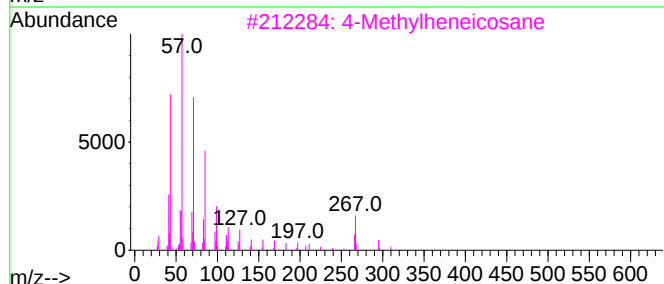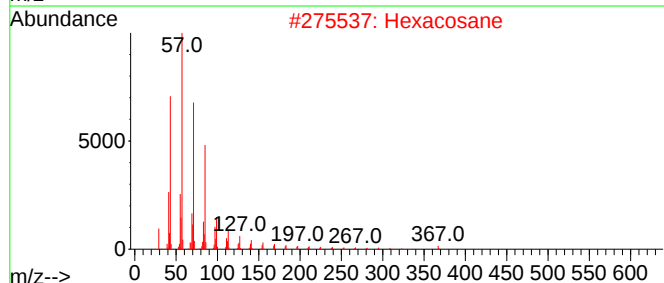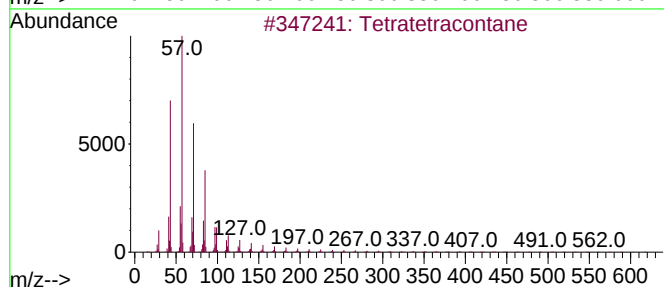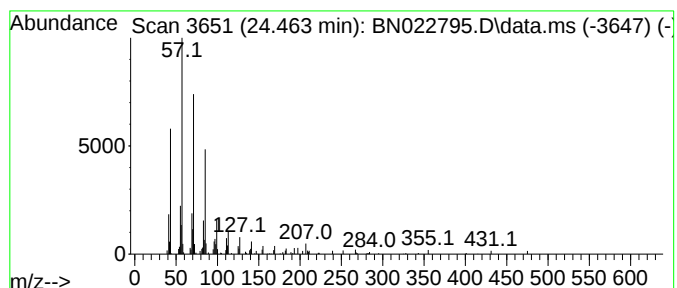

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112122\
Data File : BN022795.D
Acq On : 21 Nov 2022 20:04
Operator : CG/JU
Sample : N5690-13
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGCF4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	24.463	2.6	ng/u1	161768	6	23.869	1227690	20.0