

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112122\
 Data File : BN022800.D
 Acq On : 21 Nov 2022 23:08
 Operator : CG/JU
 Sample : N5690-03
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BGCE7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
 Title : SVOA CALIBRATION

Signal : TIC: BN022800.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.181	29	33	43	rVB	13318	21540	0.89%	0.097%
2	3.628	107	109	120	rBV	43734	80969	3.33%	0.364%
3	3.852	141	147	155	rVB2	8401	15173	0.62%	0.068%
4	3.946	159	163	166	rBV2	4663	6497	0.27%	0.029%
5	4.928	326	330	336	rVB4	2323	3814	0.16%	0.017%
6	7.016	679	685	703	rVB	71591	120334	4.95%	0.541%
7	7.181	706	713	725	rBV	272163	425644	17.50%	1.913%
8	7.375	739	746	756	rBV	253518	412341	16.95%	1.853%
9	7.446	756	758	764	rVB3	1707	2768	0.11%	0.012%
10	7.846	820	826	837	rBV	296827	472196	19.41%	2.122%
11	8.569	943	949	964	rBV	203435	348444	14.32%	1.566%
12	9.028	1020	1027	1036	rBV	357403	578551	23.78%	2.600%
13	9.405	1087	1091	1095	rVB2	2585	4346	0.18%	0.020%
14	9.752	1143	1150	1159	rBV	289176	470119	19.32%	2.113%
15	10.293	1234	1242	1259	rBV	360152	641650	26.38%	2.883%
16	10.663	1298	1305	1313	rBV	451531	748834	30.78%	3.365%
17	10.816	1324	1331	1352	rBV	277795	492590	20.25%	2.214%
18	12.087	1541	1547	1552	rVB3	3177	4973	0.20%	0.022%
19	12.269	1574	1578	1586	rVB	4430	8253	0.34%	0.037%
20	13.328	1754	1758	1762	rVB3	3341	5038	0.21%	0.023%
21	13.934	1852	1861	1871	rBV	881539	1223339	50.29%	5.497%
22	14.210	1901	1908	1924	rBV	908366	1332253	54.76%	5.987%
23	14.516	1954	1960	1971	rVB	689959	1038174	42.68%	4.665%
24	14.745	1993	1999	2020	rBV	54450	115499	4.75%	0.519%
25	14.957	2029	2035	2038	rVB4	5907	7858	0.32%	0.035%
26	15.516	2123	2130	2144	rBV	1251240	1770854	72.79%	7.958%
27	15.645	2146	2152	2167	rVB	469721	647123	26.60%	2.908%
28	15.751	2167	2170	2175	rVB3	3932	5194	0.21%	0.023%
29	15.887	2188	2193	2201	rVB2	3326	5229	0.21%	0.023%
30	17.275	2422	2429	2439	rBV	887498	1227209	50.45%	5.515%
31	17.375	2439	2446	2457	rVV	1487333	2091124	85.96%	9.397%
32	17.481	2461	2464	2467	rVB2	6620	7671	0.32%	0.034%
33	18.163	2576	2580	2590	rBV2	25589	33864	1.39%	0.152%
34	18.592	2649	2653	2657	rBV	10544	11841	0.49%	0.053%
35	19.239	2759	2763	2768	rBV3	16000	22761	0.94%	0.102%
36	19.310	2771	2775	2780	rBV	14925	21644	0.89%	0.097%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112122\
 Data File : BN022800.D
 Acq On : 21 Nov 2022 23:08
 Operator : CG/JU
 Sample : N5690-03
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BGCE7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
 Title : SVOA CALIBRATION

37	19.451	2795	2799	2804	rBV3	15358	22394	0.92%	0.101%
38	19.598	2821	2824	2827	rBV3	5821	6291	0.26%	0.028%
39	19.675	2831	2837	2848	rVV	1765470	2330156	95.78%	10.471%
40	21.180	3089	3093	3102	rBV6	20400	45644	1.88%	0.205%
41	21.474	3137	3143	3154	rBV	1014635	1344344	55.26%	6.041%
42	22.563	3325	3328	3334	rVB2	31608	44163	1.82%	0.198%
43	22.704	3348	3352	3358	rVB	65859	93702	3.85%	0.421%
44	23.110	3418	3421	3428	rVB2	49130	79892	3.28%	0.359%
45	23.710	3515	3523	3535	rBV2	1175721	2432723	100.00%	10.932%
46	23.863	3542	3549	3564	rVB2	641894	1292128	53.11%	5.806%
47	25.298	3789	3793	3802	rVB3	63396	136091	5.59%	0.612%




Sum of corrected areas: 22253239

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112122\
Data File : BN022800.D
Acq On : 21 Nov 2022 23:08
Operator : CG/JU
Sample : N5690-03
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGCE7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

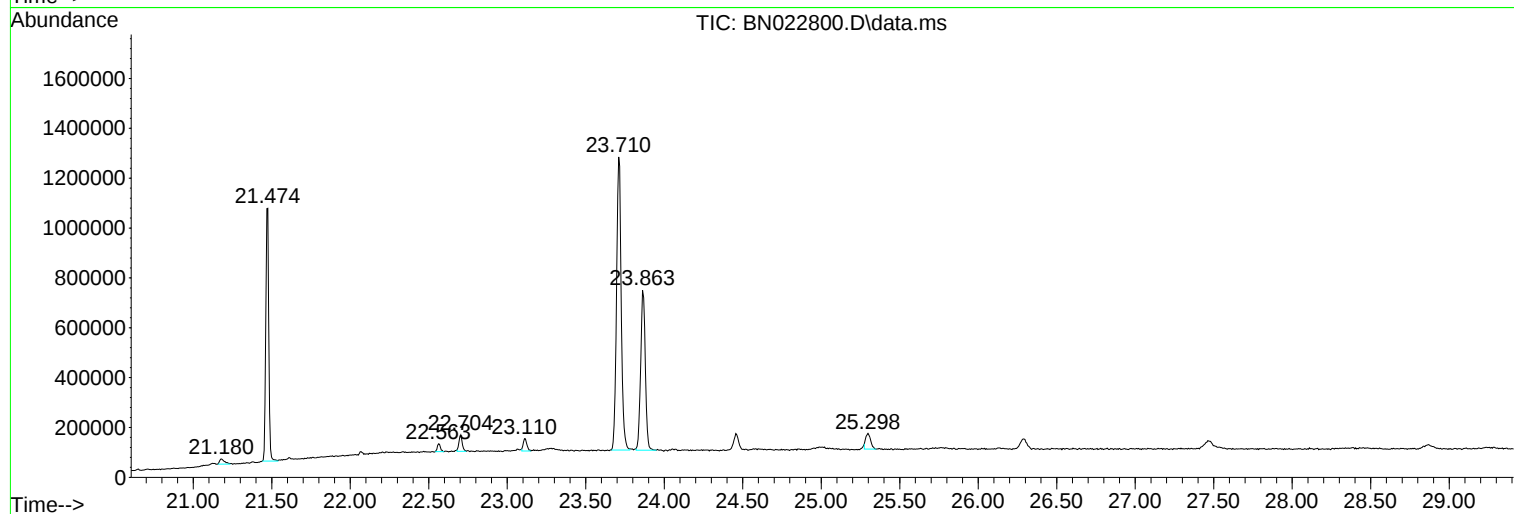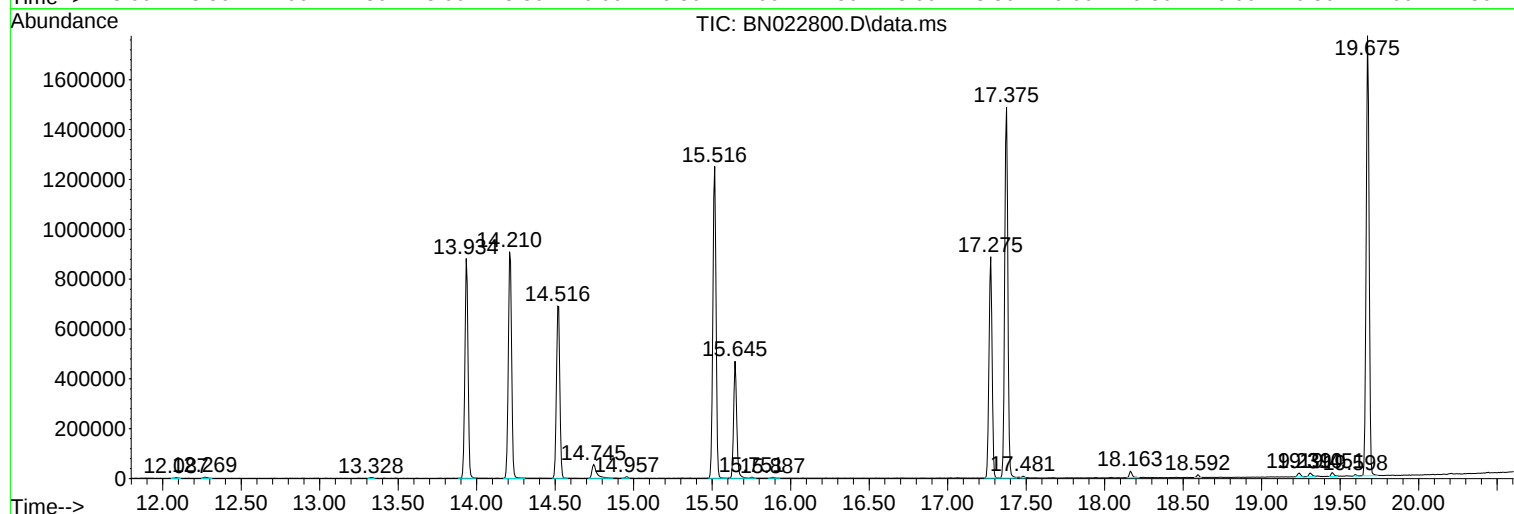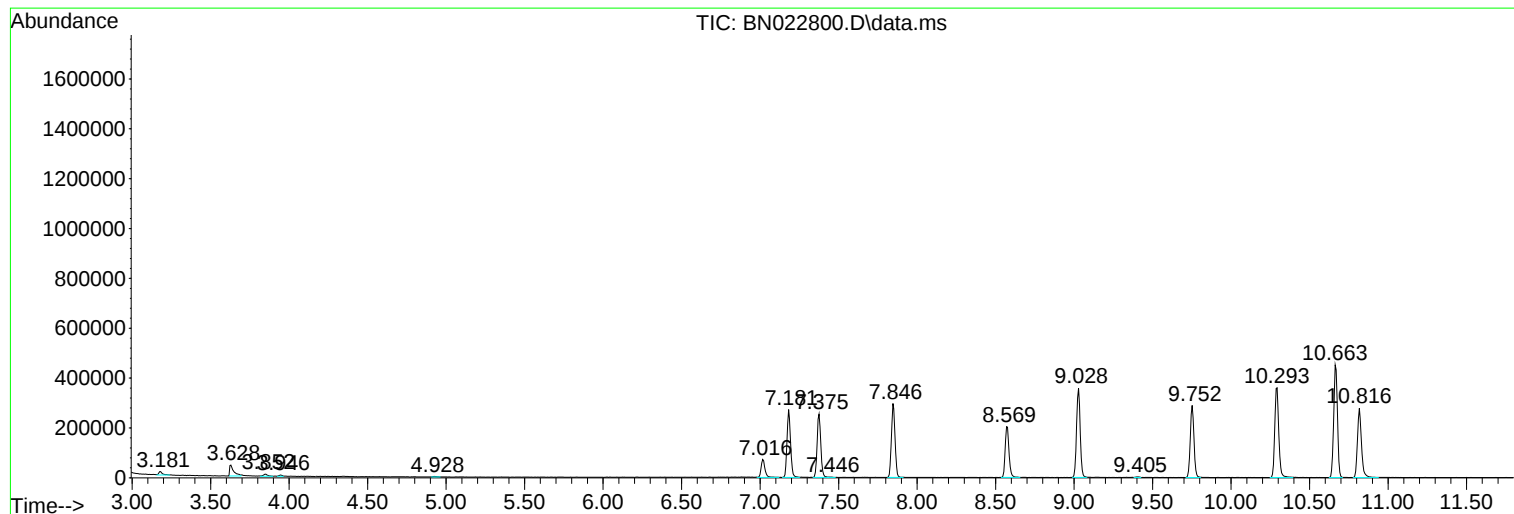

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112122\
Data File : BN022800.D
Acq On : 21 Nov 2022 23:08
Operator : CG/JU
Sample : N5690-03
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGCE7










Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
25.298	2.11 ng/ul	136091	Perylene-d12	23.863

Hit#	of 5	Tentative ID	MW	MolForm	CAS#	Qual
1		Eicosane	282	C20H42	000112-95-8	93
2		Heneicosane	296	C21H44	000629-94-7	91
3		Heneicosane	296	C21H44	000629-94-7	89
4		Pentacosane	352	C25H52	000629-99-2	87
5		Dotriacontane, 1-iodo-	576	C32H65I	1000406-32-4	87

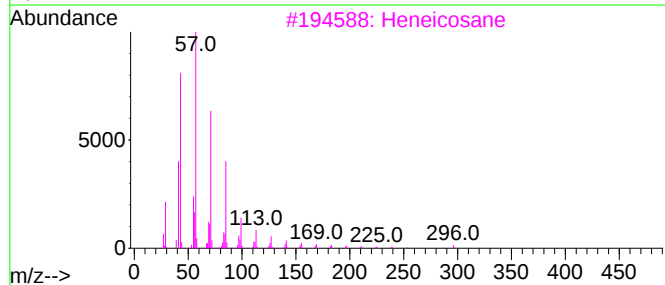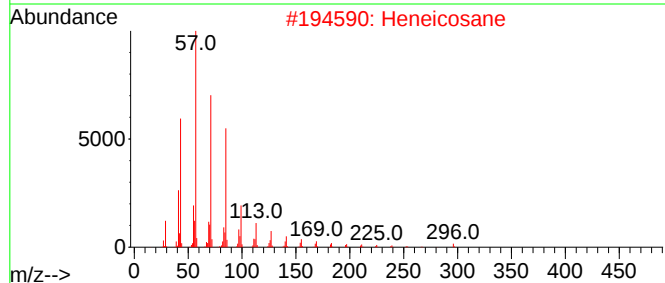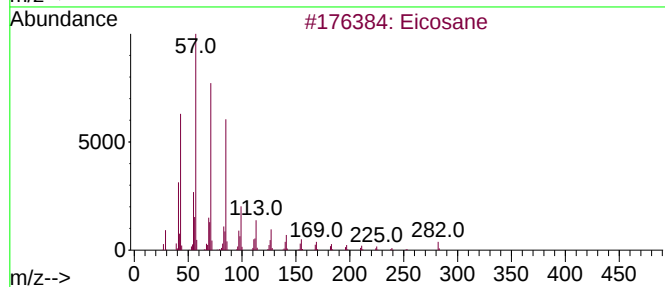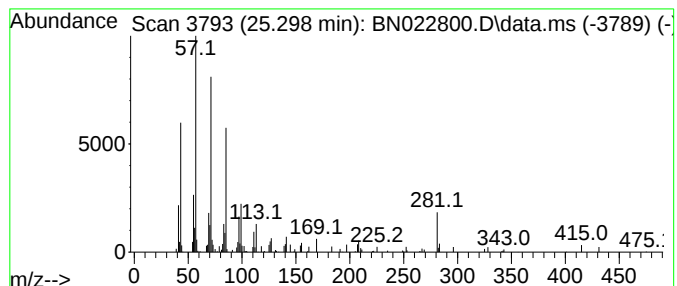

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112122\
Data File : BN022800.D
Acq On : 21 Nov 2022 23:08
Operator : CG/JU
Sample : N5690-03
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGCE7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	25.298	2.1	ng/u1	136091	6	23.863	1292130	20.0