

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112122\
 Data File : BN022806.D
 Acq On : 22 Nov 2022 02:48
 Operator : CG/JU
 Sample : N5690-09
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BGCD0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
 Title : SVOA CALIBRATION

Signal : TIC: BN022806.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.175	29	32	38	rBV	10285	13372	0.65%	0.074%
2	3.623	105	108	127	rBV	58837	112367	5.47%	0.624%
3	3.846	141	146	153	rVB2	5733	10702	0.52%	0.059%
4	3.946	158	163	167	rBV2	3813	6029	0.29%	0.033%
5	4.928	327	330	337	rVB4	1431	2587	0.13%	0.014%
6	7.016	680	685	698	rVB	58689	98392	4.79%	0.546%
7	7.181	705	713	722	rBV	223187	351518	17.10%	1.952%
8	7.375	739	746	757	rBV	199783	326902	15.91%	1.815%
9	7.846	819	826	836	rBV	221928	359619	17.50%	1.997%
10	8.569	942	949	961	rBV	169007	282546	13.75%	1.569%
11	9.028	1020	1027	1039	rBV	281722	472531	22.99%	2.623%
12	9.399	1086	1090	1095	rVB	2782	4820	0.23%	0.027%
13	9.752	1143	1150	1164	rVB	224934	367042	17.86%	2.038%
14	10.287	1235	1241	1260	rBV	283551	500902	24.37%	2.781%
15	10.663	1297	1305	1314	rBV	345950	571164	27.79%	3.171%
16	10.816	1324	1331	1346	rBV	306569	546974	26.61%	3.037%
17	12.087	1543	1547	1552	rBV	3588	5268	0.26%	0.029%
18	12.275	1574	1579	1586	rVB	3817	6876	0.33%	0.038%
19	13.328	1755	1758	1763	rVB2	5857	7279	0.35%	0.040%
20	13.934	1854	1861	1875	rVB	714439	991113	48.22%	5.503%
21	14.210	1902	1908	1918	rBV	771624	1103599	53.70%	6.127%
22	14.516	1954	1960	1969	rBV	558171	805322	39.18%	4.471%
23	14.745	1994	1999	2012	rBV	37265	83163	4.05%	0.462%
24	14.957	2030	2035	2038	rBV5	2288	2248	0.11%	0.012%
25	15.516	2123	2130	2139	rBV	1006064	1447840	70.45%	8.038%
26	15.645	2146	2152	2167	rVV	341660	464394	22.60%	2.578%
27	15.751	2167	2170	2177	rVB3	3671	4324	0.21%	0.024%
28	15.881	2189	2192	2197	rBV2	3197	4549	0.22%	0.025%
29	17.010	2378	2384	2388	rBV4	1127	2200	0.11%	0.012%
30	17.269	2422	2428	2438	rBV	678455	949063	46.18%	5.269%
31	17.369	2439	2445	2457	rVV	1175852	1708670	83.14%	9.486%
32	17.451	2457	2459	2461	rVV3	4365	5570	0.27%	0.031%
33	17.481	2461	2464	2468	rVB3	6701	8938	0.43%	0.050%
34	18.163	2574	2580	2588	rBV	20342	30130	1.47%	0.167%
35	18.592	2649	2653	2657	rVB	11299	13210	0.64%	0.073%
36	19.233	2758	2762	2769	rBV	11515	16309	0.79%	0.091%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112122\
 Data File : BN022806.D
 Acq On : 22 Nov 2022 02:48
 Operator : CG/JU
 Sample : N5690-09
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BGCD0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
 Title : SVOA CALIBRATION

37	19.310	2771	2775	2780	rBV	11693	16309	0.79%	0.091%
38	19.451	2795	2799	2803	rBV5	9696	13146	0.64%	0.073%
39	19.592	2821	2823	2828	rBV4	4312	6107	0.30%	0.034%
40	19.675	2831	2837	2850	rVV	1472957	1910413	92.96%	10.606%
41	21.175	3089	3092	3100	rVB5	23140	45228	2.20%	0.251%
42	21.469	3137	3142	3152	rBV	808686	1057392	51.45%	5.870%
43	23.110	3418	3421	3430	rVB2	42416	66205	3.22%	0.368%
44	23.710	3515	3523	3536	rVB	997635	2055197	100.00%	11.410%
45	23.863	3542	3549	3561	rVB	526942	1044098	50.80%	5.797%
46	24.457	3646	3650	3656	rVB3	59227	110335	5.37%	0.613%




Sum of corrected areas: 18011962

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112122\
Data File : BN022806.D
Acq On : 22 Nov 2022 02:48
Operator : CG/JU
Sample : N5690-09
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGCD0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

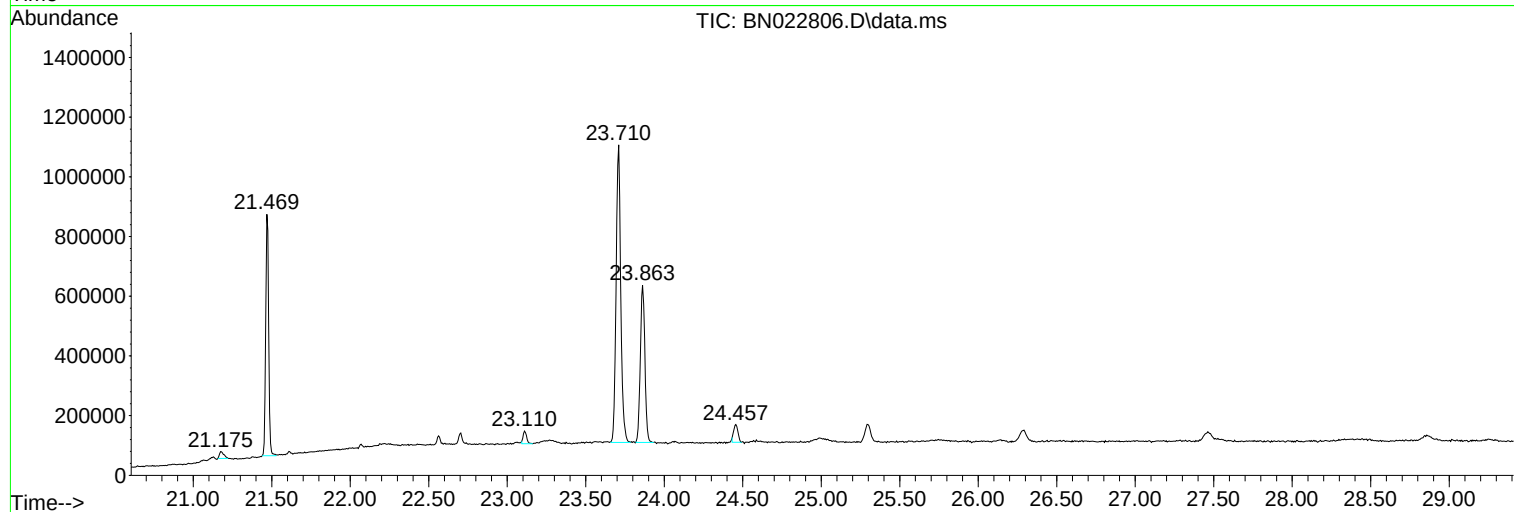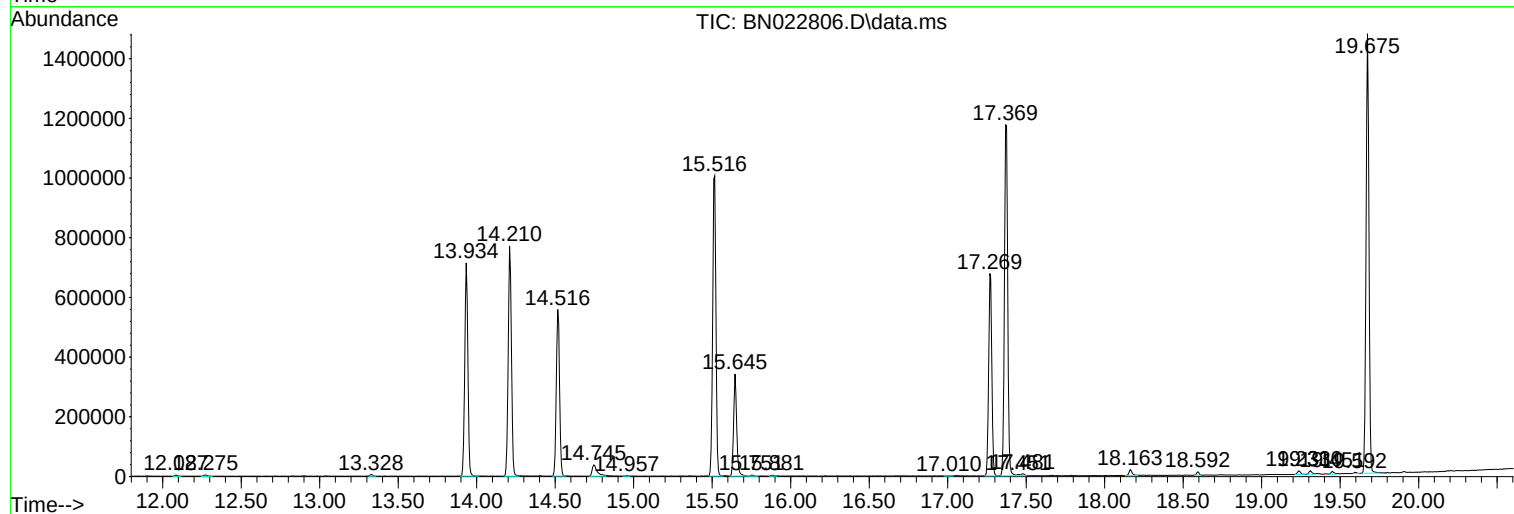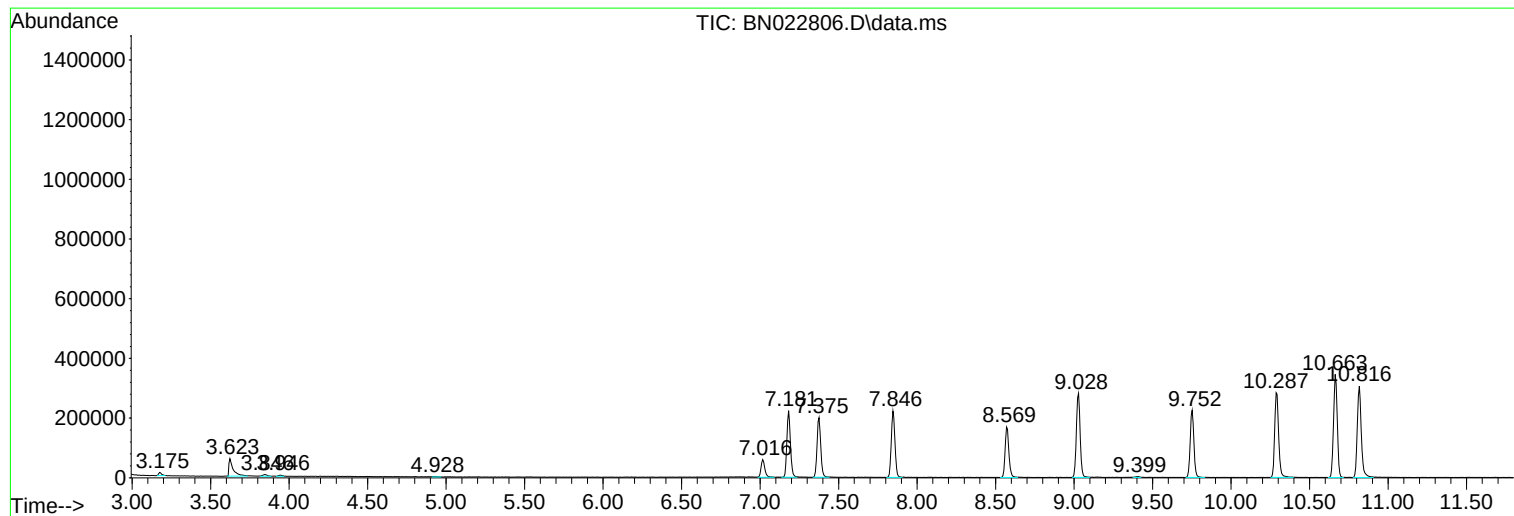

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112122\
Data File : BN022806.D
Acq On : 22 Nov 2022 02:48
Operator : CG/JU
Sample : N5690-09
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGCD0










Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
24.457	2.11 ng/ul	110335	Perylene-d12	23.863

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Octadecane	254	C18H38	000593-45-3	81
2			5,5,7,7-Tetraethylundecane	268	C19H40	1000360-42-0	80
3			Octacosane	394	C28H58	000630-02-4	80
4			Heneicosane, 11-(1-ethylpropyl)-	366	C26H54	055282-11-6	80
5			Tetracosane	338	C24H50	000646-31-1	80

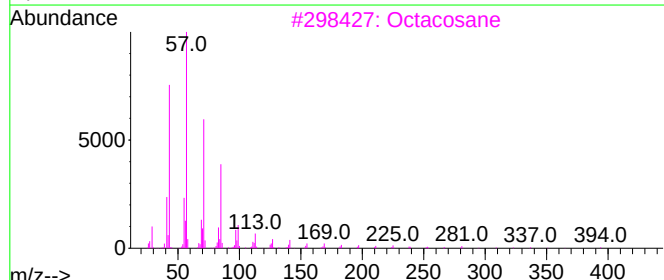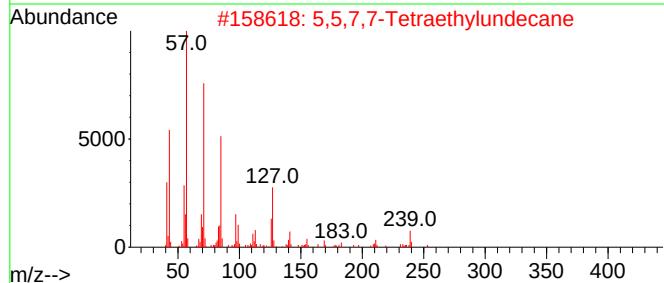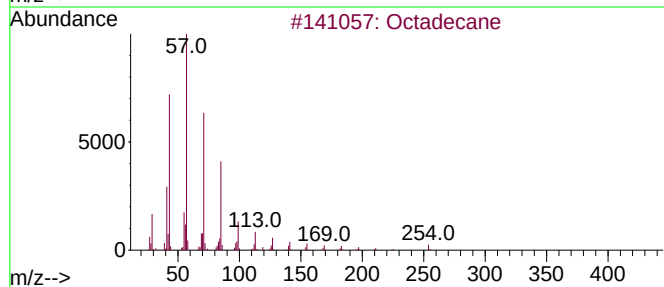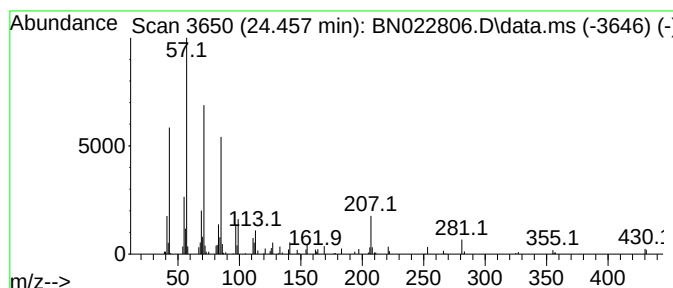

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112122\
Data File : BN022806.D
Acq On : 22 Nov 2022 02:48
Operator : CG/JU
Sample : N5690-09
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGCD0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	24.457	2.1	ng/u1	110335	6	23.863	1044100	20.0