

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112122\
 Data File : BN022808.D
 Acq On : 22 Nov 2022 04:37
 Operator : CG/JU
 Sample : PB149188BL
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK188

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
 Title : SVOA CALIBRATION

Signal : TIC: BN022808.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.175	28	32	43	rVB	21588	34833	1.63%	0.155%
2	3.611	103	106	123	rBV	274734	458775	21.41%	2.043%
3	3.940	158	162	171	rVB2	4438	7613	0.36%	0.034%
4	7.016	678	685	701	rBV	366012	597272	27.87%	2.660%
5	7.181	706	713	725	rBV	300617	467286	21.81%	2.081%
6	7.375	739	746	758	rVB	355957	582927	27.20%	2.596%
7	7.846	820	826	835	rBV	241401	385218	17.98%	1.715%
8	8.569	942	949	963	rBV	461289	752871	35.13%	3.353%
9	9.028	1019	1027	1043	rBV	372126	623548	29.10%	2.777%
10	9.751	1143	1150	1159	rBV	323359	536992	25.06%	2.391%
11	10.287	1234	1241	1261	rBV	452330	769593	35.91%	3.427%
12	10.663	1298	1305	1315	rBV	381386	615250	28.71%	2.740%
13	10.816	1323	1331	1347	rBV	450270	819678	38.25%	3.650%
14	12.275	1574	1579	1588	rVB2	4924	9113	0.43%	0.041%
15	13.410	1766	1772	1776	rVB2	1922	2557	0.12%	0.011%
16	13.934	1854	1861	1875	rVB	913932	1224126	57.13%	5.451%
17	14.210	1901	1908	1921	rBV	978770	1387924	64.77%	6.181%
18	14.516	1953	1960	1969	rBV	605694	859760	40.12%	3.829%
19	14.734	1991	1997	2017	rBV	389355	653515	30.50%	2.910%
20	15.510	2123	2129	2139	rBV	1225160	1729800	80.72%	7.703%
21	15.645	2146	2152	2167	rBV	440703	612027	28.56%	2.726%
22	15.751	2167	2170	2174	rVB2	3998	4918	0.23%	0.022%
23	16.716	2328	2334	2339	rBV4	1469	2577	0.12%	0.011%
24	17.057	2389	2392	2398	rVB4	1332	2352	0.11%	0.010%
25	17.269	2422	2428	2439	rBV	706861	1003094	46.81%	4.467%
26	17.369	2439	2445	2459	rVV	1342652	1891676	88.28%	8.424%
27	19.233	2759	2762	2766	rVB2	13182	15916	0.74%	0.071%
28	19.310	2771	2775	2780	rBV	12688	15876	0.74%	0.071%
29	19.674	2831	2837	2850	rBV	1600803	2115439	98.72%	9.421%
30	21.474	3137	3143	3152	rBV	825389	1105913	51.61%	4.925%
31	23.710	3515	3523	3534	rBV2	1076893	2142888	100.00%	9.543%
32	23.862	3542	3549	3560	rVB2	513843	1024018	47.79%	4.560%


Sum of corrected areas: 22455345

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112122\
Data File : BN022808.D
Acq On : 22 Nov 2022 04:37
Operator : CG/JU
Sample : PB149188BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK188

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

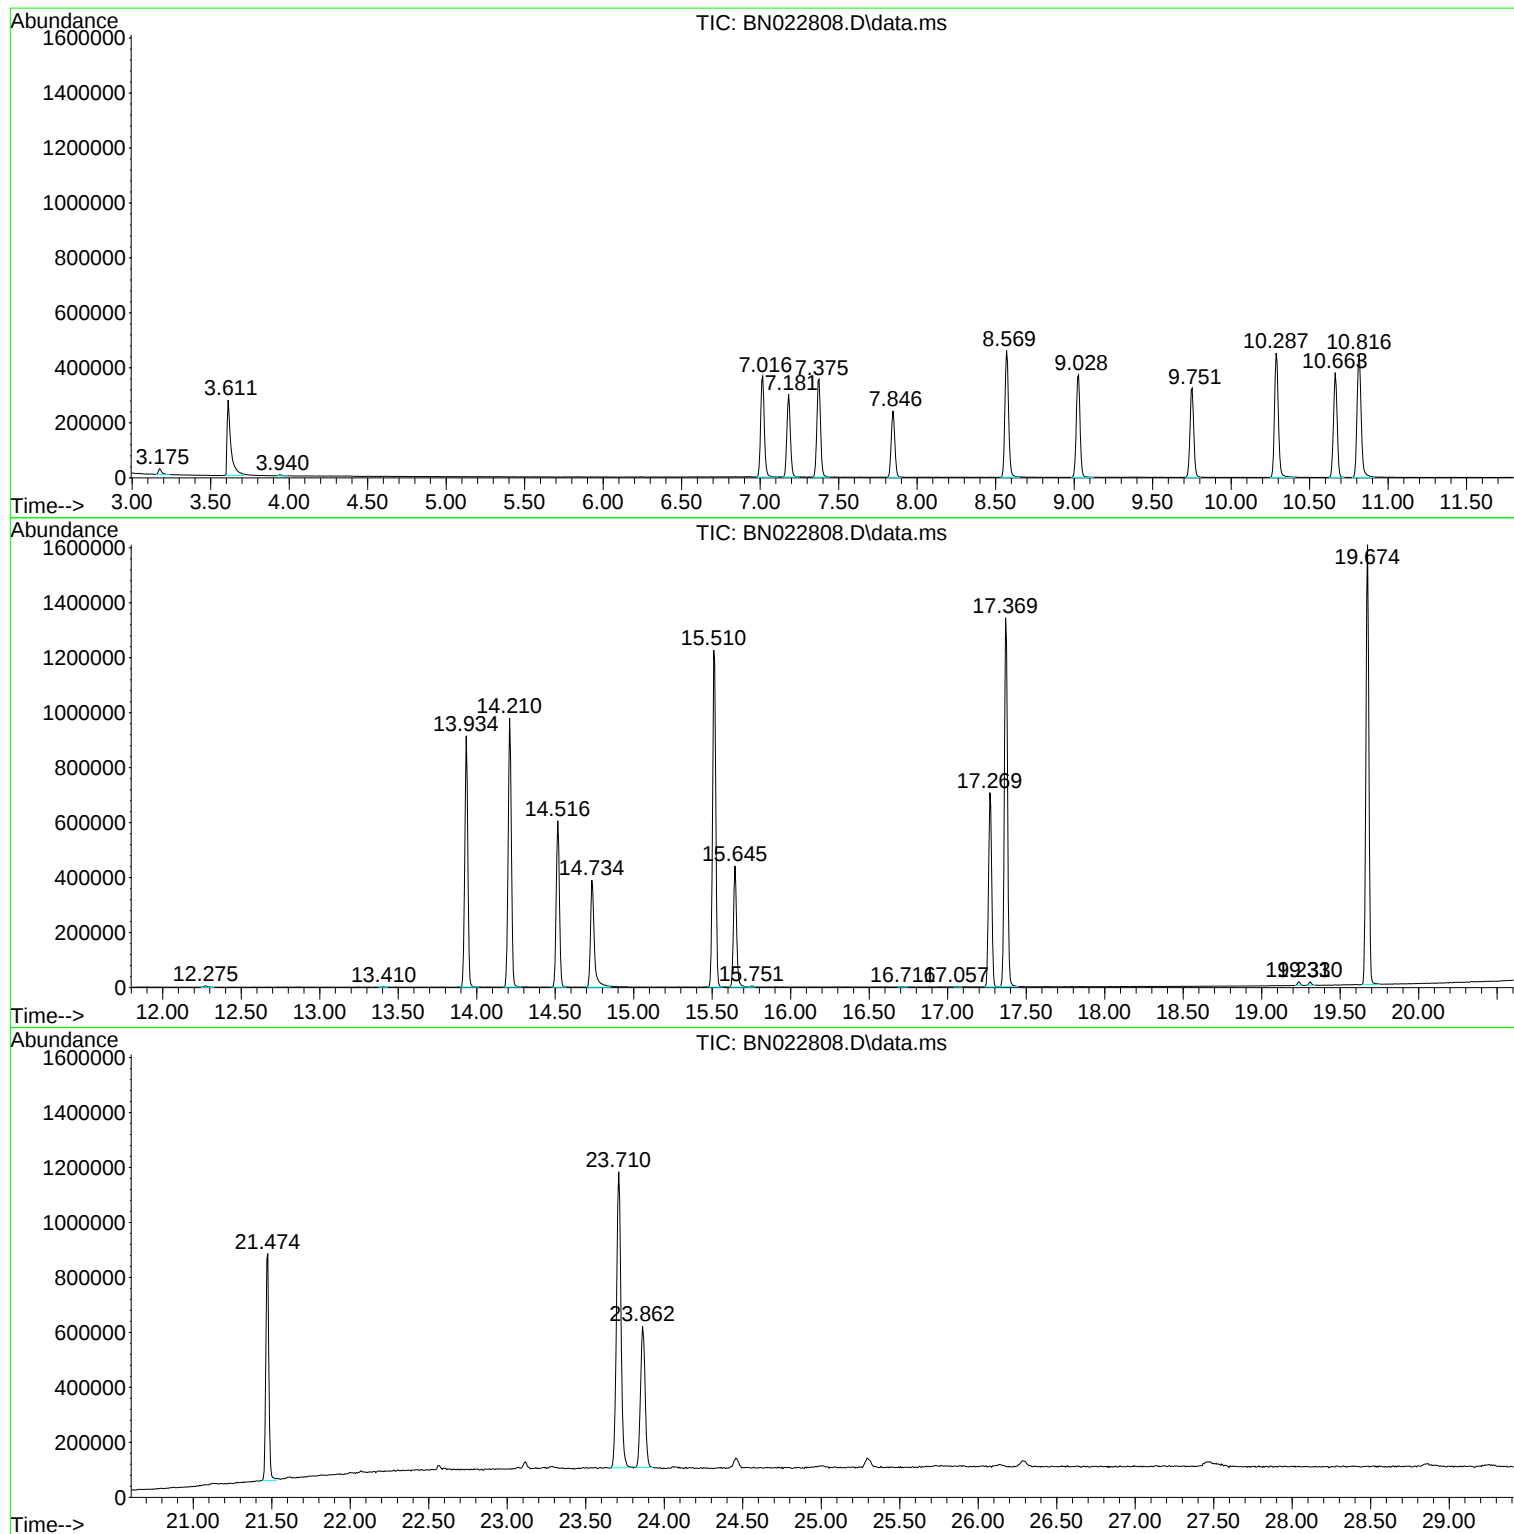

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112122\
Data File : BN022808.D
Acq On : 22 Nov 2022 04:37
Operator : CG/JU
Sample : PB149188BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK188

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112122\
Data File : BN022808.D
Acq On : 22 Nov 2022 04:37
Operator : CG/JU
Sample : PB149188BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK188

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc
