

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112122\
 Data File : BN022810.D
 Acq On : 22 Nov 2022 05:50
 Operator : CG/JU
 Sample : N5690-10
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BGCG7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
 Title : SVOA CALIBRATION

Signal : TIC: BN022810.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.175	28	32	45	rVB	14719	25158	1.48%	0.153%
2	3.617	104	107	123	rBV	78724	141722	8.33%	0.859%
3	3.846	141	146	152	rVB	7381	11148	0.66%	0.068%
4	3.940	157	162	168	rBV	4157	6955	0.41%	0.042%
5	4.928	326	330	337	rVB3	1374	2617	0.15%	0.016%
6	7.016	679	685	694	rBV	52473	88403	5.20%	0.536%
7	7.181	705	713	724	rBV	184581	295805	17.39%	1.794%
8	7.369	739	745	757	rBV	171129	288376	16.95%	1.749%
9	7.846	819	826	834	rBV	232722	367130	21.58%	2.226%
10	8.569	943	949	961	rBV	149422	248088	14.58%	1.505%
11	9.022	1019	1026	1042	rBV	230785	396552	23.31%	2.405%
12	9.405	1085	1091	1097	rVB4	4318	7977	0.47%	0.048%
13	9.752	1142	1150	1161	rBV	189033	317808	18.68%	1.927%
14	10.287	1234	1241	1257	rBV	252791	444067	26.11%	2.693%
15	10.663	1298	1305	1316	rBV	358656	596482	35.07%	3.617%
16	10.816	1324	1331	1344	rBV	302460	542562	31.90%	3.290%
17	12.087	1542	1547	1554	rBV2	6375	9839	0.58%	0.060%
18	12.275	1574	1579	1587	rVB5	2909	5579	0.33%	0.034%
19	12.716	1651	1654	1658	rBV4	1380	1733	0.10%	0.011%
20	12.899	1681	1685	1688	rVB2	2085	2635	0.15%	0.016%
21	12.987	1696	1700	1705	rBV3	1550	1941	0.11%	0.012%
22	13.034	1705	1708	1713	rVV	1640	2019	0.12%	0.012%
23	13.328	1752	1758	1766	rVB	10648	14408	0.85%	0.087%
24	13.934	1852	1861	1872	rBV	585712	828748	48.72%	5.026%
25	14.210	1901	1908	1920	rBV	650429	916075	53.85%	5.556%
26	14.404	1937	1941	1946	rVB3	2740	3573	0.21%	0.022%
27	14.516	1953	1960	1968	rBV	600991	850311	49.99%	5.157%
28	14.745	1993	1999	2017	rBV	35352	81923	4.82%	0.497%
29	15.351	2099	2102	2105	rVB3	1854	2329	0.14%	0.014%
30	15.510	2123	2129	2139	rVV	876258	1238960	72.84%	7.514%
31	15.645	2146	2152	2163	rBV	300233	414572	24.37%	2.514%
32	15.751	2167	2170	2175	rVB4	2547	3550	0.21%	0.022%
33	15.881	2187	2192	2198	rBV	17935	24488	1.44%	0.149%
34	17.016	2381	2385	2388	rBV4	1315	1884	0.11%	0.011%
35	17.063	2389	2393	2396	rVB3	1732	2389	0.14%	0.014%
36	17.269	2422	2428	2438	rBV	700058	980945	57.67%	5.949%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112122\
 Data File : BN022810.D
 Acq On : 22 Nov 2022 05:50
 Operator : CG/JU
 Sample : N5690-10
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BGCG7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
 Title : SVOA CALIBRATION

37	17.369	2439	2445	2455	rBV	1098375	1485778	87.35%	9.011%
38	17.451	2455	2459	2463	rBV	13367	16287	0.96%	0.099%
39	17.551	2473	2476	2482	rBV3	1382	2166	0.13%	0.013%
40	18.163	2575	2580	2589	rBV	51902	73306	4.31%	0.445%
41	18.233	2591	2592	2599	rVB5	1588	2626	0.15%	0.016%
42	18.363	2610	2614	2616	rVB5	1844	2435	0.14%	0.015%
43	18.592	2649	2653	2658	rVB2	23045	26345	1.55%	0.160%
44	18.733	2674	2677	2680	rBV4	1369	2056	0.12%	0.012%
45	19.233	2758	2762	2767	rBV3	11233	15304	0.90%	0.093%
46	19.310	2770	2775	2781	rBV	11382	19406	1.14%	0.118%
47	19.445	2794	2798	2804	rBV4	17746	25573	1.50%	0.155%
48	19.545	2811	2815	2818	rBV3	2098	3750	0.22%	0.023%
49	19.592	2820	2823	2827	rVB2	6306	7987	0.47%	0.048%
50	19.675	2830	2837	2846	rBV	1197282	1657066	97.42%	10.049%
51	20.645	3000	3002	3006	rVB4	4910	3427	0.20%	0.021%
52	21.175	3088	3092	3106	rBV2	51798	142507	8.38%	0.864%
53	21.375	3123	3126	3130	rBV	45587	50485	2.97%	0.306%
54	21.469	3137	3142	3150	rBV	837842	1059801	62.30%	6.427%
55	23.704	3515	3522	3536	rVB2	806374	1701013	100.00%	10.316%
56	23.863	3542	3549	3563	rVB2	502159	1023055	60.14%	6.204%


Sum of corrected areas: 16489124

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112122\
Data File : BN022810.D
Acq On : 22 Nov 2022 05:50
Operator : CG/JU
Sample : N5690-10
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGCG7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

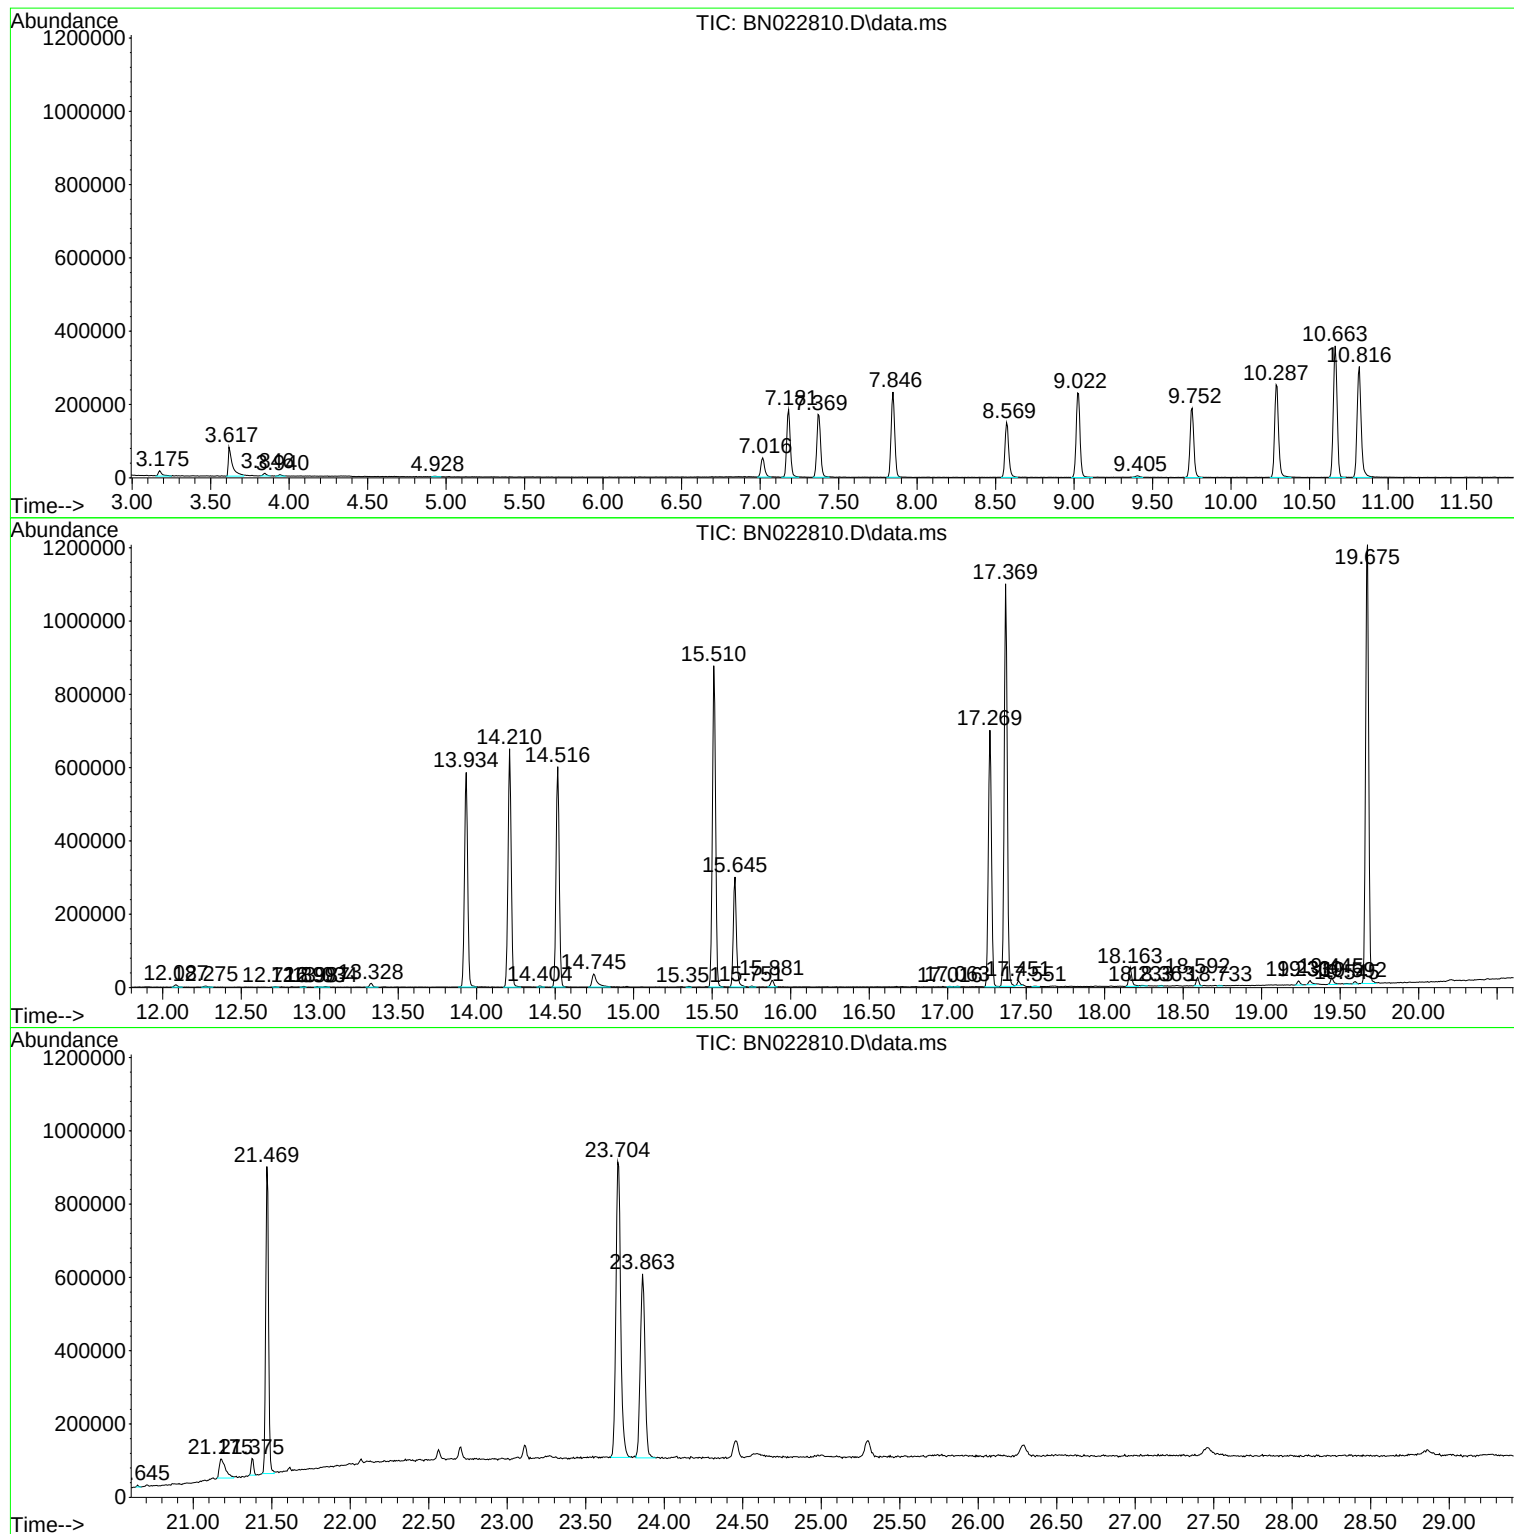

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112122\
Data File : BN022810.D
Acq On : 22 Nov 2022 05:50
Operator : CG/JU
Sample : N5690-10
Misc :
ALS Vial : 32 Sample Multiplier: 1










Instrument :
BNA_N
ClientSampleId :
BGCG7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD		R.T.	
21.174	2.69 ng/ul	142507	Chrysene-d12		21.469	
Hit# of 5	Tentative ID		MW	MolForm	CAS#	Qual
1	1-Nonadecene		266	C19H38	018435-45-5	98
2	n-Tetracosanol-1		354	C24H50O	000506-51-4	95
3	Trifluoroacetoxy hexadecane		338	C18H33F3O2	006222-03-3	95
4	Heptadecyl heptafluorobutyrate		452	C21H35F7O2	959085-66-6	95
5	Behenic alcohol		326	C22H46O	000661-19-8	95

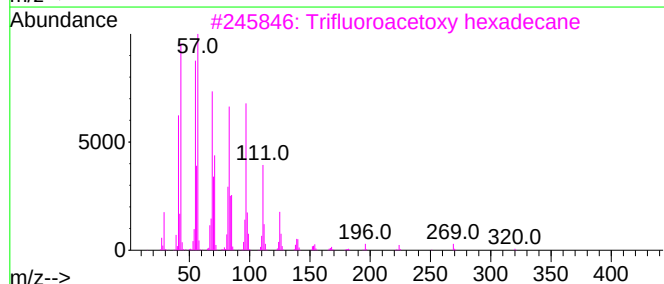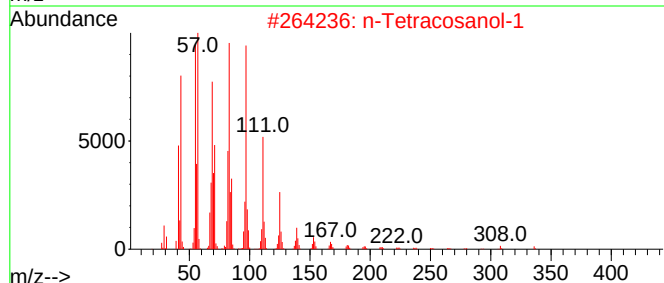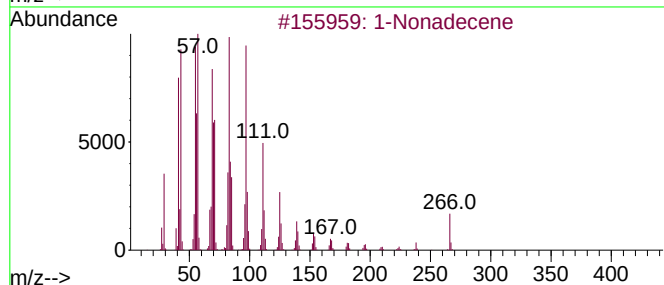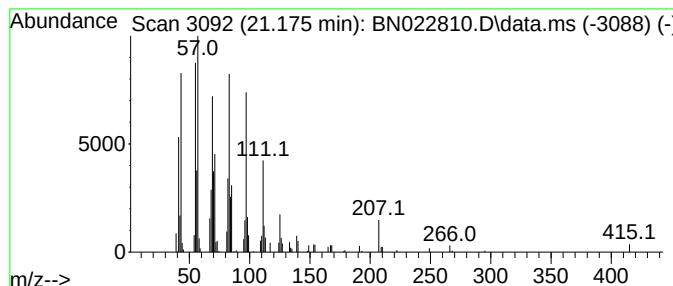

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112122\
Data File : BN022810.D
Acq On : 22 Nov 2022 05:50
Operator : CG/JU
Sample : N5690-10
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGCG7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	21.174	2.7	ng/u1	142507	5	21.469	1059800	20.0