

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112122\
 Data File : BN022829.D
 Acq On : 22 Nov 2022 17:51
 Operator : CG/JU
 Sample : PB149117BL
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK117

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
 Title : SVOA CALIBRATION

Signal : TIC: BN022829.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.176	29	32	39	rVB	17792	23298	1.34%	0.120%
2	3.611	104	106	132	rBV	215551	375217	21.60%	1.925%
3	3.940	159	162	169	rVB3	3869	6151	0.35%	0.032%
4	6.458	587	590	593	rBV3	1180	1753	0.10%	0.009%
5	7.011	678	684	704	rVB	282661	470633	27.09%	2.415%
6	7.181	707	713	725	rBV	232222	363947	20.95%	1.867%
7	7.369	736	745	758	rBV	283324	457482	26.33%	2.347%
8	7.846	819	826	835	rBV	263071	411585	23.69%	2.112%
9	8.569	941	949	960	rBV	367075	594059	34.19%	3.048%
10	9.022	1019	1026	1041	rBV	290969	491068	28.26%	2.520%
11	9.752	1142	1150	1159	rBV	249184	421891	24.28%	2.165%
12	10.287	1235	1241	1255	rBV	356804	601128	34.60%	3.084%
13	10.663	1298	1305	1314	rVB	401484	661818	38.09%	3.396%
14	10.816	1323	1331	1347	rBV	359443	651769	37.51%	3.344%
15	12.275	1573	1579	1586	rBV3	3810	7298	0.42%	0.037%
16	13.934	1854	1861	1873	rBV	712693	985187	56.70%	5.055%
17	14.210	1902	1908	1921	rBV	784357	1108758	63.82%	5.689%
18	14.516	1954	1960	1970	rBV	660959	935435	53.84%	4.800%
19	14.734	1991	1997	2014	rBV	306264	524520	30.19%	2.691%
20	15.510	2123	2129	2139	rBV	1009794	1398362	80.48%	7.175%
21	15.645	2146	2152	2166	rBV	357478	486360	27.99%	2.496%
22	15.751	2166	2170	2173	rVV	3173	3308	0.19%	0.017%
23	17.269	2422	2428	2437	rBV	793539	1112178	64.01%	5.707%
24	17.369	2438	2445	2457	rBV	1154028	1576662	90.75%	8.090%
25	19.233	2758	2762	2766	rBV2	11520	14903	0.86%	0.076%
26	19.310	2770	2775	2779	rBV	9515	13195	0.76%	0.068%
27	19.675	2831	2837	2848	rBV	1294095	1737436	100.00%	8.915%
28	21.475	3137	3143	3152	rBV	954525	1205277	69.37%	6.184%
29	23.710	3516	3523	3534	rVB2	861539	1716404	98.79%	8.807%
30	23.869	3543	3550	3563	rVB	542417	1131771	65.14%	5.807%




Sum of corrected areas: 19488853

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112122\
Data File : BN022829.D
Acq On : 22 Nov 2022 17:51
Operator : CG/JU
Sample : PB149117BL
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK117

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

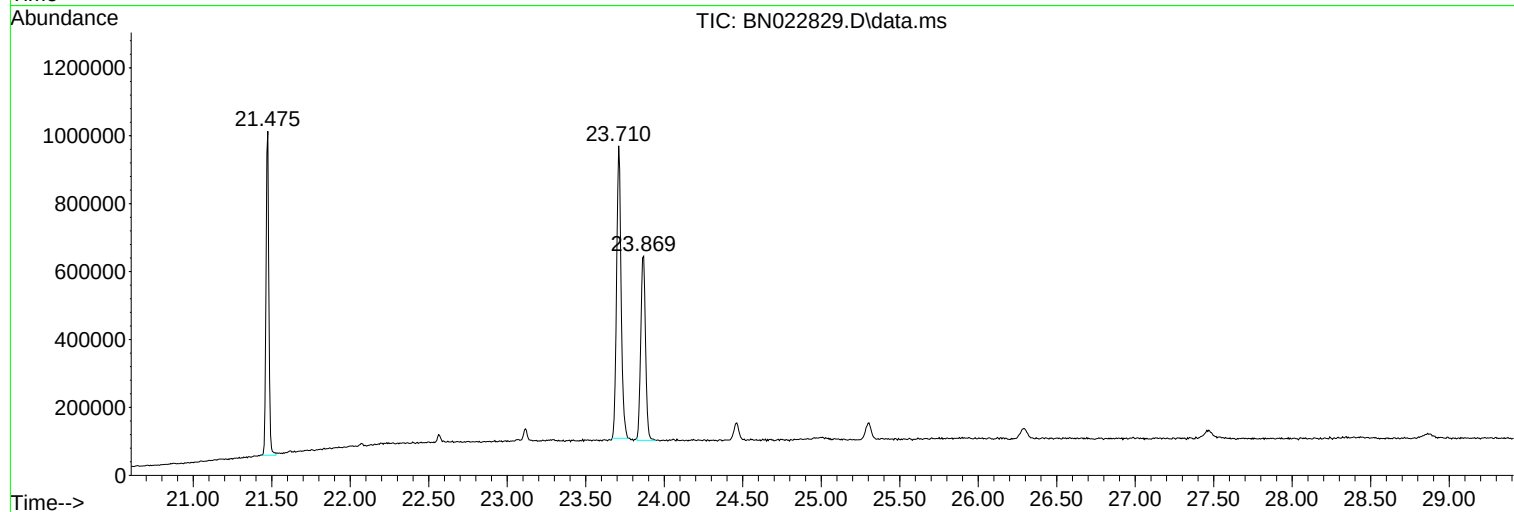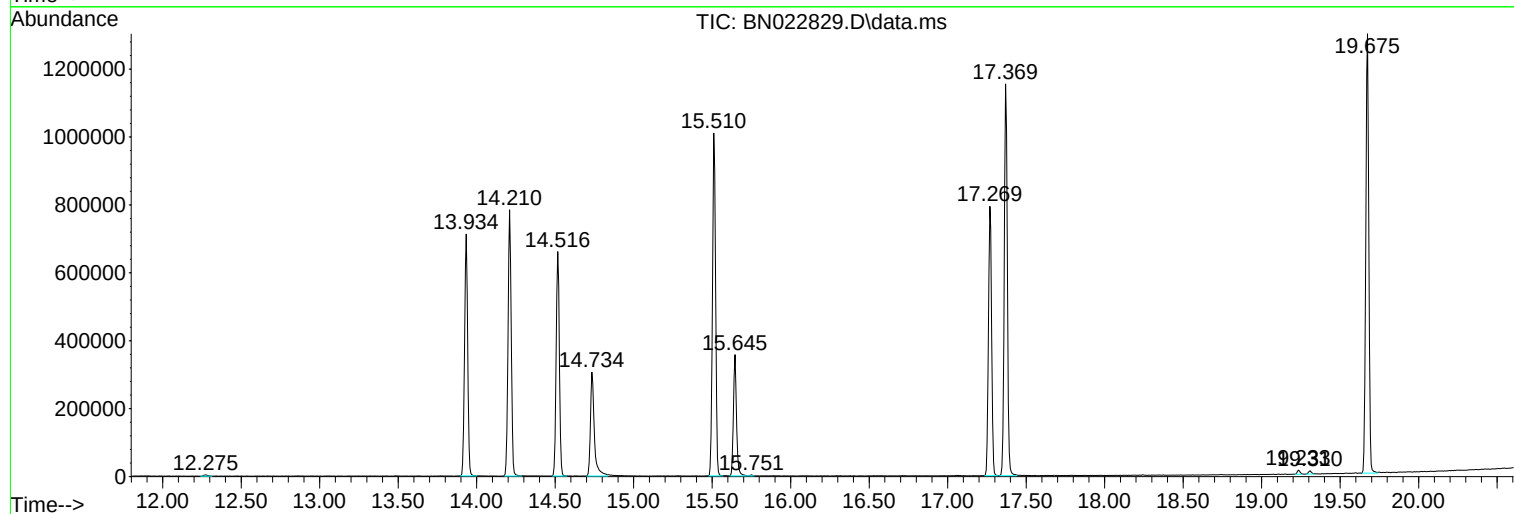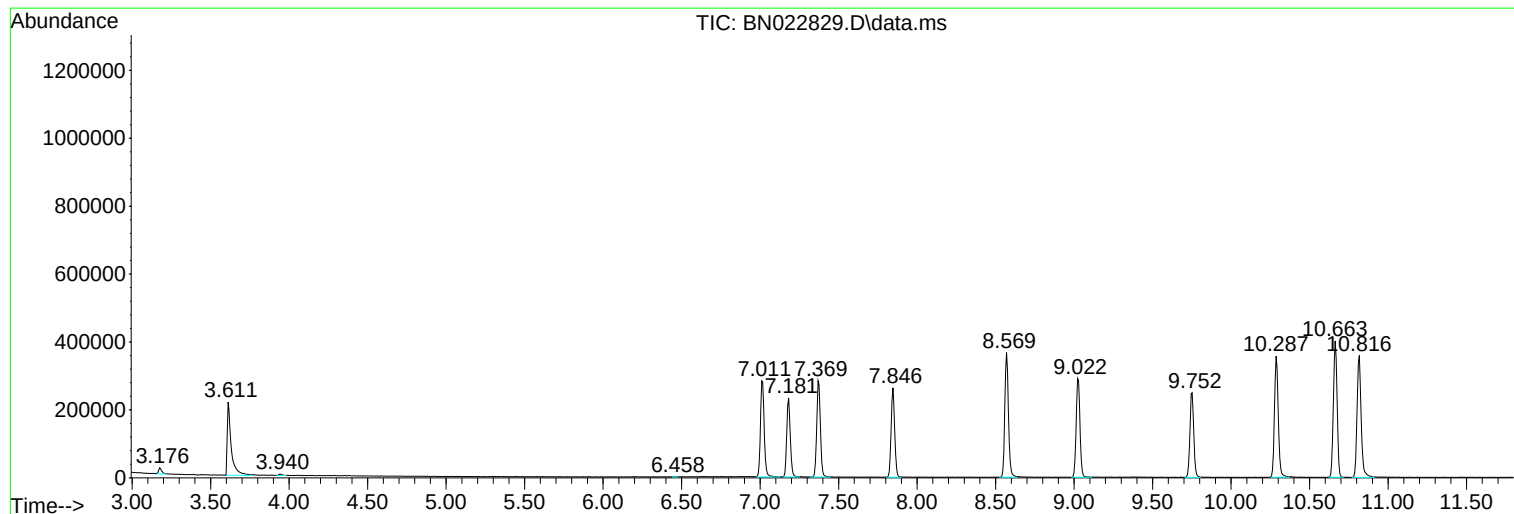

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112122\
Data File : BN022829.D
Acq On : 22 Nov 2022 17:51
Operator : CG/JU
Sample : PB149117BL
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK117

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112122\
Data File : BN022829.D
Acq On : 22 Nov 2022 17:51
Operator : CG/JU
Sample : PB149117BL
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK117

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc