

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112122\
 Data File : BN022830.D
 Acq On : 22 Nov 2022 18:29
 Operator : CG/JU
 Sample : PB149044BL
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK044

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
 Title : SVOA CALIBRATION

Signal : TIC: BN022830.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.176	28	32	39	rBV	16824	23257	1.33%	0.125%
2	3.611	103	106	128	rBV	210106	368448	21.02%	1.977%
3	3.940	159	162	168	rVB2	3286	4676	0.27%	0.025%
4	7.011	678	684	701	rVB	297774	492200	28.08%	2.641%
5	7.181	707	713	724	rBV	243395	381744	21.78%	2.048%
6	7.369	739	745	758	rBV	295780	483554	27.59%	2.594%
7	7.846	820	826	838	rBV	205178	331386	18.91%	1.778%
8	8.569	943	949	963	rBV	390094	625507	35.69%	3.356%
9	9.022	1019	1026	1036	rBV	304668	510787	29.14%	2.740%
10	9.752	1142	1150	1160	rBV	262234	442371	25.24%	2.373%
11	10.287	1233	1241	1254	rBV	377254	631950	36.05%	3.390%
12	10.663	1298	1305	1313	rBV	323474	531203	30.31%	2.850%
13	10.816	1323	1331	1348	rBV	370242	672326	38.36%	3.607%
14	11.528	1448	1452	1457	rBV2	786	1799	0.10%	0.010%
15	12.275	1571	1579	1586	rVB3	3480	7280	0.42%	0.039%
16	13.934	1855	1861	1873	rVB	754510	1020366	58.21%	5.474%
17	14.210	1901	1908	1918	rBV	797174	1146148	65.39%	6.149%
18	14.516	1954	1960	1971	rVB	517293	742913	42.39%	3.986%
19	14.734	1991	1997	2016	rBV	311298	534176	30.48%	2.866%
20	15.510	2123	2129	2138	rBV	1017418	1442524	82.30%	7.739%
21	15.645	2146	2152	2165	rBV	364693	497599	28.39%	2.669%
22	15.751	2167	2170	2175	rVB3	3027	3587	0.20%	0.019%
23	16.298	2258	2263	2267	rBV5	1049	1850	0.11%	0.010%
24	17.269	2422	2428	2438	rBV	623930	866101	49.41%	4.646%
25	17.369	2439	2445	2458	rBV2	1062624	1563541	89.20%	8.388%
26	19.233	2758	2762	2769	rBV2	10943	14653	0.84%	0.079%
27	19.310	2771	2775	2779	rVV	9535	11455	0.65%	0.061%
28	19.675	2831	2837	2847	rBV	1290735	1710056	97.56%	9.174%
29	21.475	3137	3143	3151	rBV	679459	933793	53.28%	5.010%
30	23.710	3515	3523	3536	rVB	878639	1752769	100.00%	9.403%
31	23.863	3542	3549	3558	rBV2	448593	890259	50.79%	4.776%




Sum of corrected areas: 18640278

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112122\
Data File : BN022830.D
Acq On : 22 Nov 2022 18:29
Operator : CG/JU
Sample : PB149044BL
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK044

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

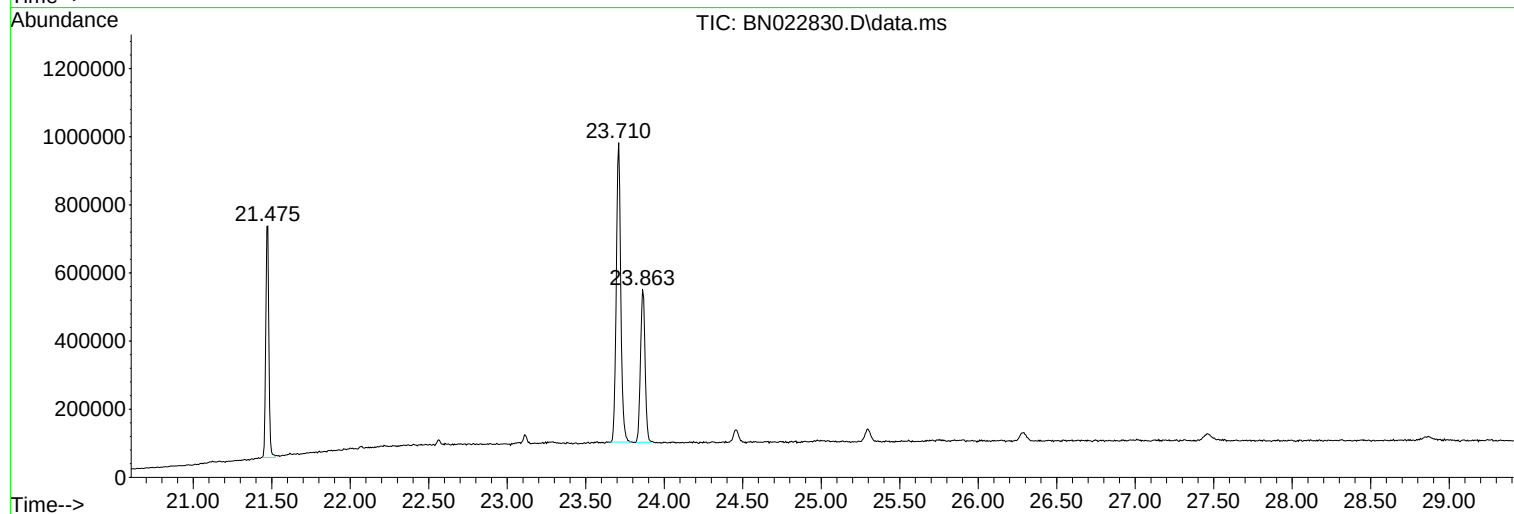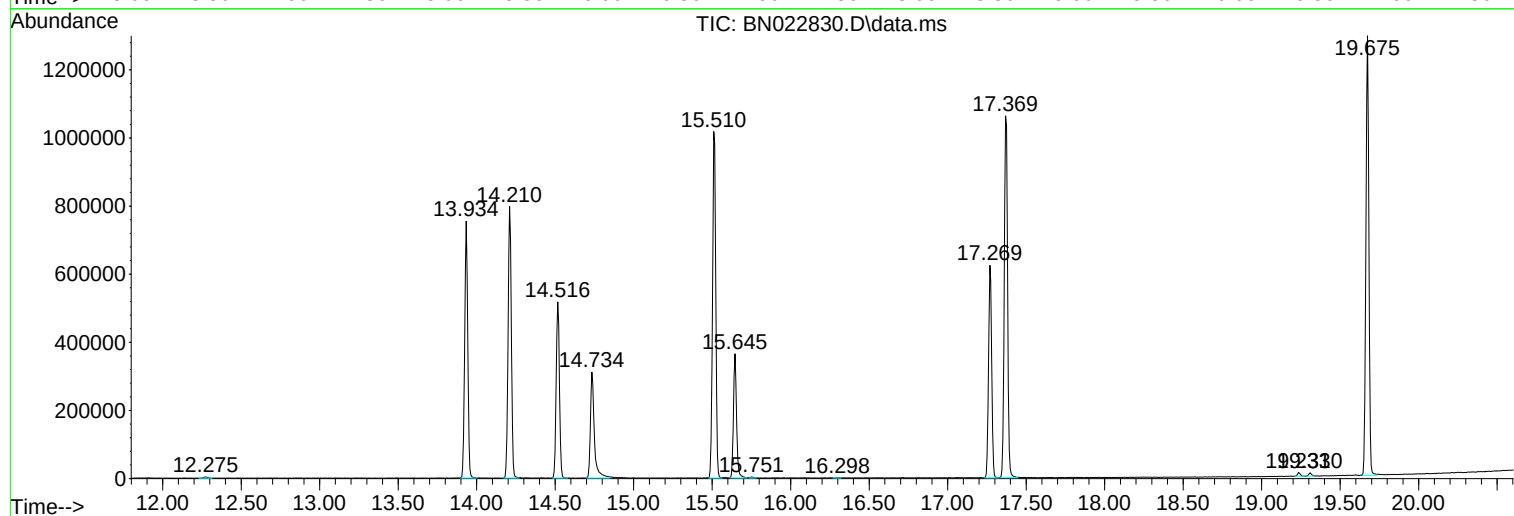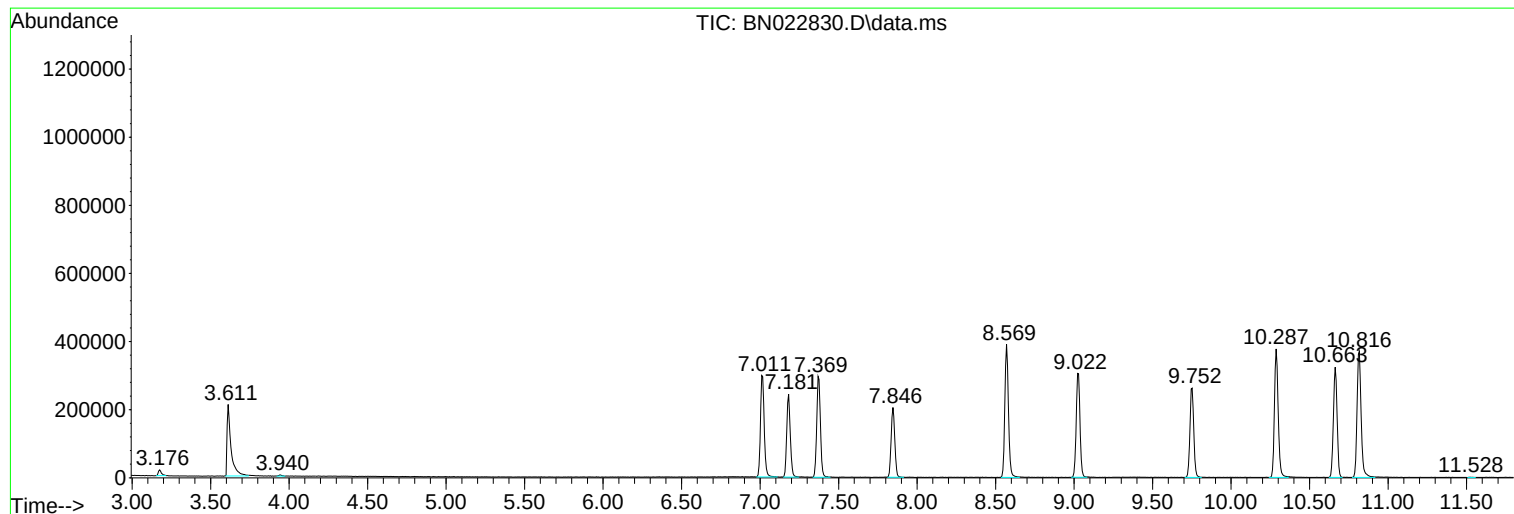

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112122\
Data File : BN022830.D
Acq On : 22 Nov 2022 18:29
Operator : CG/JU
Sample : PB149044BL
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK044

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112122\
Data File : BN022830.D
Acq On : 22 Nov 2022 18:29
Operator : CG/JU
Sample : PB149044BL
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK044

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc