

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112122\
 Data File : BN022832.D
 Acq On : 22 Nov 2022 19:44
 Operator : CG/JU
 Sample : PB149040BL
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK040

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
 Title : SVOA CALIBRATION

Signal : TIC: BN022832.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.175	28	32	39	rVB	21124	28631	1.39%	0.125%
2	3.611	103	106	127	rBV	256927	432914	20.99%	1.888%
3	3.940	158	162	170	rVB2	4455	9347	0.45%	0.041%
4	7.011	678	684	700	rBV	350491	572720	27.76%	2.498%
5	7.181	707	713	723	rBV	287983	445115	21.58%	1.941%
6	7.369	738	745	757	rBV	349138	557466	27.02%	2.431%
7	7.846	819	826	836	rVV	279761	444142	21.53%	1.937%
8	8.569	941	949	968	rBV	458352	735847	35.67%	3.209%
9	9.022	1019	1026	1038	rBV	364060	602759	29.22%	2.629%
10	9.746	1142	1149	1163	rBV	314582	523399	25.37%	2.283%
11	10.287	1233	1241	1265	rBV	434397	752936	36.50%	3.284%
12	10.663	1294	1305	1315	rBV	438425	728411	35.31%	3.177%
13	10.816	1322	1331	1352	rBV	427734	791695	38.38%	3.453%
14	12.269	1573	1578	1586	rBV3	4572	9013	0.44%	0.039%
15	13.934	1849	1861	1872	rBV	913775	1223434	59.30%	5.336%
16	14.210	1901	1908	1925	rBV2	957385	1375279	66.67%	5.998%
17	14.516	1953	1960	1975	rVB	720682	1023945	49.63%	4.466%
18	14.734	1990	1997	2019	rBV	385377	652719	31.64%	2.847%
19	15.510	2123	2129	2146	rVB	1215382	1712332	83.00%	7.468%
20	15.645	2146	2152	2166	rBV	431864	607178	29.43%	2.648%
21	15.751	2166	2170	2174	rVB2	4428	4763	0.23%	0.021%
22	16.251	2253	2255	2257	rBV	17760	6441	0.31%	0.028%
23	17.269	2422	2428	2436	rBV	865755	1183594	57.37%	5.162%
24	17.369	2439	2445	2460	rVV2	1287503	1855895	89.96%	8.094%
25	19.233	2758	2762	2767	rVB2	12090	16894	0.82%	0.074%
26	19.310	2770	2775	2780	rBV2	12141	16212	0.79%	0.071%
27	19.592	2821	2823	2826	rVB4	2347	2405	0.12%	0.010%
28	19.675	2831	2837	2847	rBV	1576841	2050627	99.40%	8.944%
29	21.474	3137	3143	3153	rBV	1003076	1284132	62.25%	5.601%
30	23.710	3515	3523	3537	rBV2	1022617	2062968	100.00%	8.998%
31	23.863	3542	3549	3561	rVB2	602494	1214906	58.89%	5.299%




Sum of corrected areas: 22928119

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112122\
Data File : BN022832.D
Acq On : 22 Nov 2022 19:44
Operator : CG/JU
Sample : PB149040BL
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK040

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

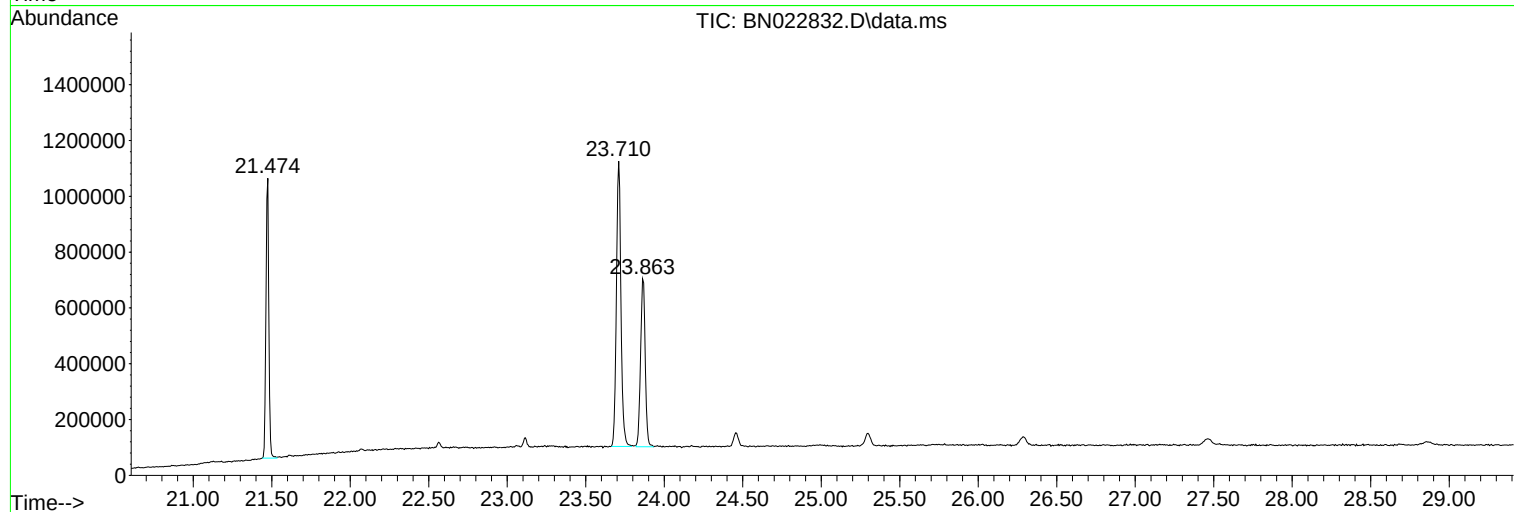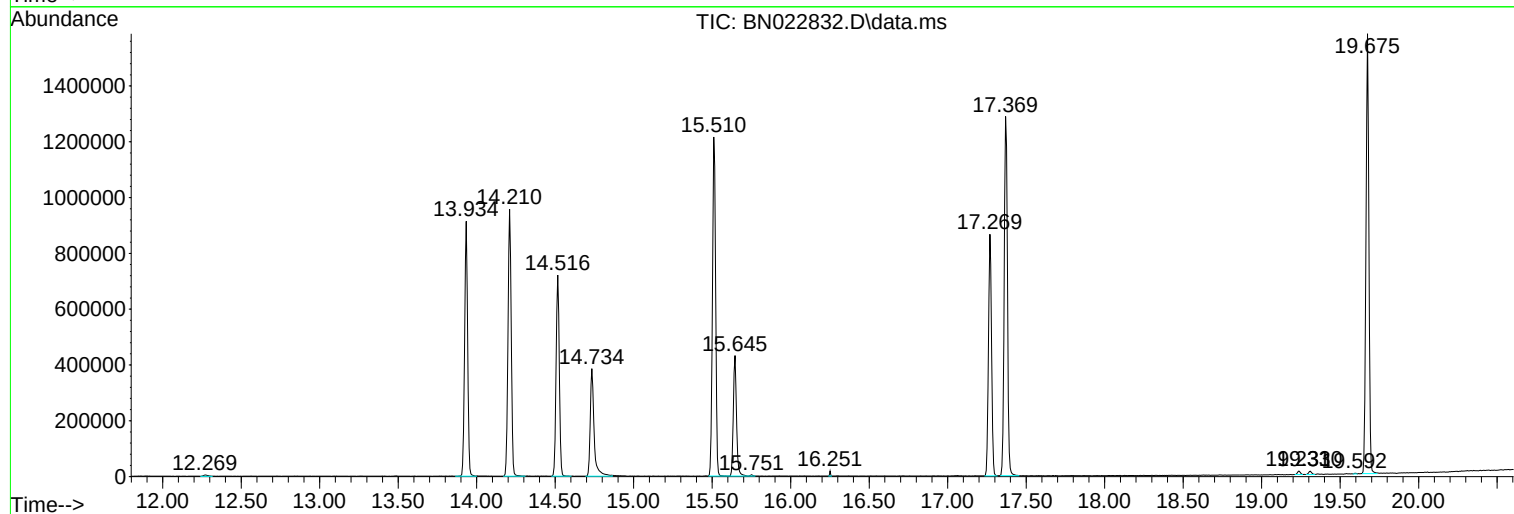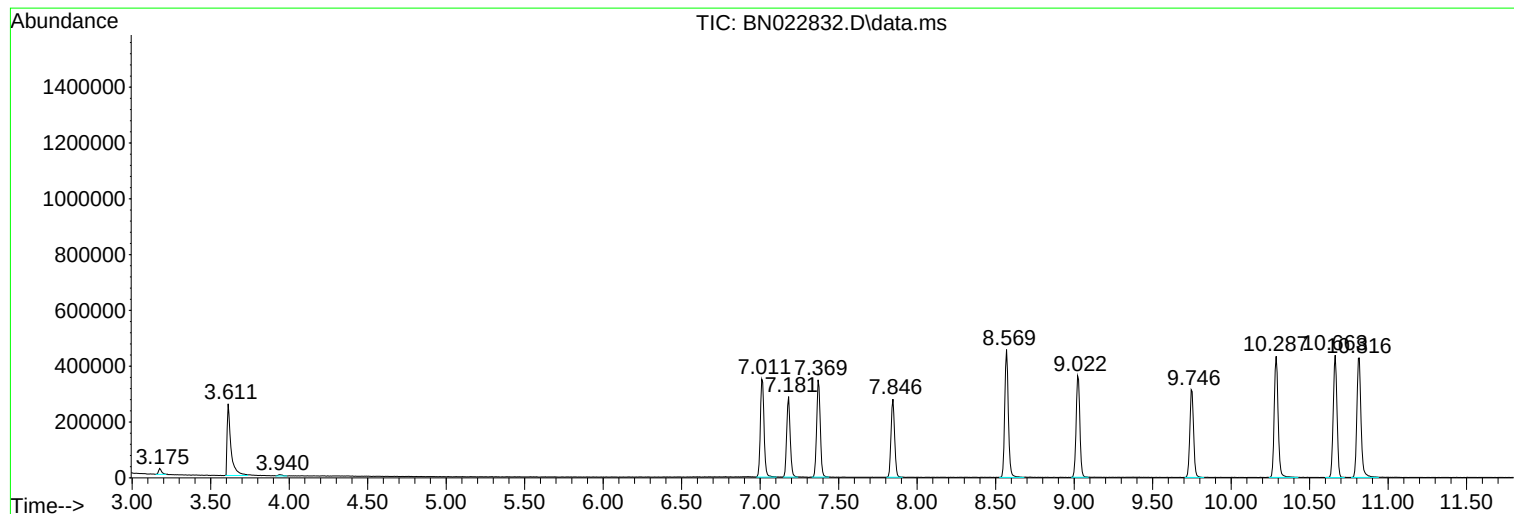

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112122\
Data File : BN022832.D
Acq On : 22 Nov 2022 19:44
Operator : CG/JU
Sample : PB149040BL
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK040

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112122\
Data File : BN022832.D
Acq On : 22 Nov 2022 19:44
Operator : CG/JU
Sample : PB149040BL
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK040

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc