

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112122\
 Data File : BN022834.D
 Acq On : 22 Nov 2022 20:58
 Operator : CG/JU
 Sample : N5593-11
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 H0AE0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
 Title : SVOA CALIBRATION

Signal : TIC: BN022834.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.134	21	25	29	rBV	29717	42826	1.70%	0.173%
2	3.176	29	32	36	rVV	18609	28886	1.15%	0.117%
3	3.211	36	38	49	rVB	16160	26427	1.05%	0.107%
4	3.617	104	107	123	rBV	101396	182440	7.25%	0.737%
5	3.846	141	146	152	rVB2	8033	14222	0.56%	0.057%
6	3.940	159	162	166	rBV3	4179	5774	0.23%	0.023%
7	4.487	248	255	267	rVB	196998	332357	13.20%	1.342%
8	4.917	323	328	342	rVB	40163	61730	2.45%	0.249%
9	7.017	679	685	693	rBV	98555	164229	6.52%	0.663%
10	7.181	706	713	724	rBV	351142	557857	22.16%	2.253%
11	7.369	737	745	756	rBV	337566	544292	21.62%	2.198%
12	7.846	819	826	835	rBV	273106	437004	17.36%	1.765%
13	8.569	942	949	964	rBV	290439	475841	18.90%	1.922%
14	9.022	1019	1026	1039	rBV	451715	751940	29.87%	3.036%
15	9.746	1143	1149	1162	rBV	368951	611353	24.28%	2.469%
16	10.287	1234	1241	1261	rBV	496129	846369	33.62%	3.418%
17	10.663	1298	1305	1314	rBV	418477	702717	27.91%	2.838%
18	10.810	1323	1330	1345	rBV	427573	783642	31.13%	3.164%
19	11.487	1440	1445	1452	rBV2	1458	3315	0.13%	0.013%
20	12.210	1565	1568	1573	rBV3	1863	3054	0.12%	0.012%
21	12.263	1573	1577	1585	rVB2	6136	10465	0.42%	0.042%
22	13.934	1854	1861	1878	rVB	1067592	1435749	57.03%	5.798%
23	14.210	1901	1908	1921	rBV	1147861	1650852	65.57%	6.666%
24	14.516	1953	1960	1969	rBV	686025	973854	38.68%	3.933%
25	14.740	1992	1998	2015	rBV	68959	143105	5.68%	0.578%
26	15.510	2123	2129	2140	rBV	1479586	2073517	82.36%	8.373%
27	15.645	2145	2152	2166	rVV	532493	746421	29.65%	3.014%
28	15.751	2166	2170	2176	rVB3	5237	7450	0.30%	0.030%
29	17.269	2422	2428	2439	rBV	821614	1137987	45.20%	4.595%
30	17.369	2439	2445	2458	rBV2	1605874	2273107	90.29%	9.179%
31	17.939	2539	2542	2545	rBV4	2984	3986	0.16%	0.016%
32	18.163	2575	2580	2590	rBV2	28871	38889	1.54%	0.157%
33	18.245	2590	2594	2595	rBV2	2000	2718	0.11%	0.011%
34	18.263	2595	2597	2602	rVB2	4224	4813	0.19%	0.019%
35	18.992	2717	2721	2725	rBV5	4144	5648	0.22%	0.023%
36	19.233	2758	2762	2768	rBV2	17722	25924	1.03%	0.105%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112122\
 Data File : BN022834.D
 Acq On : 22 Nov 2022 20:58
 Operator : CG/JU
 Sample : N5593-11
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 H0AE0

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
 Title : SVOA CALIBRATION

37	19.310	2770	2775	2781	rBV	16519	24626	0.98%	0.099%
38	19.386	2785	2788	2791	rVB4	5358	5152	0.20%	0.021%
39	19.445	2794	2798	2805	rBV	29246	40734	1.62%	0.164%
40	19.592	2821	2823	2827	rVB4	4841	5067	0.20%	0.020%
41	19.675	2830	2837	2851	rBV	1911142	2517538	100.00%	10.166%
42	20.704	3009	3012	3015	rBV4	7615	11347	0.45%	0.046%
43	21.469	3137	3142	3151	rBV	934035	1221563	48.52%	4.933%
44	23.110	3419	3421	3427	rVB	40467	55763	2.21%	0.225%
45	23.710	3515	3523	3535	rBV2	1237241	2506601	99.57%	10.122%
46	23.863	3542	3549	3559	rVB2	573523	1156357	45.93%	4.670%
47	24.451	3646	3649	3658	rVB2	54097	108482	4.31%	0.438%




Sum of corrected areas: 24763990

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112122\
Data File : BN022834.D
Acq On : 22 Nov 2022 20:58
Operator : CG/JU
Sample : N5593-11
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
H0AE0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

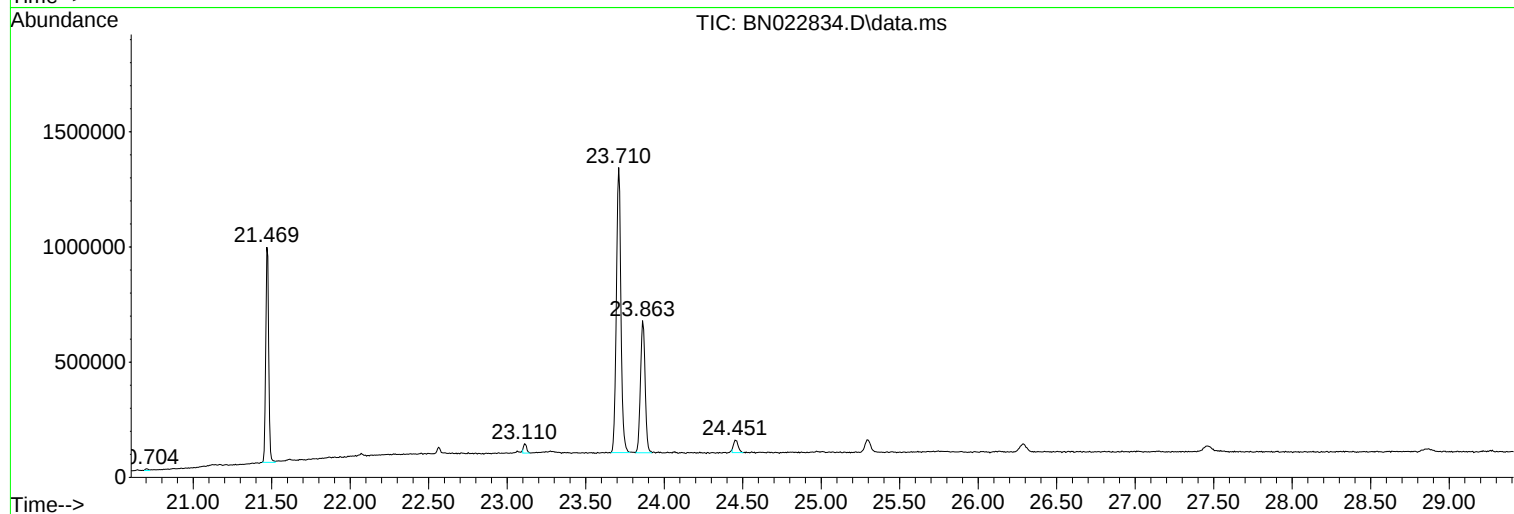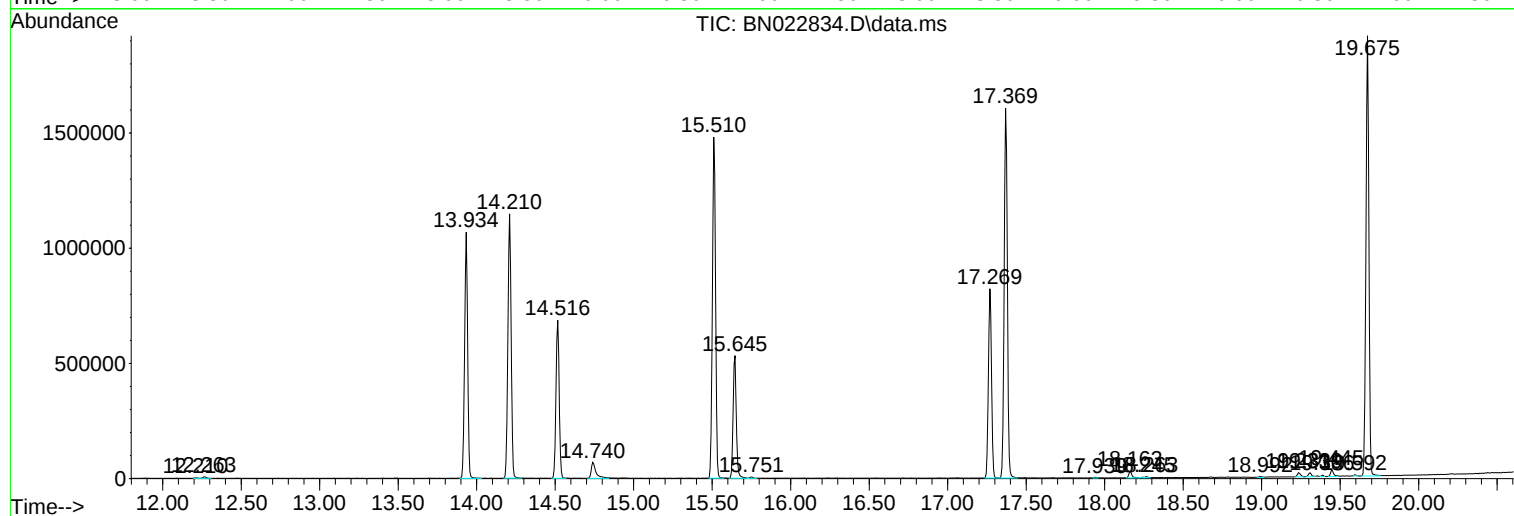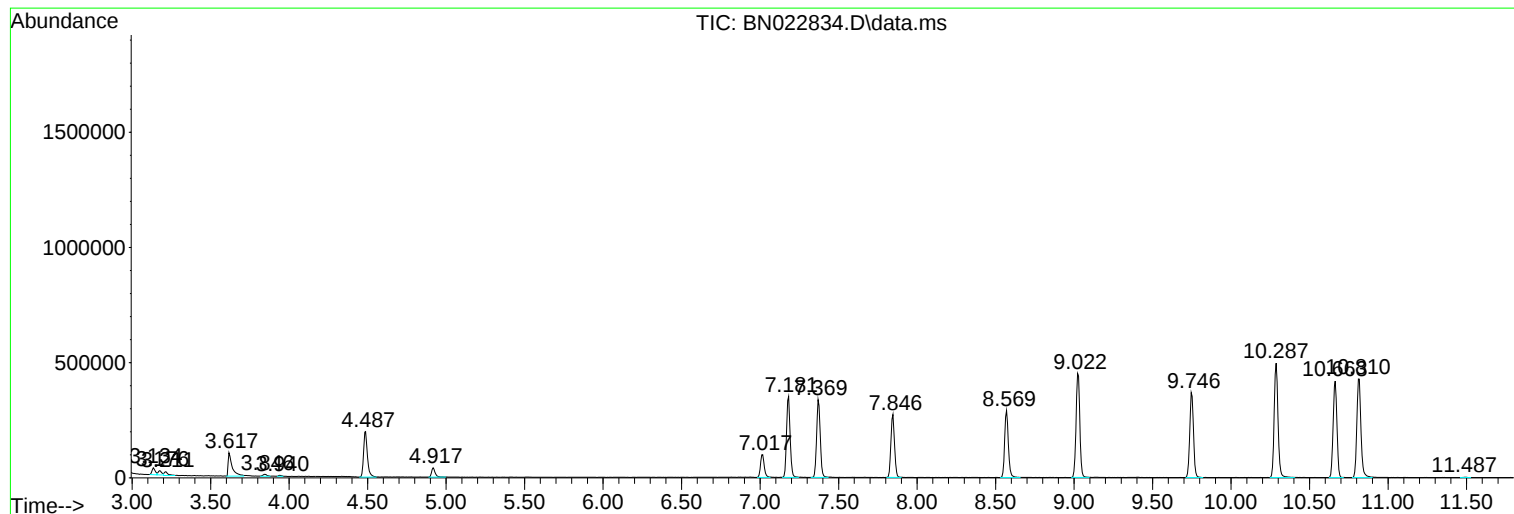

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112122\
Data File : BN022834.D
Acq On : 22 Nov 2022 20:58
Operator : CG/JU
Sample : N5593-11
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
H0AE0










Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.917	2.83 ng/ul	61730	1,4-Dichlorobenzene-d4	7.846

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	72
2			2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	64
3			2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	56
4			2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	25
5			2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	23

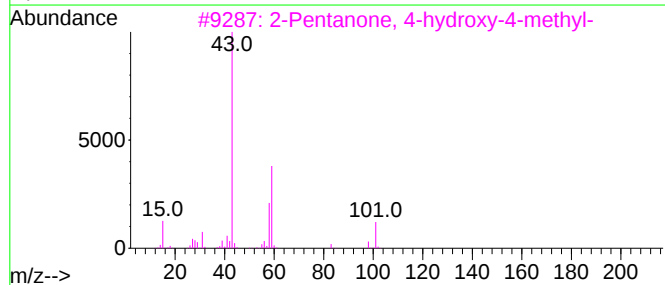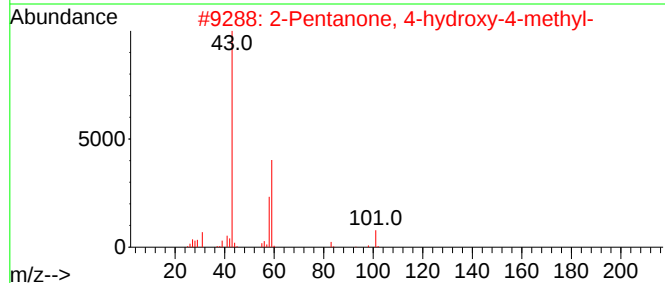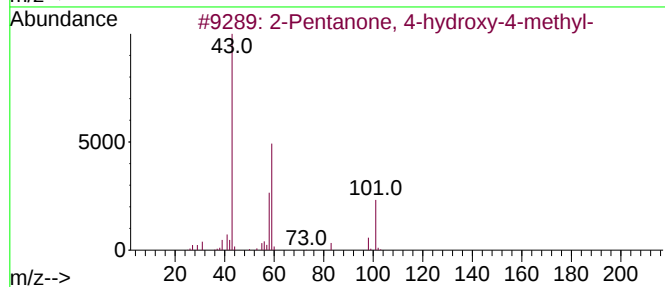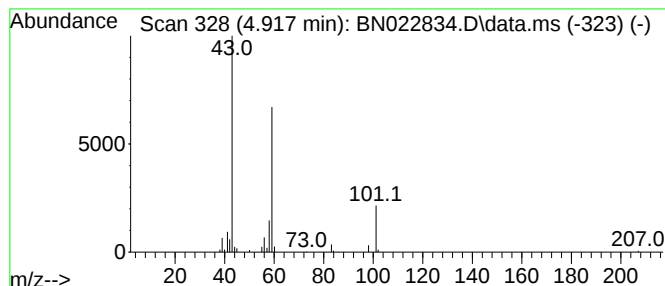

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112122\
Data File : BN022834.D
Acq On : 22 Nov 2022 20:58
Operator : CG/JU
Sample : N5593-11
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
H0AE0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	4.917	2.8	ng/u1	61730	1	7.846	437004	20.0