

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112122\
 Data File : BN022840.D
 Acq On : 23 Nov 2022 00:40
 Operator : CG/JU
 Sample : N5593-05
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 H0AD3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
 Title : SVOA CALIBRATION

Signal : TIC: BN022840.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.134	22	25	29	rBV2	7280	10430	0.45%	0.051%
2	3.175	29	32	36	rVV	14867	20113	0.87%	0.098%
3	3.211	36	38	49	rVB	9051	14544	0.63%	0.071%
4	3.617	104	107	126	rBV	72833	139288	6.05%	0.677%
5	3.846	141	146	154	rVB3	6376	11928	0.52%	0.058%
6	3.940	158	162	169	rVB	4050	6282	0.27%	0.031%
7	4.481	249	254	262	rBV	55000	91411	3.97%	0.444%
8	4.916	324	328	336	rVB	11823	18243	0.79%	0.089%
9	7.010	678	684	698	rVB	69413	125422	5.45%	0.610%
10	7.181	706	713	725	rBV	248652	402878	17.50%	1.958%
11	7.369	738	745	755	rBV	240827	392329	17.04%	1.907%
12	7.846	819	826	835	rBV	236950	377682	16.40%	1.836%
13	8.569	943	949	963	rBV	211949	348891	15.15%	1.696%
14	9.022	1019	1026	1039	rBV	335694	553786	24.05%	2.692%
15	9.746	1142	1149	1160	rBV	267127	439062	19.07%	2.134%
16	10.287	1234	1241	1254	rBV	356742	612050	26.58%	2.975%
17	10.663	1298	1305	1312	rBV	367025	619414	26.90%	3.011%
18	10.810	1322	1330	1346	rBV	341294	617633	26.82%	3.002%
19	12.269	1574	1578	1586	rVB2	4324	7314	0.32%	0.036%
20	13.934	1854	1861	1872	rVB	855523	1196650	51.97%	5.816%
21	14.210	1901	1908	1923	rBV	901425	1282736	55.71%	6.235%
22	14.516	1953	1960	1968	rBV	586005	857166	37.23%	4.166%
23	14.739	1990	1998	2022	rBV	52434	120422	5.23%	0.585%
24	14.951	2032	2034	2040	rVB3	3981	4102	0.18%	0.020%
25	15.510	2123	2129	2142	rVV	1238762	1708502	74.20%	8.304%
26	15.645	2146	2152	2166	rVV	438848	618745	26.87%	3.007%
27	15.751	2166	2170	2174	rVB2	3572	4754	0.21%	0.023%
28	17.269	2422	2428	2435	rBV	739011	1013223	44.00%	4.925%
29	17.369	2439	2445	2461	rVB	1441169	1984097	86.17%	9.644%
30	18.163	2575	2580	2589	rBV	18853	25584	1.11%	0.124%
31	19.233	2758	2762	2766	rBV	14841	19280	0.84%	0.094%
32	19.304	2770	2774	2780	rBV	15641	24741	1.07%	0.120%
33	19.445	2794	2798	2804	rBV3	15038	19389	0.84%	0.094%
34	19.592	2820	2823	2830	rBV5	4571	6482	0.28%	0.032%
35	19.675	2830	2837	2849	rVV	1627818	2219832	96.41%	10.789%
36	21.469	3137	3142	3149	rBV	859616	1090790	47.37%	5.302%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112122\
Data File : BN022840.D
Acq On : 23 Nov 2022 00:40
Operator : CG/JU
Sample : N5593-05
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
H0AD3

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Title : SVOA CALIBRATION

37	23.110	3418	3421	3427	rVB3	43935	66661	2.90%	0.324%
38	23.704	3515	3522	3535	rVB2	1119402	2302593	100.00%	11.192%
39	23.863	3541	3549	3560	rVB2	532610	1079386	46.88%	5.246%
40	24.457	3645	3650	3658	rVB2	58577	120546	5.24%	0.586%




Sum of corrected areas: 20574381

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112122\
Data File : BN022840.D
Acq On : 23 Nov 2022 00:40
Operator : CG/JU
Sample : N5593-05
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
H0AD3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

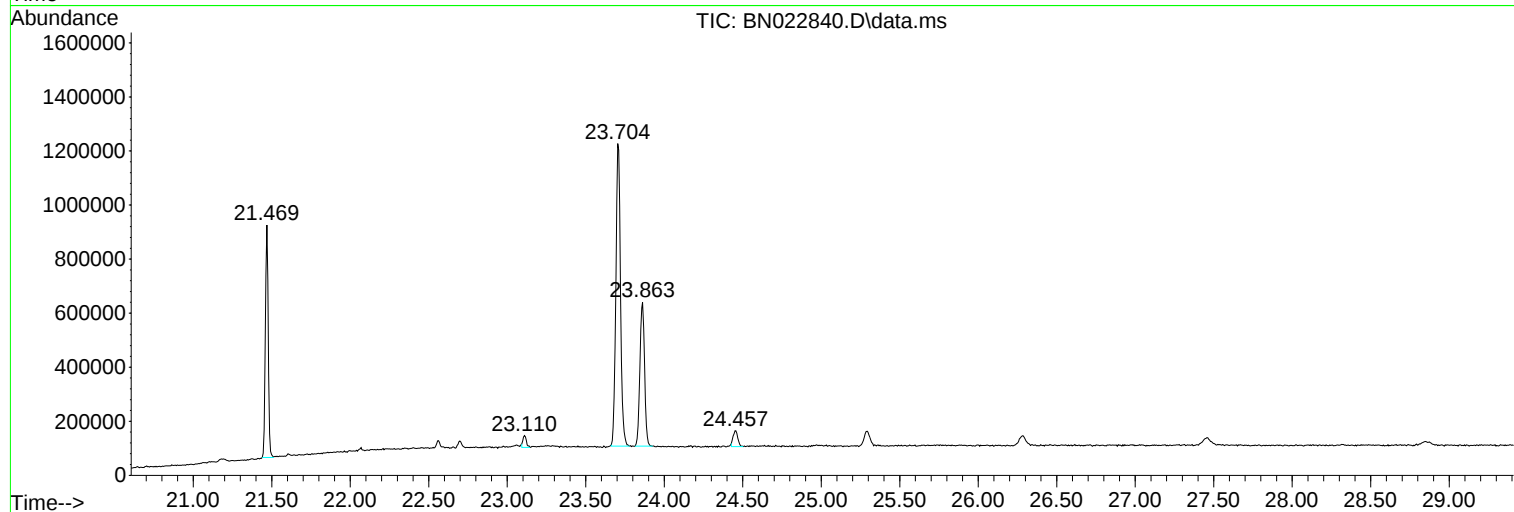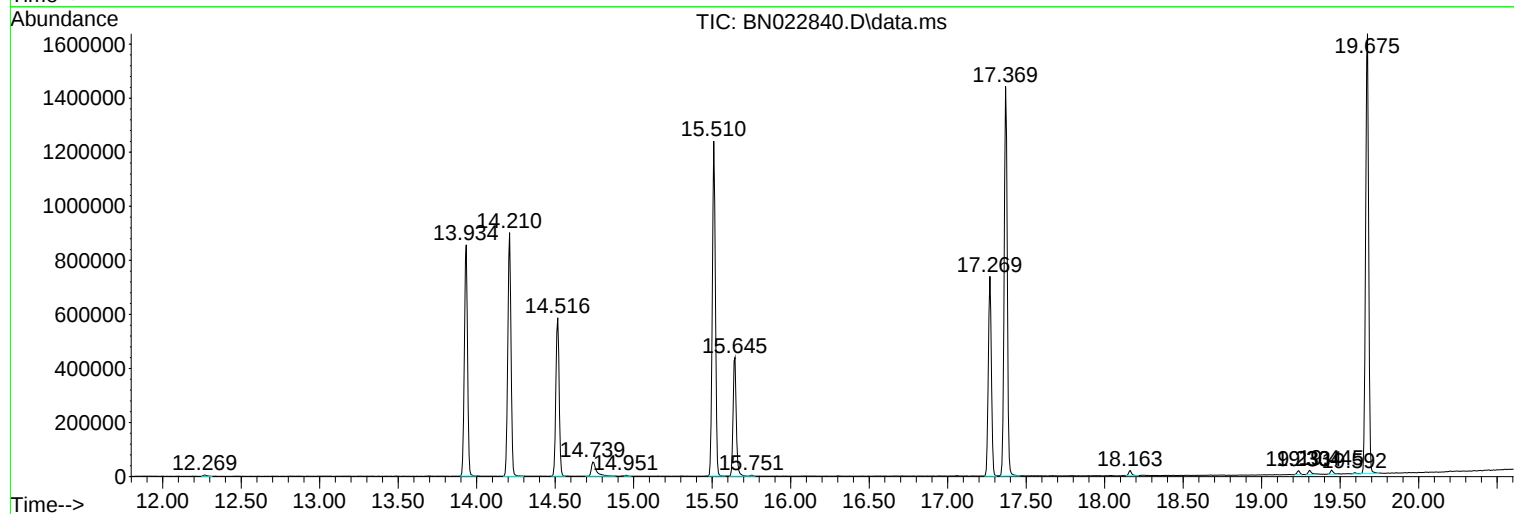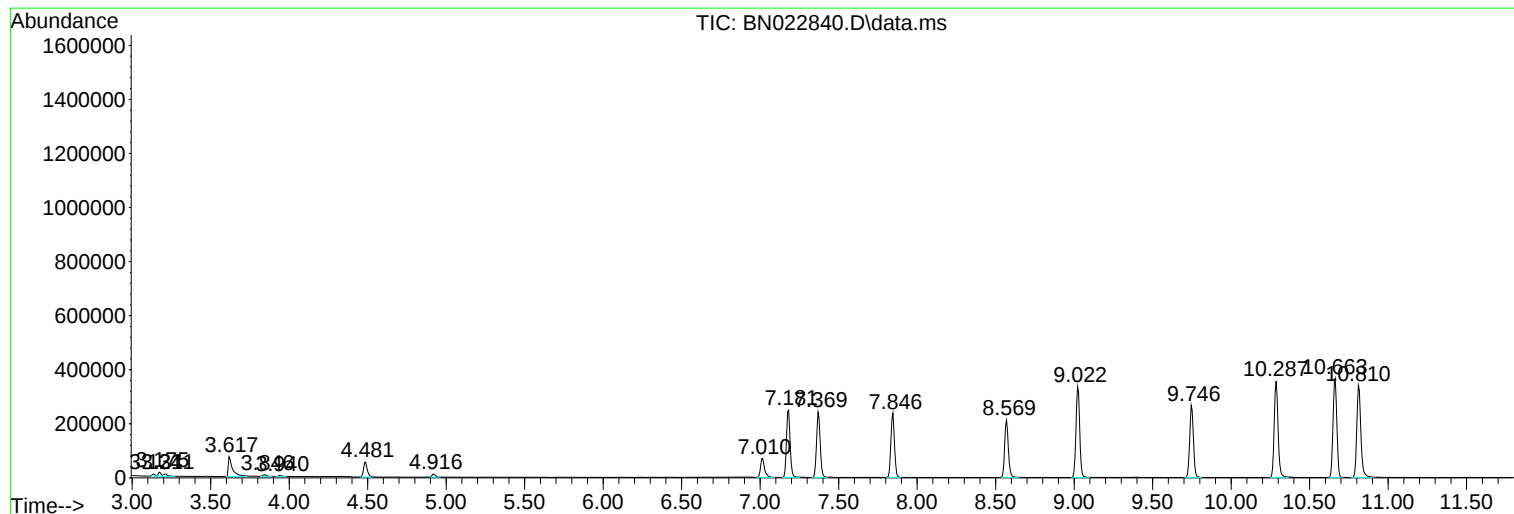

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112122\
Data File : BN022840.D
Acq On : 23 Nov 2022 00:40
Operator : CG/JU
Sample : N5593-05
Misc :
ALS Vial : 62 Sample Multiplier: 1










Instrument :
BNA_N
ClientSampleId :
H0AD3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 (DEL) Alkane: Straight-Chai... Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD		R.T.	
24.457	2.23 ng/ul	120546	Perylene-d12		23.863	
Hit# of 5	Tentative ID		MW	MolForm	CAS#	Qual
1	Heneicosane		296	C21H44	000629-94-7	90
2	Octacosane, 2-methyl-		408	C29H60	001560-98-1	90
3	Hentriacontane		437	C31H64	000630-04-6	90
4	Tetracosane		338	C24H50	000646-31-1	90
5	Heneicosane, 11-decyl-		437	C31H64	055320-06-4	87

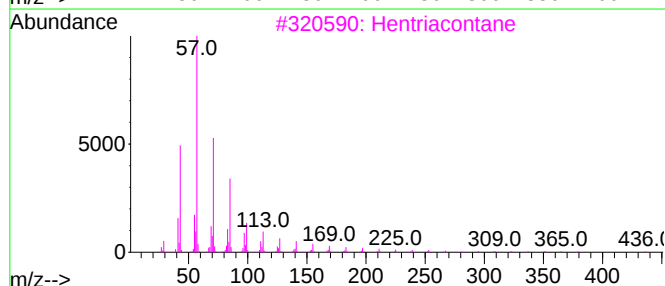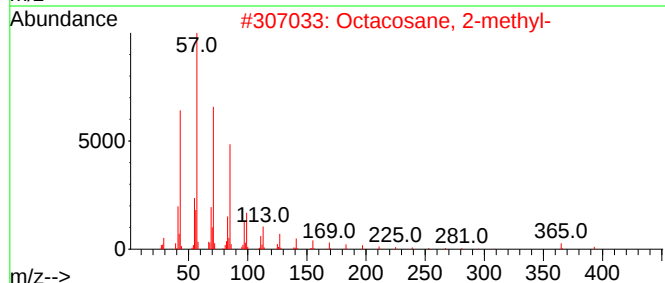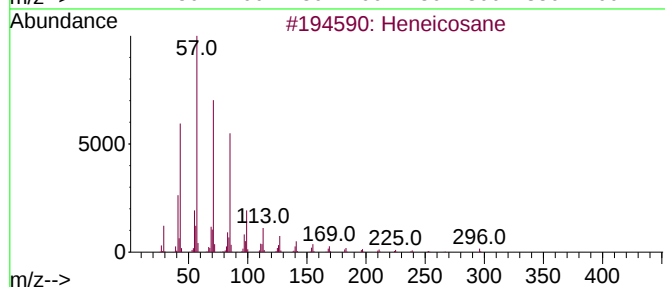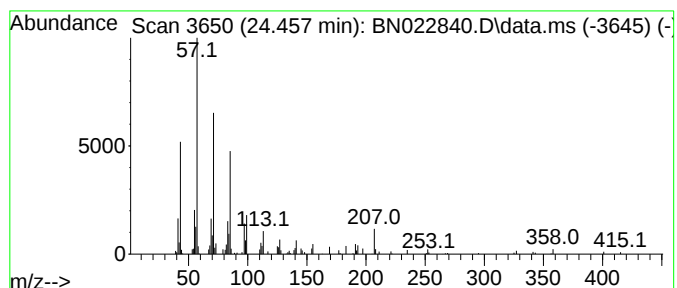

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112122\
Data File : BN022840.D
Acq On : 23 Nov 2022 00:40
Operator : CG/JU
Sample : N5593-05
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
H0AD3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	24.457	2.2	ng/u1	120546	6	23.863	1079390	20.0