
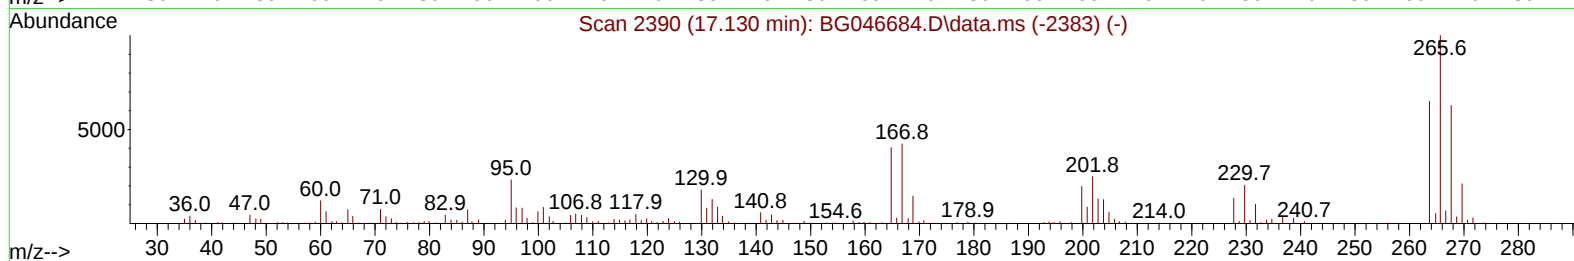
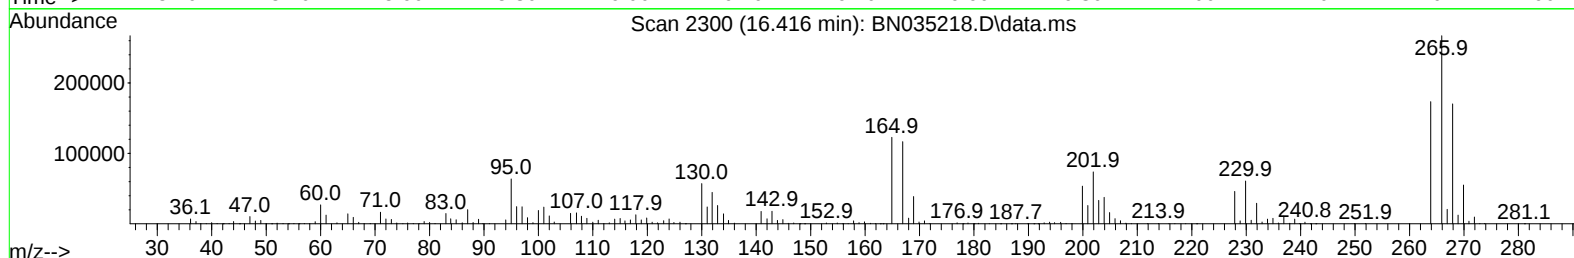


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112124\
Data File : BN035218.D
Acq On : 21 Nov 2024 12:43
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 21 15:34:38 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 21 03:21:56 2024
Response via : Initial Calibration

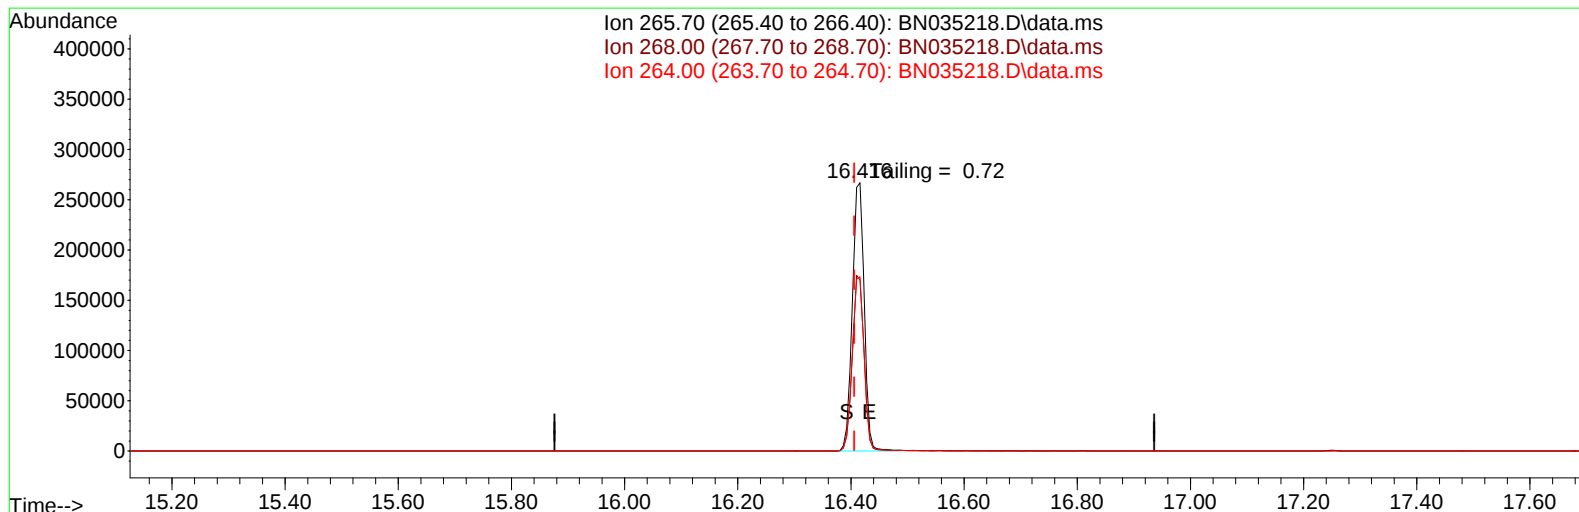

TIC: BN035218.D\data.ms

(70) Pentachlorophenol (C)




16.416min (+ 0.010) 32791.32 ng m

response 386007

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.76
264.00	61.60	64.93
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112124\
Data File : BN035218.D
Acq On : 21 Nov 2024 12:43
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 21 15:39:01 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 21 03:21:56 2024
Response via : Initial Calibration

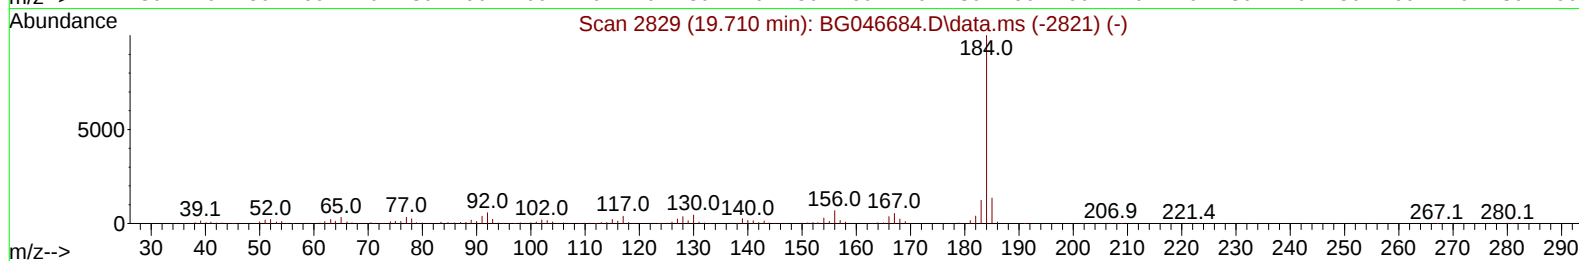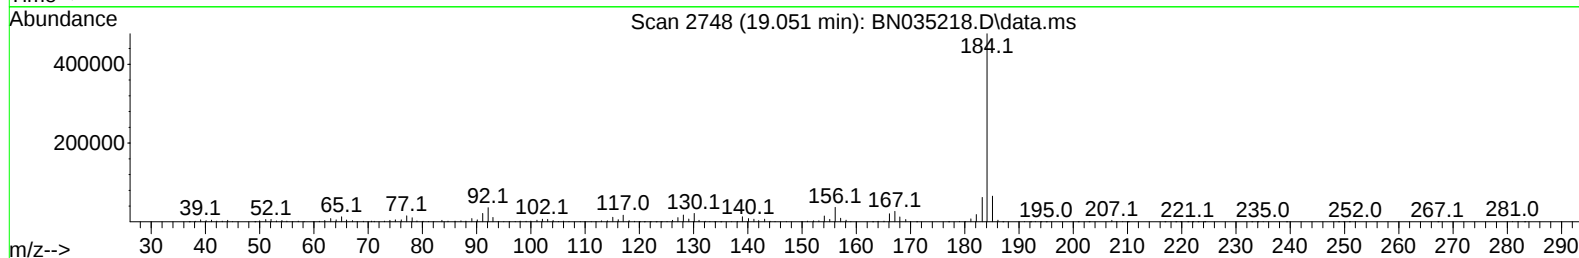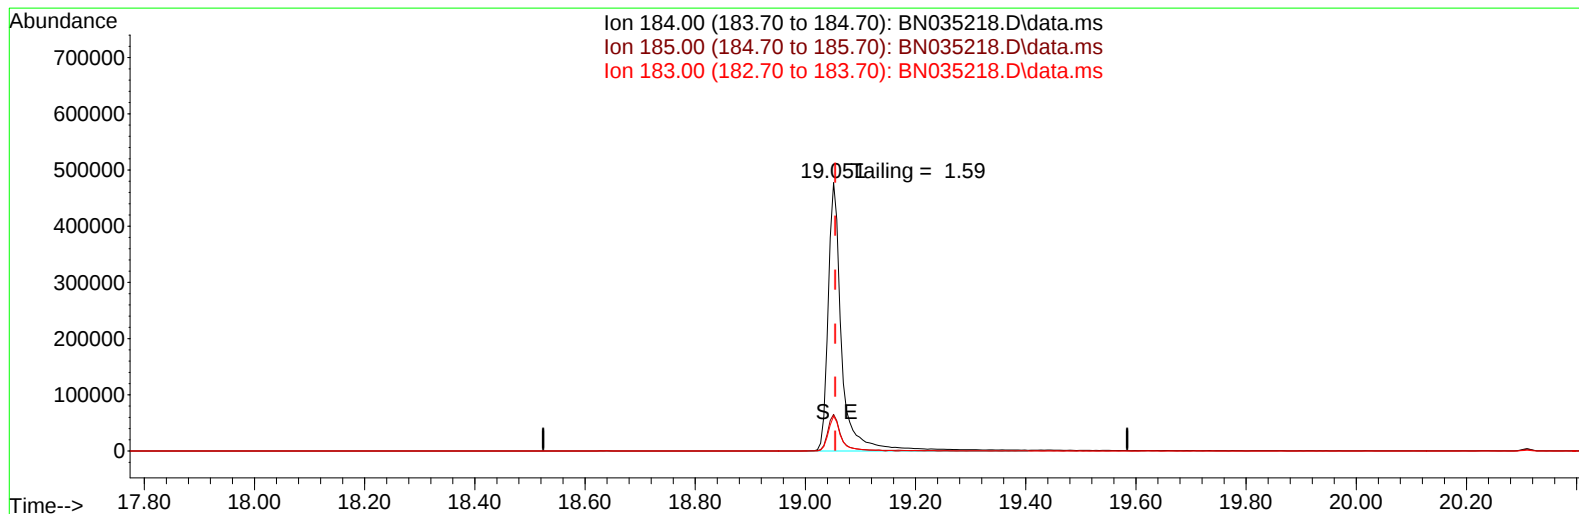

TIC: BN035218.D\data.ms

(77) Benzidine

19.051min (-0.003) 13099.41 ng m

response 829797

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.69
183.00	13.20	13.01
0.00	0.00	0.00