

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112221\
 Data File : BN017544.D
 Acq On : 22 Nov 2021 13:26
 Operator : CG/JU
 Sample : SSTD16050
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTD160250

Quant Time: Nov 22 14:53:55 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN112221.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Nov 22 14:49:39 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.846	152	270887	20.000	ng/u1	0.00
20) Naphthalene-d8	10.646	136	1133645	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.487	164	622972	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.228	188	1048699	20.000	ng/u1	0.00
79) Chrysene-d12	21.416	240	675407	20.000	ng/u1	0.00
88) Perylene-d12	23.786	264	719513	20.000	ng/u1	0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.305	96	453990	60.709	ng/uL	0.00
4) Pyridine-d5	3.711	84	3011552	150.348	ng/u1	0.00
7) Phenol-d5	7.028	99	3754456	149.155	ng/u1	0.02
9) Bis-(2-Chloroethyl)eth...	7.187	67	2221048	148.659	ng/u1	0.01
11) 2-Chlorophenol-d4	7.387	132	2846091	143.775	ng/u1	0.01
15) 4-Methylphenol-d8	8.569	113	2829508	137.700	ng/u1	0.02
21) Nitrobenzene-d5	9.016	128	1418789	161.603	ng/u1	0.02
24) 2-Nitrophenol-d4	9.734	143	1510495	155.410	ng/u1	0.01
28) 2,4-Dichlorophenol-d3	10.275	165	2512101	141.077	ng/u1	0.02
31) 4-Chloroaniline-d4	10.787	131	3267397	123.199	ng/u1	0.02
46) Dimethylphthalate-d6	13.904	166	6046124	129.642	ng/u1	0.01
49) Acenaphthylene-d8	14.181	160	7911366	134.567	ng/u1	0.01
54) 4-Nitrophenol-d4	14.698	143	1130958	122.901	ng/u1	0.04
60) Fluorene-d10	15.481	176	4740964	119.019	ng/u1	0.01
65) 4,6-Dinitro-2-methylph...	15.604	200	924839	136.192	ng/u1	0.02
73) Anthracene-d10	17.334	188	6451403	127.418	ng/u1	0.01
81) Pyrene-d10	19.622	212	6441611	162.622	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.645	264	5690118	148.798	ng/u1	0.02
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.340	88	462294	62.512	ng/uL	96
5) Pyridine	3.728	79	2970823	146.556	ng/u1	97
6) Benzaldehyde	6.981	77	943206	62.889	ng/u1	92
8) Phenol	7.058	94	3665748	143.956	ng/u1	93
10) Bis(2-Chloroethyl)ether	7.281	93	2896930	144.783	ng/u1	98
12) 2-Chlorophenol	7.422	128	2807136	137.128	ng/u1	97
13) 2-Methylphenol	8.299	108	2741687	141.517	ng/u1	99
14) 2,2'-oxybis(1-Chloropr...	8.387	45	3867326	131.746	ng/u1	96
16) Acetophenone	8.681	105	3866297	126.957	ng/u1	94
17) N-Nitroso-di-n-propyla...	8.699	70	2042247	133.587	ng/u1	93
18) 4-Methylphenol	8.652	108	2862679	133.749	ng/u1	97
19) Hexachloroethane	8.934	117	1213299	153.899	ng/u1	96
22) Nitrobenzene	9.058	77	3267083	165.489	ng/u1	95
23) Isophorone	9.605	82	6084692	151.803	ng/u1	97
25) 2-Nitrophenol	9.769	139	1514151	143.079	ng/u1#	87
26) 2,4-Dimethylphenol	9.834	107	3140585	148.085	ng/u1	90
27) Bis(2-Chloroethoxy)met...	10.069	93	3675963	143.382	ng/u1	99
29) 2,4-Dichlorophenol	10.305	162	2365040	133.730	ng/u1	96
30) Naphthalene	10.705	128	8011784	129.896	ng/u1	99
32) 4-Chloroaniline	10.810	127	3186225	121.441	ng/u1	99
33) Hexachlorobutadiene	10.993	225	1599952	148.568	ng/u1	97
34) Caprolactam	11.622	113	459219	72.164	ng/u1	94
35) 4-Chloro-3-methylphenol	11.952	107	2756254	140.080	ng/u1	94
36) 2-Methylnaphthalene	12.310	142	5135017	120.592	ng/u1	100

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112221\
 Data File : BN017544.D
 Acq On : 22 Nov 2021 13:26
 Operator : CG/JU
 Sample : SSTD16050
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTD160250


Quant Time: Nov 22 14:53:55 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN112221.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Nov 22 14:49:39 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.534	142	5206348	118.692	ng/ul#	96
39) 1,2,4,5-Tetrachloroben...	12.687	216	2563212	141.164	ng/ul	96
40) Hexachlorocyclopentadiene	12.669	237	1897869	164.458	ng/ul	98
41) 2,4,6-Trichlorophenol	12.922	196	1781531	151.322	ng/ul	100
42) 2,4,5-Trichlorophenol	12.993	196	1905826	145.366	ng/ul	100
43) 1,1'-Biphenyl	13.328	154	6303991	130.697	ng/ul	96
44) 2-Chloronaphthalene	13.369	162	5037853	137.143	ng/ul	95
45) 2-Nitroaniline	13.569	65	1741988	174.202	ng/ul	92
47) Dimethylphthalate	13.957	163	5882960	125.602	ng/ul	99
48) 2,6-Dinitrotoluene	14.069	165	1339129	145.599	ng/ul#	88
50) Acenaphthylene	14.210	152	7515895	124.819	ng/ul	99
51) 3-Nitroaniline	14.393	138	1166566	109.585	ng/ul	88
52) Acenaphthene	14.551	153	4986083	128.054	ng/ul	98
53) 2,4-Dinitrophenol	14.598	184	780705	132.714	ng/ul	93
55) 4-Nitrophenol	14.716	109	988080	152.159	ng/ul#	76
56) Dibenzofuran	14.887	168	6757349	121.551	ng/ul	91
57) 2,4-Dinitrotoluene	14.857	165	1746014	131.635	ng/ul	95
58) 2,3,4,6-Tetrachlorophenol	15.116	232	1357707	125.447	ng/ul	99
59) Diethylphthalate	15.322	149	5801192	124.207	ng/ul	99
61) Fluorene	15.540	166	4635183	105.774	ng/ul	97
62) 4-Chlorophenyl-phenyle...	15.528	204	2370281	110.000	ng/ul	91
63) 4-Nitroaniline	15.563	138	809595	76.966	ng/ul#	81
66) 4,6-Dinitro-2-methylph...	15.622	198	892109	131.672	ng/ul#	83
67) N-Nitrosodiphenylamine	15.745	169	4499334	140.955	ng/ul	99
68) 4-Bromophenyl-phenylether	16.422	248	1568729	140.373	ng/ul	91
69) Hexachlorobenzene	16.545	284	1575392	121.140	ng/ul#	88
70) Atrazine	16.704	200	1622544	138.531	ng/ul	98
71) Pentachlorophenol	16.881	266	1035380	132.618	ng/ul	100
72) Phenanthrene	17.275	178	7457313	129.062	ng/ul	99
74) Anthracene	17.369	178	7099124	121.326	ng/ul	96
75) 1,2,3,4-Tetrachloroben...	13.287	216	2719707	177.407	ng/ul	97
76) Pentachlorobenzene	14.810	250	2338050	150.602	ng/ul	94
77) Carbazole	17.634	167	6534117	126.482	ng/ul	99
78) Di-n-butylphthalate	18.204	149	8259999	135.264	ng/ul#	99
80) Fluoranthene	19.292	202	7543373	159.472	ng/ul	97
82) Pyrene	19.657	202	7202782	148.764	ng/ul	95
83) Butylbenzylphthalate	20.557	149	3402854	188.753	ng/ul	94
84) 3,3'-Dichlorobenzidine	21.333	252	1737968	115.595	ng/ul	93
85) Benzo(a)anthracene	21.404	228	6672579	150.074	ng/ul	100
86) Bis(2-ethylhexyl)phtha...	21.339	149	4381414	161.028	ng/ul	98
87) Chrysene	21.457	228	6188508	141.220	ng/ul	100
89) Di-n-octyl phthalate	22.257	149	8261416	157.094	ng/ul	100
90) Benzo(b)fluoranthene	23.074	252	7041869	144.969	ng/ul	96
91) Benzo(k)fluoranthene	23.122	252	6592020	139.515	ng/ul	98
93) Benzo(a)pyrene	23.698	252	6645681	142.185	ng/ul	98
94) Indeno(1,2,3-cd)pyrene	26.263	276	8163058	171.202	ng/ul	98
95) Dibenzo(a,h)anthracene	26.280	278	6650829	165.018	ng/ul	93
96) Benzo(g,h,i)perylene	27.015	276	7217238	180.777	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: Nov 22 14:53:55 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN112221.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Nov 22 14:49:39 2021
Response via : Initial Calibration









#2
1,4-Dioxane
Concen: 62.512 ng/uL
RT: 3.340 min Scan# 60
Delta R.T. 0.000 min
Lab File: BN017544.D
Acq: 22 Nov 2021 13:26




Instrument :
BNA_N
ClientSampleId :
SSTD160250


Tgt Ion: 88 Resp: 462294
Ion Ratio Lower Upper
88 100
43 29.0 24.4 36.6
58 73.7 61.9 92.9

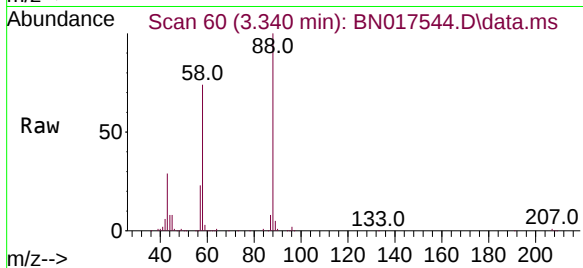

#5
Pyridine
Concen: 146.556 ng/uL
RT: 3.728 min Scan# 126
Delta R.T. 0.000 min
Lab File: BN017544.D
Acq: 22 Nov 2021 13:26

Tgt Ion: 79 Resp: 2970823
Ion Ratio Lower Upper
79 100
52 79.9 66.7 100.1
51 36.8 30.6 46.0




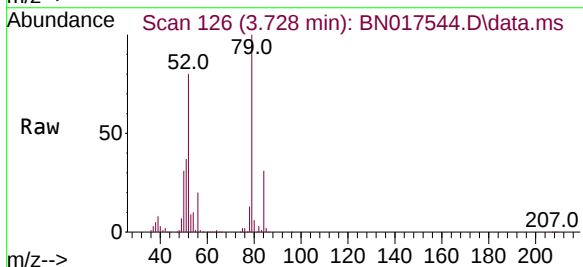




#6
Benzaldehyde
Concen: 62.889 ng/ul
RT: 6.981 min Scan# 61
Delta R.T. 0.000 min
Lab File: BN017544.D
Acq: 22 Nov 2021 13:26




Instrument :
BNA_N
ClientSampleId :
SSTD160250


Tgt Ion: 77 Resp: 943206
Ion Ratio Lower Upper
77 100
105 95.4 83.8 125.6
106 91.6 79.6 119.4

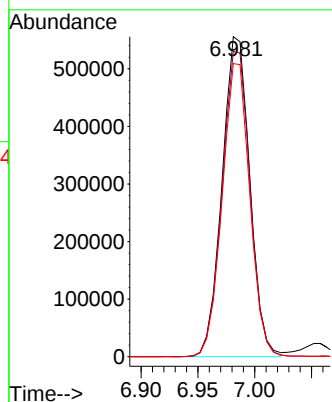

#8
Phenol
Concen: 143.956 ng/ul
RT: 7.058 min Scan# 692
Delta R.T. 0.024 min
Lab File: BN017544.D
Acq: 22 Nov 2021 13:26

Tgt Ion: 94 Resp: 3665748
Ion Ratio Lower Upper
94 100
65 28.9 21.7 32.5
66 40.8 28.3 42.5









#10
 Bis(2-Chloroethyl)ether
 Concen: 144.783 ng/ul
 RT: 7.281 min Scan# 71
 Delta R.T. 0.012 min
 Lab File: BN017544.D
 Acq: 22 Nov 2021 13:26




Instrument :
 BNA_N
 ClientSampleId :
 SSTD160250


Tgt Ion: 93 Resp: 2896930
 Ion Ratio Lower Upper
 93 100
 63 77.5 63.6 95.4
 95 32.7 26.2 39.2

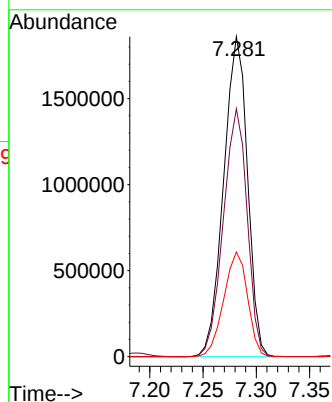

#12
 2-Chlorophenol
 Concen: 137.128 ng/ul
 RT: 7.422 min Scan# 754
 Delta R.T. 0.018 min
 Lab File: BN017544.D
 Acq: 22 Nov 2021 13:26

Tgt Ion:128 Resp: 2807136
 Ion Ratio Lower Upper
 128 100
 64 48.2 36.2 54.2
 130 32.1 26.4 39.6









#13
2-Methylphenol
Concen: 141.517 ng/ul
RT: 8.299 min Scan# 901
Delta R.T. 0.018 min
Lab File: BN017544.D
Acq: 22 Nov 2021 13:26




Instrument :
BNA_N
ClientSampleId :
SSTD160250


Tgt Ion:108 Resp: 2741687
Ion Ratio Lower Upper
108 100
107 88.2 71.1 106.7

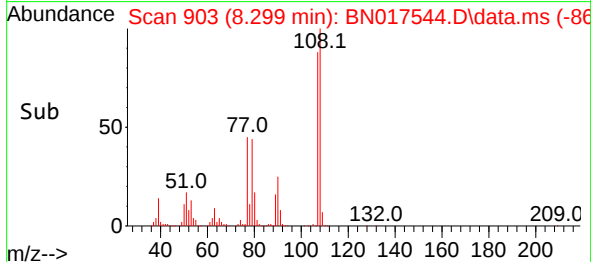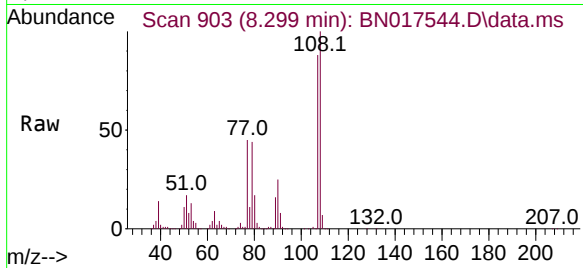

#14
2,2'-oxybis(1-Chloropropane)
Concen: 131.746 ng/ul
RT: 8.387 min Scan# 918
Delta R.T. 0.006 min
Lab File: BN017544.D
Acq: 22 Nov 2021 13:26

Tgt Ion: 45 Resp: 3867326
Ion Ratio Lower Upper
45 100
77 15.1 10.7 16.1
79 11.6 8.1 12.1




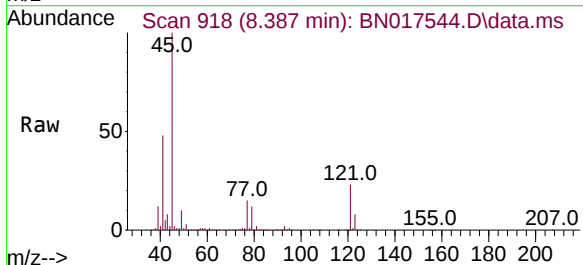




#16
Acetophenone
Concen: 126.957 ng/ul
RT: 8.681 min Scan# 90
Delta R.T. 0.018 min
Lab File: BN017544.D
Acq: 22 Nov 2021 13:26




Instrument :
BNA_N
ClientSampleId :
SSTD160250


Tgt Ion:105 Resp: 3866297
Ion Ratio Lower Upper
105 100
77 79.6 58.6 87.8
51 28.1 21.3 31.9

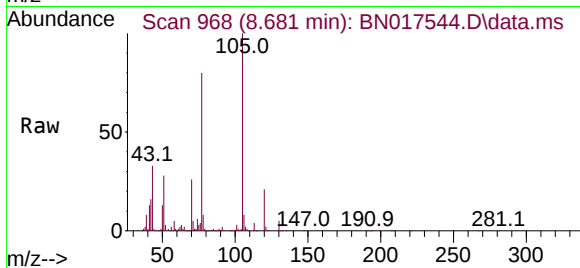

#17
N-Nitroso-di-n-propylamine
Concen: 133.587 ng/ul
RT: 8.699 min Scan# 971
Delta R.T. 0.048 min
Lab File: BN017544.D
Acq: 22 Nov 2021 13:26

Tgt Ion: 70 Resp: 2042247
Ion Ratio Lower Upper
70 100
42 55.1 49.8 74.8
101 9.5 8.2 12.2
130 20.2 18.0 27.0




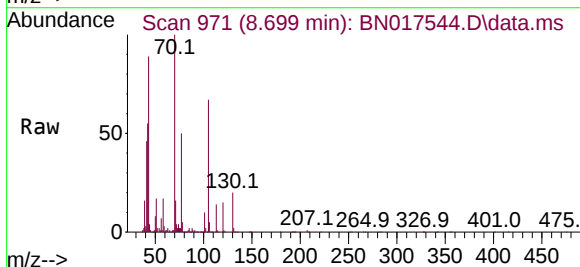




#18
4-Methylphenol
Concen: 133.749 ng/ul
RT: 8.652 min Scan# 910
Delta R.T. 0.042 min
Lab File: BN017544.D
Acq: 22 Nov 2021 13:26




Instrument :
BNA_N
ClientSampleId :
SSTD160250


Tgt Ion:108 Resp: 2862679
Ion Ratio Lower Upper
108 100
107 107.7 88.7 133.1

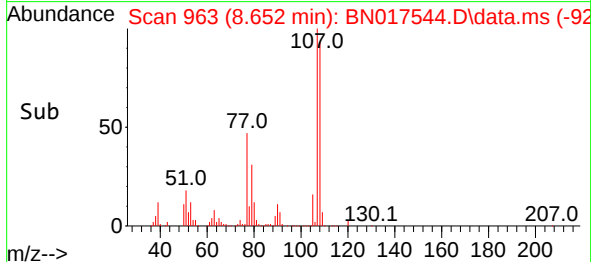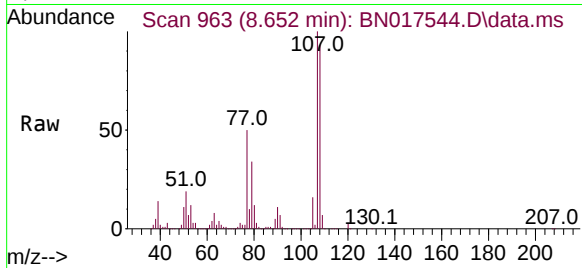

#19
Hexachloroethane
Concen: 153.899 ng/ul
RT: 8.934 min Scan# 1011
Delta R.T. 0.006 min
Lab File: BN017544.D
Acq: 22 Nov 2021 13:26

Tgt Ion:117 Resp: 1213299
Ion Ratio Lower Upper
117 100
201 93.2 78.1 117.1
199 56.7 46.6 70.0




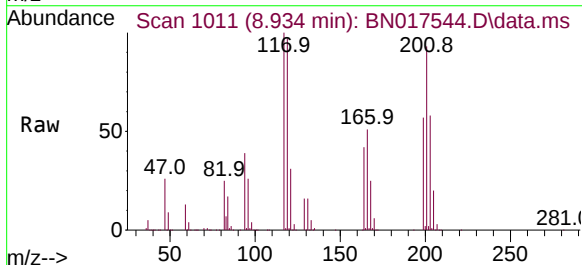




#22
Nitrobenzene
Concen: 165.489 ng/ul
RT: 9.058 min Scan# 1102
Delta R.T. 0.018 min
Lab File: BN017544.D
Acq: 22 Nov 2021 13:26




Instrument :
BNA_N
ClientSampleId :
SSTD160250


Tgt Ion: 77 Resp: 3267083
Ion Ratio Lower Upper
77 100
123 43.1 37.9 56.9
65 13.9 10.6 16.0

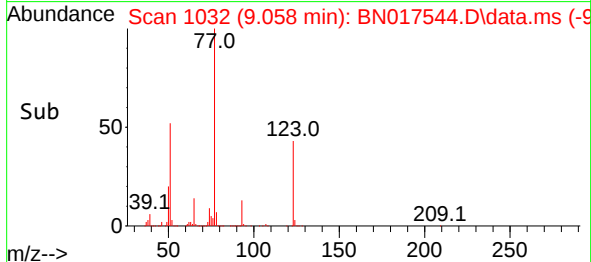

#23
Isophorone
Concen: 151.803 ng/ul
RT: 9.605 min Scan# 1125
Delta R.T. 0.042 min
Lab File: BN017544.D
Acq: 22 Nov 2021 13:26

Tgt Ion: 82 Resp: 6084692
Ion Ratio Lower Upper
82 100
95 7.8 5.6 8.4
138 17.1 15.0 22.4

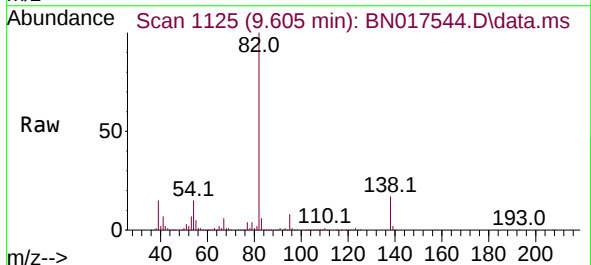



#25

2-Nitrophenol

Concen: 143.079 ng/ul

RT: 9.769 min Scan# 1153

Delta R.T. 0.018 min

Lab File: BN017544.D

Acq: 22 Nov 2021 13:26

Instrument :

BNA_N

ClientSampleId :

SSTD160250





Tgt Ion:139 Resp: 1514151

Ion Ratio Lower Upper

139 100

65 55.6 38.4 57.6

109 36.2 21.9 32.9#

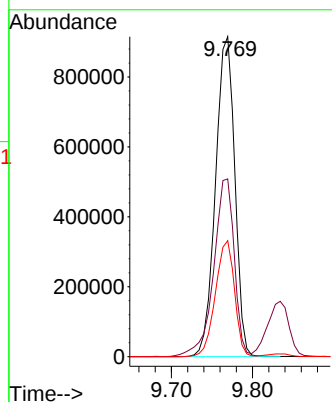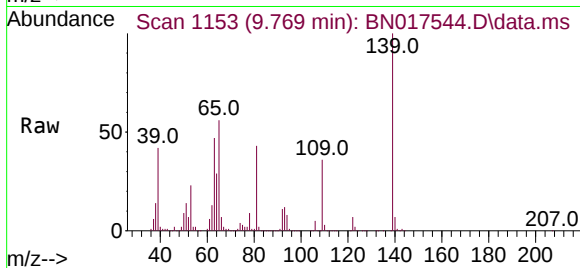

#26

2,4-Dimethylphenol

Concen: 148.085 ng/ul

RT: 9.834 min Scan# 1164

Delta R.T. 0.018 min

Lab File: BN017544.D

Acq: 22 Nov 2021 13:26




Tgt Ion:107 Resp: 3140585


Ion Ratio Lower Upper

107 100

121 47.0 41.2 61.8

122 78.6 71.4 107.0




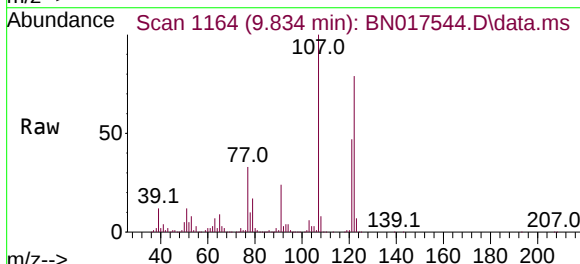




#27
 Bis(2-Chloroethoxy)methane
 Concen: 143.382 ng/ul
 RT: 10.069 min Scan# 1204
 Delta R.T. 0.018 min
 Lab File: BN017544.D
 Acq: 22 Nov 2021 13:26




Instrument :
 BNA_N
 ClientSampleId :
 SSTD160250


Tgt Ion: 93 Resp: 3675963
 Ion Ratio Lower Upper
 93 100
 95 31.9 25.4 38.2
 123 10.7 9.0 13.6

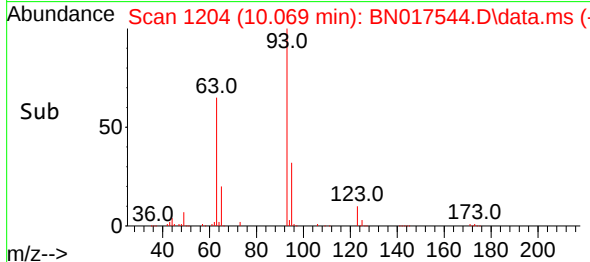

#29
 2,4-Dichlorophenol
 Concen: 133.730 ng/ul
 RT: 10.305 min Scan# 1244
 Delta R.T. 0.018 min
 Lab File: BN017544.D
 Acq: 22 Nov 2021 13:26

Tgt Ion:162 Resp: 2365040
 Ion Ratio Lower Upper
 162 100
 164 64.7 53.6 80.4
 98 40.3 29.9 44.9

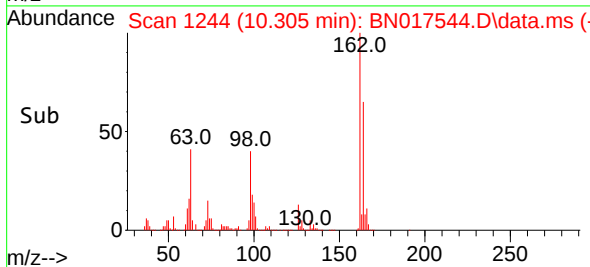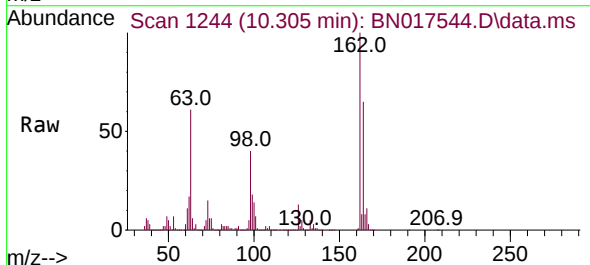



#30

Naphthalene

Concen: 129.896 ng/ul

RT: 10.705 min Scan# 11

Delta R.T. 0.012 min

Lab File: BN017544.D

Acq: 22 Nov 2021 13:26

Instrument :

BNA_N

ClientSampleId :

SSTD160250





Tgt Ion:128 Resp: 8011784

Ion Ratio Lower Upper

128 100

129 10.9 8.4 12.6

127 13.6 10.3 15.5

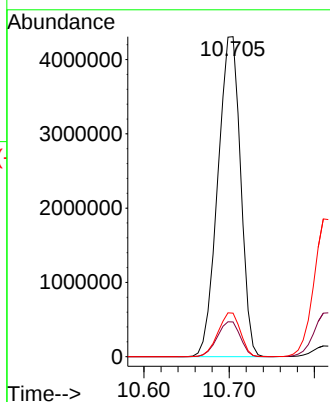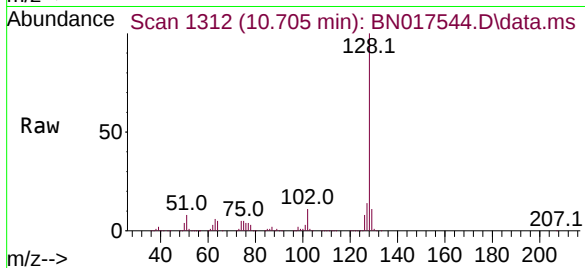

#32

4-Chloroaniline

Concen: 121.441 ng/ul

RT: 10.810 min Scan# 1330

Delta R.T. 0.018 min

Lab File: BN017544.D




Acq: 22 Nov 2021 13:26


Tgt Ion:127 Resp: 3186225

Ion Ratio Lower Upper

127 100

129 31.5 25.8 38.6




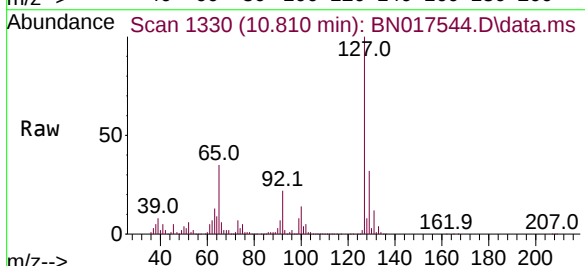




#33
Hexachlorobutadiene
Concen: 148.568 ng/ul
RT: 10.993 min Scan# 11
Delta R.T. 0.006 min
Lab File: BN017544.D
Acq: 22 Nov 2021 13:26




Instrument :
BNA_N
ClientSampleId :
SSTD160250


Tgt Ion:225 Resp: 1599952
Ion Ratio Lower Upper
225 100
223 63.7 49.4 74.2
227 64.3 49.0 73.6

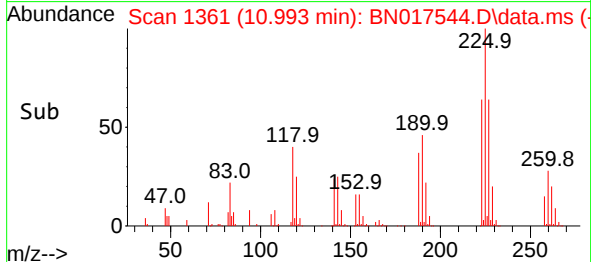

#34
Caprolactam
Concen: 72.164 ng/ul
RT: 11.622 min Scan# 1468
Delta R.T. 0.083 min
Lab File: BN017544.D
Acq: 22 Nov 2021 13:26

Tgt Ion:113 Resp: 459219
Ion Ratio Lower Upper
113 100
55 165.7 141.4 212.2
56 125.2 103.9 155.9




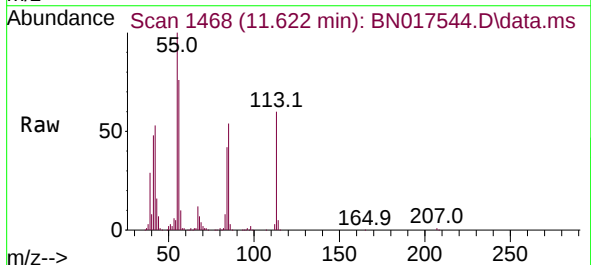




#35
4-Chloro-3-methylphenol
Concen: 140.080 ng/ul
RT: 11.952 min Scan# 11
Delta R.T. 0.030 min
Lab File: BN017544.D
Acq: 22 Nov 2021 13:26




Instrument :
BNA_N
ClientSampleId :
SSTD160250


Tgt Ion:107 Resp: 2756254
Ion Ratio Lower Upper
107 100
144 23.7 20.6 30.8
142 73.8 64.1 96.1



#36
2-Methylnaphthalene
Concen: 120.592 ng/ul
RT: 12.310 min Scan# 1585
Delta R.T. 0.006 min
Lab File: BN017544.D
Acq: 22 Nov 2021 13:26

Tgt Ion:142 Resp: 5135017
Ion Ratio Lower Upper
142 100
141 87.9 70.2 105.2









#37
1-Methylnaphthalene
Concen: 118.692 ng/ul
RT: 12.534 min Scan# 1623
Delta R.T. 0.012 min
Lab File: BN017544.D
Acq: 22 Nov 2021 13:26




Instrument :
BNA_N
ClientSampleId :
SSTD160250


Tgt Ion:142 Resp: 5206348
Ion Ratio Lower Upper
142 100
141 93.9 72.2 108.2
116 4.7 3.0 4.6#

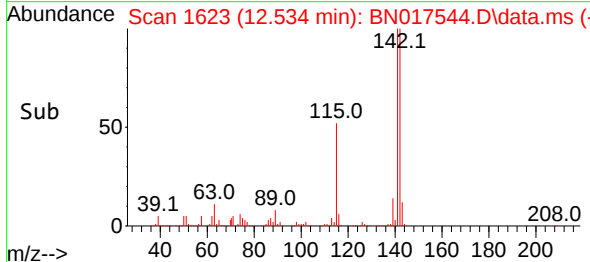

#39
1,2,4,5-Tetrachlorobenzene
Concen: 141.164 ng/ul
RT: 12.687 min Scan# 1649
Delta R.T. 0.012 min
Lab File: BN017544.D
Acq: 22 Nov 2021 13:26

Tgt Ion:216 Resp: 2563212
Ion Ratio Lower Upper
216 100
214 77.1 65.6 98.4
179 22.1 17.4 26.0
108 18.8 14.0 21.0


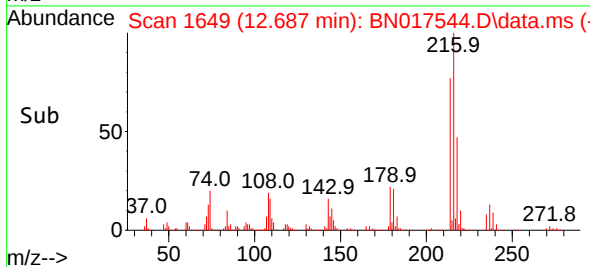

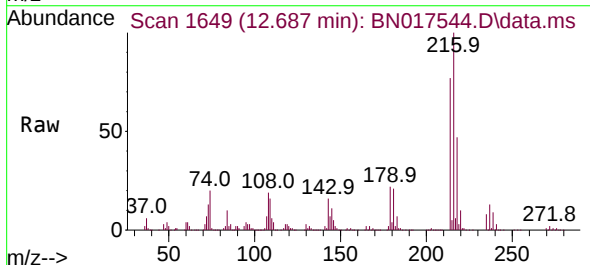




#40
Hexachlorocyclopentadiene
Concen: 164.458 ng/ul
RT: 12.669 min Scan# 1645
Delta R.T. 0.006 min
Lab File: BN017544.D
Acq: 22 Nov 2021 13:26




Instrument :
BNA_N
ClientSampleId :
SSTD160250


Tgt Ion:237 Resp: 1897869
Ion Ratio Lower Upper
237 100
235 65.8 51.9 77.9
272 11.5 10.9 16.3

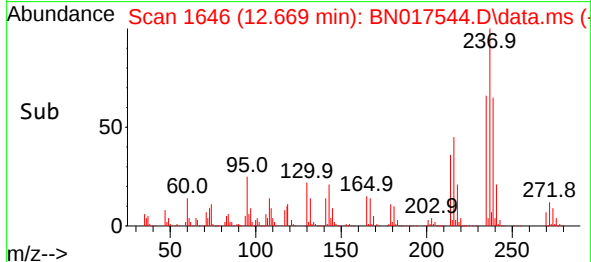

#41
2,4,6-Trichlorophenol
Concen: 151.322 ng/ul
RT: 12.922 min Scan# 1689
Delta R.T. 0.012 min
Lab File: BN017544.D
Acq: 22 Nov 2021 13:26

Tgt Ion:196 Resp: 1781531
Ion Ratio Lower Upper
196 100
198 94.7 75.8 113.8
200 29.9 24.0 36.0


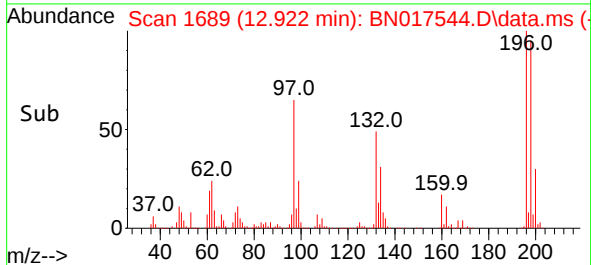






#42
2,4,5-Trichlorophenol
Concen: 145.366 ng/ul
RT: 12.993 min Scan# 11
Delta R.T. 0.012 min
Lab File: BN017544.D
Acq: 22 Nov 2021 13:26




Instrument :
BNA_N
ClientSampleId :
SSTD160250


Tgt Ion:196 Resp: 1905826
Ion Ratio Lower Upper
196 100
198 95.1 76.4 114.6
200 30.5 24.4 36.6

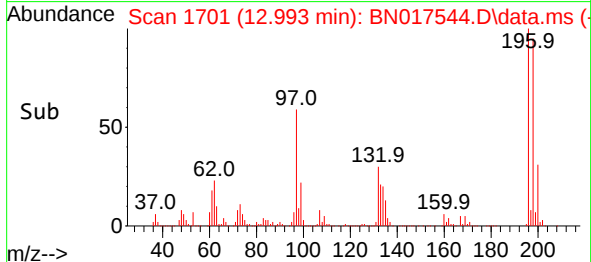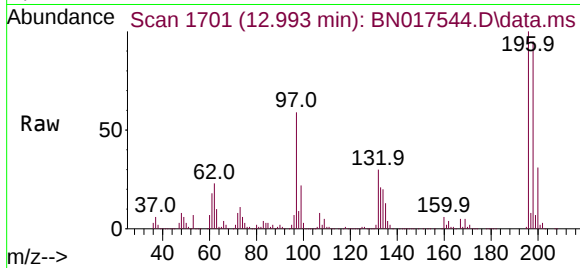

#43
1,1'-Biphenyl
Concen: 130.697 ng/ul
RT: 13.328 min Scan# 1758
Delta R.T. 0.012 min
Lab File: BN017544.D
Acq: 22 Nov 2021 13:26

Tgt Ion:154 Resp: 6303991
Ion Ratio Lower Upper
154 100
153 43.1 32.1 48.1
76 13.5 10.6 15.8

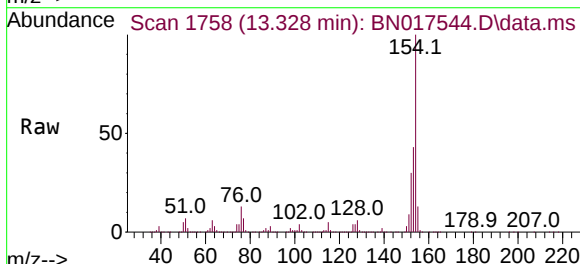



#44

2-Chloronaphthalene

Concen: 137.143 ng/ul

RT: 13.369 min Scan# 1765

Delta R.T. 0.018 min

Lab File: BN017544.D

Acq: 22 Nov 2021 13:26

Instrument :

BNA_N

ClientSampleId :

SSTD160250





Tgt Ion:162 Resp: 5037853

Ion Ratio Lower Upper

162 100

164 32.7 25.6 38.4

127 44.3 31.1 46.7

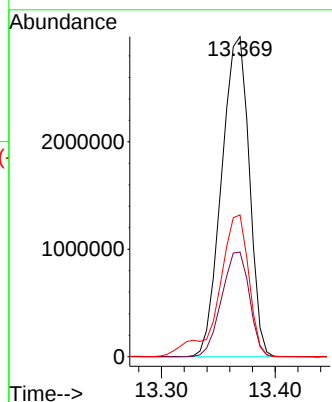

#45

2-Nitroaniline

Concen: 174.202 ng/ul

RT: 13.569 min Scan# 1799

Delta R.T. 0.018 min

Lab File: BN017544.D

Acq: 22 Nov 2021 13:26




Tgt Ion: 65 Resp: 1741988


Ion Ratio Lower Upper

65 100

92 69.3 56.9 85.3

138 99.8 89.3 133.9


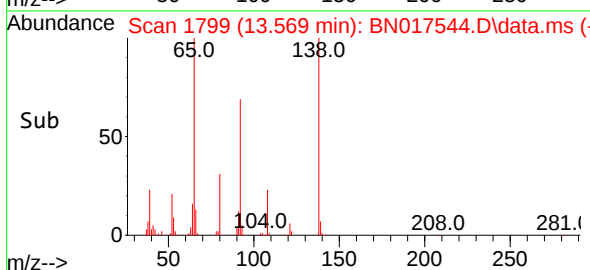






#47
Dimethylphthalate
Concen: 125.602 ng/ul
RT: 13.957 min Scan# 1865
Delta R.T. 0.018 min
Lab File: BN017544.D
Acq: 22 Nov 2021 13:26




Instrument :
BNA_N
ClientSampleId :
SSTD160250


Tgt Ion:163 Resp: 5882960
Ion Ratio Lower Upper
163 100
194 3.9 3.3 4.9
164 10.1 7.8 11.8



#48
2,6-Dinitrotoluene
Concen: 145.599 ng/ul
RT: 14.069 min Scan# 1884
Delta R.T. 0.018 min
Lab File: BN017544.D
Acq: 22 Nov 2021 13:26

Tgt Ion:165 Resp: 1339129
Ion Ratio Lower Upper
165 100
89 63.8 42.3 63.5#
121 22.3 16.9 25.3


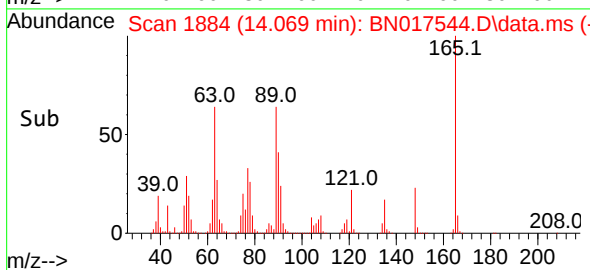






#50
Acenaphthylene
Concen: 124.819 ng/ul
RT: 14.210 min Scan# 1906
Delta R.T. 0.012 min
Lab File: BN017544.D
Acq: 22 Nov 2021 13:26




Instrument :
BNA_N
ClientSampleId :
SSTD160250


Tgt Ion:152 Resp: 7515895
Ion Ratio Lower Upper
152 100
151 20.6 15.9 23.9
153 13.4 10.6 15.8

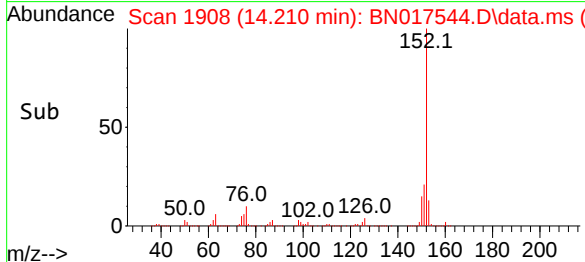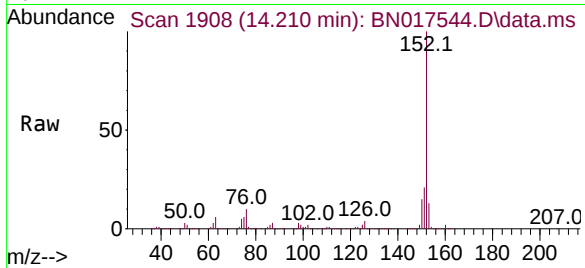

#51
3-Nitroaniline
Concen: 109.585 ng/ul
RT: 14.393 min Scan# 1939
Delta R.T. 0.018 min
Lab File: BN017544.D
Acq: 22 Nov 2021 13:26

Tgt Ion:138 Resp: 1166566
Ion Ratio Lower Upper
138 100
108 12.1 8.5 12.7
92 124.9 89.4 134.0


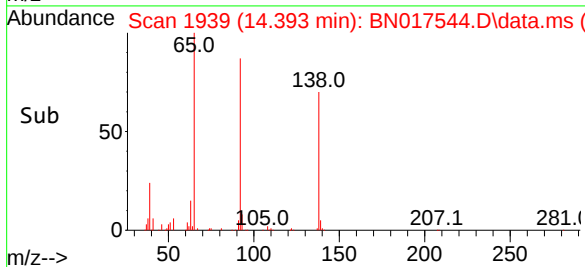

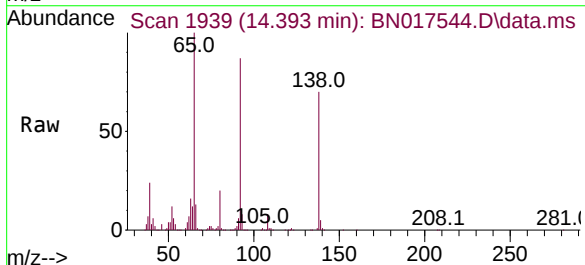




#52
Acenaphthene
Concen: 128.054 ng/ul
RT: 14.551 min Scan# 1966
Delta R.T. 0.006 min
Lab File: BN017544.D
Acq: 22 Nov 2021 13:26




Instrument :
BNA_N
ClientSampleId :
SSTD160250


Tgt Ion:153 Resp: 4986083
Ion Ratio Lower Upper
153 100
152 47.1 37.6 56.4
154 87.3 72.2 108.4



#53
2,4-Dinitrophenol
Concen: 132.714 ng/ul
RT: 14.598 min Scan# 1974
Delta R.T. 0.018 min
Lab File: BN017544.D
Acq: 22 Nov 2021 13:26

Tgt Ion:184 Resp: 780705
Ion Ratio Lower Upper
184 100
63 71.6 54.2 81.4
154 70.3 50.2 75.2


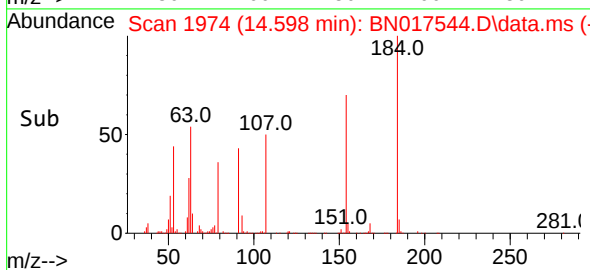






#55
4-Nitrophenol
Concen: 152.159 ng/ul
RT: 14.716 min Scan# 1988
Delta R.T. 0.036 min
Lab File: BN017544.D
Acq: 22 Nov 2021 13:26




Instrument :
BNA_N
ClientSampleId :
SSTD160250


Tgt Ion:109 Resp: 988080
Ion Ratio Lower Upper
109 100
139 110.0 121.5 182.3#
65 119.7 109.4 164.0



#56
Dibenzofuran
Concen: 121.551 ng/ul
RT: 14.887 min Scan# 2023
Delta R.T. 0.012 min
Lab File: BN017544.D
Acq: 22 Nov 2021 13:26

Tgt Ion:168 Resp: 6757349
Ion Ratio Lower Upper
168 100
139 42.9 29.9 44.9


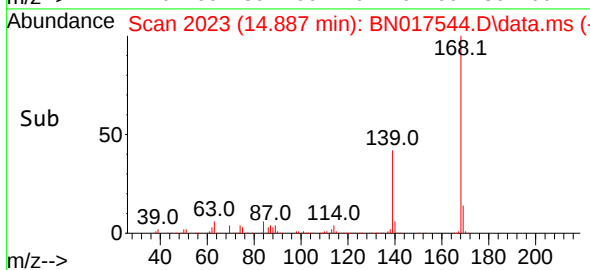






#57
2,4-Dinitrotoluene
Concen: 131.635 ng/ul
RT: 14.857 min Scan# 2014
Delta R.T. 0.024 min
Lab File: BN017544.D
Acq: 22 Nov 2021 13:26




Instrument :
BNA_N
ClientSampleId :
SSTD160250


Tgt Ion:165 Resp: 1746014
Ion Ratio Lower Upper
165 100
63 48.0 35.4 53.0
182 2.7 2.3 3.5



#58
2,3,4,6-Tetrachlorophenol
Concen: 125.447 ng/ul
RT: 15.116 min Scan# 2062
Delta R.T. 0.012 min
Lab File: BN017544.D
Acq: 22 Nov 2021 13:26

Tgt Ion:232 Resp: 1357707
Ion Ratio Lower Upper
232 100
131 50.4 40.1 60.1
130 2.7 2.0 3.0
166 33.5 26.2 39.4

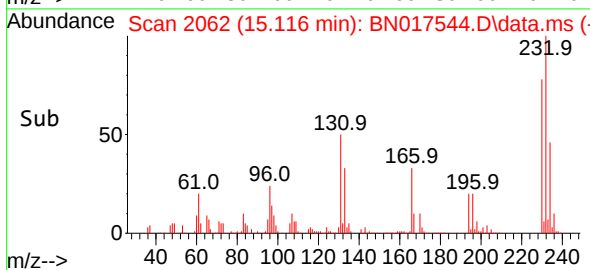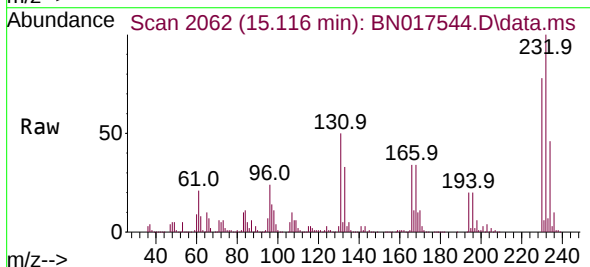



#59

Diethylphthalate

Concen: 124.207 ng/ul

RT: 15.322 min Scan# 2097

Delta R.T. 0.018 min

Lab File: BN017544.D

Acq: 22 Nov 2021 13:26

Instrument :





BNA_N

ClientSampleId :

SSTD160250

Tgt Ion:149 Resp: 5801192

Ion	Ratio	Lower	Upper
149	100		
177	21.5	17.6	26.4
150	12.6	10.0	15.0



#61

Fluorene

Concen: 105.774 ng/ul

RT: 15.540 min Scan# 2134




Delta R.T. 0.012 min


Lab File: BN017544.D

Acq: 22 Nov 2021 13:26

Tgt Ion:166 Resp: 4635183

Ion	Ratio	Lower	Upper
166	100		
165	100.4	77.4	116.0
167	13.8	11.0	16.6


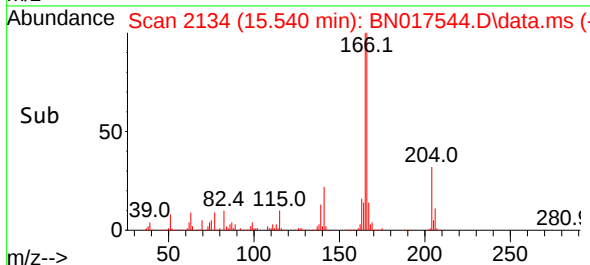

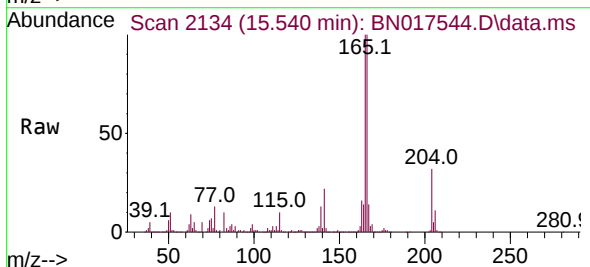




#62
4-Chlorophenyl-phenylether
Concen: 110.000 ng/ul
RT: 15.528 min Scan# 2131
Delta R.T. 0.006 min
Lab File: BN017544.D
Acq: 22 Nov 2021 13:26




Instrument :
BNA_N
ClientSampleId :
SSTD160250


Tgt Ion:204 Resp: 2370281
Ion Ratio Lower Upper
204 100
206 34.4 27.0 40.4
141 69.3 47.2 70.8



#63
4-Nitroaniline
Concen: 76.966 ng/ul
RT: 15.563 min Scan# 2138
Delta R.T. 0.024 min
Lab File: BN017544.D
Acq: 22 Nov 2021 13:26

Tgt Ion:138 Resp: 809595
Ion Ratio Lower Upper
138 100
92 54.8 39.0 58.4
108 91.9 56.7 85.1#


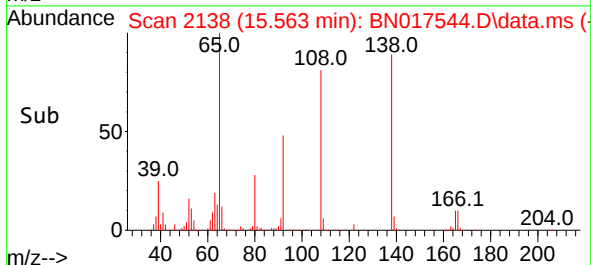






#66
4,6-Dinitro-2-methylphenol
Concen: 131.672 ng/ul
RT: 15.622 min Scan# 2148
Delta R.T. 0.024 min
Lab File: BN017544.D
Acq: 22 Nov 2021 13:26




Instrument :
BNA_N
ClientSampleId :
SSTD160250


Tgt Ion:198 Resp: 892109
Ion Ratio Lower Upper
198 100
182 3.6 3.1 4.7
77 31.1 17.4 26.2#



#67
N-Nitrosodiphenylamine
Concen: 140.955 ng/ul
RT: 15.745 min Scan# 2169
Delta R.T. 0.012 min
Lab File: BN017544.D
Acq: 22 Nov 2021 13:26

Tgt Ion:169 Resp: 4499334
Ion Ratio Lower Upper
169 100
168 65.2 50.8 76.2
167 36.4 29.0 43.6


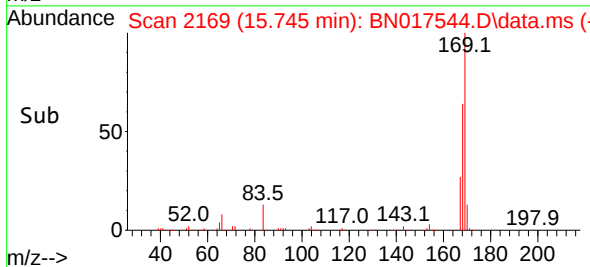

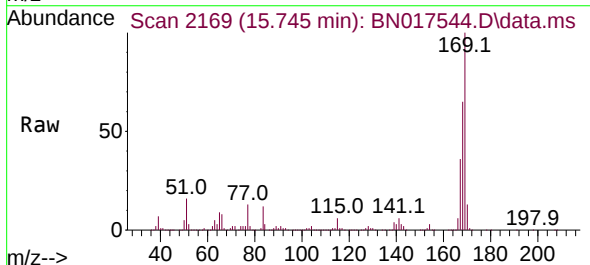




#68
4-Bromophenyl-phenylether
Concen: 140.373 ng/ul
RT: 16.422 min Scan# 21
Delta R.T. 0.006 min
Lab File: BN017544.D
Acq: 22 Nov 2021 13:26




Instrument :
BNA_N
ClientSampleId :
SSTD160250


Tgt Ion:248 Resp: 1568729
Ion Ratio Lower Upper
248 100
250 96.4 78.9 118.3
141 89.2 59.8 89.6

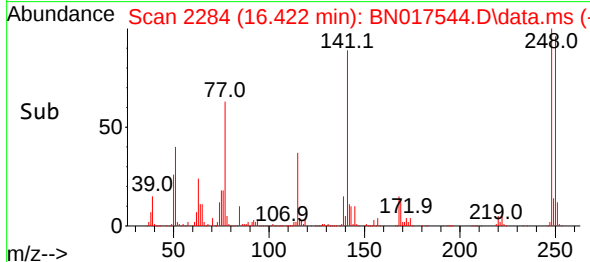

#69
Hexachlorobenzene
Concen: 121.140 ng/ul
RT: 16.545 min Scan# 2305
Delta R.T. 0.012 min
Lab File: BN017544.D
Acq: 22 Nov 2021 13:26

Tgt Ion:284 Resp: 1575392
Ion Ratio Lower Upper
284 100
142 42.7 28.2 42.2#
249 36.5 24.5 36.7


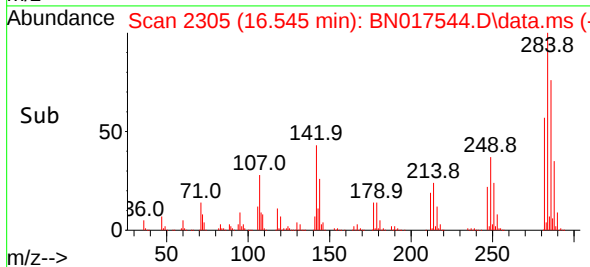

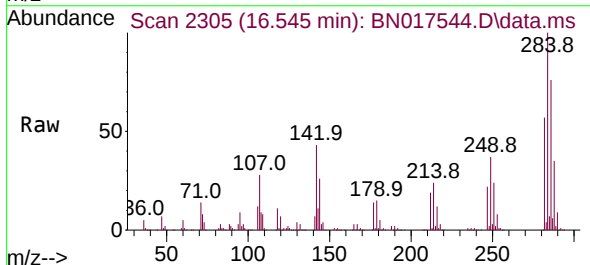




#70
Atrazine
Concen: 138.531 ng/ul
RT: 16.704 min Scan# 21
Delta R.T. 0.018 min
Lab File: BN017544.D
Acq: 22 Nov 2021 13:26




Instrument :
BNA_N
ClientSampleId :
SSTD160250


Tgt Ion:200 Resp: 1622544
Ion Ratio Lower Upper
200 100
173 27.3 21.6 32.4
215 46.8 38.8 58.2

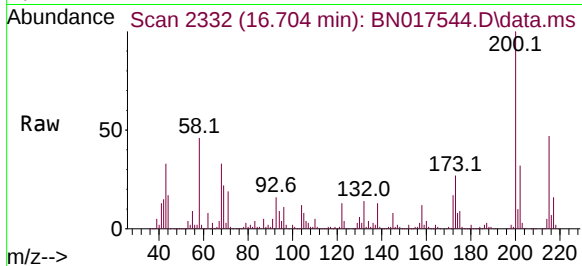

#71
Pentachlorophenol
Concen: 132.618 ng/ul
RT: 16.881 min Scan# 2362
Delta R.T. 0.006 min
Lab File: BN017544.D
Acq: 22 Nov 2021 13:26

Tgt Ion:266 Resp: 1035380
Ion Ratio Lower Upper
266 100
264 64.6 52.2 78.2
268 64.3 51.4 77.0

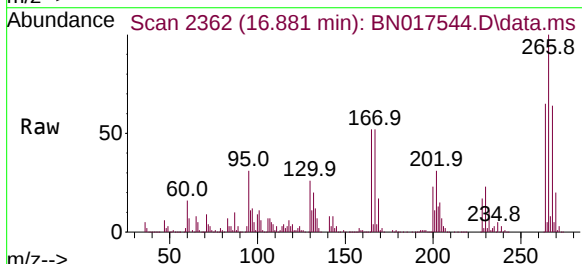



#72

Phenanthrene

Concen: 129.062 ng/u1

RT: 17.275 min Scan# 2427

Delta R.T. 0.012 min

Lab File: BN017544.D

Acq: 22 Nov 2021 13:26

Instrument :

BNA_N

ClientSampleId :

SSTD160250





Tgt Ion:178 Resp: 7457313

Ion Ratio Lower Upper

178 100

179 15.6 12.5 18.7

176 19.5 14.6 22.0

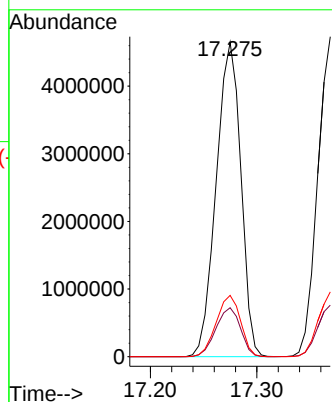

#74

Anthracene

Concen: 121.326 ng/u1

RT: 17.369 min Scan# 2445

Delta R.T. 0.012 min

Lab File: BN017544.D

Acq: 22 Nov 2021 13:26




Tgt Ion:178 Resp: 7099124


Ion Ratio Lower Upper

178 100

179 16.1 12.2 18.2

176 20.3 14.2 21.2


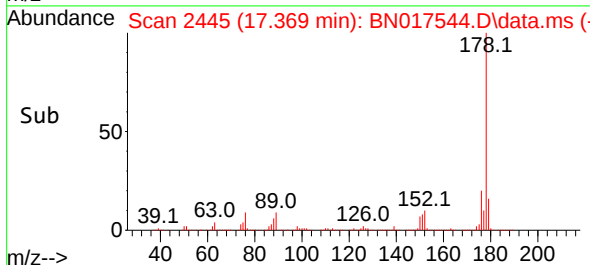

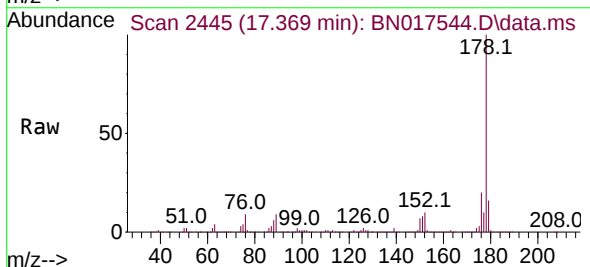




#75
1,2,3,4-Tetrachlorobenzene
Concen: 177.407 ng/uL
RT: 13.287 min Scan# 1751
Delta R.T. 0.006 min
Lab File: BN017544.D
Acq: 22 Nov 2021 13:26




Instrument :
BNA_N
ClientSampleId :
SSTD160250


Tgt Ion:216 Resp: 2719707
Ion Ratio Lower Upper
216 100
214 79.9 61.5 92.3
218 50.0 40.6 61.0



#76
Pentachlorobenzene
Concen: 150.602 ng/uL
RT: 14.810 min Scan# 2010
Delta R.T. 0.006 min
Lab File: BN017544.D
Acq: 22 Nov 2021 13:26

Tgt Ion:250 Resp: 2338050
Ion Ratio Lower Upper
250 100
248 62.0 53.2 79.8
252 60.1 52.5 78.7



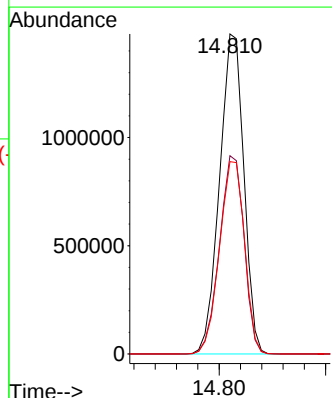





#77
Carbazole
Concen: 126.482 ng/ul
RT: 17.634 min Scan# 2488
Delta R.T. 0.012 min
Lab File: BN017544.D
Acq: 22 Nov 2021 13:26




Instrument :
BNA_N
ClientSampleId :
SSTD160250


Tgt Ion:167 Resp: 6534117
Ion Ratio Lower Upper
167 100
166 21.7 17.6 26.4
139 14.2 10.6 16.0

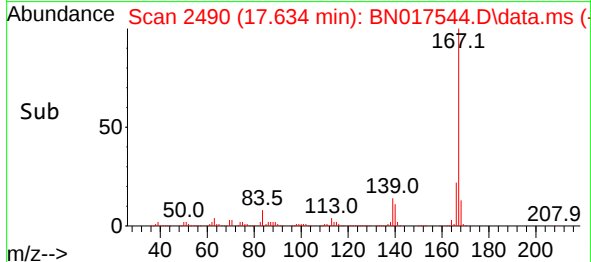

#78
Di-n-butylphthalate
Concen: 135.264 ng/ul
RT: 18.204 min Scan# 2587
Delta R.T. 0.006 min
Lab File: BN017544.D
Acq: 22 Nov 2021 13:26

Tgt Ion:149 Resp: 8259999
Ion Ratio Lower Upper
149 100
150 9.3 7.4 11.2
104 6.0 3.8 5.6#




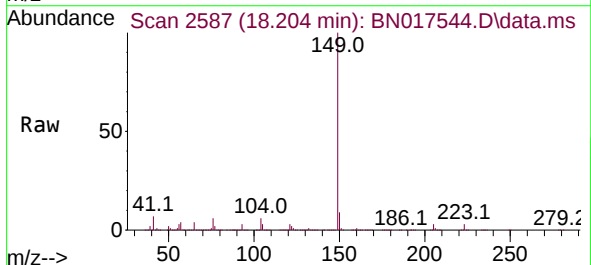




#80
Fluoranthene
Concen: 159.472 ng/ul
RT: 19.292 min Scan# 21
Delta R.T. 0.012 min
Lab File: BN017544.D
Acq: 22 Nov 2021 13:26




Instrument :
BNA_N
ClientSampleId :
SSTD160250


Tgt Ion:202 Resp: 7543373
Ion Ratio Lower Upper
202 100
101 10.6 9.6 14.4
100 8.2 7.3 10.9



#82
Pyrene
Concen: 148.764 ng/ul
RT: 19.657 min Scan# 2834
Delta R.T. 0.012 min
Lab File: BN017544.D
Acq: 22 Nov 2021 13:26

Tgt Ion:202 Resp: 7202782
Ion Ratio Lower Upper
202 100
101 12.3 11.8 17.6
100 10.4 9.6 14.4









#83
Butylbenzylphthalate
Concen: 188.753 ng/ul
RT: 20.557 min Scan# 2986
Delta R.T. 0.006 min
Lab File: BN017544.D
Acq: 22 Nov 2021 13:26




Instrument :
BNA_N
ClientSampleId :
SSTD160250


Tgt Ion:149 Resp: 3402854
Ion Ratio Lower Upper
149 100
91 73.5 54.5 81.7
206 20.7 17.7 26.5



#84
3,3'-Dichlorobenzidine
Concen: 115.595 ng/ul
RT: 21.333 min Scan# 3119
Delta R.T. 0.006 min
Lab File: BN017544.D
Acq: 22 Nov 2021 13:26

Tgt Ion:252 Resp: 1737968
Ion Ratio Lower Upper
252 100
254 65.4 47.6 71.4
126 11.2 10.1 15.1









#85
Benzo(a)anthracene
Concen: 150.074 ng/ul
RT: 21.404 min Scan# 3131
Delta R.T. 0.006 min
Lab File: BN017544.D
Acq: 22 Nov 2021 13:26




Instrument :
BNA_N
ClientSampleId :
SSTD160250


Tgt Ion:228 Resp: 6672579
Ion Ratio Lower Upper
228 100
229 19.8 15.8 23.8
226 27.6 21.8 32.8



#86
Bis(2-ethylhexyl)phthalate
Concen: 161.028 ng/ul
RT: 21.339 min Scan# 3120
Delta R.T. 0.000 min
Lab File: BN017544.D
Acq: 22 Nov 2021 13:26

Tgt Ion:149 Resp: 4381414
Ion Ratio Lower Upper
149 100
167 26.8 22.6 33.8
279 4.4 3.8 5.6









#87
Chrysene
Concen: 141.220 ng/ul
RT: 21.457 min Scan# 3138
Delta R.T. 0.012 min
Lab File: BN017544.D
Acq: 22 Nov 2021 13:26




Instrument :
BNA_N
ClientSampleId :
SSTD160250


Tgt Ion:228 Resp: 6188508
Ion Ratio Lower Upper
228 100
226 29.8 24.1 36.1
229 19.6 15.6 23.4

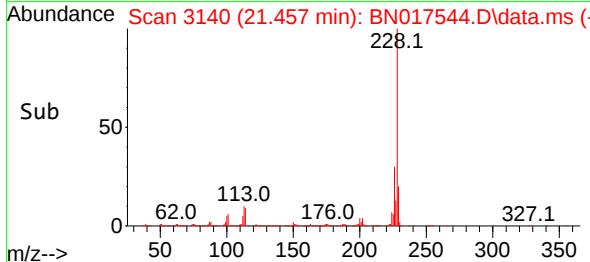

#89
Di-n-octyl phthalate
Concen: 157.094 ng/ul
RT: 22.257 min Scan# 3276
Delta R.T. 0.006 min
Lab File: BN017544.D
Acq: 22 Nov 2021 13:26

Tgt Ion:149 Resp: 8261416


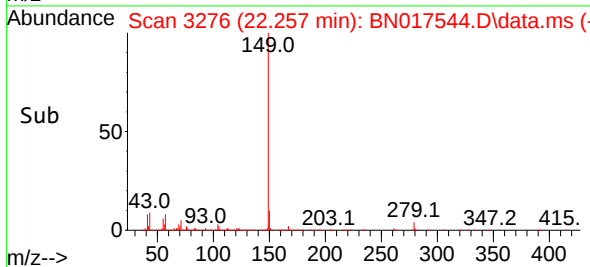

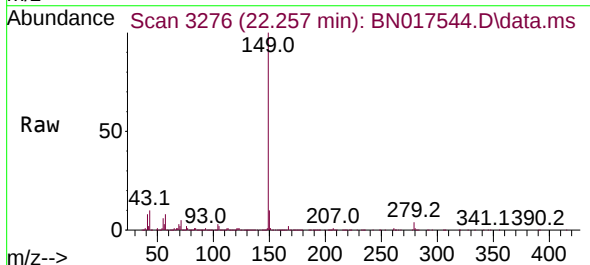




#90
Benzo(b)fluoranthene
Concen: 144.969 ng/ul
RT: 23.074 min Scan# 3412
Delta R.T. 0.018 min
Lab File: BN017544.D
Acq: 22 Nov 2021 13:26




Instrument :
BNA_N
ClientSampleId :
SSTD160250


Tgt Ion:252 Resp: 7041869
Ion Ratio Lower Upper
252 100
253 21.8 18.4 27.6
125 9.4 9.4 14.0

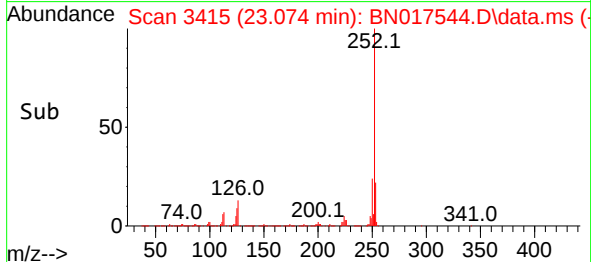

#91
Benzo(k)fluoranthene
Concen: 139.515 ng/ul
RT: 23.122 min Scan# 3423
Delta R.T. 0.018 min
Lab File: BN017544.D
Acq: 22 Nov 2021 13:26

Tgt Ion:252 Resp: 6592020
Ion Ratio Lower Upper
252 100
253 20.9 17.4 26.2
125 9.8 8.6 13.0




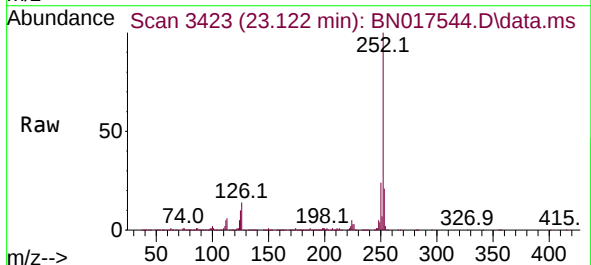




#93
Benzo(a)pyrene
Concen: 142.185 ng/ul
RT: 23.698 min Scan# 3521
Delta R.T. 0.024 min
Lab File: BN017544.D
Acq: 22 Nov 2021 13:26




Instrument :
BNA_N
ClientSampleId :
SSTD160250


Tgt Ion:252 Resp: 6645681
Ion Ratio Lower Upper
252 100
253 22.9 17.5 26.3
125 10.9 9.7 14.5



#94
Indeno(1,2,3-cd)pyrene
Concen: 171.202 ng/ul
RT: 26.263 min Scan# 3957
Delta R.T. 0.036 min
Lab File: BN017544.D
Acq: 22 Nov 2021 13:26

Tgt Ion:276 Resp: 8163058
Ion Ratio Lower Upper
276 100
138 25.5 21.4 32.2
277 23.3 19.5 29.3





#95

Dibenzo(a,h)anthracene

Concen: 165.018 ng/ul

RT: 26.280 min Scan# 3953

Delta R.T. 0.042 min

Lab File: BN017544.D

Acq: 22 Nov 2021 13:26

Instrument :

BNA_N

ClientSampleId :

SSTD160250





Tgt Ion:278 Resp: 6650829

Ion Ratio Lower Upper

278 100

139 15.0 14.7 22.1

279 21.8 19.7 29.5

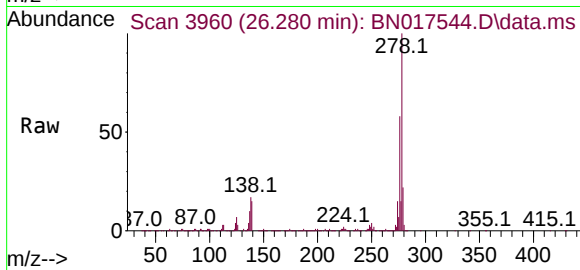

#96

Benzo(g,h,i)perylene

Concen: 180.777 ng/ul

RT: 27.015 min Scan# 4085

Delta R.T. 0.048 min

Lab File: BN017544.D

Acq: 22 Nov 2021 13:26

Tgt Ion:276 Resp: 7217238

Ion Ratio Lower Upper

276 100

138 21.7 18.2 27.4

277 22.1 17.4 26.0

