

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112221\
 Data File : BN017545.D
 Acq On : 22 Nov 2021 15:06
 Operator : CG/JU
 Sample : SSTDICV020
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SICV201

Quant Time: Nov 22 16:19:29 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN112221.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Nov 22 16:16:36 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.840	152	257695	20.000	ng/u1	0.00
20) Naphthalene-d8	10.640	136	1166884	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.475	164	743802	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.222	188	1541498	20.000	ng/u1	0.00
79) Chrysene-d12	21.416	240	1417072	20.000	ng/u1	0.00
88) Perylene-d12	23.786	264	1400506	20.000	ng/u1	0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.299	96	51636	7.161	ng/uL	-0.01
4) Pyridine-d5	3.699	84	342296	18.091	ng/u1	-0.01
7) Phenol-d5	6.999	99	424494	18.095	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.163	67	266173	18.106	ng/u1	-0.01
11) 2-Chlorophenol-d4	7.369	132	323050	18.187	ng/u1	0.00
15) 4-Methylphenol-d8	8.540	113	345847	18.742	ng/u1	-0.01
21) Nitrobenzene-d5	8.993	128	165532	18.725	ng/u1	0.00
24) 2-Nitrophenol-d4	9.716	143	165017	18.867	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.251	165	323692	18.798	ng/u1	0.00
31) 4-Chloroaniline-d4	10.763	131	486999	19.696	ng/u1	0.00
46) Dimethylphthalate-d6	13.886	166	1009010	18.658	ng/u1	0.00
49) Acenaphthylene-d8	14.169	160	1280302	18.439	ng/u1	0.00
54) 4-Nitrophenol-d4	14.663	143	186906	20.424	ng/u1	0.00
60) Fluorene-d10	15.469	176	870174	19.077	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.581	200	143374	17.907	ng/u1	0.00
73) Anthracene-d10	17.322	188	1336498	18.654	ng/u1	0.00
81) Pyrene-d10	19.616	212	1568908	17.441	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.627	264	1334131	18.119	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.334	88	53459	7.509	ng/uL	96
5) Pyridine	3.722	79	348308	18.292	ng/u1	94
6) Benzaldehyde	6.969	77	280420	22.533	ng/u1	92
8) Phenol	7.022	94	438135	18.440	ng/u1	95
10) Bis(2-Chloroethyl)ether	7.257	93	352253	18.081	ng/u1	98
12) 2-Chlorophenol	7.399	128	337186	18.421	ng/u1	96
13) 2-Methylphenol	8.275	108	328498	18.356	ng/u1	99
14) 2,2'-oxybis(1-Chloropr...	8.369	45	481076	18.316	ng/u1	95
16) Acetophenone	8.657	105	535576	19.408	ng/u1	92
17) N-Nitroso-di-n-propyla...	8.646	70	282186	19.619	ng/u1	94
18) 4-Methylphenol	8.604	108	359697	18.763	ng/u1	95
19) Hexachloroethane	8.922	117	139802	18.077	ng/u1	98
22) Nitrobenzene	9.034	77	413290	18.499	ng/u1	95
23) Isophorone	9.557	82	791514	18.928	ng/u1	97
25) 2-Nitrophenol	9.746	139	183789	19.050	ng/u1	91
26) 2,4-Dimethylphenol	9.810	107	411415	18.439	ng/u1	97
27) Bis(2-Chloroethoxy)met...	10.046	93	491365	18.054	ng/u1	98
29) 2,4-Dichlorophenol	10.281	162	323152	18.611	ng/u1	98
30) Naphthalene	10.687	128	1124058	18.006	ng/u1	99
32) 4-Chloroaniline	10.787	127	491760	19.601	ng/u1	99
33) Hexachlorobutadiene	10.987	225	206178	18.053	ng/u1	96
34) Caprolactam	11.534	113	106627	20.249	ng/u1	93
35) 4-Chloro-3-methylphenol	11.916	107	376873	19.293	ng/u1	96
36) 2-Methylnaphthalene	12.298	142	767089	18.411	ng/u1	100


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112221\
 Data File : BN017545.D
 Acq On : 22 Nov 2021 15:06
 Operator : CG/JU
 Sample : SSTDICV020
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SICV201

Quant Time: Nov 22 16:19:29 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN112221.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Nov 22 16:16:36 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.516	142	802607	19.025	ng/ul	99
39) 1,2,4,5-Tetrachloroben...	12.675	216	394868	17.899	ng/ul	94
40) Hexachlorocyclopentadiene	12.657	237	234036	16.540	ng/ul	97
41) 2,4,6-Trichlorophenol	12.910	196	248093	18.408	ng/ul	97
42) 2,4,5-Trichlorophenol	12.975	196	276409	18.808	ng/ul	99
43) 1,1'-Biphenyl	13.310	154	1057271	18.023	ng/ul	99
44) 2-Chloronaphthalene	13.351	162	798986	17.912	ng/ul	96
45) 2-Nitroaniline	13.545	65	242769	19.664	ng/ul	91
47) Dimethylphthalate	13.934	163	1026236	19.145	ng/ul	99
48) 2,6-Dinitrotoluene	14.045	165	200690	19.949	ng/ul	90
50) Acenaphthylene	14.198	152	1311014	18.526	ng/ul	99
51) 3-Nitroaniline	14.375	138	220685	20.720	ng/ul	93
52) Acenaphthene	14.539	153	840374	18.419	ng/ul	98
53) 2,4-Dinitrophenol	14.575	184	88538	17.508	ng/ul	91
55) 4-Nitrophenol	14.675	109	163309	20.461	ng/ul#	82
56) Dibenzofuran	14.875	168	1199398	18.312	ng/ul	95
57) 2,4-Dinitrotoluene	14.833	165	295472	20.727	ng/ul	98
58) 2,3,4,6-Tetrachlorophenol	15.104	232	214851	19.759	ng/ul	99
59) Diethylphthalate	15.304	149	1033835	19.257	ng/ul	100
61) Fluorene	15.522	166	932463	18.965	ng/ul	99
62) 4-Chlorophenyl-phenyle...	15.522	204	460784	19.205	ng/ul	92
63) 4-Nitroaniline	15.533	138	210899	23.485	ng/ul#	84
66) 4,6-Dinitro-2-methylph...	15.598	198	147844	18.393	ng/ul#	87
67) N-Nitrosodiphenylamine	15.733	169	837547	18.025	ng/ul	97
68) 4-Bromophenyl-phenylether	16.416	248	269485	17.706	ng/ul#	87
69) Hexachlorobenzene	16.533	284	294874	18.179	ng/ul#	88
70) Atrazine	16.686	200	308225	18.783	ng/ul	99
71) Pentachlorophenol	16.875	266	168916	18.314	ng/ul	95
72) Phenanthrene	17.263	178	1550257	18.432	ng/ul	99
74) Anthracene	17.357	178	1559122	18.693	ng/ul	99
75) 1,2,3,4-Tetrachloroben...	13.275	216	396432	16.402	ng/uL	98
76) Pentachlorobenzene	14.798	250	384112	17.478	ng/uL	95
77) Carbazole	17.622	167	1437239	20.078	ng/ul	99
78) Di-n-butylphthalate	18.204	149	1733906	19.932	ng/ul	99
80) Fluoranthene	19.280	202	1807259	16.701	ng/ul	100
82) Pyrene	19.645	202	1847659	17.055	ng/ul	98
83) Butylbenzylphthalate	20.551	149	761788	19.262	ng/ul	90
84) 3,3'-Dichlorobenzidine	21.333	252	567231	21.042	ng/ul	96
85) Benzo(a)anthracene	21.398	228	1779733	18.960	ng/ul	98
86) Bis(2-ethylhexyl)phtha...	21.339	149	1164667	20.347	ng/ul#	98
87) Chrysene	21.451	228	1706763	18.504	ng/ul	98
89) Di-n-octyl phthalate	22.257	149	1966354	18.486	ng/ul	100
90) Benzo(b)fluoranthene	23.062	252	1736198	17.929	ng/ul	96
91) Benzo(k)fluoranthene	23.110	252	1642289	17.961	ng/ul	99
93) Benzo(a)pyrene	23.680	252	1678443	18.255	ng/ul	99
94) Indeno(1,2,3-cd)pyrene	26.227	276	1698184	17.788	ng/ul	98
95) Dibenzo(a,h)anthracene	26.251	278	1456976	17.968	ng/ul	99
96) Benzo(g,h,i)perylene	26.974	276	1418434	17.383	ng/ul	95





(#) = qualifier out of range (m) = manual integration (+) = signals summed



#2
1,4-Dioxane
Concen: 7.509 ng/uL
RT: 3.334 min Scan# 51
Delta R.T. -0.006 min
Lab File: BN017545.D
Acq: 22 Nov 2021 15:06




Instrument :
BNA_N
ClientSampleId :
SICV201


Tgt Ion: 88 Resp: 53459
Ion Ratio Lower Upper
88 100
43 27.8 24.4 36.6
58 74.4 61.9 92.9

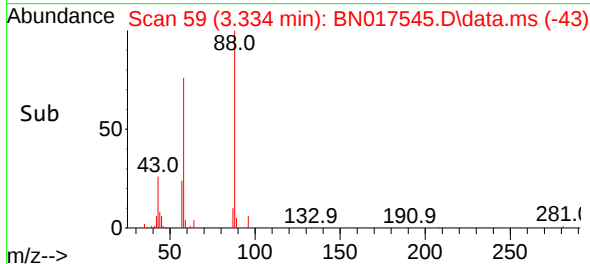

#5
Pyridine
Concen: 18.292 ng/uL
RT: 3.722 min Scan# 125
Delta R.T. -0.006 min
Lab File: BN017545.D
Acq: 22 Nov 2021 15:06

Tgt Ion: 79 Resp: 348308
Ion Ratio Lower Upper
79 100
52 76.4 66.7 100.1
51 36.3 30.6 46.0


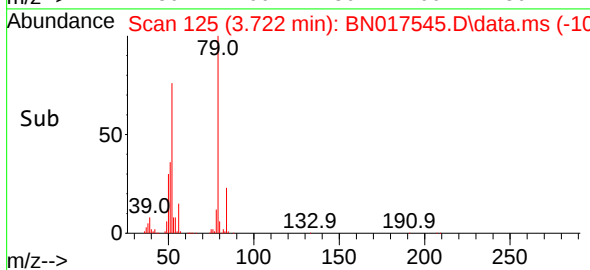

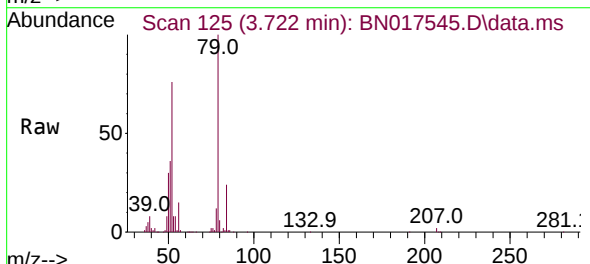




#6
Benzaldehyde
Concen: 22.533 ng/ul
RT: 6.969 min Scan# 677
Delta R.T. -0.012 min
Lab File: BN017545.D
Acq: 22 Nov 2021 15:06




Instrument :
BNA_N
ClientSampleId :
SICV201


Tgt Ion: 77 Resp: 280420
Ion Ratio Lower Upper
77 100
105 95.3 83.8 125.6
106 92.0 79.6 119.4



#8
Phenol
Concen: 18.440 ng/ul
RT: 7.022 min Scan# 686
Delta R.T. -0.012 min
Lab File: BN017545.D
Acq: 22 Nov 2021 15:06

Tgt Ion: 94 Resp: 438135
Ion Ratio Lower Upper
94 100
65 28.7 21.7 32.5
66 39.0 28.3 42.5


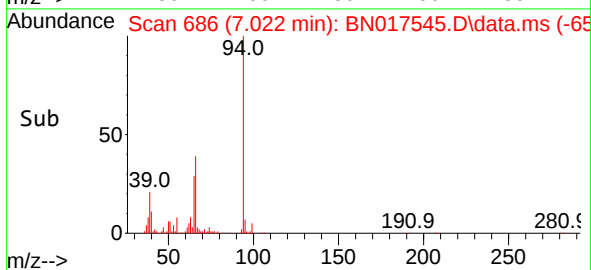






#10
Bis(2-Chloroethyl)ether
Concen: 18.081 ng/ul
RT: 7.257 min Scan# 71
Delta R.T. -0.012 min
Lab File: BN017545.D
Acq: 22 Nov 2021 15:06




Instrument :
BNA_N
ClientSampleId :
SICV201


Tgt Ion: 93 Resp: 352253
Ion Ratio Lower Upper
93 100
63 76.8 63.6 95.4
95 32.8 26.2 39.2



#12
2-Chlorophenol
Concen: 18.421 ng/ul
RT: 7.399 min Scan# 750
Delta R.T. -0.006 min
Lab File: BN017545.D
Acq: 22 Nov 2021 15:06

Tgt Ion:128 Resp: 337186
Ion Ratio Lower Upper
128 100
64 49.9 36.2 54.2
130 32.8 26.4 39.6









#13
2-Methylphenol
Concen: 18.356 ng/ul
RT: 8.275 min Scan# 899
Delta R.T. -0.006 min
Lab File: BN017545.D
Acq: 22 Nov 2021 15:06




Instrument :
BNA_N
ClientSampleId :
SICV201


Tgt Ion:108 Resp: 328498
Ion Ratio Lower Upper
108 100
107 89.6 71.1 106.7



#14
2,2'-oxybis(1-Chloropropane)
Concen: 18.316 ng/ul
RT: 8.369 min Scan# 915
Delta R.T. -0.012 min
Lab File: BN017545.D
Acq: 22 Nov 2021 15:06

Tgt Ion: 45 Resp: 481076
Ion Ratio Lower Upper
45 100
77 15.4 10.7 16.1
79 11.7 8.1 12.1









#16
Acetophenone
Concen: 19.408 ng/ul
RT: 8.657 min Scan# 965
Delta R.T. -0.006 min
Lab File: BN017545.D
Acq: 22 Nov 2021 15:06




Instrument :
BNA_N
ClientSampleId :
SICV201


Tgt Ion:105 Resp: 535576
Ion Ratio Lower Upper
105 100
77 81.7 58.6 87.8
51 28.3 21.3 31.9

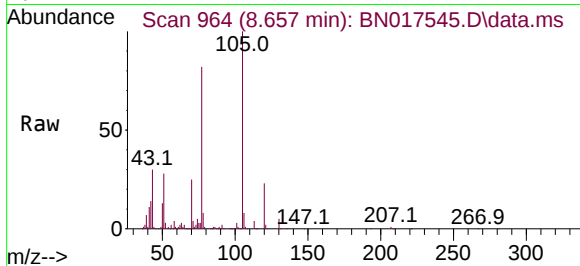

#17
N-Nitroso-di-n-propylamine
Concen: 19.619 ng/ul
RT: 8.646 min Scan# 962
Delta R.T. -0.006 min
Lab File: BN017545.D
Acq: 22 Nov 2021 15:06

Tgt Ion: 70 Resp: 282186
Ion Ratio Lower Upper
70 100
42 56.4 49.8 74.8
101 10.0 8.2 12.2
130 21.3 18.0 27.0




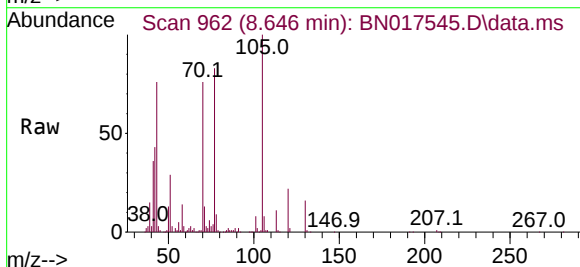




#18
4-Methylphenol
Concen: 18.763 ng/ul
RT: 8.604 min Scan# 91
Delta R.T. -0.006 min
Lab File: BN017545.D
Acq: 22 Nov 2021 15:06




Instrument :
BNA_N
ClientSampleId :
SICV201


Tgt Ion:108 Resp: 359697
Ion Ratio Lower Upper
108 100
107 116.3 88.7 133.1



#19
Hexachloroethane
Concen: 18.077 ng/ul
RT: 8.922 min Scan# 1009
Delta R.T. -0.006 min
Lab File: BN017545.D
Acq: 22 Nov 2021 15:06

Tgt Ion:117 Resp: 139802
Ion Ratio Lower Upper
117 100
201 95.1 78.1 117.1
199 59.8 46.6 70.0









#22
Nitrobenzene
Concen: 18.499 ng/ul
RT: 9.034 min Scan# 1028
Delta R.T. -0.006 min
Lab File: BN017545.D
Acq: 22 Nov 2021 15:06




Instrument :
BNA_N
ClientSampleId :
SICV201


Tgt Ion: 77 Resp: 413290
Ion Ratio Lower Upper
77 100
123 43.0 37.9 56.9
65 13.2 10.6 16.0



#23
Isophorone
Concen: 18.928 ng/ul
RT: 9.557 min Scan# 1117
Delta R.T. -0.006 min
Lab File: BN017545.D
Acq: 22 Nov 2021 15:06

Tgt Ion: 82 Resp: 791514
Ion Ratio Lower Upper
82 100
95 7.3 5.6 8.4
138 17.1 15.0 22.4

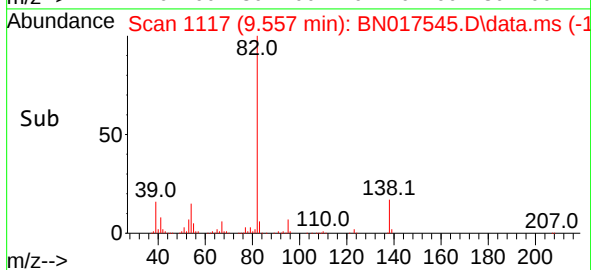



#25

2-Nitrophenol

Concen: 19.050 ng/ul

RT: 9.746 min Scan# 1149

Delta R.T. -0.006 min

Lab File: BN017545.D

Acq: 22 Nov 2021 15:06

Instrument :

BNA_N

ClientSampleId :

SICV201





Tgt Ion:139 Resp: 183789

Ion Ratio Lower Upper

139 100

65 54.1 38.4 57.6

109 32.4 21.9 32.9

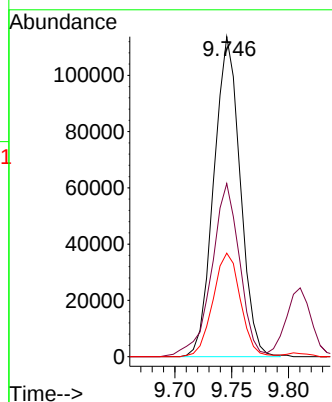

#26

2,4-Dimethylphenol

Concen: 18.439 ng/ul

RT: 9.810 min Scan# 1160

Delta R.T. -0.006 min

Lab File: BN017545.D

Acq: 22 Nov 2021 15:06




Tgt Ion:107 Resp: 411415


Ion Ratio Lower Upper

107 100

121 49.5 41.2 61.8

122 86.7 71.4 107.0









#27
 Bis(2-Chloroethoxy)methane
 Concen: 18.054 ng/ul
 RT: 10.046 min Scan# 11
 Delta R.T. -0.006 min
 Lab File: BN017545.D
 Acq: 22 Nov 2021 15:06




Instrument :
 BNA_N
 ClientSampleId :
 SICV201


Tgt Ion: 93 Resp: 491365
 Ion Ratio Lower Upper
 93 100
 95 32.8 25.4 38.2
 123 11.1 9.0 13.6

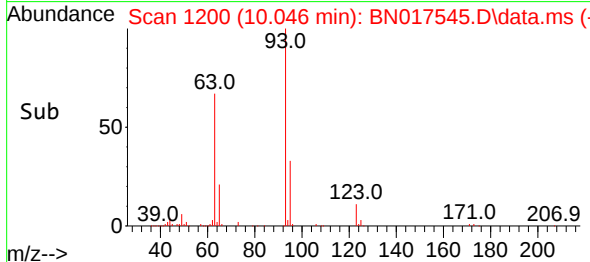

#29
 2,4-Dichlorophenol
 Concen: 18.611 ng/ul
 RT: 10.281 min Scan# 1240
 Delta R.T. -0.006 min
 Lab File: BN017545.D
 Acq: 22 Nov 2021 15:06

Tgt Ion:162 Resp: 323152
 Ion Ratio Lower Upper
 162 100
 164 66.2 53.6 80.4
 98 39.3 29.9 44.9




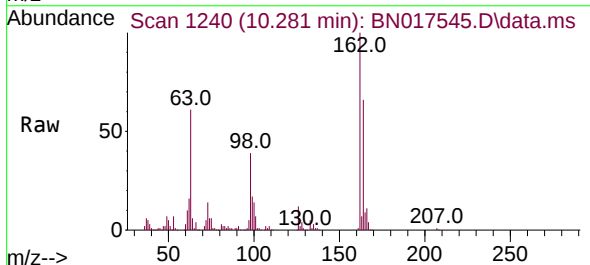




#30
Naphthalene
Concen: 18.006 ng/ul
RT: 10.687 min Scan# 1309
Delta R.T. -0.006 min
Lab File: BN017545.D
Acq: 22 Nov 2021 15:06




Instrument :
BNA_N
ClientSampleId :
SICV201


Tgt Ion:128 Resp: 1124058
Ion Ratio Lower Upper
128 100
129 10.8 8.4 12.6
127 13.2 10.3 15.5

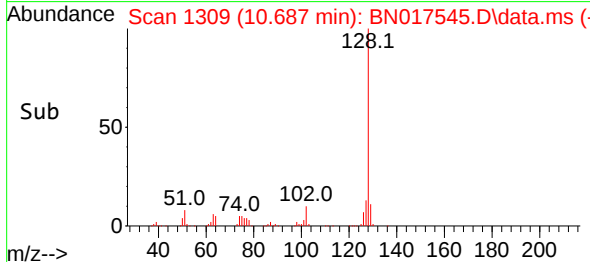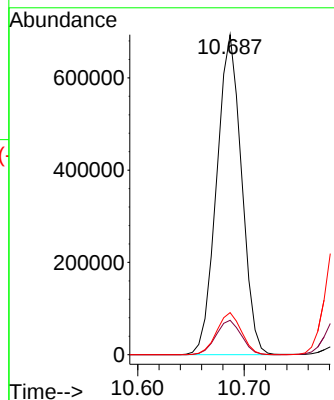

#32
4-Chloroaniline
Concen: 19.601 ng/ul
RT: 10.787 min Scan# 1326
Delta R.T. -0.006 min
Lab File: BN017545.D
Acq: 22 Nov 2021 15:06

Tgt Ion:127 Resp: 491760
Ion Ratio Lower Upper
127 100
129 32.9 25.8 38.6


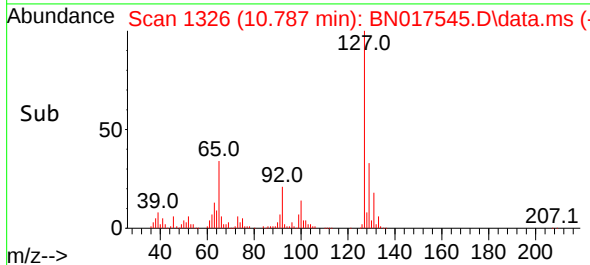
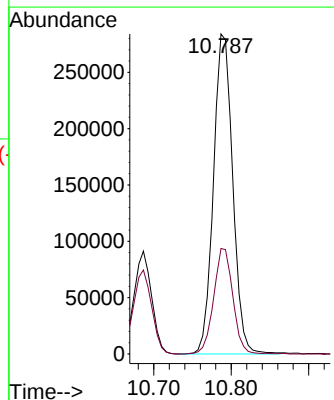





#33
Hexachlorobutadiene
Concen: 18.053 ng/ul
RT: 10.987 min Scan# 1360
Delta R.T. 0.000 min
Lab File: BN017545.D
Acq: 22 Nov 2021 15:06




Instrument :
BNA_N
ClientSampleId :
SICV201


Tgt Ion:225 Resp: 206178
Ion Ratio Lower Upper
225 100
223 65.5 49.4 74.2
227 63.5 49.0 73.6



#34
Caprolactam
Concen: 20.249 ng/ul
RT: 11.534 min Scan# 1453
Delta R.T. -0.006 min
Lab File: BN017545.D
Acq: 22 Nov 2021 15:06

Tgt Ion:113 Resp: 106627
Ion Ratio Lower Upper
113 100
55 164.7 141.4 212.2
56 125.0 103.9 155.9









#35
4-Chloro-3-methylphenol
Concen: 19.293 ng/ul
RT: 11.916 min Scan# 1518
Delta R.T. -0.006 min
Lab File: BN017545.D
Acq: 22 Nov 2021 15:06




Instrument :
BNA_N
ClientSampleId :
SICV201


Tgt Ion:107 Resp: 376873
Ion Ratio Lower Upper
107 100
144 24.5 20.6 30.8
142 76.5 64.1 96.1

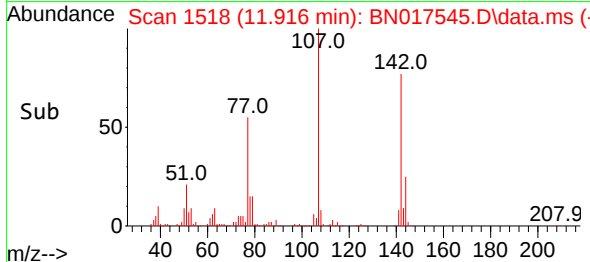

#36
2-Methylnaphthalene
Concen: 18.411 ng/ul
RT: 12.298 min Scan# 1583
Delta R.T. -0.006 min
Lab File: BN017545.D
Acq: 22 Nov 2021 15:06

Tgt Ion:142 Resp: 767089
Ion Ratio Lower Upper
142 100
141 87.5 70.2 105.2

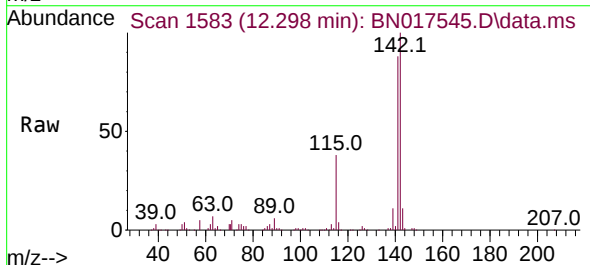



#37

1-Methylnaphthalene

Concen: 19.025 ng/ul

RT: 12.516 min Scan# 1620

Delta R.T. -0.006 min

Lab File: BN017545.D

Acq: 22 Nov 2021 15:06

Instrument :

BNA_N

ClientSampleId :

SICV201





Tgt Ion:142 Resp: 802607

Ion Ratio Lower Upper

142 100

141 91.2 72.2 108.2

116 4.0 3.0 4.6

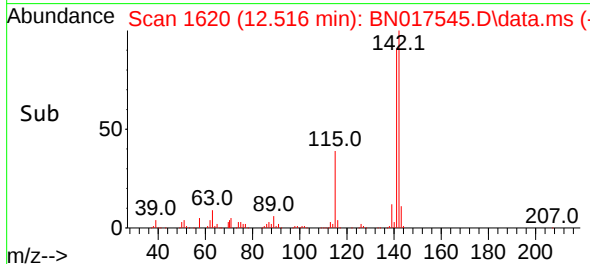

#39

1,2,4,5-Tetrachlorobenzene

Concen: 17.899 ng/ul

RT: 12.675 min Scan# 1647

Delta R.T. 0.000 min

Lab File: BN017545.D

Acq: 22 Nov 2021 15:06

Tgt Ion:216 Resp: 394868




Ion Ratio Lower Upper


216 100

214 74.6 65.6 98.4

179 21.4 17.4 26.0

108 18.3 14.0 21.0




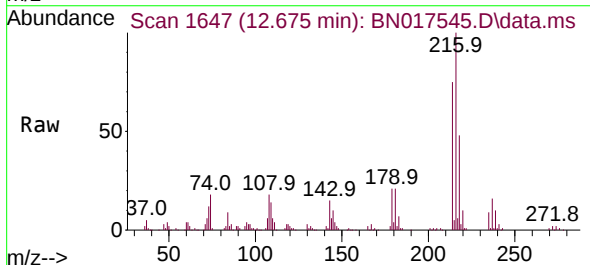




#40
Hexachlorocyclopentadiene
Concen: 16.540 ng/ul
RT: 12.657 min Scan# 1644
Delta R.T. -0.006 min
Lab File: BN017545.D
Acq: 22 Nov 2021 15:06




Instrument :
BNA_N
ClientSampleId :
SICV201


Tgt Ion:237 Resp: 234036
Ion Ratio Lower Upper
237 100
235 61.8 51.9 77.9
272 13.2 10.9 16.3



#41
2,4,6-Trichlorophenol
Concen: 18.408 ng/ul
RT: 12.910 min Scan# 1687
Delta R.T. 0.000 min
Lab File: BN017545.D
Acq: 22 Nov 2021 15:06

Tgt Ion:196 Resp: 248093
Ion Ratio Lower Upper
196 100
198 92.8 75.8 113.8
200 32.5 24.0 36.0





#42

2,4,5-Trichlorophenol

Concen: 18.808 ng/ul

RT: 12.975 min Scan# 1

Delta R.T. -0.006 min

Lab File: BN017545.D

Acq: 22 Nov 2021 15:06

Instrument :

BNA_N

ClientSampleId :

SICV201





Tgt Ion:196 Resp: 276409

Ion Ratio Lower Upper

196 100

198 94.7 76.4 114.6

200 29.9 24.4 36.6

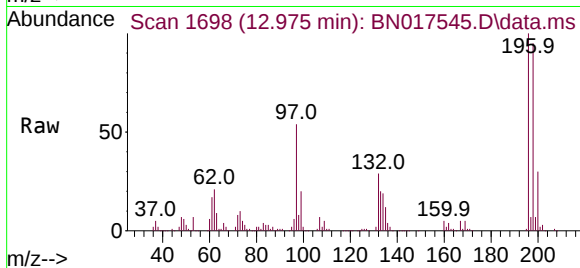

#43

1,1'-Biphenyl

Concen: 18.023 ng/ul

RT: 13.310 min Scan# 1755

Delta R.T. -0.006 min

Lab File: BN017545.D

Acq: 22 Nov 2021 15:06




Tgt Ion:154 Resp: 1057271


Ion Ratio Lower Upper

154 100

153 40.8 32.1 48.1

76 14.1 10.6 15.8




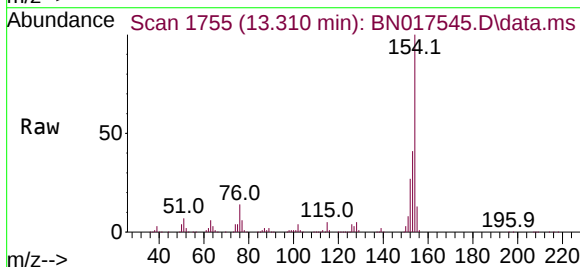




#44
2-Chloronaphthalene
Concen: 17.912 ng/ul
RT: 13.351 min Scan# 1762
Delta R.T. 0.000 min
Lab File: BN017545.D
Acq: 22 Nov 2021 15:06




Instrument :
BNA_N
ClientSampleId :
SICV201


Tgt Ion:162 Resp: 798986
Ion Ratio Lower Upper
162 100
164 33.0 25.6 38.4
127 42.4 31.1 46.7

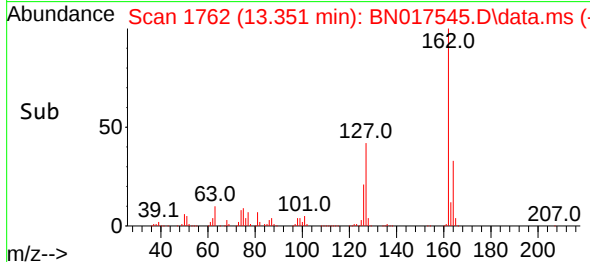

#45
2-Nitroaniline
Concen: 19.664 ng/ul
RT: 13.545 min Scan# 1795
Delta R.T. -0.006 min
Lab File: BN017545.D
Acq: 22 Nov 2021 15:06

Tgt Ion: 65 Resp: 242769
Ion Ratio Lower Upper
65 100
92 68.0 56.9 85.3
138 99.1 89.3 133.9




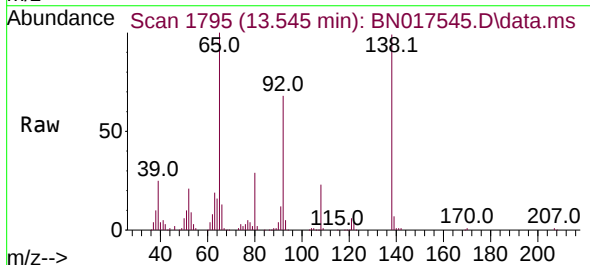




#47
Dimethylphthalate
Concen: 19.145 ng/ul
RT: 13.934 min Scan# 1861
Delta R.T. -0.006 min
Lab File: BN017545.D
Acq: 22 Nov 2021 15:06




Instrument :
BNA_N
ClientSampleId :
SICV201


Tgt Ion:163 Resp: 1026236
Ion Ratio Lower Upper
163 100
194 3.9 3.3 4.9
164 10.1 7.8 11.8



#48
2,6-Dinitrotoluene
Concen: 19.949 ng/ul
RT: 14.045 min Scan# 1880
Delta R.T. -0.006 min
Lab File: BN017545.D
Acq: 22 Nov 2021 15:06

Tgt Ion:165 Resp: 200690
Ion Ratio Lower Upper
165 100
89 61.4 42.3 63.5
121 22.9 16.9 25.3









#50
Acenaphthylene
Concen: 18.526 ng/ul
RT: 14.198 min Scan# 1906
Delta R.T. 0.000 min
Lab File: BN017545.D
Acq: 22 Nov 2021 15:06




Instrument :
BNA_N
ClientSampleId :
SICV201


Tgt Ion:152 Resp: 1311014
Ion Ratio Lower Upper
152 100
151 20.3 15.9 23.9
153 12.9 10.6 15.8



#51
3-Nitroaniline
Concen: 20.720 ng/ul
RT: 14.375 min Scan# 1936
Delta R.T. 0.000 min
Lab File: BN017545.D
Acq: 22 Nov 2021 15:06

Tgt Ion:138 Resp: 220685
Ion Ratio Lower Upper
138 100
108 11.3 8.5 12.7
92 120.0 89.4 134.0







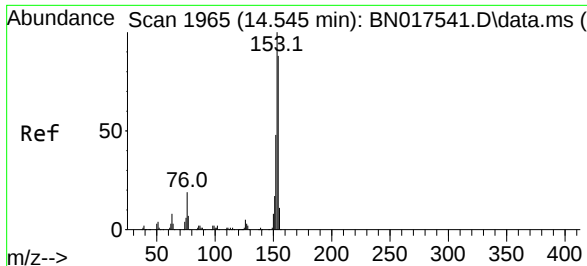

#52
Acenaphthene
Concen: 18.419 ng/ul
RT: 14.539 min Scan# 1964
Delta R.T. -0.006 min
Lab File: BN017545.D
Acq: 22 Nov 2021 15:06




Instrument :
BNA_N
ClientSampleId :
SICV201


Tgt Ion:153 Resp: 840374
Ion Ratio Lower Upper
153 100
152 47.9 37.6 56.4
154 88.5 72.2 108.4

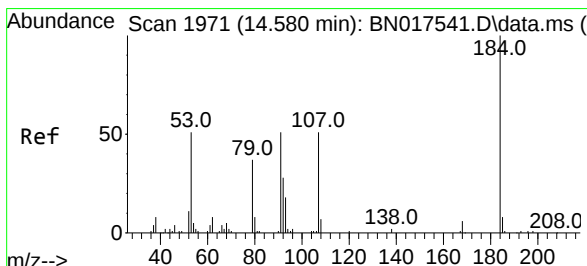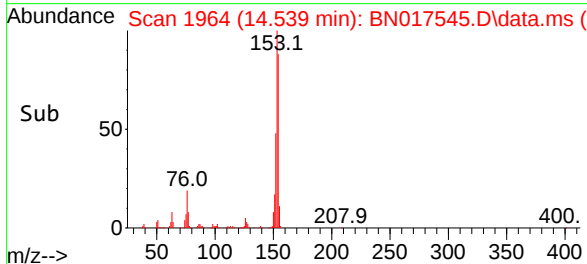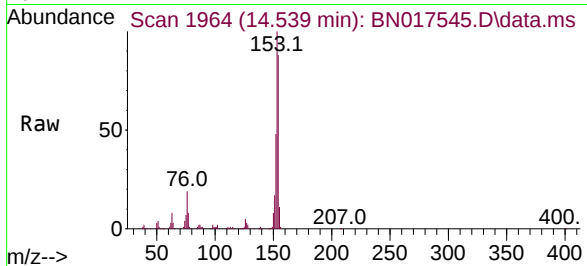

#53
2,4-Dinitrophenol
Concen: 17.508 ng/ul
RT: 14.575 min Scan# 1970
Delta R.T. -0.006 min
Lab File: BN017545.D
Acq: 22 Nov 2021 15:06

Tgt Ion:184 Resp: 88538
Ion Ratio Lower Upper
184 100
63 75.2 54.2 81.4
154 68.7 50.2 75.2


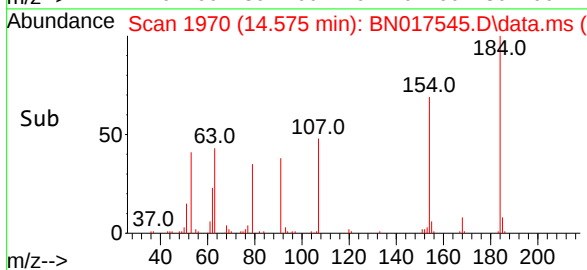

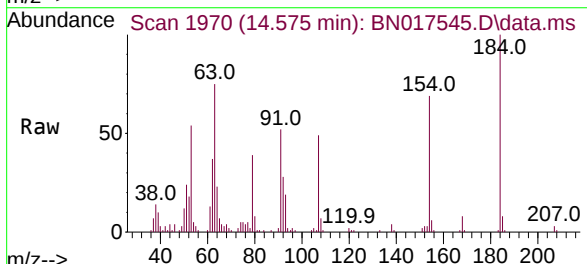




#55
4-Nitrophenol
Concen: 20.461 ng/ul
RT: 14.675 min Scan# 1988
Delta R.T. -0.006 min
Lab File: BN017545.D
Acq: 22 Nov 2021 15:06




Instrument :
BNA_N
ClientSampleId :
SICV201


Tgt Ion:109 Resp: 163309
Ion Ratio Lower Upper
109 100
139 119.1 121.5 182.3#
65 125.8 109.4 164.0

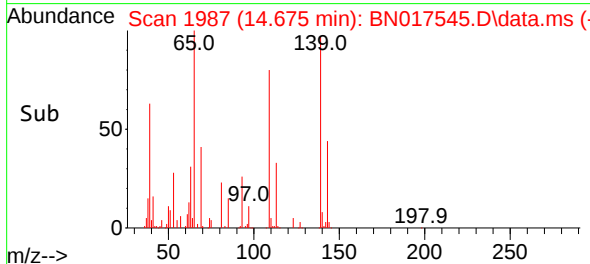

#56
Dibenzofuran
Concen: 18.312 ng/ul
RT: 14.875 min Scan# 2021
Delta R.T. 0.000 min
Lab File: BN017545.D
Acq: 22 Nov 2021 15:06

Tgt Ion:168 Resp: 1199398
Ion Ratio Lower Upper
168 100
139 40.1 29.9 44.9


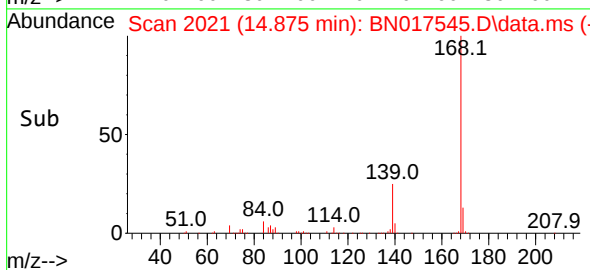






#57
2,4-Dinitrotoluene
Concen: 20.727 ng/ul
RT: 14.833 min Scan# 2014
Delta R.T. 0.000 min
Lab File: BN017545.D
Acq: 22 Nov 2021 15:06




Instrument :
BNA_N
ClientSampleId :
SICV201


Tgt Ion:165 Resp: 295472
Ion Ratio Lower Upper
165 100
63 45.9 35.4 53.0
182 2.8 2.3 3.5

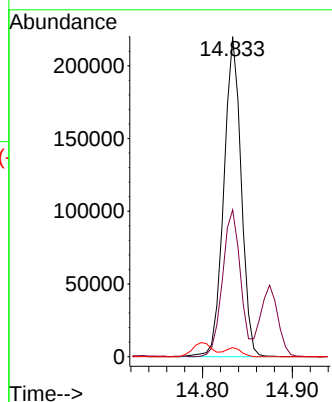

#58
2,3,4,6-Tetrachlorophenol
Concen: 19.759 ng/ul
RT: 15.104 min Scan# 2060
Delta R.T. 0.000 min
Lab File: BN017545.D
Acq: 22 Nov 2021 15:06

Tgt Ion:232 Resp: 214851
Ion Ratio Lower Upper
232 100
131 49.6 40.1 60.1
130 2.9 2.0 3.0
166 32.3 26.2 39.4

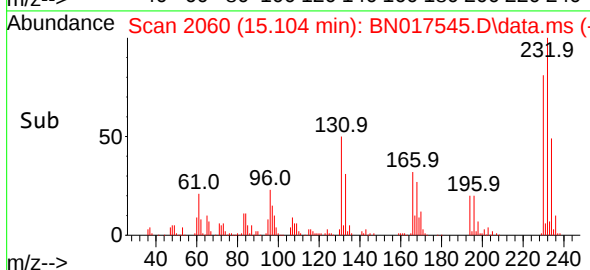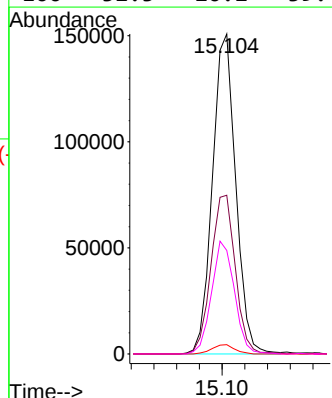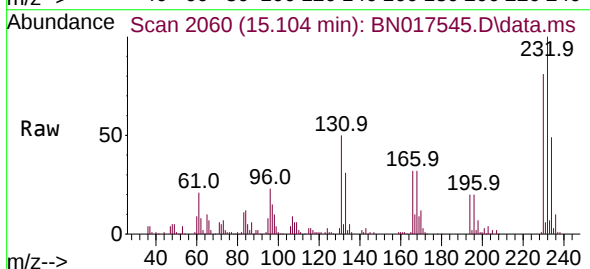



#59

Diethylphthalate

Concen: 19.257 ng/ul

RT: 15.304 min Scan# 2094

Delta R.T. 0.000 min

Lab File: BN017545.D

Acq: 22 Nov 2021 15:06

Instrument :





BNA_N

ClientSampleId :

SICV201

Tgt Ion:149 Resp: 1033835

Ion	Ratio	Lower	Upper
149	100		
177	21.8	17.6	26.4
150	12.5	10.0	15.0

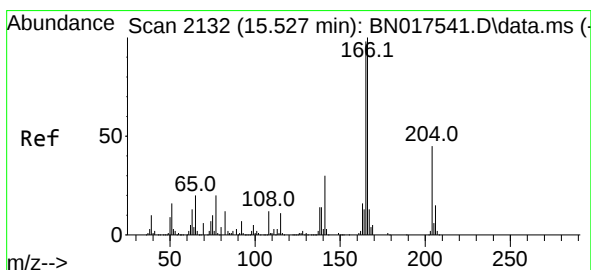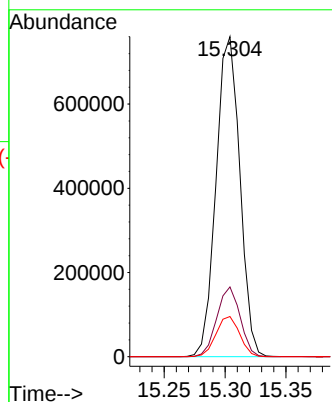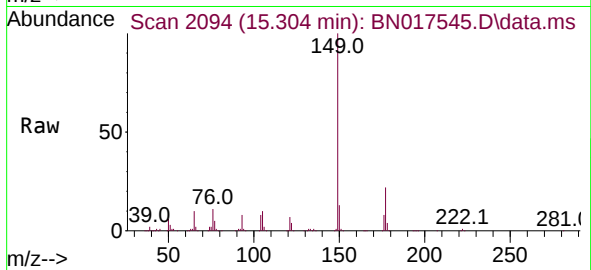

#61

Fluorene

Concen: 18.965 ng/ul

RT: 15.522 min Scan# 2131




Delta R.T. -0.006 min


Lab File: BN017545.D

Acq: 22 Nov 2021 15:06

Tgt Ion:166 Resp: 932463

Ion	Ratio	Lower	Upper
166	100		
165	95.4	77.4	116.0
167	13.5	11.0	16.6


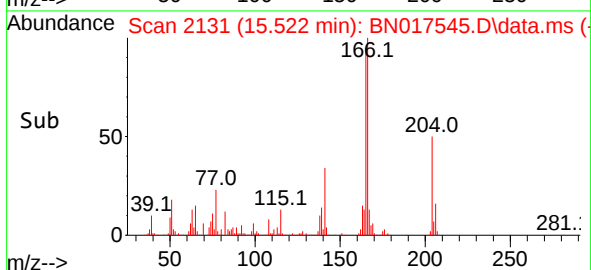

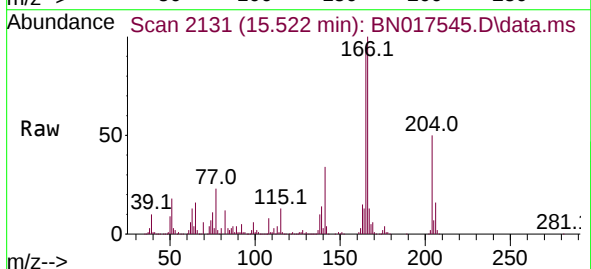




#62
4-Chlorophenyl-phenylether
Concen: 19.205 ng/ul
RT: 15.522 min Scan# 2131
Delta R.T. 0.000 min
Lab File: BN017545.D
Acq: 22 Nov 2021 15:06




Instrument :
BNA_N
ClientSampleId :
SICV201


Tgt Ion:204 Resp: 460784
Ion Ratio Lower Upper
204 100
206 32.6 27.0 40.4
141 67.2 47.2 70.8



#63
4-Nitroaniline
Concen: 23.485 ng/ul
RT: 15.533 min Scan# 2133
Delta R.T. -0.006 min
Lab File: BN017545.D
Acq: 22 Nov 2021 15:06

Tgt Ion:138 Resp: 210899
Ion Ratio Lower Upper
138 100
92 54.8 39.0 58.4
108 88.5 56.7 85.1#









#66
4,6-Dinitro-2-methylphenol
Concen: 18.393 ng/ul
RT: 15.598 min Scan# 2144
Delta R.T. 0.000 min
Lab File: BN017545.D
Acq: 22 Nov 2021 15:06




Instrument :
BNA_N
ClientSampleId :
SICV201


Tgt Ion:198 Resp: 147844
Ion Ratio Lower Upper
198 100
182 4.1 3.1 4.7
77 28.9 17.4 26.2#

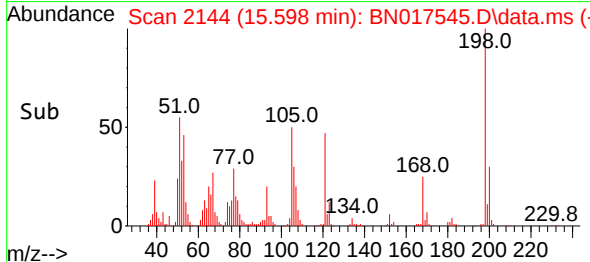

#67
N-Nitrosodiphenylamine
Concen: 18.025 ng/ul
RT: 15.733 min Scan# 2167
Delta R.T. 0.000 min
Lab File: BN017545.D
Acq: 22 Nov 2021 15:06

Tgt Ion:169 Resp: 837547
Ion Ratio Lower Upper
169 100
168 66.8 50.8 76.2
167 36.7 29.0 43.6




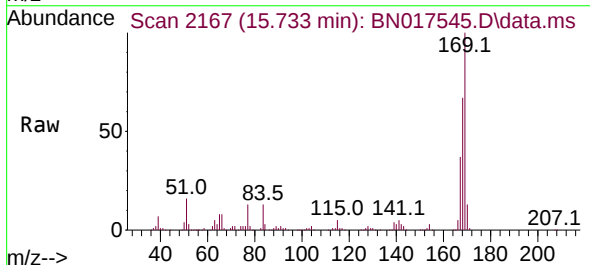




#68
4-Bromophenyl-phenylether
Concen: 17.706 ng/ul
RT: 16.416 min Scan# 211
Delta R.T. 0.000 min
Lab File: BN017545.D
Acq: 22 Nov 2021 15:06




Instrument :
BNA_N
ClientSampleId :
SICV201


Tgt Ion:248 Resp: 269485
Ion Ratio Lower Upper
248 100
250 106.3 78.9 118.3
141 92.4 59.8 89.6#

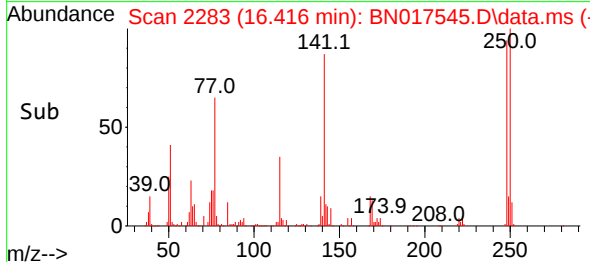

#69
Hexachlorobenzene
Concen: 18.179 ng/ul
RT: 16.533 min Scan# 2303
Delta R.T. 0.000 min
Lab File: BN017545.D
Acq: 22 Nov 2021 15:06

Tgt Ion:284 Resp: 294874
Ion Ratio Lower Upper
284 100
142 43.7 28.2 42.2#
249 35.4 24.5 36.7

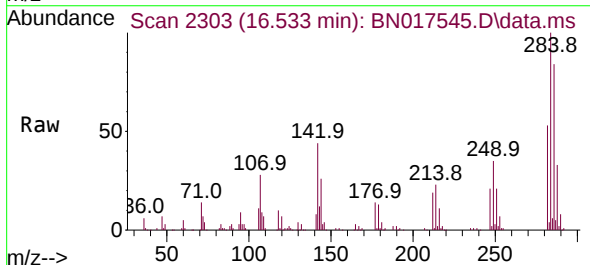



#70

Atrazine

Concen: 18.783 ng/ul

RT: 16.686 min Scan# 2329

Delta R.T. 0.000 min

Lab File: BN017545.D

Acq: 22 Nov 2021 15:06

Instrument :

BNA_N

ClientSampleId :

SICV201





Tgt Ion:200 Resp: 308225

Ion Ratio Lower Upper

200 100

173 26.1 21.6 32.4

215 47.6 38.8 58.2



#71

Pentachlorophenol

Concen: 18.314 ng/ul

RT: 16.875 min Scan# 2361

Delta R.T. 0.000 min

Lab File: BN017545.D

Acq: 22 Nov 2021 15:06




Tgt Ion:266 Resp: 168916


Ion Ratio Lower Upper

266 100

264 63.3 52.2 78.2

268 57.6 51.4 77.0









#72
Phenanthrene
Concen: 18.432 ng/u1
RT: 17.263 min Scan# 2427
Delta R.T. 0.000 min
Lab File: BN017545.D
Acq: 22 Nov 2021 15:06




Instrument :
BNA_N
ClientSampleId :
SICV201


Tgt Ion:178 Resp: 1550257
Ion Ratio Lower Upper
178 100
179 15.0 12.5 18.7
176 18.8 14.6 22.0



#74
Anthracene
Concen: 18.693 ng/u1
RT: 17.357 min Scan# 2443
Delta R.T. 0.000 min
Lab File: BN017545.D
Acq: 22 Nov 2021 15:06

Tgt Ion:178 Resp: 1559122
Ion Ratio Lower Upper
178 100
179 15.6 12.2 18.2
176 17.6 14.2 21.2









#75
1,2,3,4-Tetrachlorobenzene
Concen: 16.402 ng/uL
RT: 13.275 min Scan# 11
Delta R.T. -0.006 min
Lab File: BN017545.D
Acq: 22 Nov 2021 15:06




Instrument :
BNA_N
ClientSampleId :
SICV201


Tgt Ion:216 Resp: 396432
Ion Ratio Lower Upper
216 100
214 79.2 61.5 92.3
218 49.6 40.6 61.0

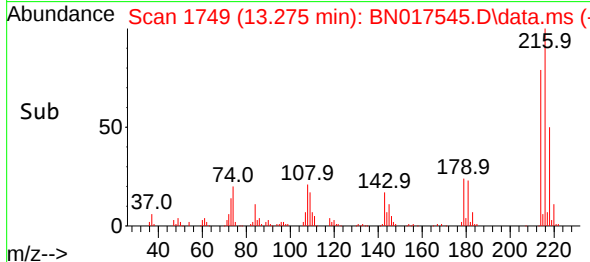

#76
Pentachlorobenzene
Concen: 17.478 ng/uL
RT: 14.798 min Scan# 2008
Delta R.T. -0.006 min
Lab File: BN017545.D
Acq: 22 Nov 2021 15:06

Tgt Ion:250 Resp: 384112
Ion Ratio Lower Upper
250 100
248 62.1 53.2 79.8
252 61.7 52.5 78.7

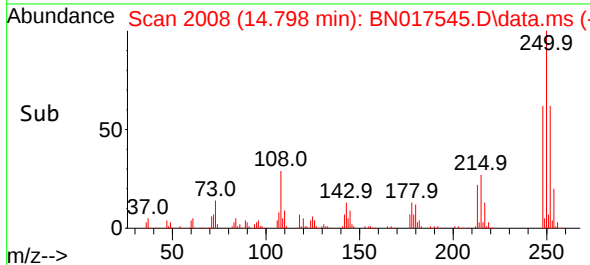







#77
 Carbazole
 Concen: 20.078 ng/ul
 RT: 17.622 min Scan# 2488
 Delta R.T. 0.000 min
 Lab File: BN017545.D
 Acq: 22 Nov 2021 15:06

Instrument :
 BNA_N
 ClientSampleId :
 SICV201

Tgt Ion:167 Resp: 1437239




Ion	Ratio	Lower	Upper
167	100		
166	21.2	17.6	26.4
139	13.2	10.6	16.0

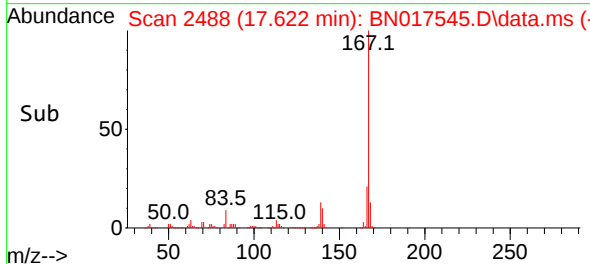


#78
 Di-n-butylphthalate
 Concen: 19.932 ng/ul
 RT: 18.204 min Scan# 2587
 Delta R.T. 0.006 min
 Lab File: BN017545.D
 Acq: 22 Nov 2021 15:06

Tgt Ion:149 Resp: 1733906

Ion	Ratio	Lower	Upper
149	100		
150	8.8	7.4	11.2
104	5.2	3.8	5.6


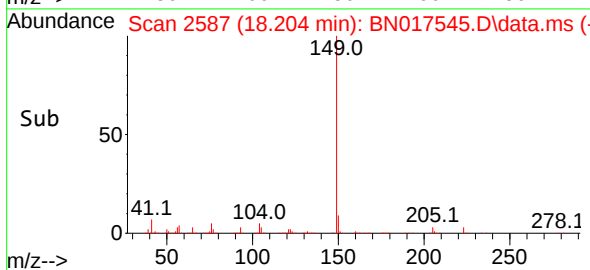

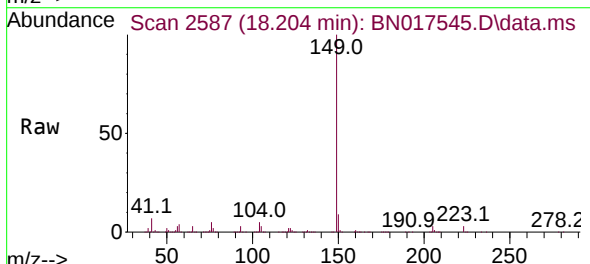




#80
Fluoranthene
Concen: 16.701 ng/u1
RT: 19.280 min Scan# 2770
Delta R.T. 0.000 min
Lab File: BN017545.D
Acq: 22 Nov 2021 15:06




Instrument :
BNA_N
ClientSampleId :
SICV201


Tgt Ion:202 Resp: 1807259
Ion Ratio Lower Upper
202 100
101 11.7 9.6 14.4
100 9.1 7.3 10.9

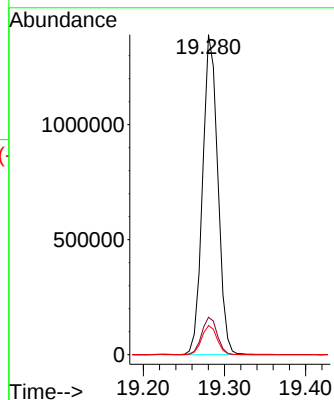

#82
Pyrene
Concen: 17.055 ng/u1
RT: 19.645 min Scan# 2832
Delta R.T. 0.000 min
Lab File: BN017545.D
Acq: 22 Nov 2021 15:06

Tgt Ion:202 Resp: 1847659
Ion Ratio Lower Upper
202 100
101 13.9 11.8 17.6
100 11.5 9.6 14.4



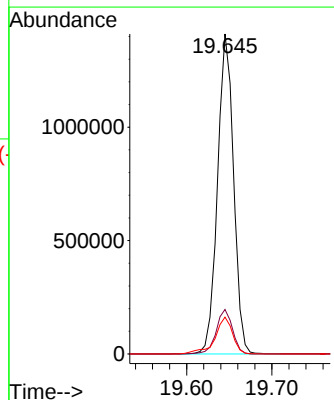





#83
Butylbenzylphthalate
Concen: 19.262 ng/ul
RT: 20.551 min Scan# 2986
Delta R.T. 0.000 min
Lab File: BN017545.D
Acq: 22 Nov 2021 15:06




Instrument :
BNA_N
ClientSampleId :
SICV201


Tgt Ion:149 Resp: 761788
Ion Ratio Lower Upper
149 100
91 77.0 54.5 81.7
206 19.6 17.7 26.5



#84
3,3'-Dichlorobenzidine
Concen: 21.042 ng/ul
RT: 21.333 min Scan# 3119
Delta R.T. 0.006 min
Lab File: BN017545.D
Acq: 22 Nov 2021 15:06

Tgt Ion:252 Resp: 567231
Ion Ratio Lower Upper
252 100
254 63.0 47.6 71.4
126 12.0 10.1 15.1


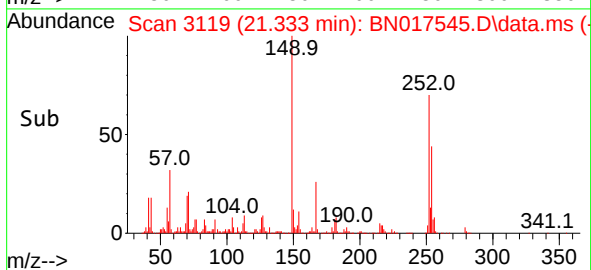






#85
Benzo(a)anthracene
Concen: 18.960 ng/ul
RT: 21.398 min Scan# 3130
Delta R.T. 0.000 min
Lab File: BN017545.D
Acq: 22 Nov 2021 15:06




Instrument :
BNA_N
ClientSampleId :
SICV201


Tgt Ion:228 Resp: 1779733
Ion Ratio Lower Upper
228 100
229 19.0 15.8 23.8
226 25.7 21.8 32.8

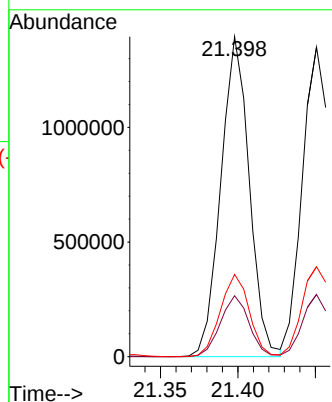

#86
Bis(2-ethylhexyl)phthalate
Concen: 20.347 ng/ul
RT: 21.339 min Scan# 3120
Delta R.T. 0.000 min
Lab File: BN017545.D
Acq: 22 Nov 2021 15:06

Tgt Ion:149 Resp: 1164667
Ion Ratio Lower Upper
149 100
167 27.6 22.6 33.8
279 3.5 3.8 5.6#





#87

Chrysene

Concen: 18.504 ng/ul

RT: 21.451 min Scan# 3138

Delta R.T. 0.006 min

Lab File: BN017545.D

Acq: 22 Nov 2021 15:06

Instrument :

BNA_N

ClientSampleId :

SICV201





Tgt Ion:228 Resp: 1706763

Ion Ratio Lower Upper

228 100

226 29.0 24.1 36.1

229 20.1 15.6 23.4



#89

Di-n-octyl phthalate

Concen: 18.486 ng/ul




RT: 22.257 min Scan# 3276


Delta R.T. 0.006 min

Lab File: BN017545.D

Acq: 22 Nov 2021 15:06

Tgt Ion:149 Resp: 1966354









#90
Benzo(b)fluoranthene
Concen: 17.929 ng/ul
RT: 23.062 min Scan# 3412
Delta R.T. 0.006 min
Lab File: BN017545.D
Acq: 22 Nov 2021 15:06




Instrument :
BNA_N
ClientSampleId :
SICV201


Tgt Ion:252 Resp: 1736198
Ion Ratio Lower Upper
252 100
253 21.0 18.4 27.6
125 10.4 9.4 14.0

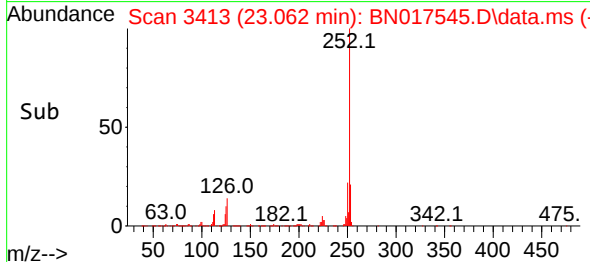

#91
Benzo(k)fluoranthene
Concen: 17.961 ng/ul
RT: 23.110 min Scan# 3421
Delta R.T. 0.006 min
Lab File: BN017545.D
Acq: 22 Nov 2021 15:06

Tgt Ion:252 Resp: 1642289
Ion Ratio Lower Upper
252 100
253 22.3 17.4 26.2
125 11.1 8.6 13.0




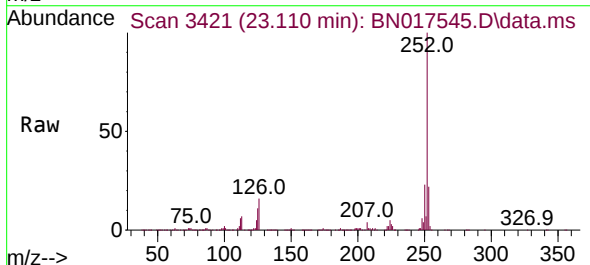




#93
Benzo(a)pyrene
Concen: 18.255 ng/ul
RT: 23.680 min Scan# 3518
Delta R.T. 0.006 min
Lab File: BN017545.D
Acq: 22 Nov 2021 15:06




Instrument :
BNA_N
ClientSampleId :
SICV201


Tgt Ion:252 Resp: 1678443
Ion Ratio Lower Upper
252 100
253 21.4 17.5 26.3
125 11.7 9.7 14.5

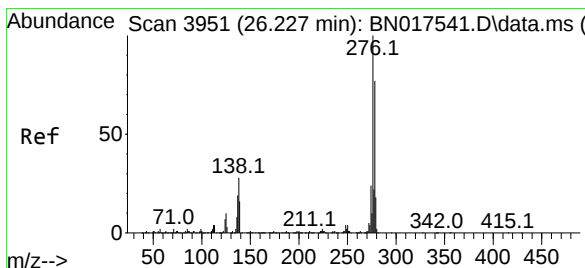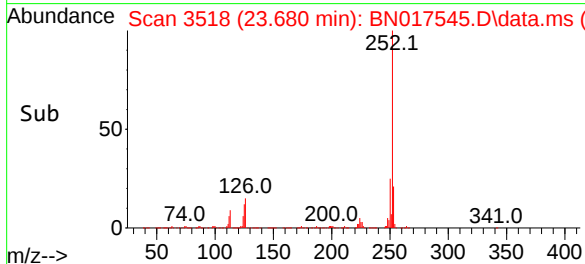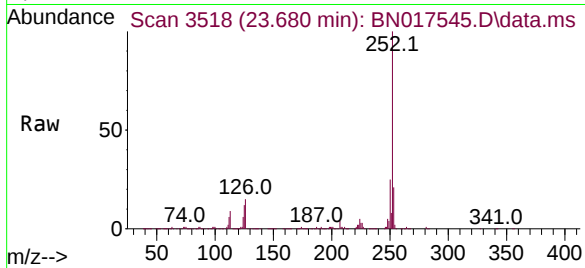

#94
Indeno(1,2,3-cd)pyrene
Concen: 17.788 ng/ul
RT: 26.227 min Scan# 3951
Delta R.T. 0.000 min
Lab File: BN017545.D
Acq: 22 Nov 2021 15:06

Tgt Ion:276 Resp: 1698184
Ion Ratio Lower Upper
276 100
138 27.9 21.4 32.2
277 25.7 19.5 29.3


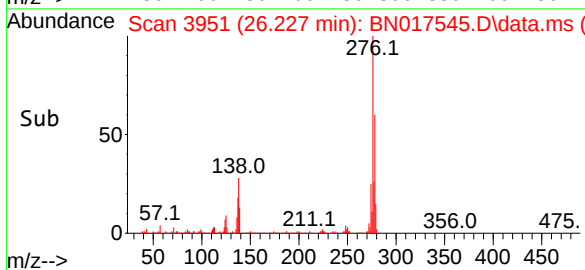

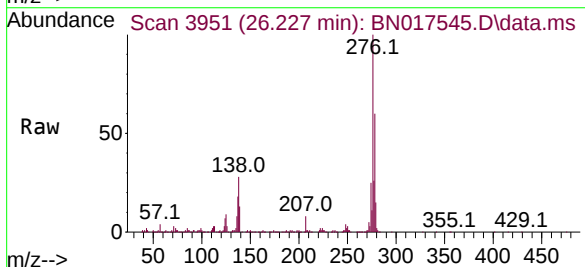




#95
 Dibenzo(a,h)anthracene
 Concen: 17.968 ng/ul
 RT: 26.251 min Scan# 3955
 Delta R.T. 0.012 min
 Lab File: BN017545.D
 Acq: 22 Nov 2021 15:06

Instrument :
 BNA_N
 ClientSampleId :
 SICV201

Tgt Ion:278 Resp: 1456976
 Ion Ratio Lower Upper
 278 100
 139 18.0 14.7 22.1
 279 25.1 19.7 29.5



#96
 Benzo(g,h,i)perylene
 Concen: 17.383 ng/ul
 RT: 26.974 min Scan# 4078
 Delta R.T. 0.006 min
 Lab File: BN017545.D
 Acq: 22 Nov 2021 15:06

Tgt Ion:276 Resp: 1418434
 Ion Ratio Lower Upper
 276 100
 138 24.6 18.2 27.4
 277 24.7 17.4 26.0

