

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112223\
 Data File : BN028841.D
 Acq On : 22 Nov 2023 16:00
 Operator : MA/JU
 Sample : 05233-02
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH377

Quant Time: Nov 22 21:37:09 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 21 23:49:43 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.690	152	6805	0.400	ng/ul	-0.05
4) Naphthalene-d8	10.440	136	26154	0.400	ng/ul	#-0.02
9) Acenaphthene-d10	14.297	164	12949	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.056	188	23582	0.400	ng/ul	0.00
17) Chrysene-d12	21.281	240	15686	0.400	ng/ul	# 0.01
23) Perylene-d12	23.546	264	19735	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.108	96	37446	4.979	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.079	152	4850	0.123	ng/ul	0.00
18) Fluoranthene-d10	19.094	212	19484	0.386	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.146	88	5426	0.653	ng/ul#	84
20) Pyrene	19.452	202	3252	0.047	ng/ul#	1
26) Benzo(a)pyrene	23.388	252	5847	0.084	ng/ul#	48


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112223\
Data File : BN028841.D
Acq On : 22 Nov 2023 16:00
Operator : MA/JU
Sample : 05233-02
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH377

Quant Time: Nov 22 21:37:09 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 21 23:49:43 2023
Response via : Initial Calibration




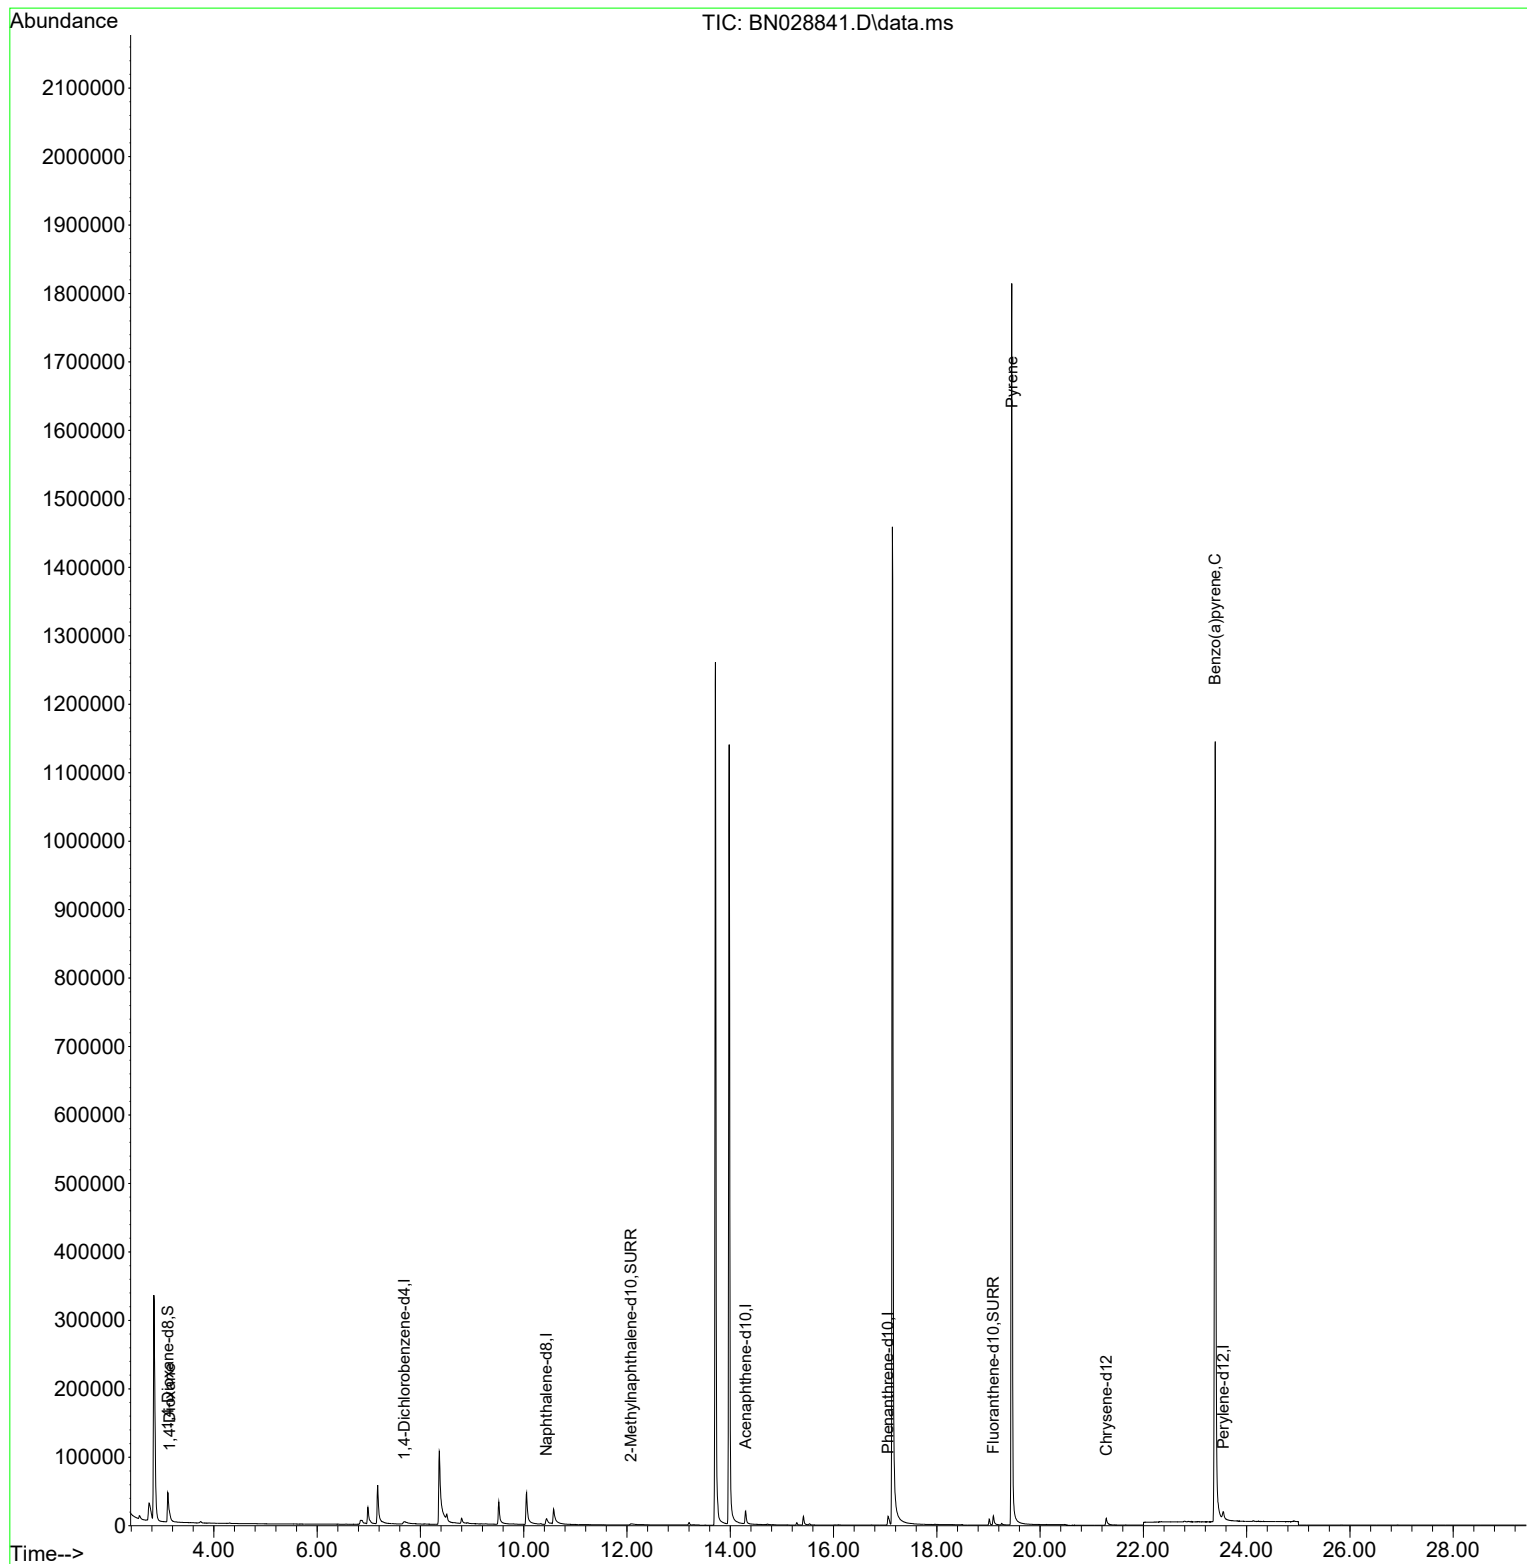


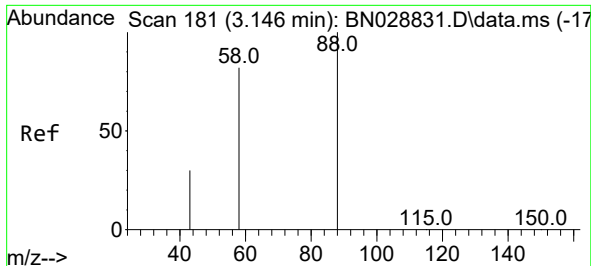

#2
1,4-Dioxane
Concen: 0.653 ng/ul
RT: 3.146 min Scan# 11
Delta R.T. 0.004 min
Lab File: BN028841.D
Acq: 22 Nov 2023 16:00




Instrument :
BNA_N
ClientSampleId :
BH377


Tgt Ion: 88 Resp: 5426
Ion Ratio Lower Upper
88 100
43 31.4 32.9 49.3#
58 40.8 41.8 62.8#

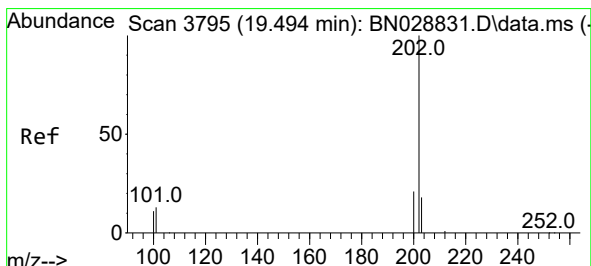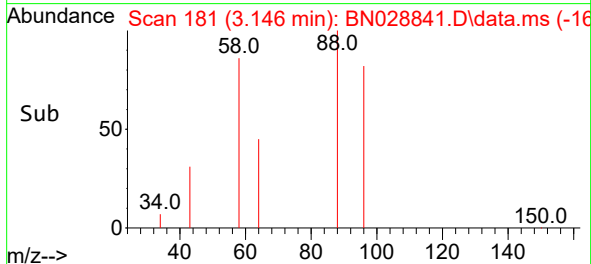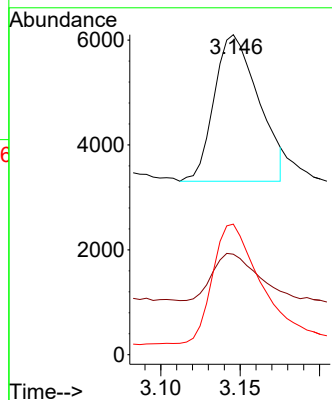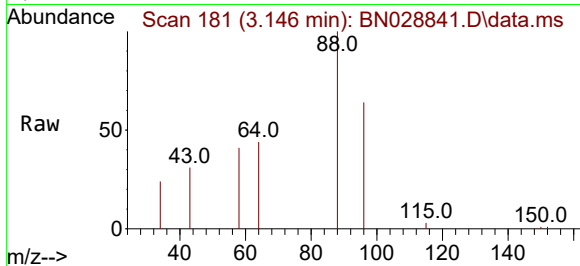

#20
Pyrene
Concen: 0.047 ng/ul
RT: 19.452 min Scan# 3786
Delta R.T. -0.033 min
Lab File: BN028841.D
Acq: 22 Nov 2023 16:00


Tgt Ion: 202 Resp: 3252
Ion Ratio Lower Upper
202 100
101 153.5 10.3 15.5#
100 1091.7 8.2 12.2#

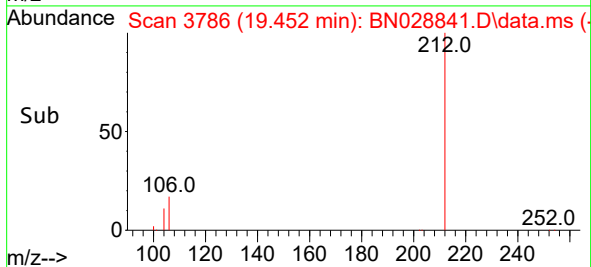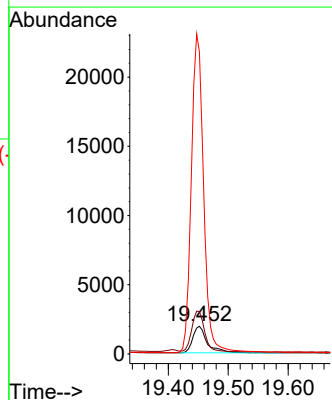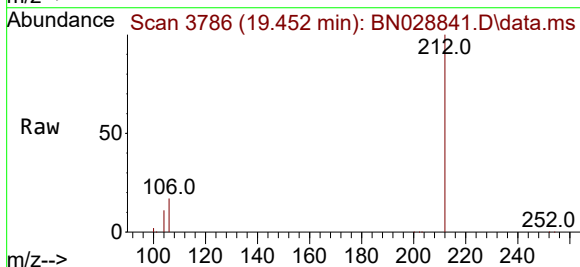

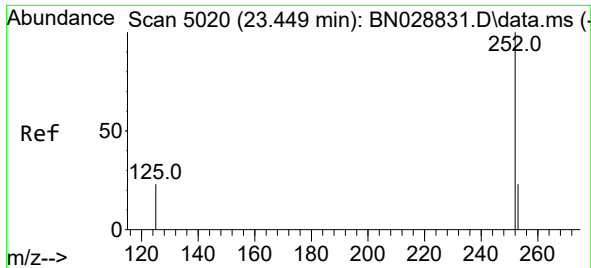

#26
Benzo(a)pyrene
Concen: 0.084 ng/ul
RT: 23.388 min Scan# 4999
Delta R.T. -0.056 min
Lab File: BN028841.D
Acq: 22 Nov 2023 16:00

Instrument :
BNA_N
ClientSampleId :
BH377

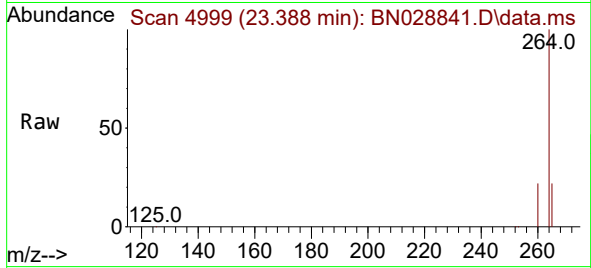

Tgt Ion:252 Resp: 5847
Ion Ratio Lower Upper
252 100
253 47.3 19.0 28.6#
125 41.8 13.2 19.8#

