




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112223\
 Data File : BN028819.D
 Acq On : 21 Nov 2023 20:17
 Operator : MA/JU
 Sample : 05281-02
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AC3

Manual IntegrationsAPPROVED

Quant Time: Nov 21 23:52:47 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 21 23:49:43 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/23/2023
 Supervised By :mohammad ahmed 11/25/2023

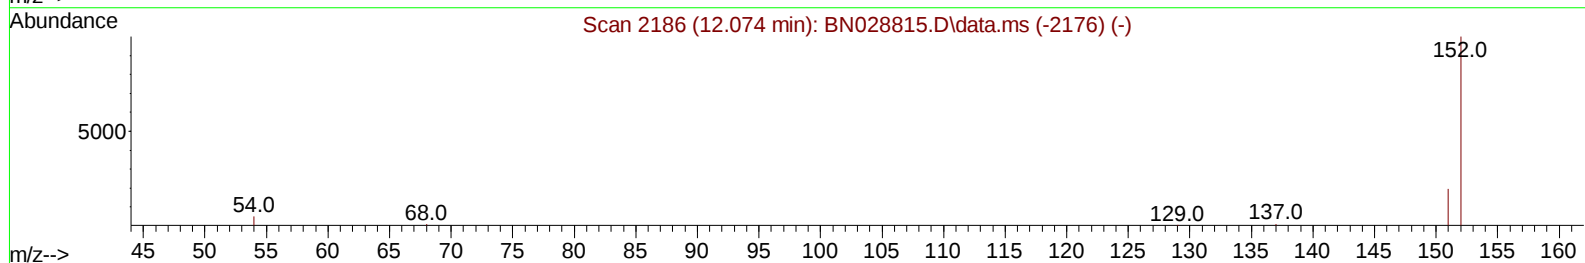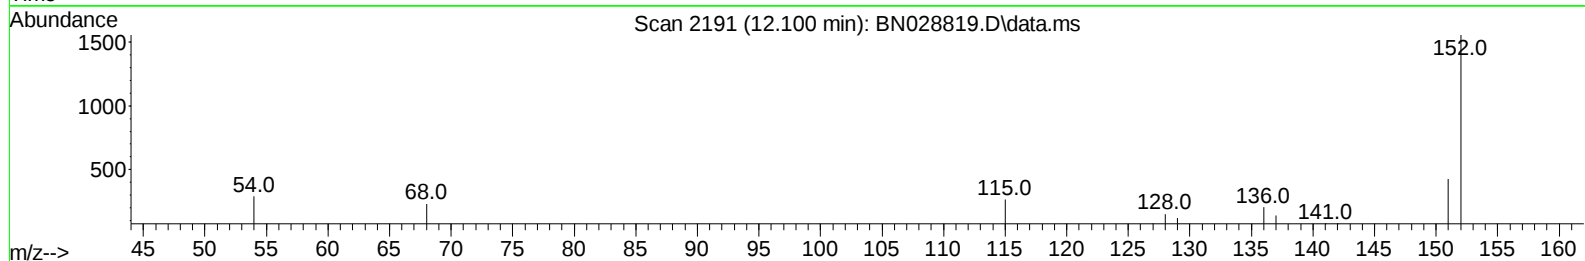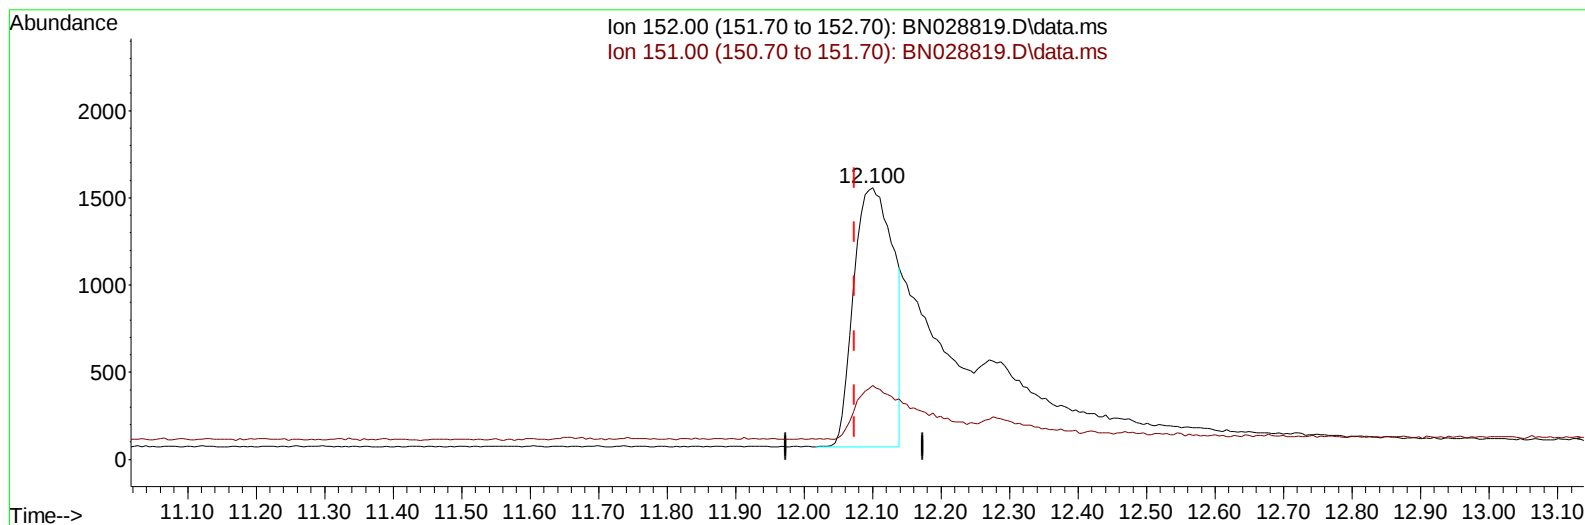

TIC: BN028819.D\data.ms

(6) 2-Methylnaphthalene-d10 (SURR)

12.100min (+ 0.026) 0.23 ng/u1

response 5908

Ion	Exp%	Act%
152.00	100.00	100.00
151.00	20.50	18.43
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112223\
 Data File : BN028819.D
 Acq On : 21 Nov 2023 20:17
 Operator : MA/JU
 Sample : 05281-02
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AC3

Manual IntegrationsAPPROVED

Quant Time: Nov 21 23:52:47 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 21 23:49:43 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/23/2023
 Supervised By :mohammad ahmed 11/25/2023

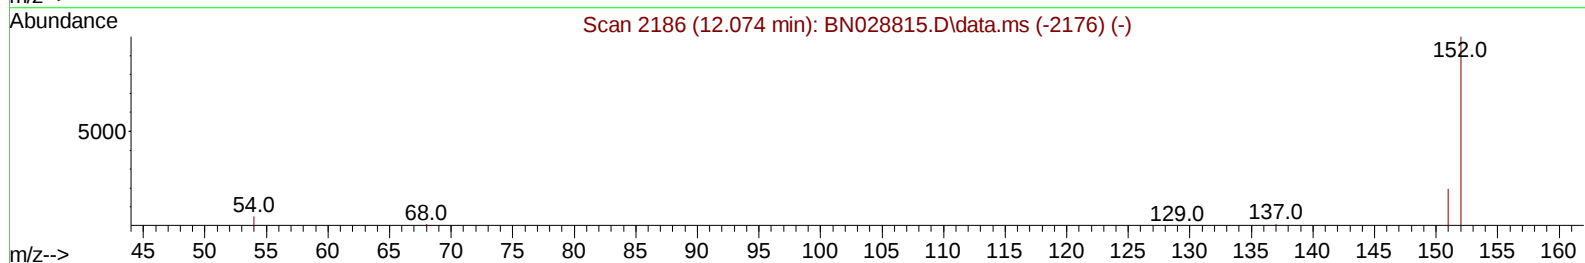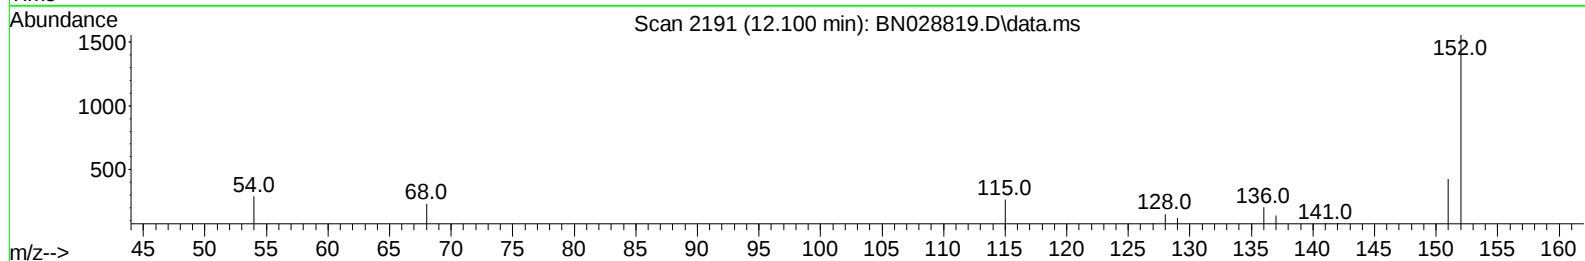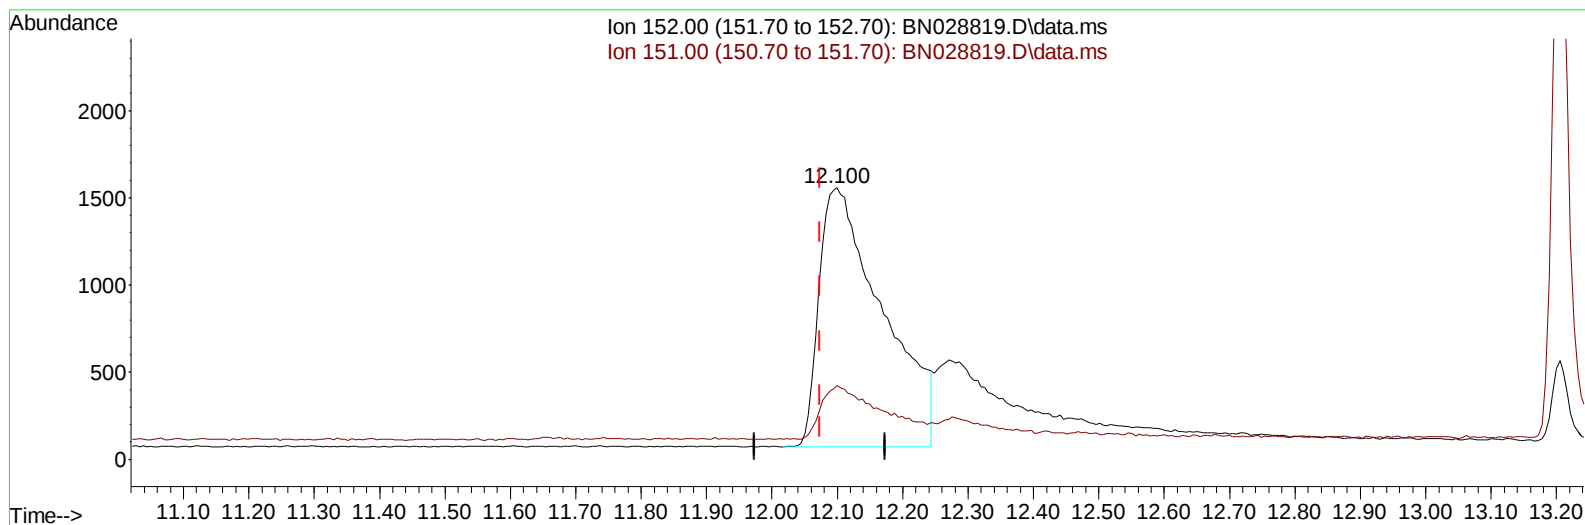

TIC: BN028819.D\data.ms

(6) 2-Methylnaphthalene-d10 (SURR)

12.100min (+ 0.026) 0.40 ng/ul m

response 10014

Ion	Exp%	Act%
152.00	100.00	100.00
151.00	20.50	10.87#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112223\
 Data File : BN028819.D
 Acq On : 21 Nov 2023 20:17
 Operator : MA/JU
 Sample : 05281-02
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AC3

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/23/2023
 Supervised By :mohammad ahmed 11/25/2023

Quant Time: Nov 21 23:52:47 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 21 23:49:43 2023
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.711	152		5215	0.400	ng/ul	#-0.03
4) Naphthalene-d8	10.450	136		16837	0.400	ng/ul	#-0.01
9) Acenaphthene-d10	14.301	164		12957	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.059	188		24599	0.400	ng/ul	0.00
17) Chrysene-d12	21.283	240		14850	0.400	ng/ul	# 0.01
23) Perylene-d12	23.545	264		18452	0.400	ng/ul	# 0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.103	96		36405	6.316	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.100	152		10014m	0.395	ng/ul	0.03
18) Fluoranthene-d10	19.093	212		31265	0.654	ng/ul	0.00
Target Compounds							Qvalue
2) 1,4-Dioxane	3.137	88		1934	0.304	ng/ul#	81

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112223\
Data File : BN028819.D
Acq On : 21 Nov 2023 20:17
Operator : MA/JU
Sample : 05281-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AC3

Manual IntegrationsAPPROVED

Quant Time: Nov 21 23:52:47 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 21 23:49:43 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/23/2023
Supervised By :mohammad ahmed 11/25/2023

