




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112223\
 Data File : BN028822.D
 Acq On : 21 Nov 2023 22:04
 Operator : MA/JU
 Sample : 05281-05
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AC6

Manual IntegrationsAPPROVED

Quant Time: Nov 21 23:53:08 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 21 23:49:43 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/23/2023
 Supervised By :mohammad ahmed 11/25/2023

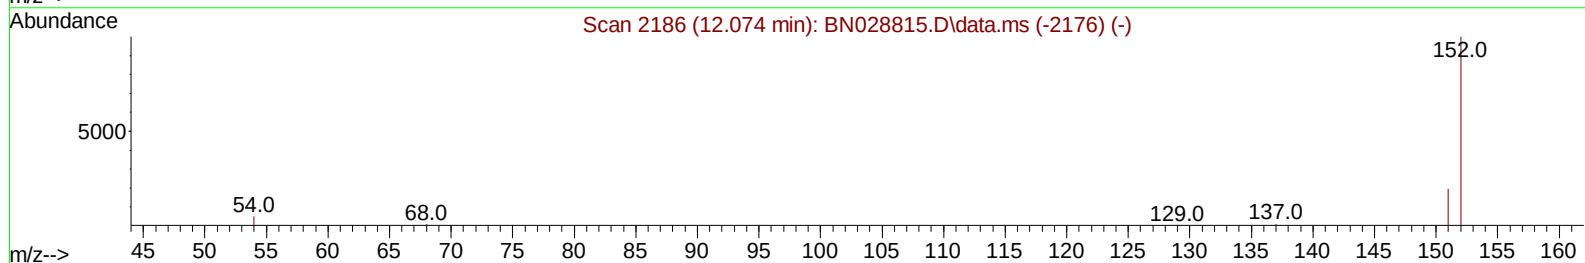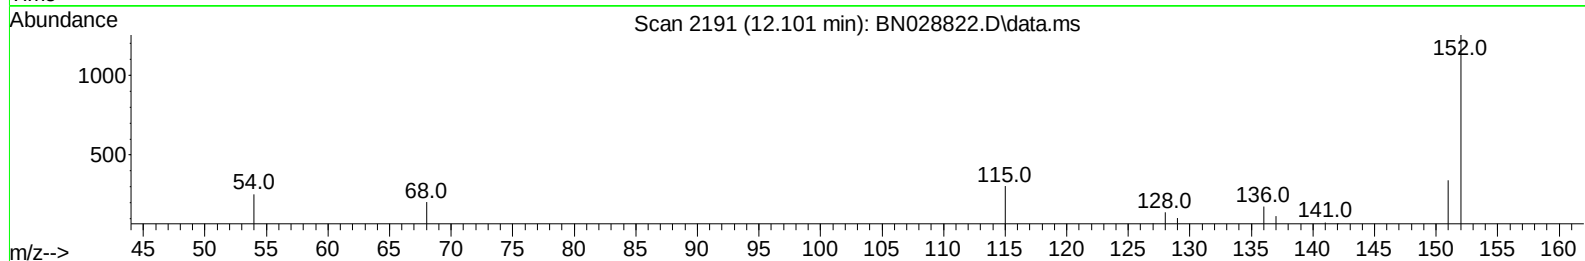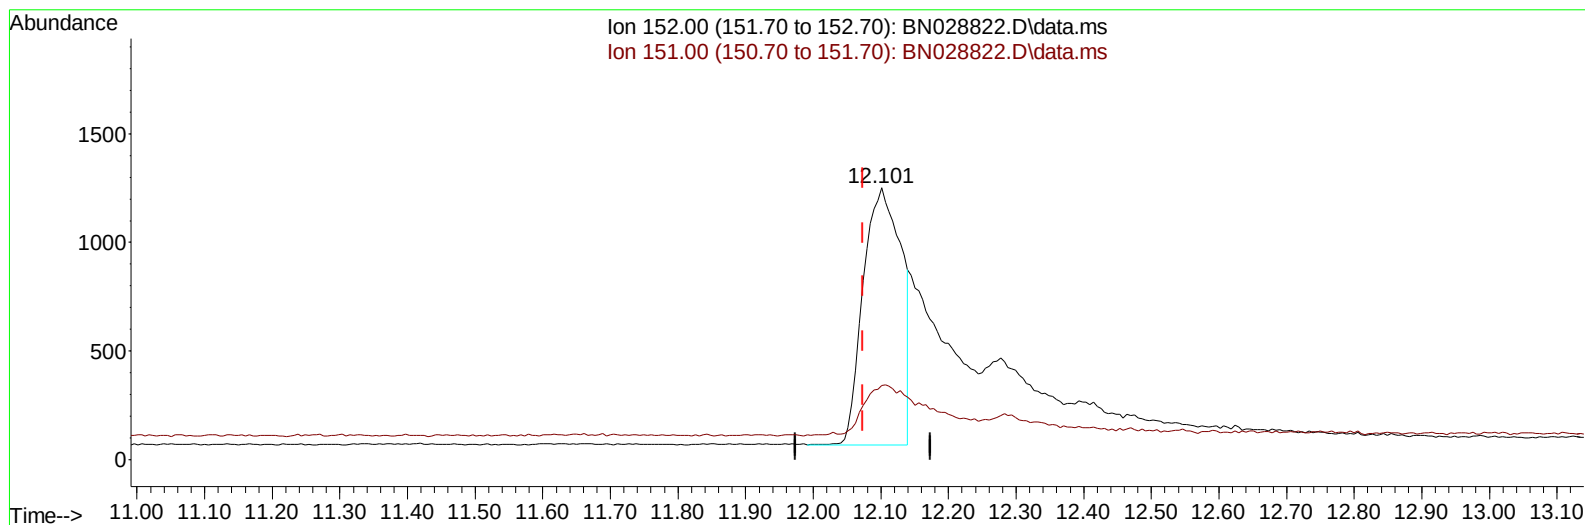

TIC: BN028822.D\data.ms

(6) 2-Methylnaphthalene-d10 (SURR)

12.101min (+ 0.027) 0.14 ng/u1

response 4654

Ion	Exp%	Act%
152.00	100.00	100.00
151.00	20.50	19.04
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112223\
Data File : BN028822.D
Acq On : 21 Nov 2023 22:04
Operator : MA/JU
Sample : 05281-05
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AC6

Manual IntegrationsAPPROVED

Quant Time: Nov 21 23:53:08 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 21 23:49:43 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/23/2023
Supervised By :mohammad ahmed 11/25/2023

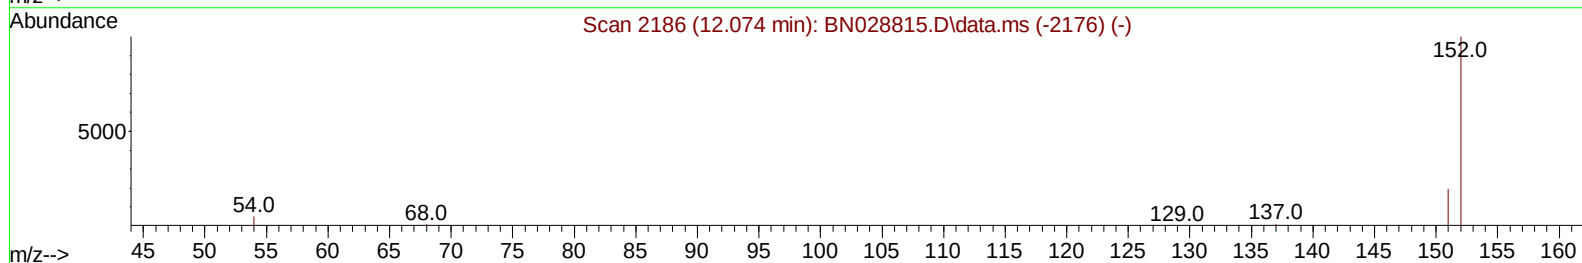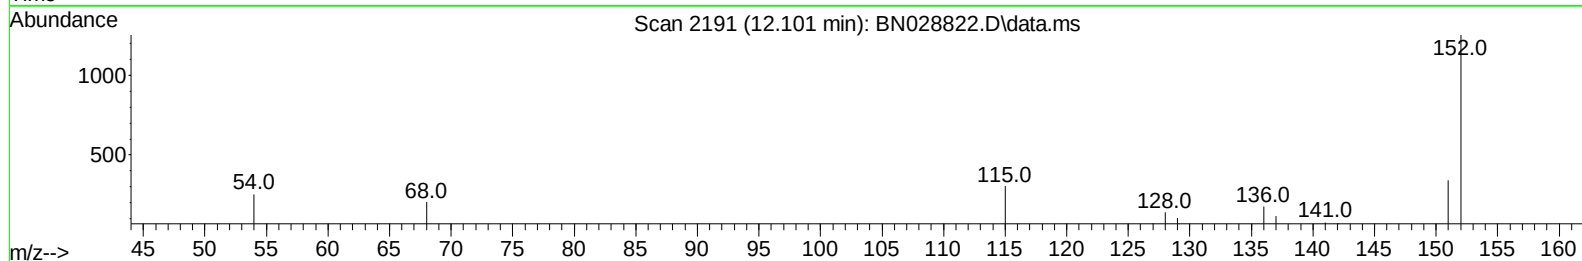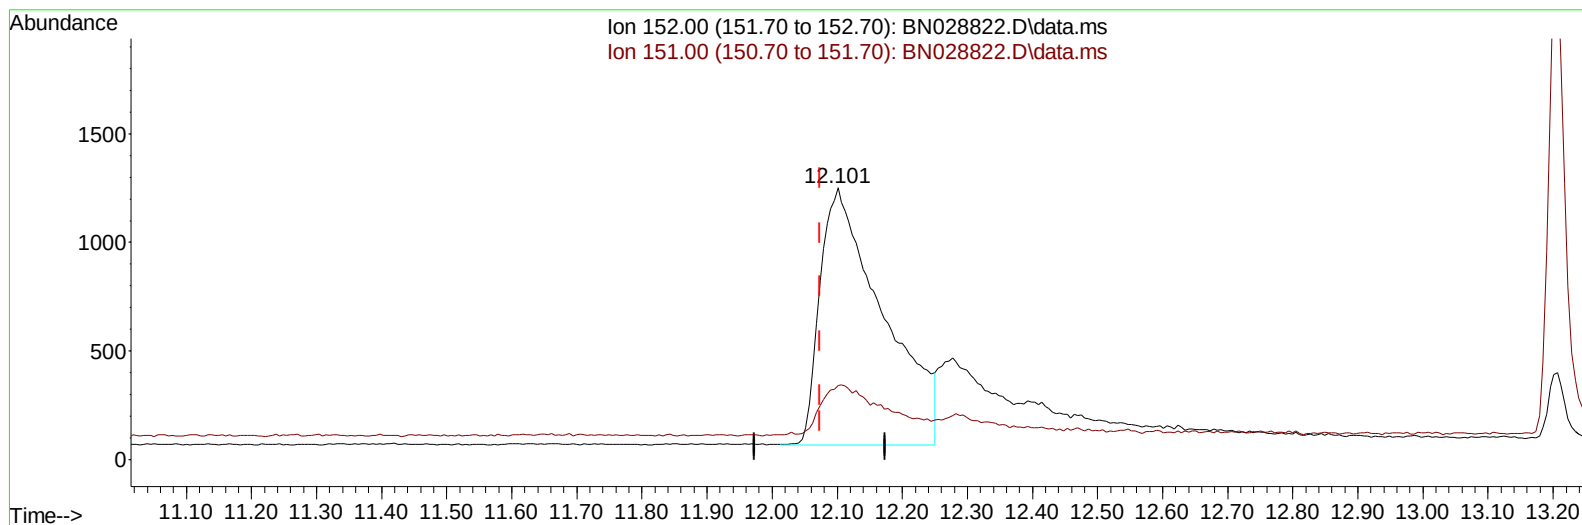

TIC: BN028822.D\data.ms

(6) 2-Methylnaphthalene-d10 (SURR)

12.101min (+ 0.027) 0.23 ng/ul m

response 7952

Ion	Exp%	Act%
152.00	100.00	100.00
151.00	20.50	11.14#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112223\
 Data File : BN028822.D
 Acq On : 21 Nov 2023 22:04
 Operator : MA/JU
 Sample : 05281-05
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AC6

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/23/2023
 Supervised By :mohammad ahmed 11/25/2023

Quant Time: Nov 21 23:53:08 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 21 23:49:43 2023
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.711	152		5494	0.400	ng/ul	#-0.03
4) Naphthalene-d8	10.451	136		22656	0.400	ng/ul	#-0.01
9) Acenaphthene-d10	14.298	164		13967	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.056	188		28357	0.400	ng/ul	0.00
17) Chrysene-d12	21.279	240		19710	0.400	ng/ul	0.00
23) Perylene-d12	23.538	264		25108	0.400	ng/ul	# 0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.099	96		33472	5.512	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.101	152		7952m	0.233	ng/ul	0.03
18) Fluoranthene-d10	19.095	212		28453	0.449	ng/ul	0.00
Target Compounds							Qvalue
2) 1,4-Dioxane	3.137	88		9288	1.384	ng/ul	93

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112223\
Data File : BN028822.D
Acq On : 21 Nov 2023 22:04
Operator : MA/JU
Sample : 05281-05
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AC6

Manual IntegrationsAPPROVED

Quant Time: Nov 21 23:53:08 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 21 23:49:43 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/23/2023
Supervised By :mohammad ahmed 11/25/2023

