




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112223\
 Data File : BN028826.D
 Acq On : 22 Nov 2023 00:27
 Operator : MA/JU
 Sample : 05281-06
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AC7

Manual IntegrationsAPPROVED

Quant Time: Nov 22 00:58:12 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 21 23:49:43 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/23/2023
 Supervised By :mohammad ahmed 11/25/2023

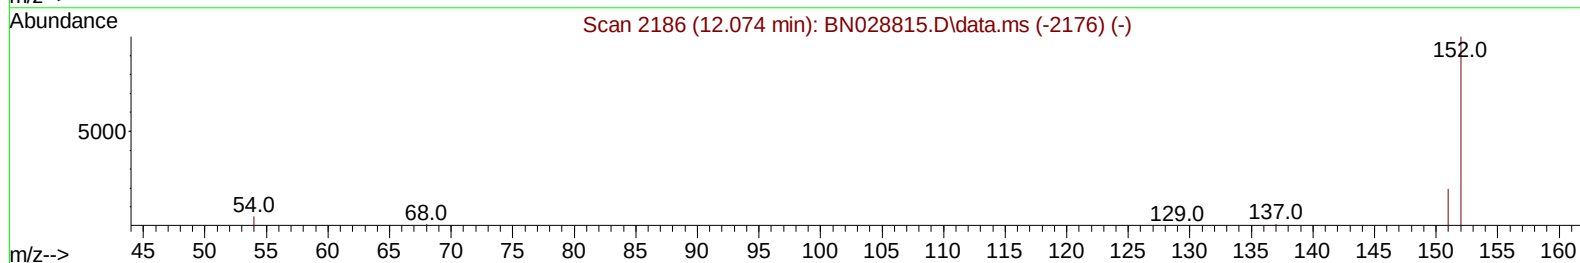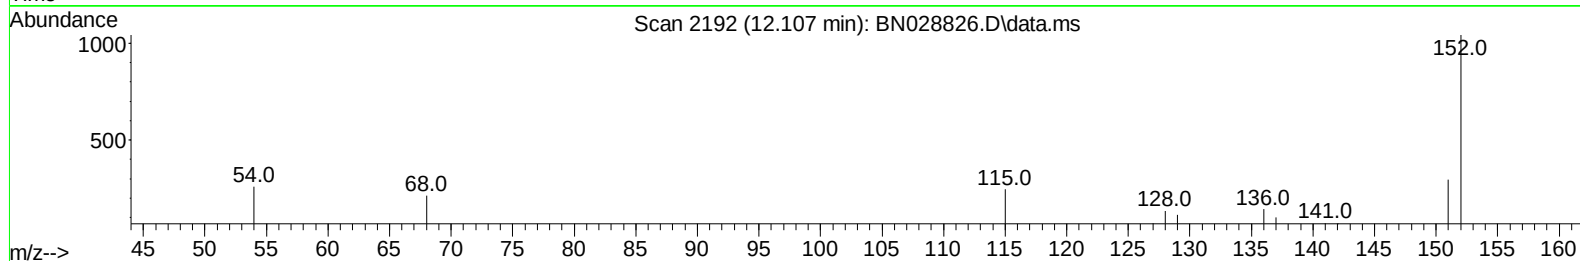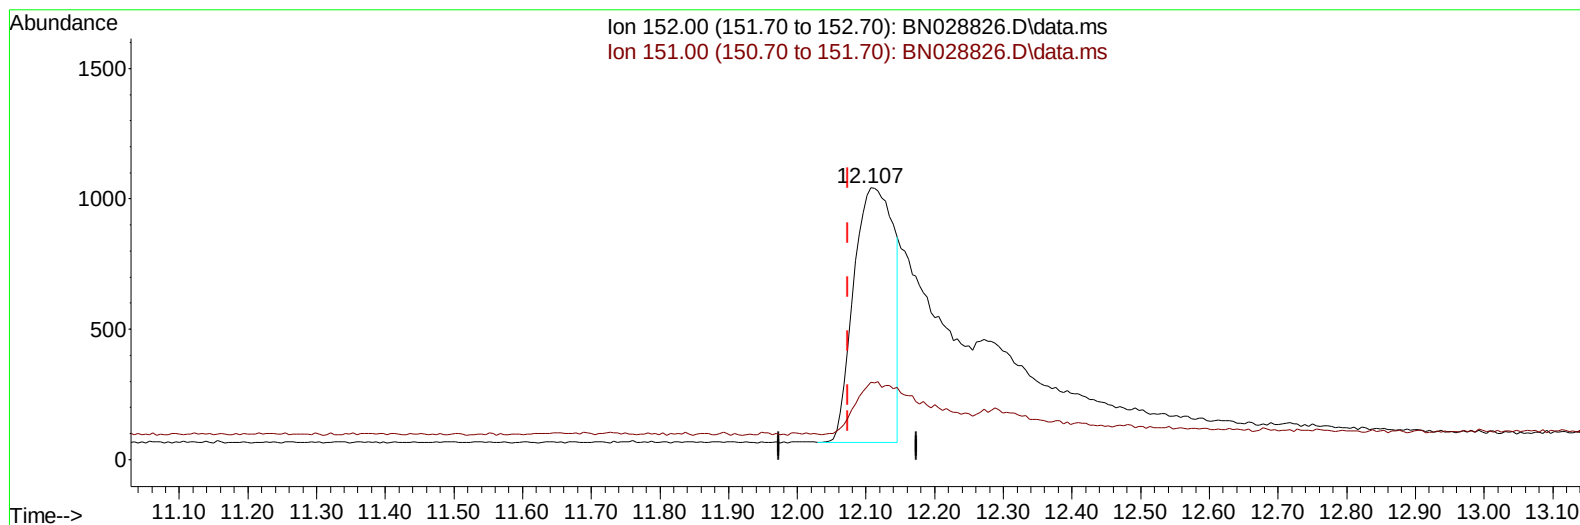

TIC: BN028826.D\data.ms

(6) 2-Methylnaphthalene-d10 (SURR)

12.107min (+ 0.033) 0.16 ng/u1

response 3932

Ion	Exp%	Act%
152.00	100.00	100.00
151.00	20.50	18.54
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112223\
 Data File : BN028826.D
 Acq On : 22 Nov 2023 00:27
 Operator : MA/JU
 Sample : 05281-06
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AC7

Manual IntegrationsAPPROVED

Quant Time: Nov 22 00:58:12 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 21 23:49:43 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/23/2023
 Supervised By :mohammad ahmed 11/25/2023

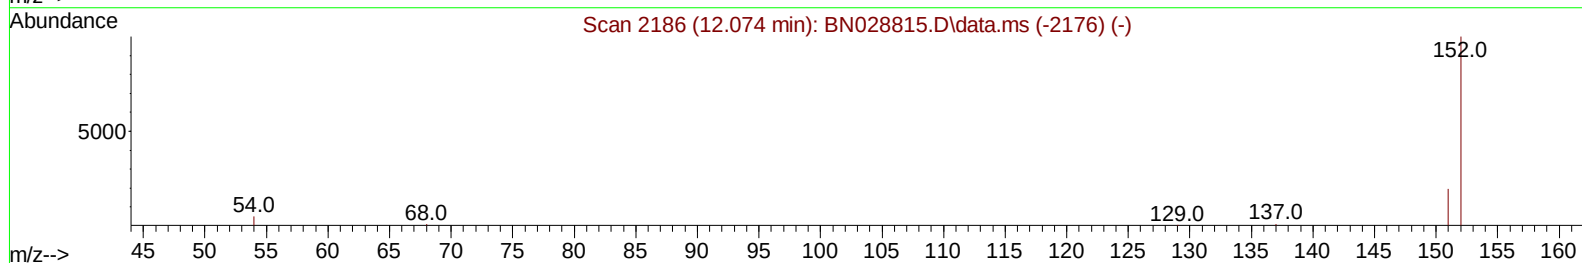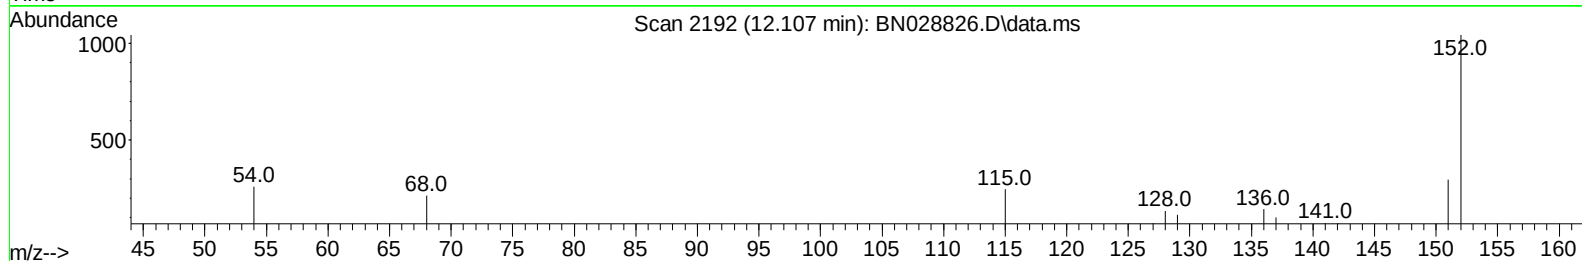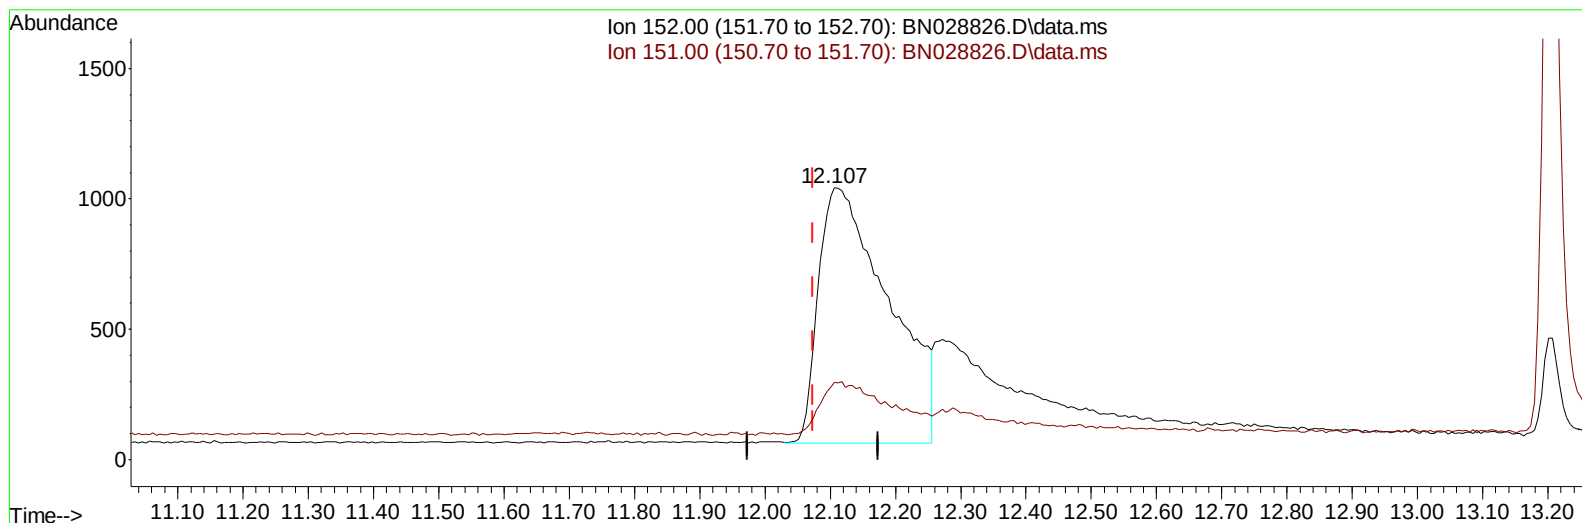

TIC: BN028826.D\data.ms

(6) 2-Methylnaphthalene-d10 (SURR)

12.107min (+ 0.033) 0.30 ng/ul m

response 7352

Ion	Exp%	Act%
152.00	100.00	100.00
151.00	20.50	9.92#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112223\
 Data File : BN028826.D
 Acq On : 22 Nov 2023 00:27
 Operator : MA/JU
 Sample : 05281-06
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AC7

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/23/2023
 Supervised By :mohammad ahmed 11/25/2023

Quant Time: Nov 22 00:58:12 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 21 23:49:43 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.723	152	5097	0.400	ng/ul	#-0.01
4) Naphthalene-d8	10.457	136	16140	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.298	164	13258	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.061	188	26409	0.400	ng/ul	0.00
17) Chrysene-d12	21.279	240	18969	0.400	ng/ul	0.00
23) Perylene-d12	23.538	264	25017	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.099	96	30011	5.327	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.107	152	7352m	0.303	ng/ul	0.03
18) Fluoranthene-d10	19.095	212	26339	0.431	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.137	88	3993	0.641	ng/ul#	84

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112223\
Data File : BN028826.D
Acq On : 22 Nov 2023 00:27
Operator : MA/JU
Sample : 05281-06
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AC7

Manual IntegrationsAPPROVED

Quant Time: Nov 22 00:58:12 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 21 23:49:43 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/23/2023
Supervised By :mohammad ahmed 11/25/2023

