




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112223\
 Data File : BN028827.D
 Acq On : 22 Nov 2023 01:03
 Operator : MA/JU
 Sample : 05281-07
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AC8

Manual IntegrationsAPPROVED

Quant Time: Nov 22 01:59:17 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 21 23:49:43 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/23/2023
 Supervised By :mohammad ahmed 11/25/2023

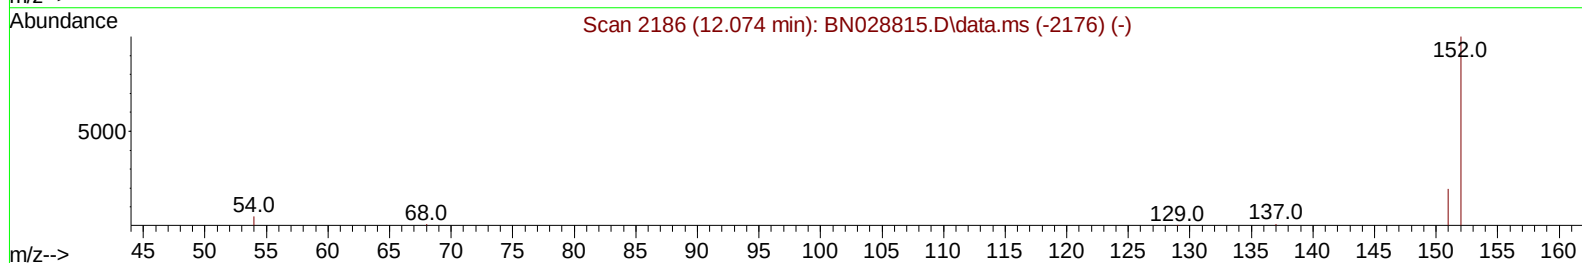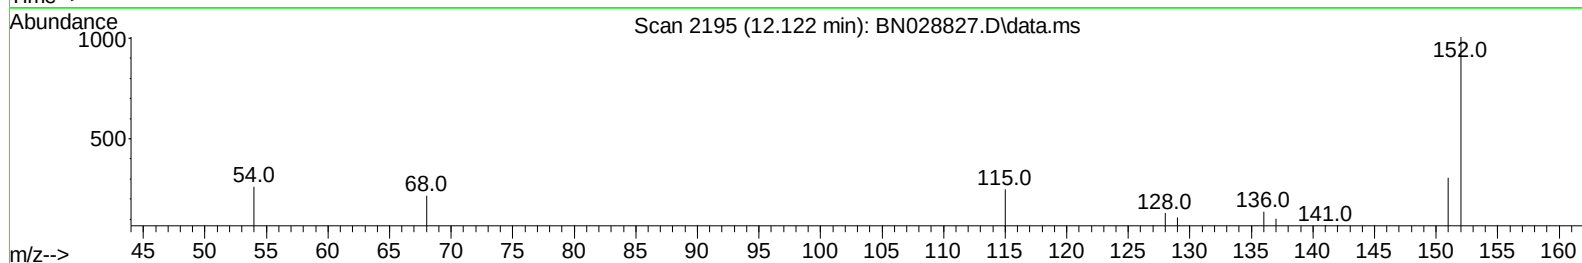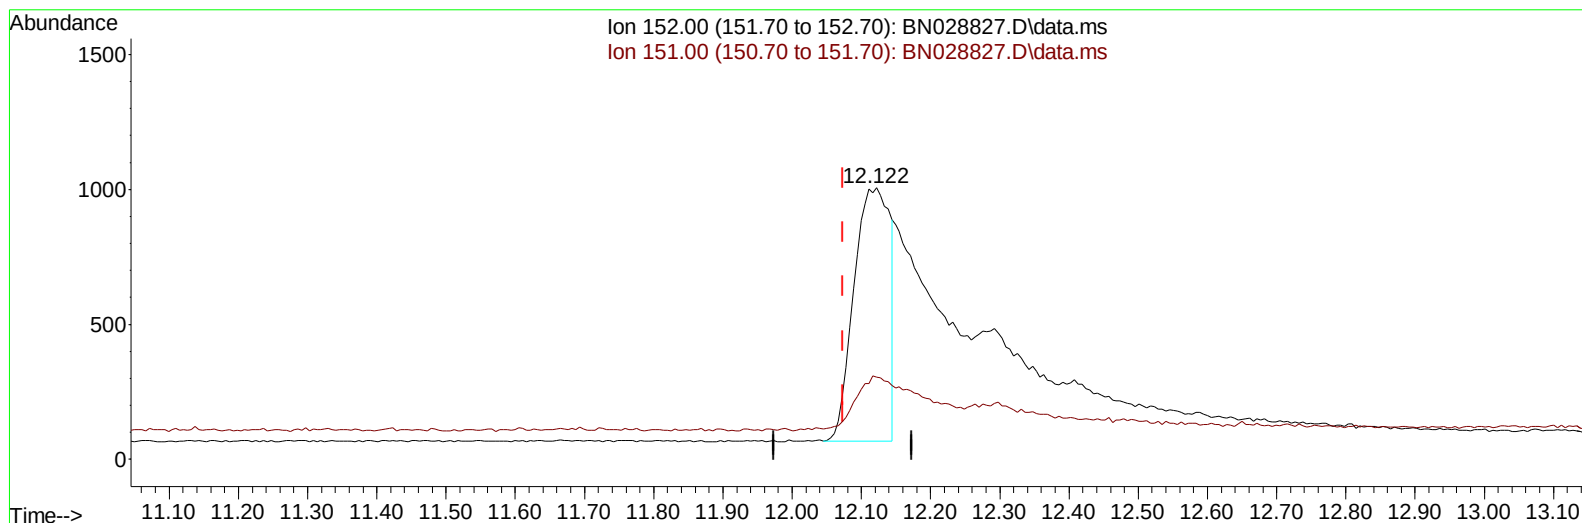

TIC: BN028827.D\data.ms

(6) 2-Methylnaphthalene-d10 (SURR)

12.122min (+ 0.048) 0.18 ng/u1

response 3362

Ion	Exp%	Act%
152.00	100.00	100.00
151.00	20.50	19.24
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112223\
 Data File : BN028827.D
 Acq On : 22 Nov 2023 01:03
 Operator : MA/JU
 Sample : 05281-07
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AC8

Manual IntegrationsAPPROVED

Quant Time: Nov 22 01:59:17 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 21 23:49:43 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/23/2023
 Supervised By :mohammad ahmed 11/25/2023

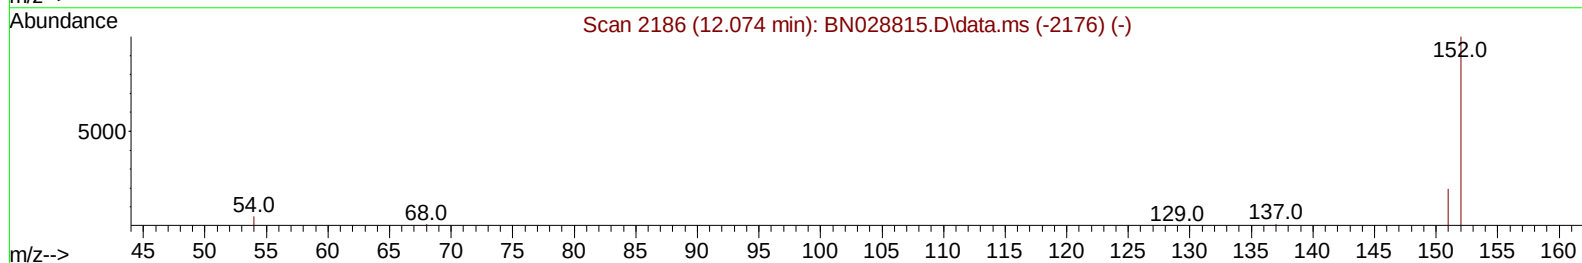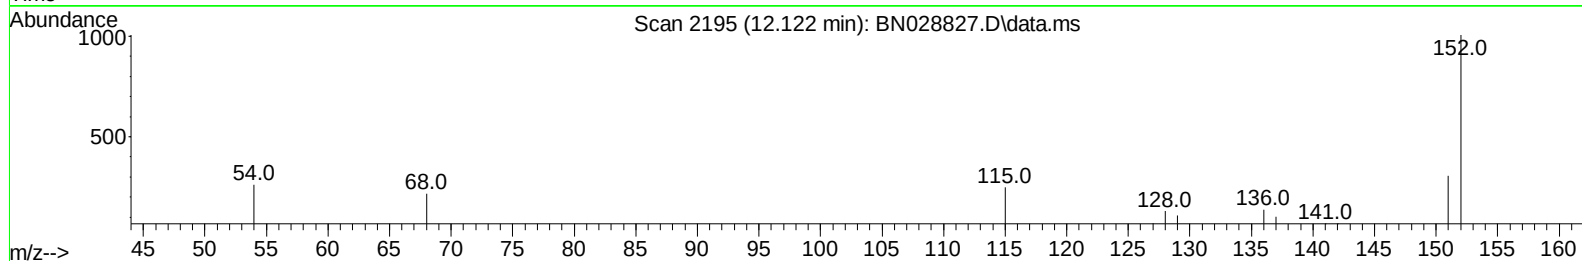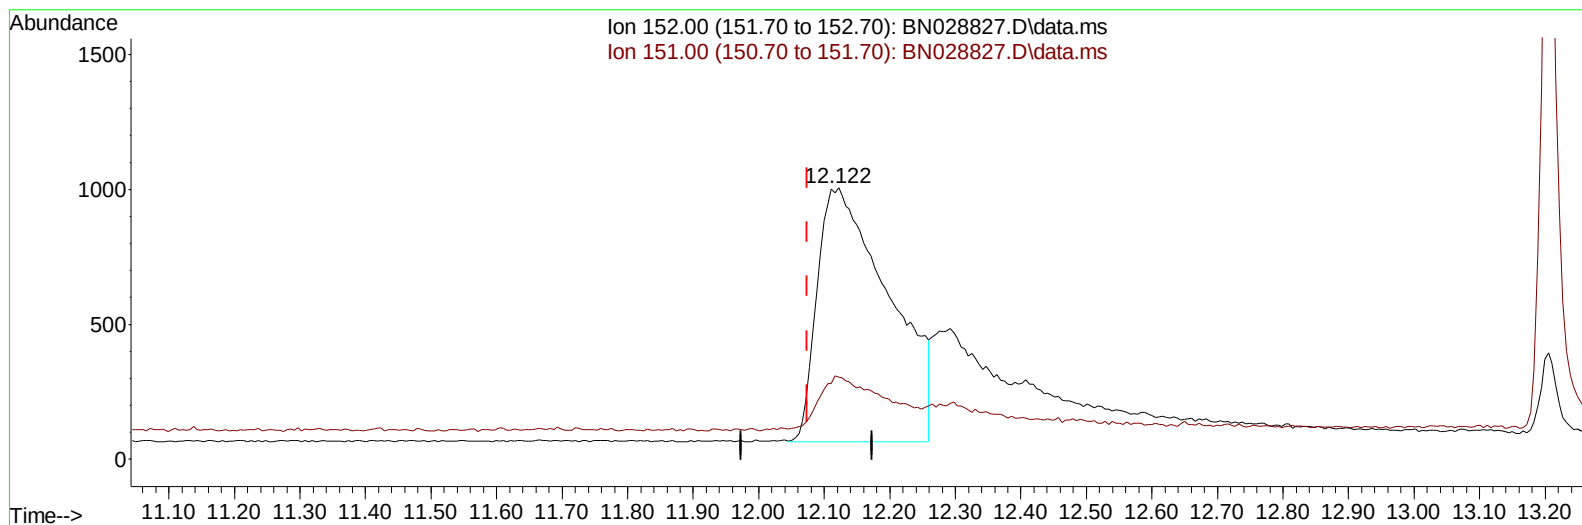

TIC: BN028827.D\data.ms

(6) 2-Methylnaphthalene-d10 (SURR)

12.122min (+ 0.048) 0.39 ng/ul m

response 7175

Ion	Exp%	Act%
152.00	100.00	100.00
151.00	20.50	9.02#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112223\
 Data File : BN028827.D
 Acq On : 22 Nov 2023 01:03
 Operator : MA/JU
 Sample : 05281-07
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AC8

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/23/2023
 Supervised By :mohammad ahmed 11/25/2023

Quant Time: Nov 22 01:59:17 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 21 23:49:43 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.736	152	3911	0.400	ng/ul	# 0.00
4) Naphthalene-d8	10.455	136	12253	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.301	164	10404	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.064	188	20299	0.400	ng/ul	0.00
17) Chrysene-d12	21.283	240	14637	0.400	ng/ul	# 0.01
23) Perylene-d12	23.542	264	19623	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.099	96	35226	8.149	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.122	152	7175m	0.389	ng/ul	0.05
18) Fluoranthene-d10	19.093	212	26932	0.572	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112223\
Data File : BN028827.D
Acq On : 22 Nov 2023 01:03
Operator : MA/JU
Sample : 05281-07
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AC8

Manual IntegrationsAPPROVED

Quant Time: Nov 22 01:59:17 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 21 23:49:43 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/23/2023
Supervised By :mohammad ahmed 11/25/2023

