




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112223\
Data File : BN028830.D
Acq On : 22 Nov 2023 02:50
Operator : MA/JU
Sample : 05281-10
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AD1

Manual IntegrationsAPPROVED

Quant Time: Nov 22 03:21:58 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 21 23:49:43 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/23/2023
Supervised By :mohammad ahmed 11/25/2023

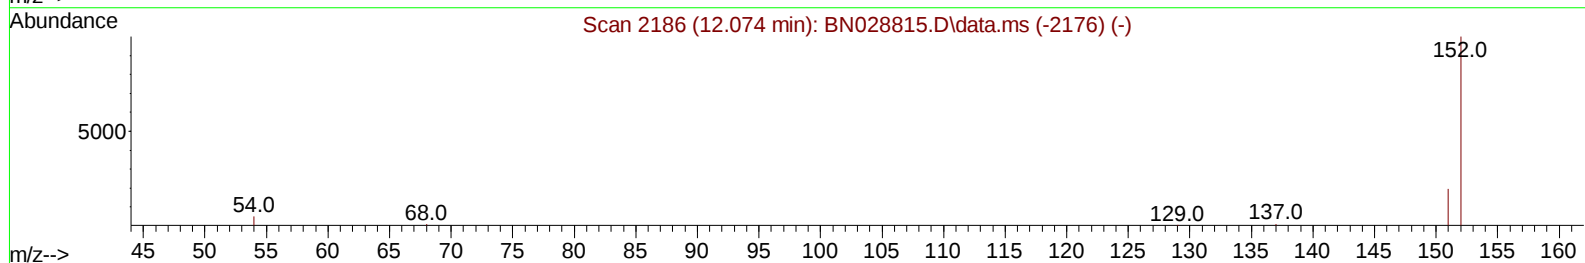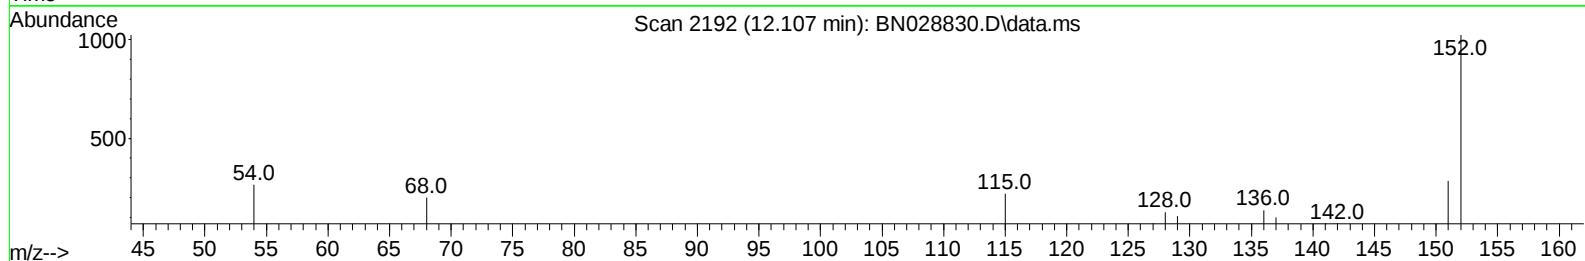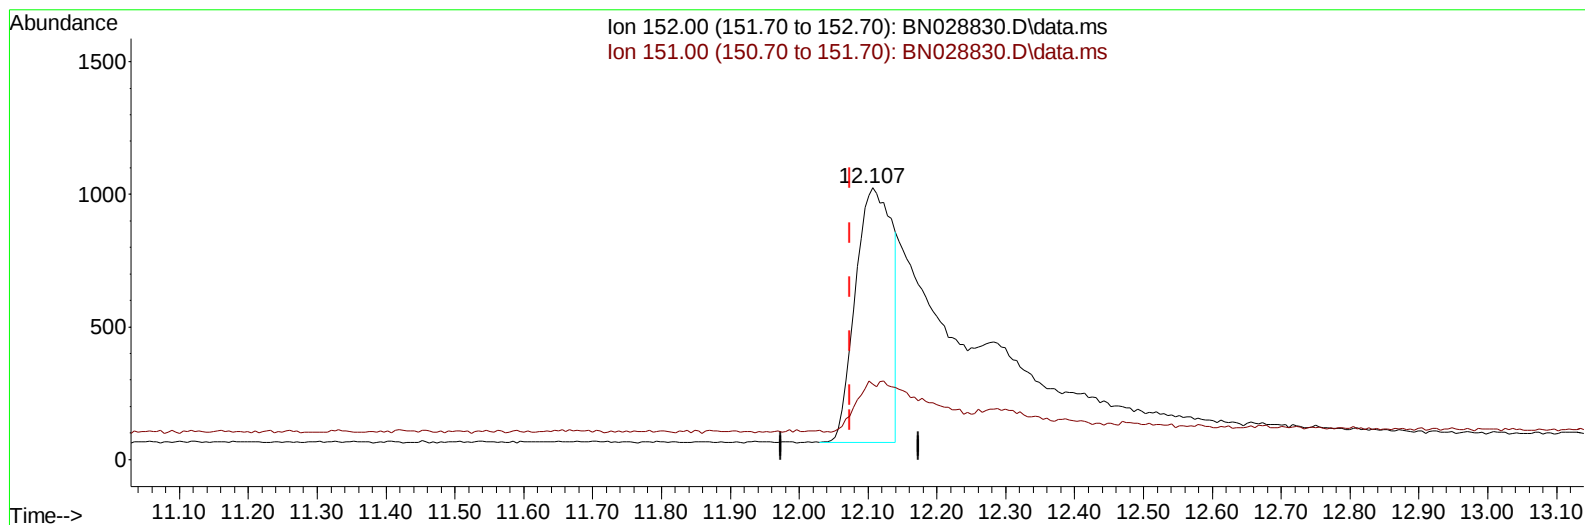

TIC: BN028830.D\data.ms

(6) 2-Methylnaphthalene-d10 (SURR)

12.107min (+ 0.033) 0.14 ng/u1

response 3549

Ion	Exp%	Act%
152.00	100.00	100.00
151.00	20.50	19.67
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112223\
 Data File : BN028830.D
 Acq On : 22 Nov 2023 02:50
 Operator : MA/JU
 Sample : 05281-10
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AD1

Manual IntegrationsAPPROVED

Quant Time: Nov 22 03:21:58 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 21 23:49:43 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/23/2023
 Supervised By :mohammad ahmed 11/25/2023

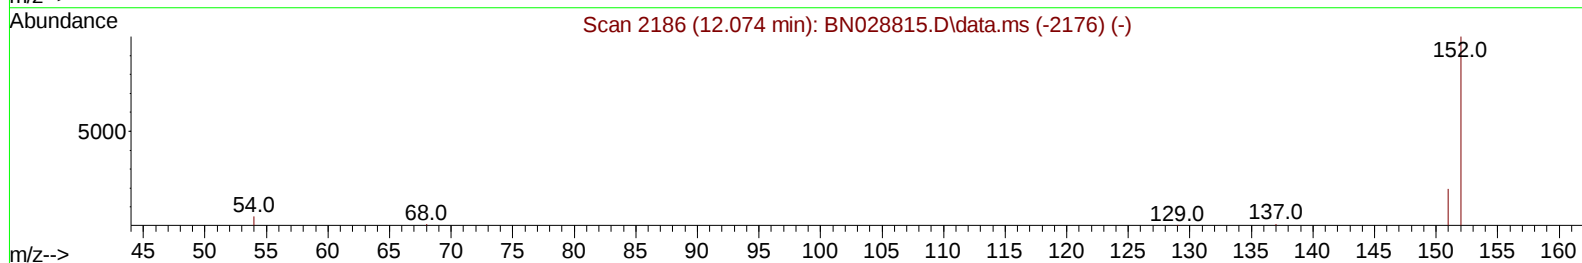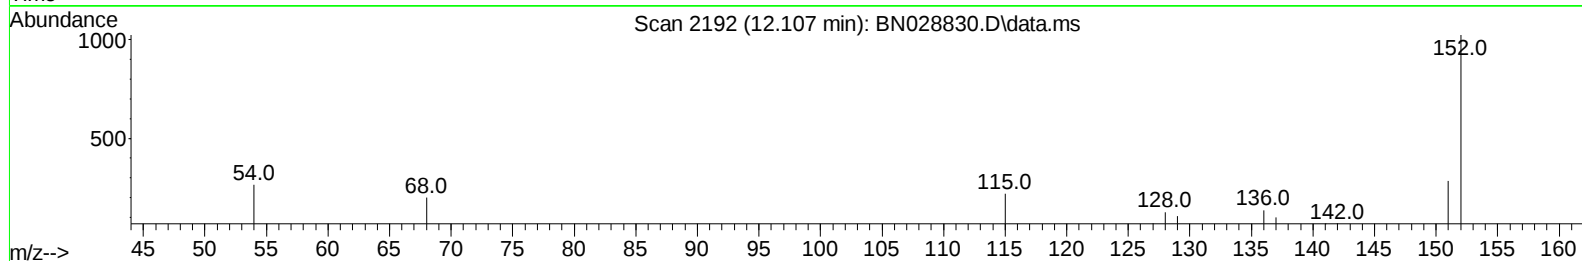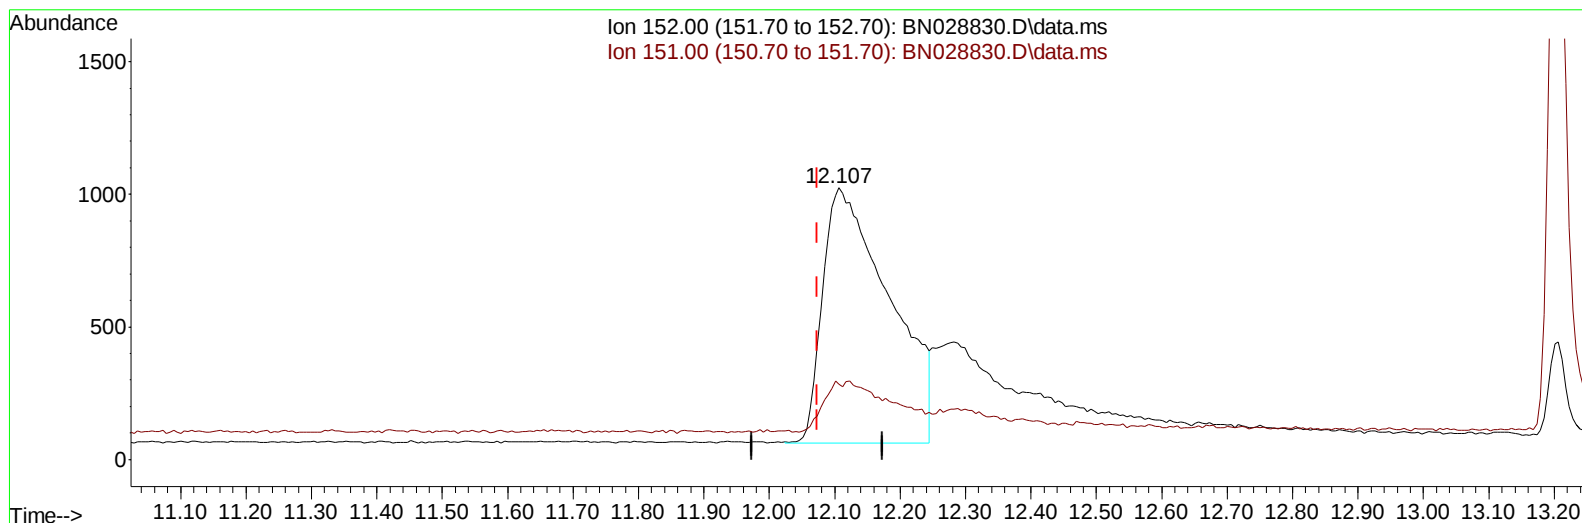

TIC: BN028830.D\data.ms

(6) 2-Methylnaphthalene-d10 (SURR)

12.107min (+ 0.033) 0.27 ng/ul m

response 6826

Ion	Exp%	Act%
152.00	100.00	100.00
151.00	20.50	10.23#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112223\
 Data File : BN028830.D
 Acq On : 22 Nov 2023 02:50
 Operator : MA/JU
 Sample : 05281-10
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AD1

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/23/2023
 Supervised By :mohammad ahmed 11/25/2023

Quant Time: Nov 22 03:21:58 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 21 23:49:43 2023
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.723	152		5131	0.400	ng/ul	#-0.01
4) Naphthalene-d8	10.451	136		16888	0.400	ng/ul	#-0.01
9) Acenaphthene-d10	14.297	164		13081	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.060	188		25539	0.400	ng/ul	0.00
17) Chrysene-d12	21.281	240		16715	0.400	ng/ul	# 0.01
23) Perylene-d12	23.540	264		20886	0.400	ng/ul	# 0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.103	96		39851	7.027	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.107	152		6826m	0.268	ng/ul	0.03
18) Fluoranthene-d10	19.094	212		26890	0.500	ng/ul	0.00
Target Compounds							
							Qvalue
2) 1,4-Dioxane	3.141	88		3887	0.620	ng/ul#	80

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112223\
Data File : BN028830.D
Acq On : 22 Nov 2023 02:50
Operator : MA/JU
Sample : 05281-10
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AD1

Manual IntegrationsAPPROVED

Quant Time: Nov 22 03:21:58 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 21 23:49:43 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/23/2023
Supervised By :mohammad ahmed 11/25/2023

