




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112223\
 Data File : BN028843.D
 Acq On : 22 Nov 2023 17:30
 Operator : MA/JU
 Sample : 05268-20
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SLCS054

Manual IntegrationsAPPROVED

Quant Time: Nov 22 23:01:07 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 21 23:49:43 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/25/2023
 Supervised By :mohammad ahmed 11/25/2023

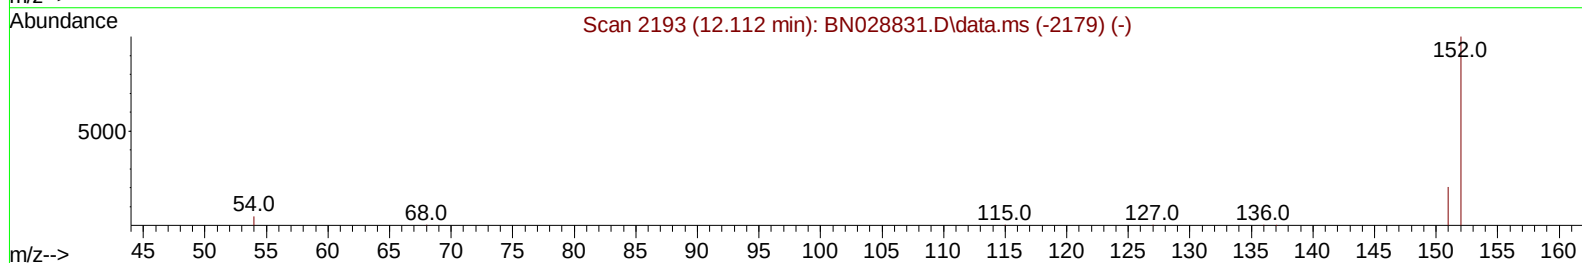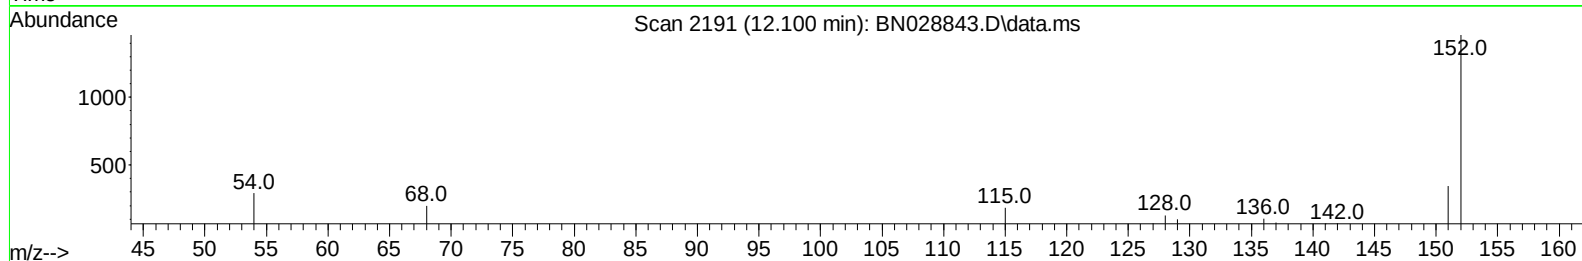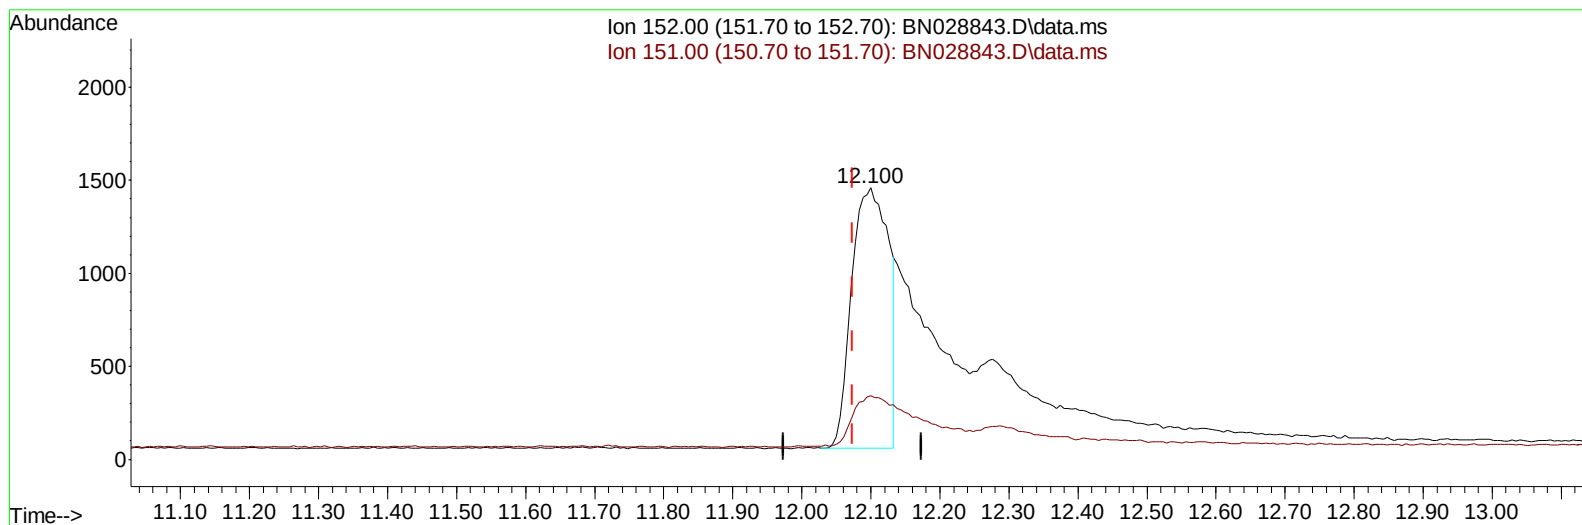

TIC: BN028843.D\data.ms

(6) 2-Methylnaphthalene-d10 (SURR)

12.100min (+ 0.026) 0.21 ng/u1

response 5219

Ion	Exp%	Act%
152.00	100.00	100.00
151.00	20.50	17.88
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112223\
Data File : BN028843.D
Acq On : 22 Nov 2023 17:30
Operator : MA/JU
Sample : 05268-20
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SLCS054

Manual IntegrationsAPPROVED

Quant Time: Nov 22 23:01:07 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 21 23:49:43 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/25/2023
Supervised By :mohammad ahmed 11/25/2023

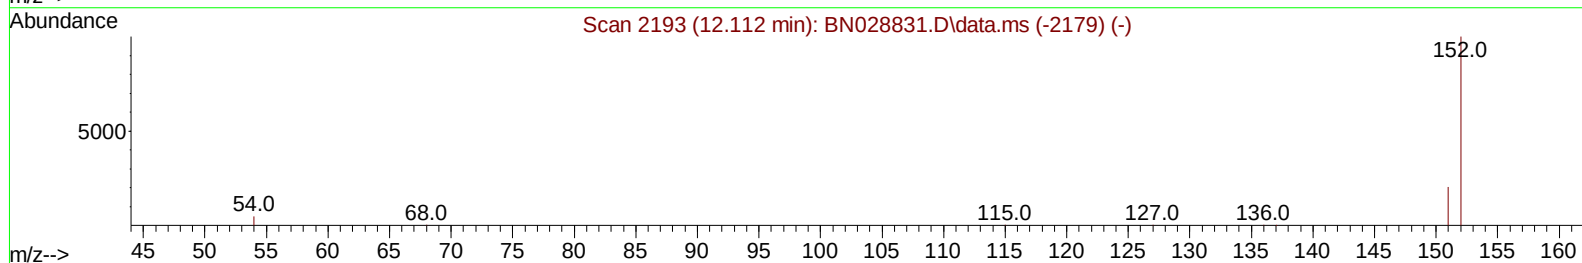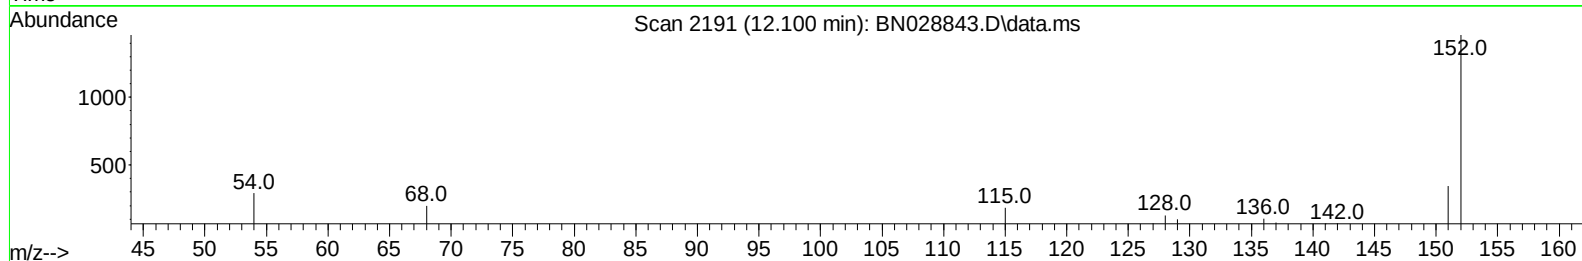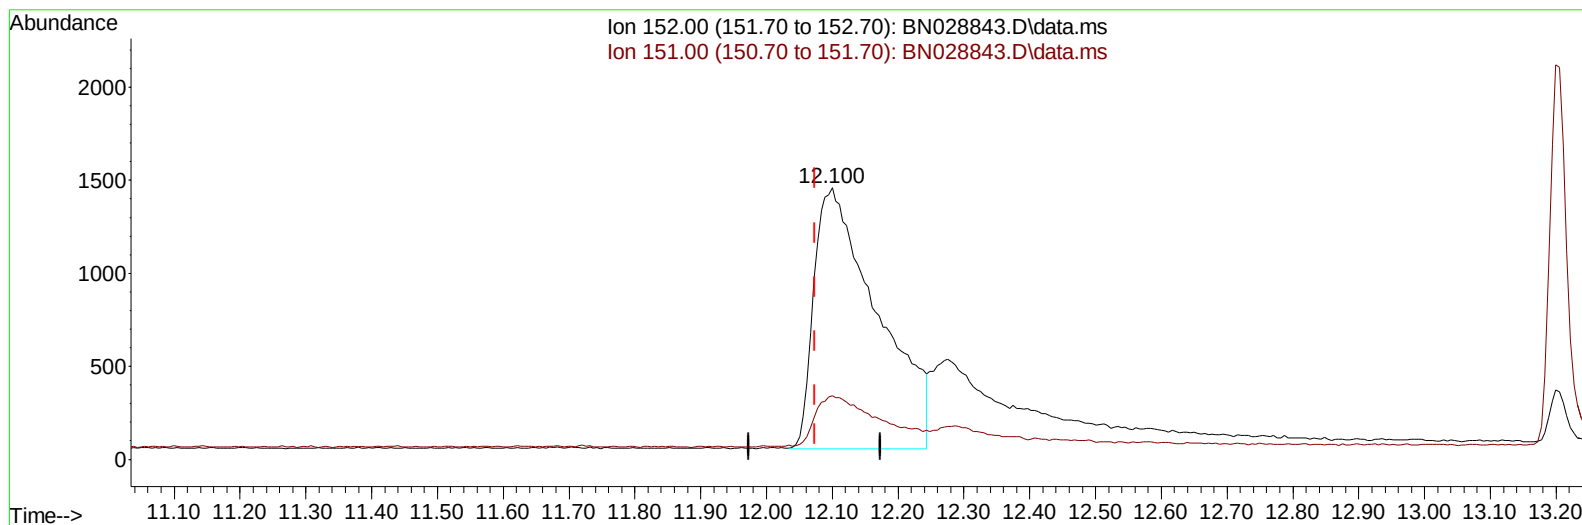

TIC: BN028843.D\data.ms

(6) 2-Methylnaphthalene-d10 (SURR)

12.100min (+ 0.026) 0.39 ng/ul m

response 9410

Ion	Exp%	Act%
152.00	100.00	100.00
151.00	20.50	9.91#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112223\
 Data File : BN028843.D
 Acq On : 22 Nov 2023 17:30
 Operator : MA/JU
 Sample : 05268-20
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SLCS054

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/25/2023
 Supervised By :mohammad ahmed 11/25/2023

Quant Time: Nov 22 23:01:07 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 21 23:49:43 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.706	152	5457	0.400	ng/ul	-0.03
4) Naphthalene-d8	10.444	136	16171	0.400	ng/ul	#-0.02
9) Acenaphthene-d10	14.297	164	10354	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.059	188	18353	0.400	ng/ul	0.00
17) Chrysene-d12	21.286	240	11795	0.400	ng/ul	# 0.02
23) Perylene-d12	23.551	264	15747	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.112	96	37855	6.277	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.100	152	9410m	0.387	ng/ul	0.03
18) Fluoranthene-d10	19.093	212	25040	0.660	ng/ul	0.00

Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112223\
Data File : BN028843.D
Acq On : 22 Nov 2023 17:30
Operator : MA/JU
Sample : 05268-20
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SLCS054

Manual IntegrationsAPPROVED

Quant Time: Nov 22 23:01:07 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 21 23:49:43 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/25/2023
Supervised By :mohammad ahmed 11/25/2023

