

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112223\
 Data File : BN028834.D
 Acq On : 22 Nov 2023 10:06
 Operator : MA/JU
 Sample : 05268-16
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DCKD9

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/23/2023
 Supervised By :mohammad ahmed 11/25/2023

Quant Time: Nov 22 21:36:16 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 21 23:49:43 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.723	152	5279	0.400	ng/ul	#-0.01
4) Naphthalene-d8	10.434	136	24469	0.400	ng/ul	#-0.03
9) Acenaphthene-d10	14.297	164	13294	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.055	188	27902	0.400	ng/ul	0.00
17) Chrysene-d12	21.275	240	21516	0.400	ng/ul	0.00
23) Perylene-d12	23.546	264	25937	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.099	96	33111	5.675	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.067	152	8181m	0.222	ng/ul	0.00
18) Fluoranthene-d10	19.094	212	26186	0.378	ng/ul	0.00
Target Compounds						
16) Anthracene	17.182	178	22559	0.287	ng/ul	Qvalue 95

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112223\
Data File : BN028834.D
Acq On : 22 Nov 2023 10:06
Operator : MA/JU
Sample : 05268-16
Misc :
ALS Vial : 22 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
DCKD9

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/23/2023
Supervised By :mohammad ahmed 11/25/2023


Quant Time: Nov 22 21:36:16 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 21 23:49:43 2023
Response via : Initial Calibration

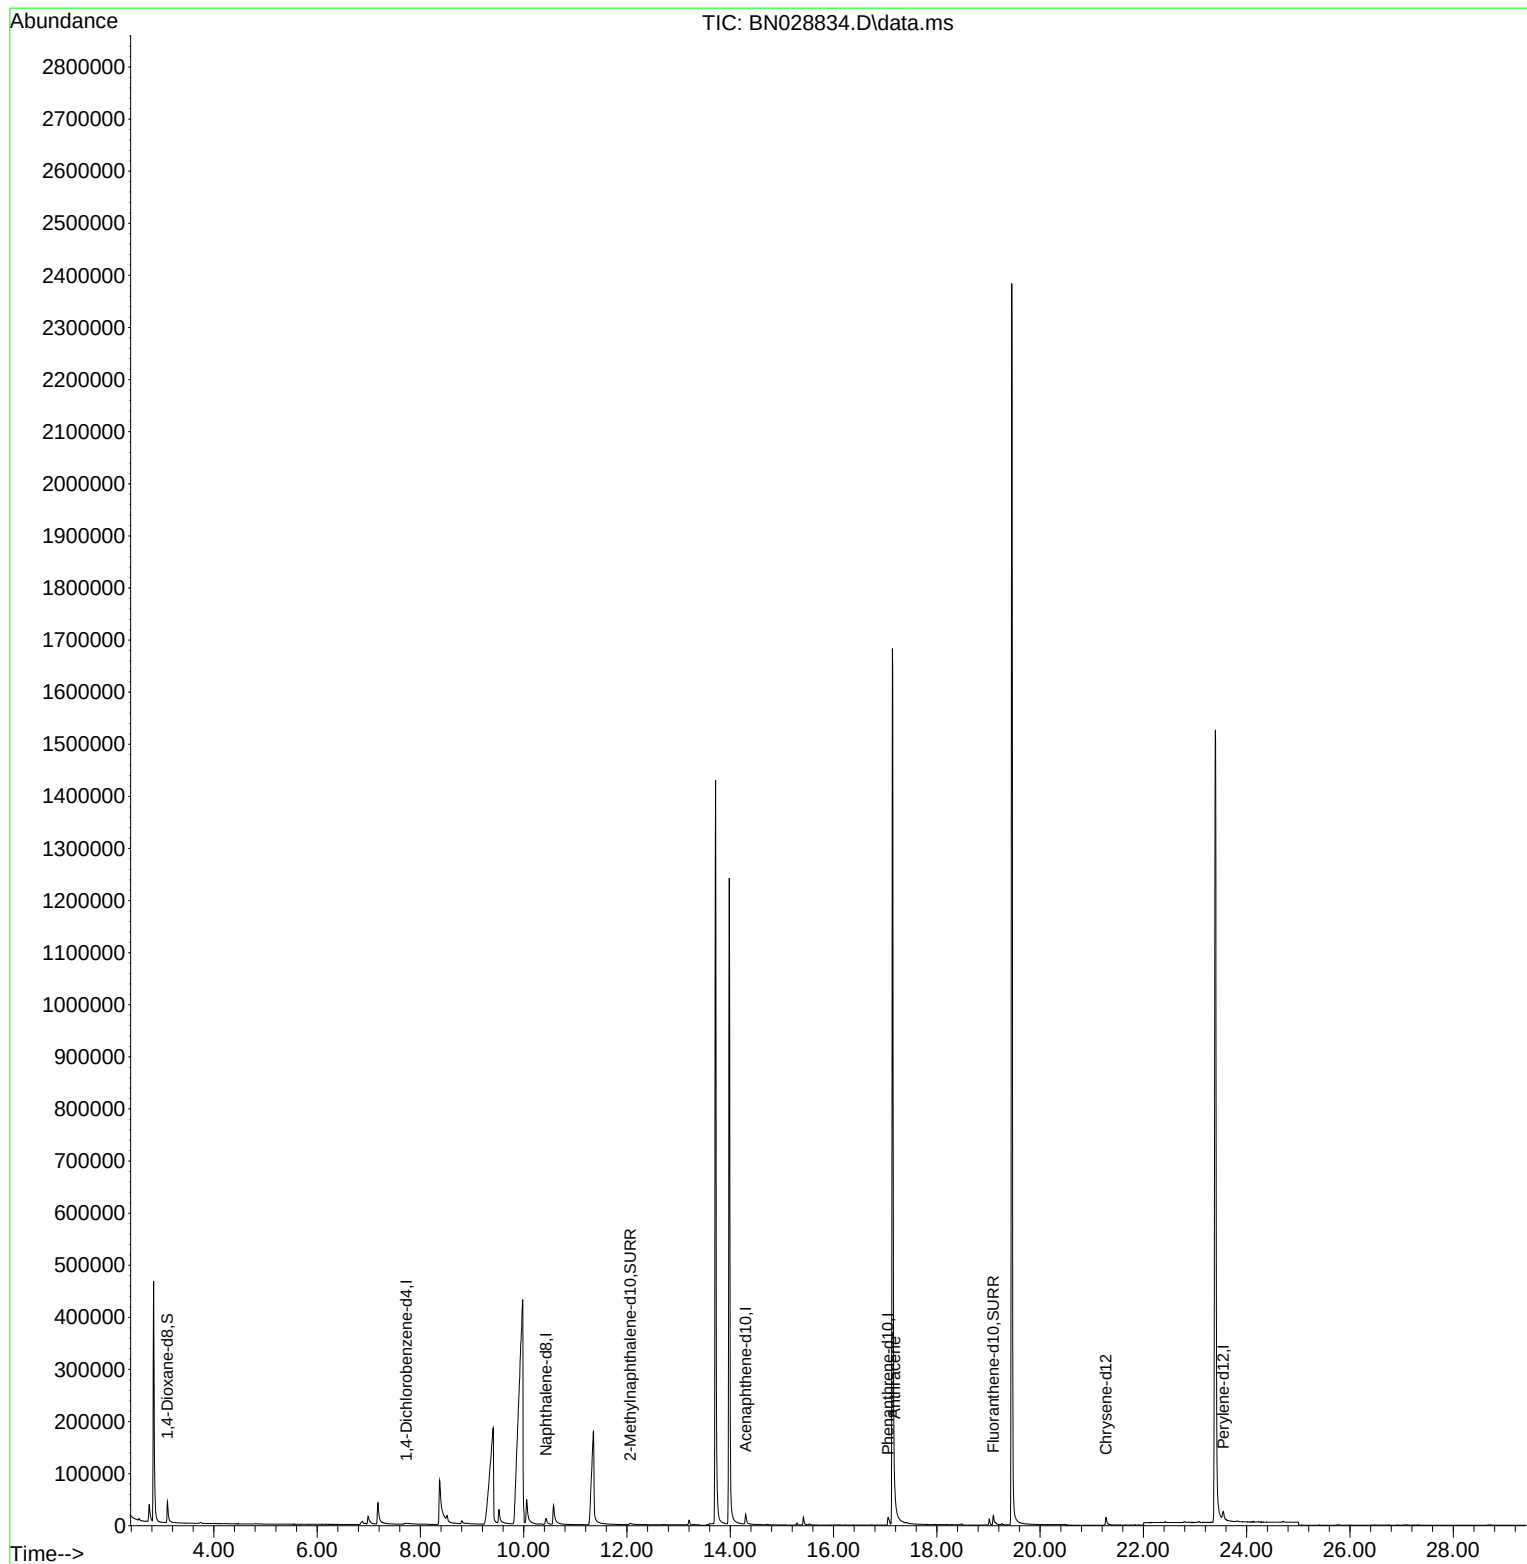

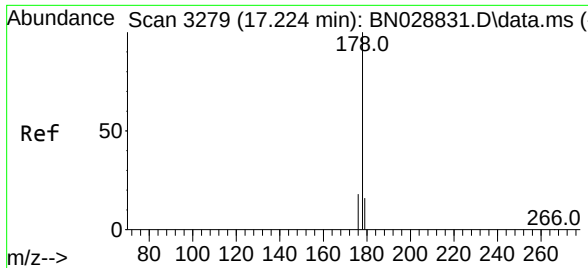

#16
 Anthracene
 Concen: 0.287 ng/ul
 RT: 17.182 min Scan# 31
 Delta R.T. -0.022 min
 Lab File: BN028834.D
 Acq: 22 Nov 2023 10:06

Instrument :
 BNA_N
 ClientSampleId :
 DCKD9

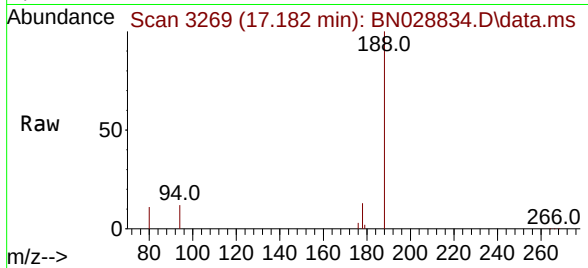

Tgt Ion:178 Resp: 22559
 Ion Ratio Lower Upper
 178 100
 179 18.5 12.6 18.8
 176 20.3 14.9 22.3

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/23/2023
 Supervised By :mohammad ahmed 11/25/2023

